

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 14:54
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 16:51:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 16:50:41 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	172.6E6	50739755	23.594	23.977
28)	SA Decachlor...	8.048	9.040	207.6E6	57263495	25.447	25.999
Target Compounds							
23)	Chlordane-1	4.211	4.975	81333725	27493696	235.719	245.864
24)	Chlordane-2	4.703	5.443	94841126	30293254	247.337	254.956
25)	Chlordane-3	5.261	6.088	277.6E6	93394345	232.010	238.372
26)	Chlordane-4	5.317	6.162	257.2E6	113.1E6	235.147	242.010
27)	Chlordane-5	6.142	6.966	82852264	22242148	233.498	243.470



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 14:54
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 16:51:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 16:50:41 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

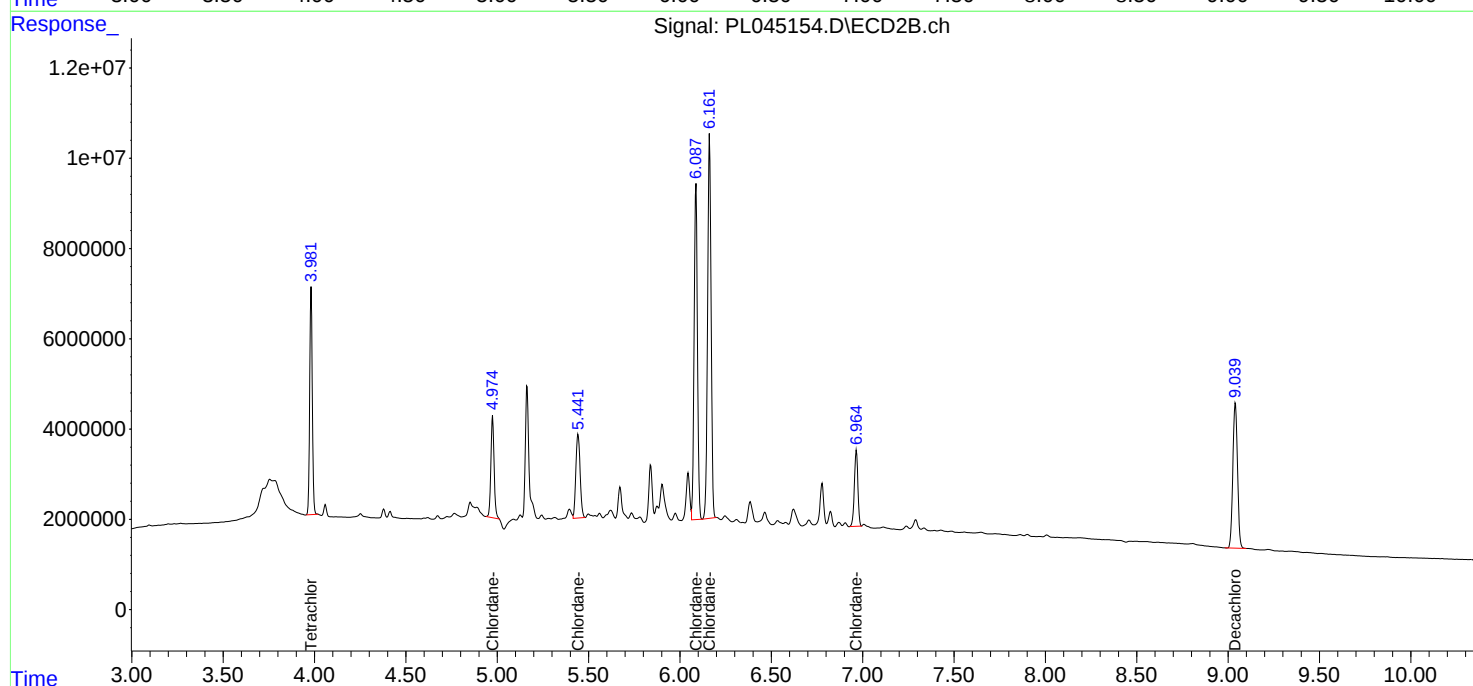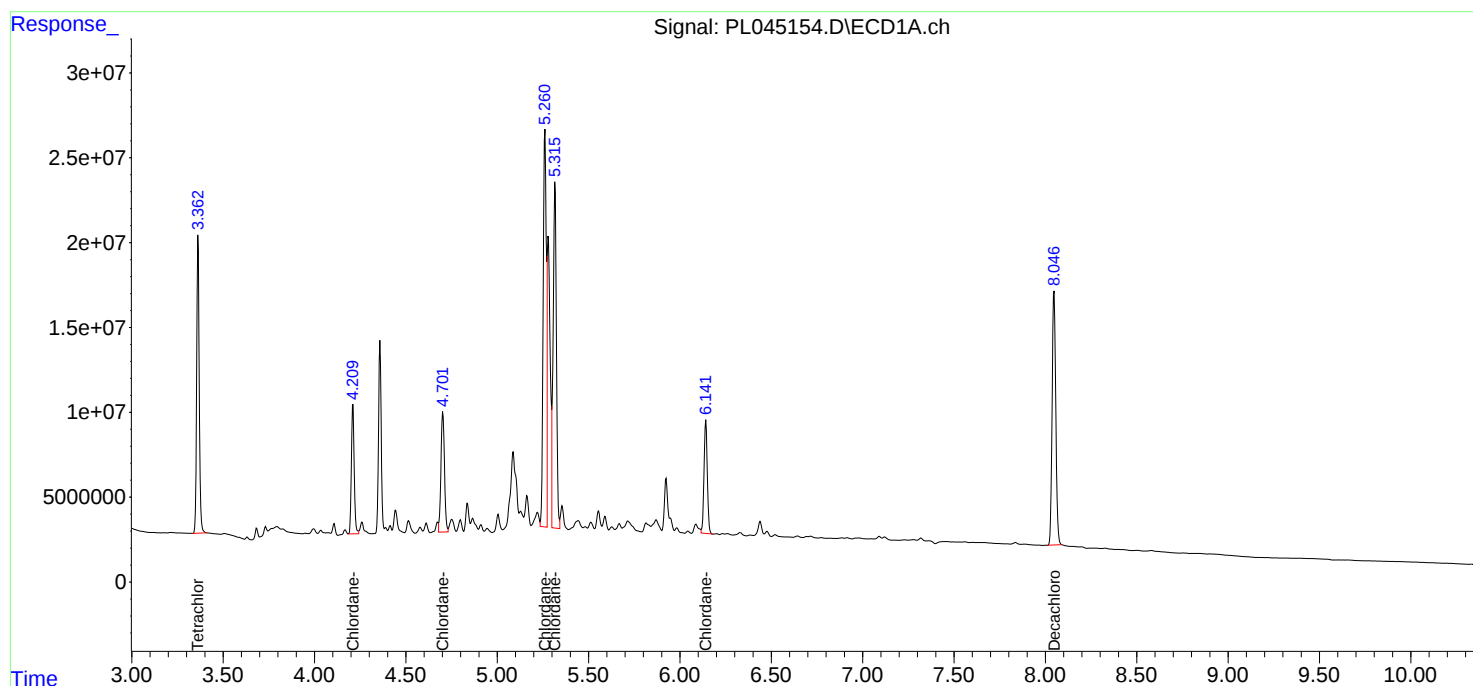


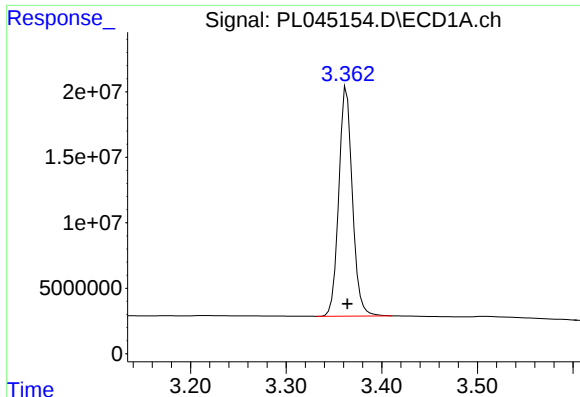

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 172610818
Conc: 23.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

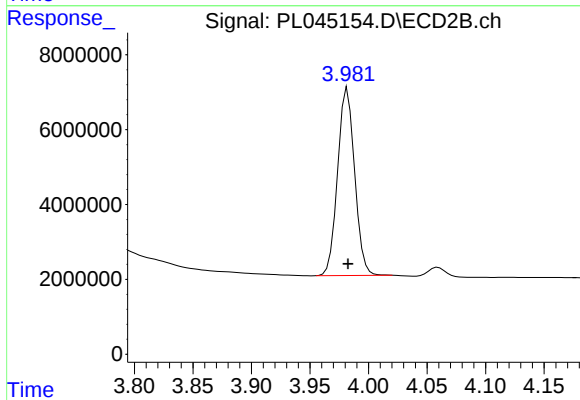


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 50739755
Conc: 23.98 ng/ml

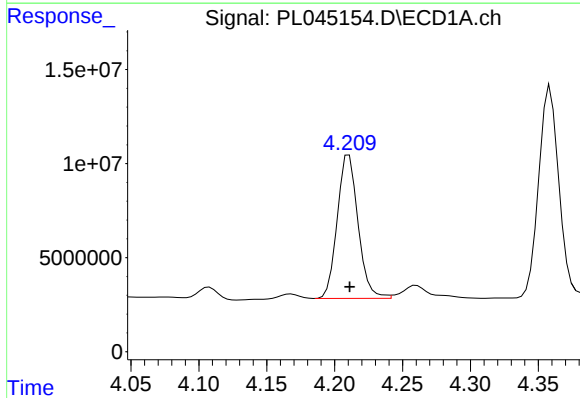


#23 Chlordane-1

R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 81333725
Conc: 235.72 ng/ml

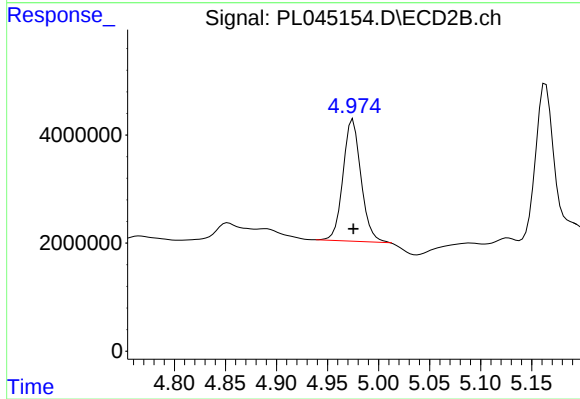

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 27493696
Conc: 245.86 ng/ml

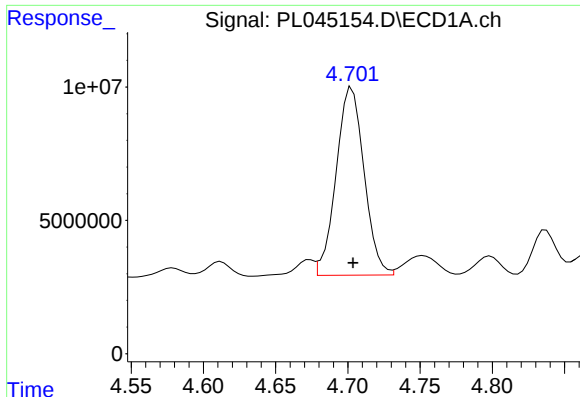

#24 Chlordane-2


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 94841126
Conc: 247.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

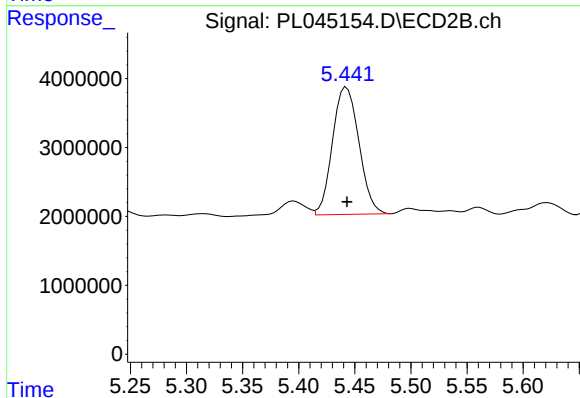


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 30293254
Conc: 254.96 ng/ml

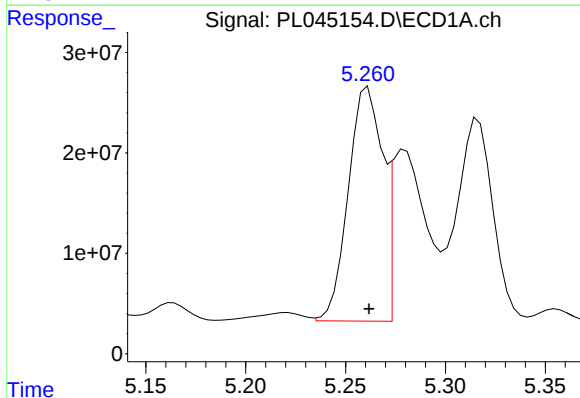


#25 Chlordane-3

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 277589484
Conc: 232.01 ng/ml

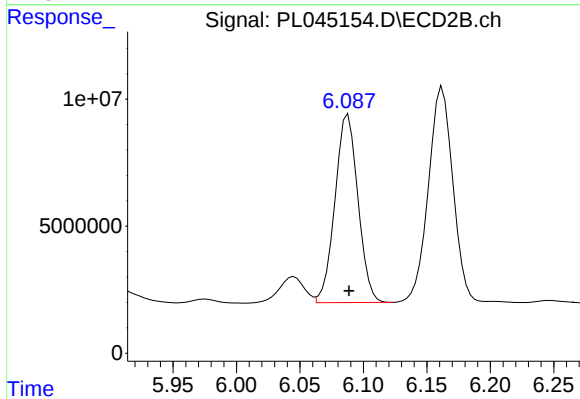

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 93394345
Conc: 238.37 ng/ml

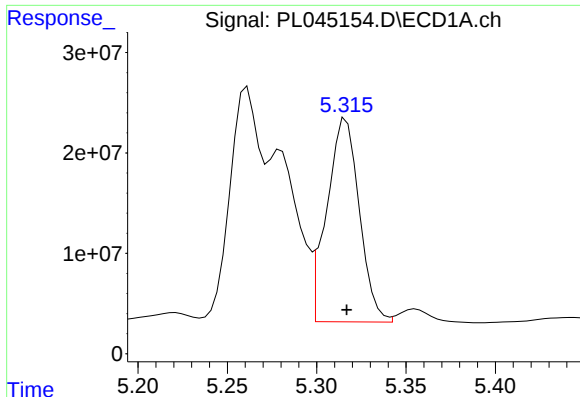

#26 Chlordane-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 257166267
Conc: 235.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

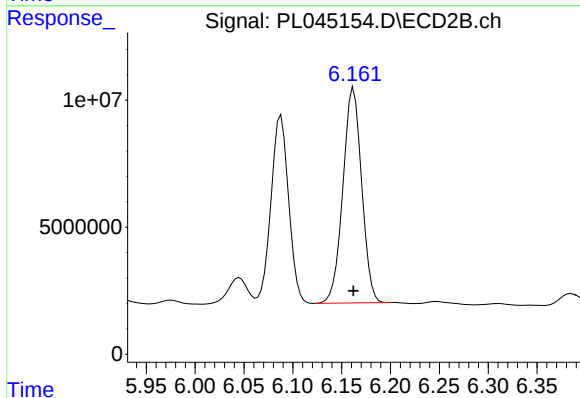


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 113091952
Conc: 242.01 ng/ml

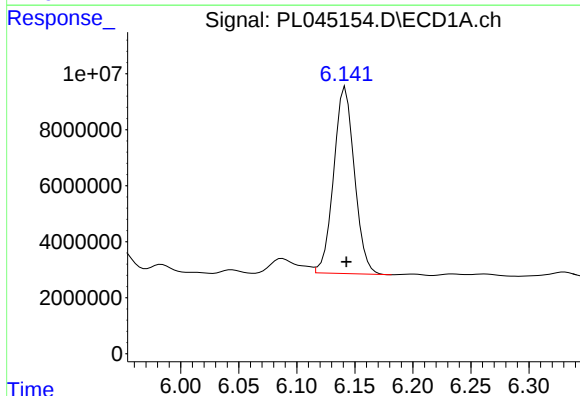


#27 Chlordane-5

R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 82852264
Conc: 233.50 ng/ml

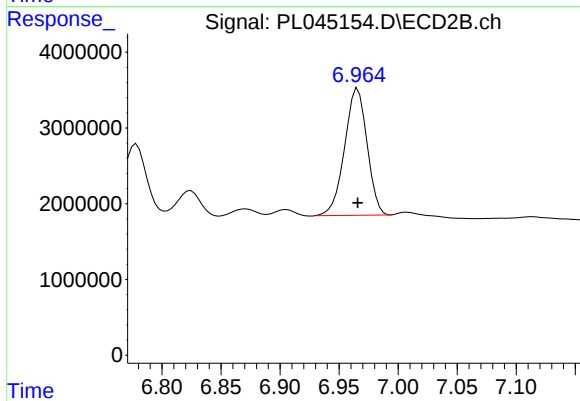

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 22242148
Conc: 243.47 ng/ml

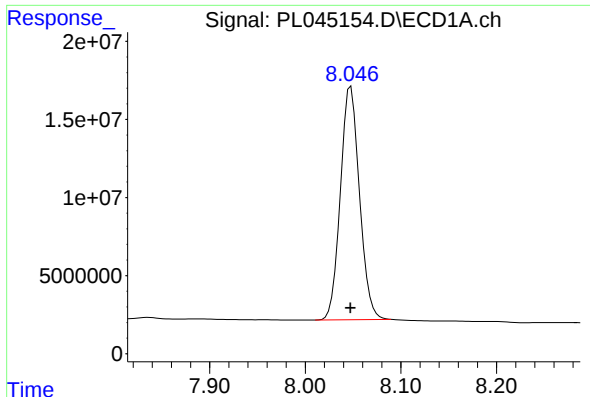

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 207555996
Conc: 25.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

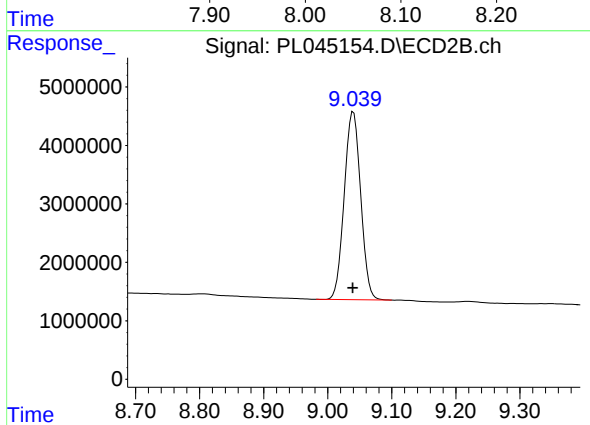

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 57263495
Conc: 26.00 ng/ml