

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 14:26
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 16:51:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 16:50:41 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.983	561.5E6	160.6E6	76.748	75.911
28)	SA Decachlor...	8.048	9.040	602.4E6	160.7E6	73.862	72.969
Target Compounds							
23)	Chlordane-1	4.211	4.975	266.2E6	84547489	771.355	756.070
24)	Chlordane-2	4.703	5.443	286.5E6	87516480	747.265	736.561
25)	Chlordane-3	5.261	6.089	906.3E6	301.4E6	757.448	769.175
26)	Chlordane-4	5.317	6.163	842.4E6	357.1E6	770.274	764.268
27)	Chlordane-5	6.143	6.966	275.8E6	69955083	777.288	765.751


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 14:26
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 16:51:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 16:50:41 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

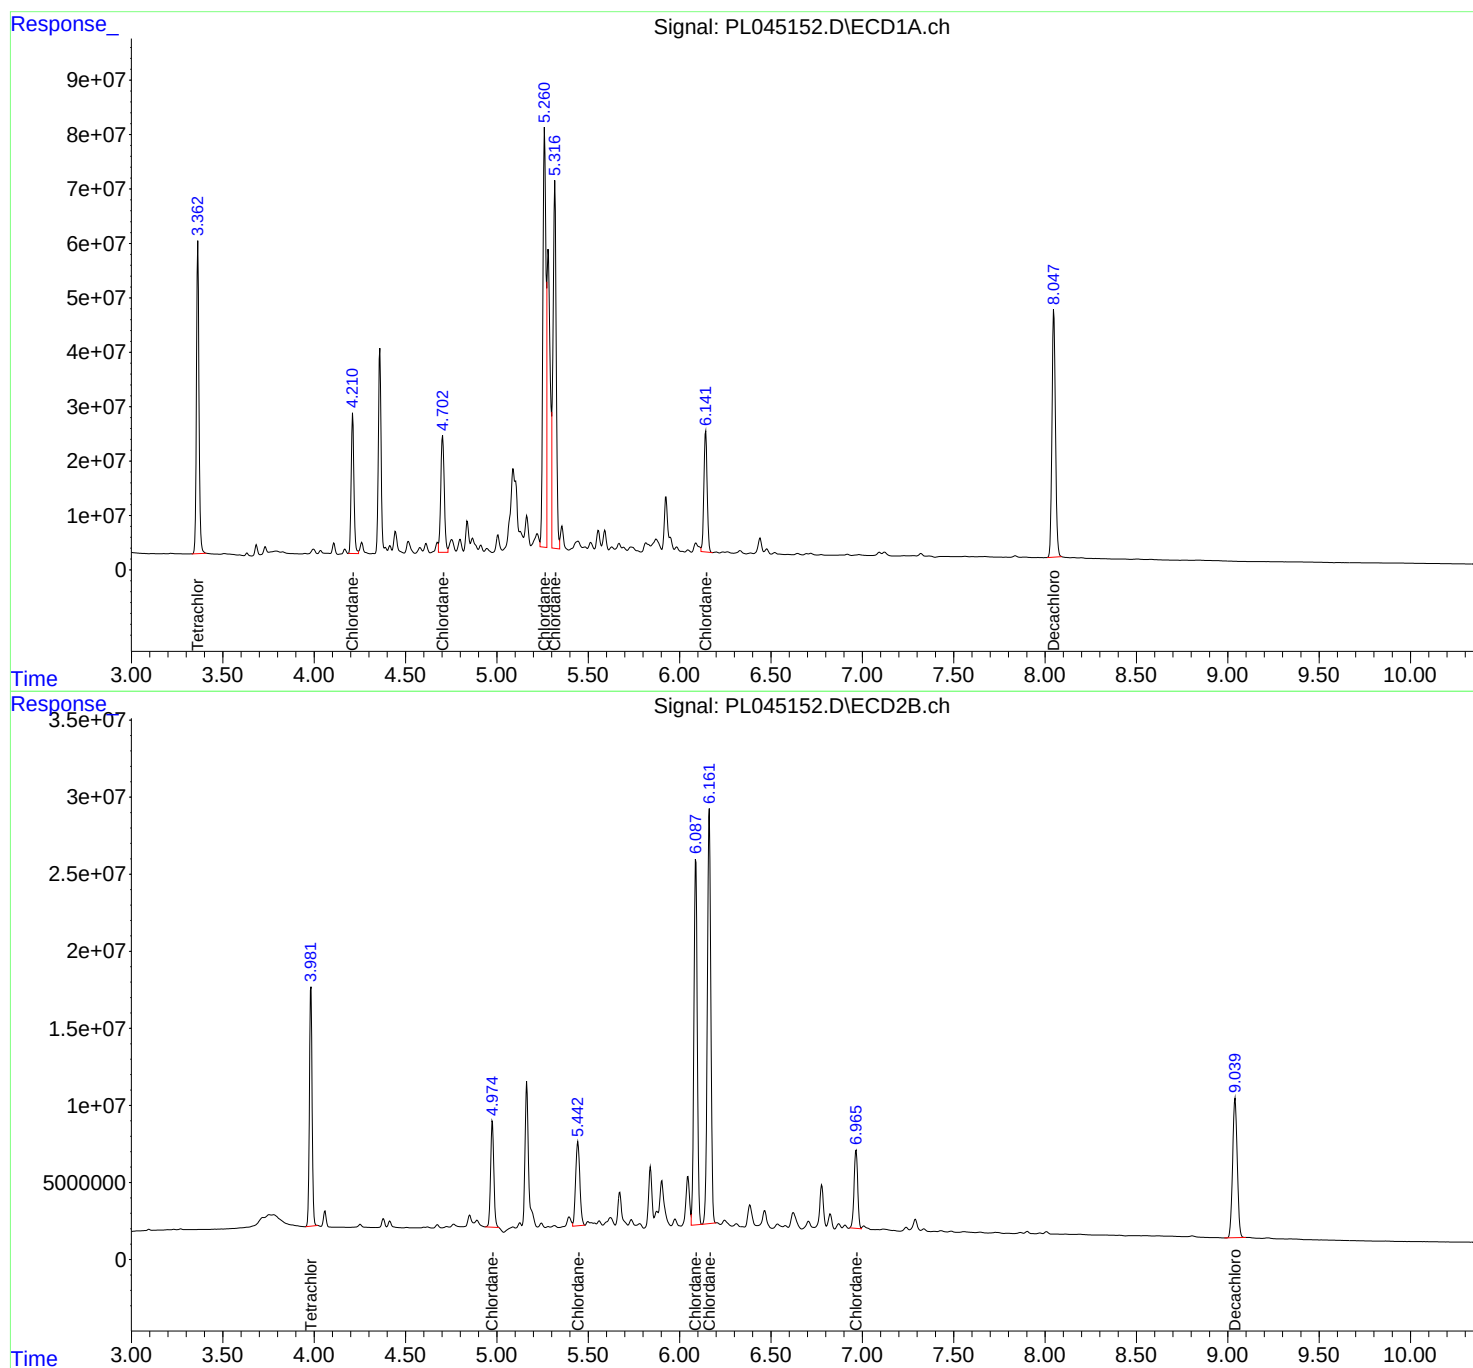


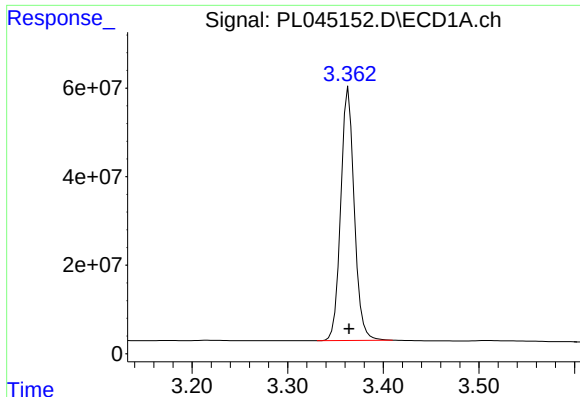

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 561476454
Conc: 76.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

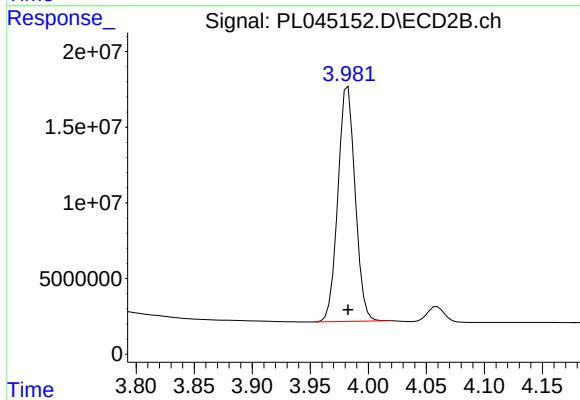


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 160639099
Conc: 75.91 ng/ml

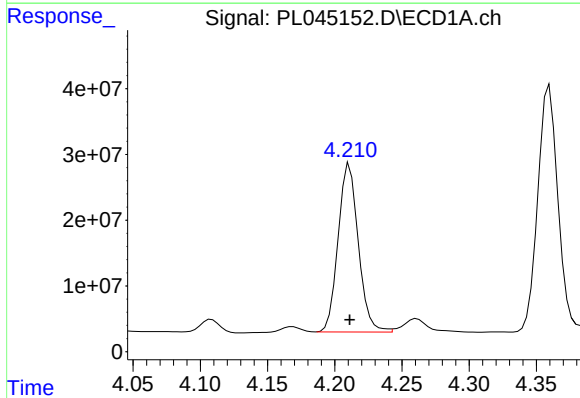


#23 Chlordane-1

R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 266152634
Conc: 771.35 ng/ml

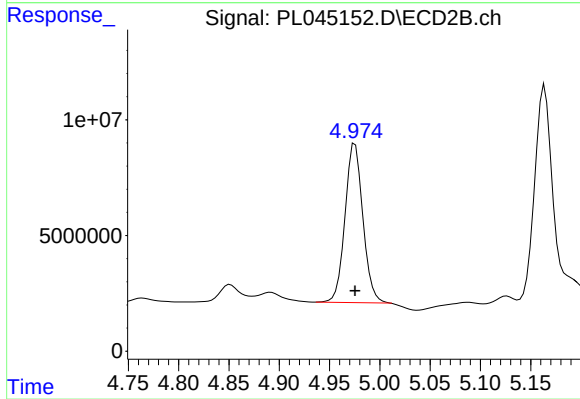

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 84547489
Conc: 756.07 ng/ml

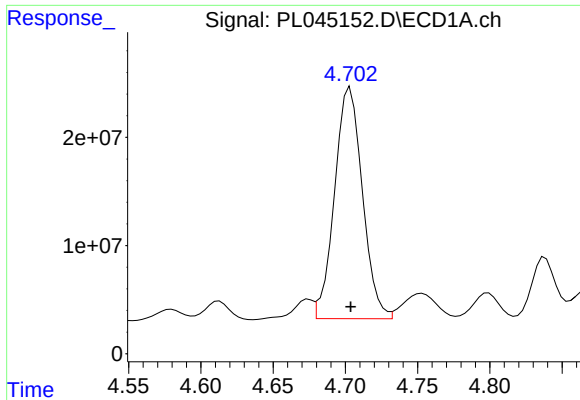

#24 Chlordane-2


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 286538006
Conc: 747.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

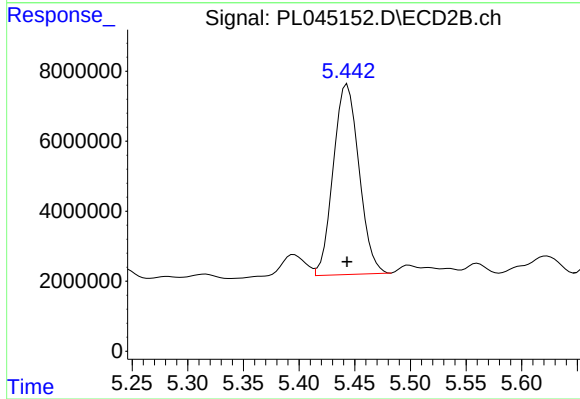


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 87516480
Conc: 736.56 ng/ml

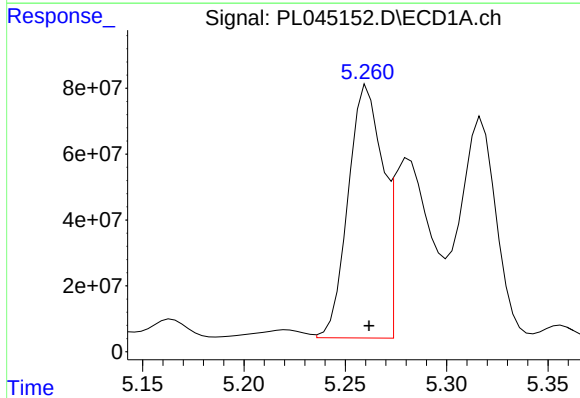


#25 Chlordane-3

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 906254006
Conc: 757.45 ng/ml

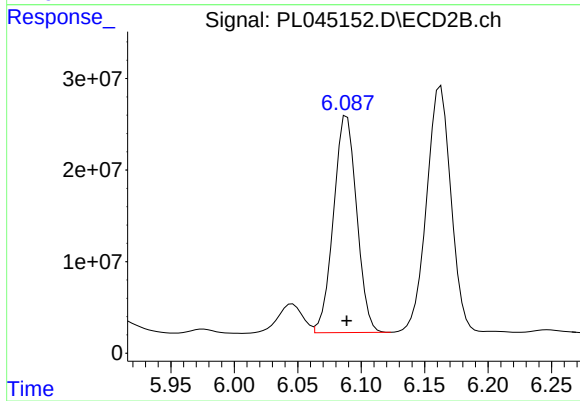

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 301363198
Conc: 769.17 ng/ml

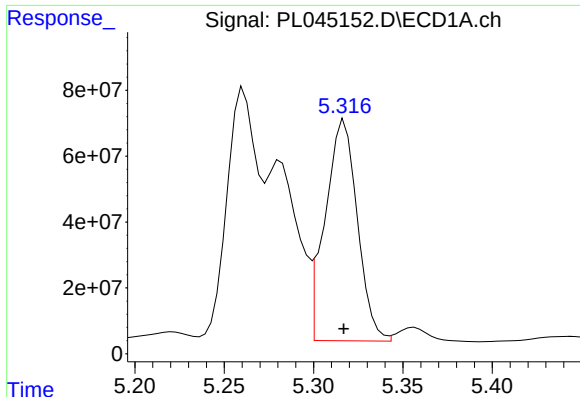

#26 Chlordane-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 842402129
Conc: 770.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

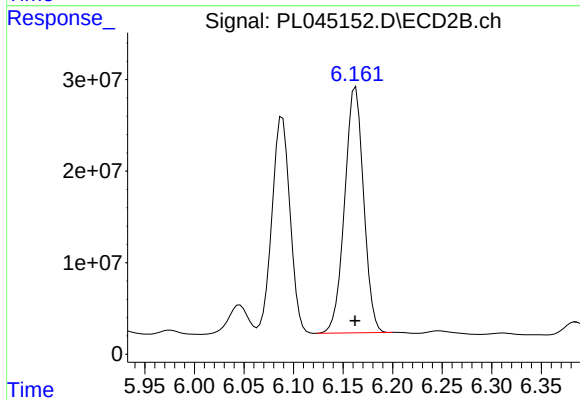


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 357144817
Conc: 764.27 ng/ml

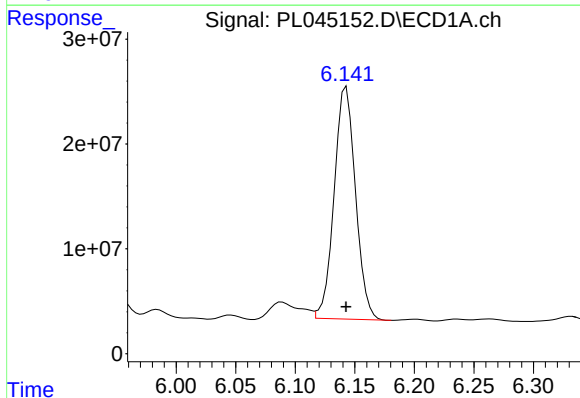


#27 Chlordane-5

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 275805847
Conc: 777.29 ng/ml

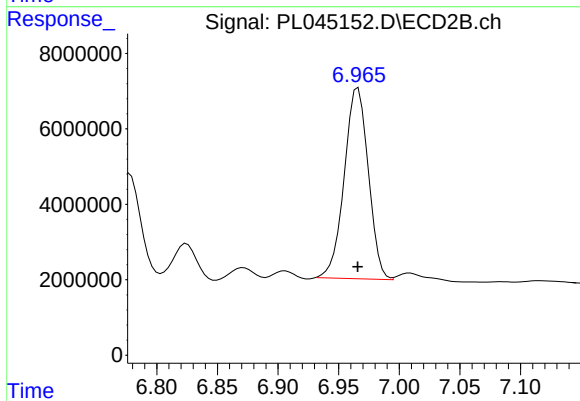

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 69955083
Conc: 765.75 ng/ml

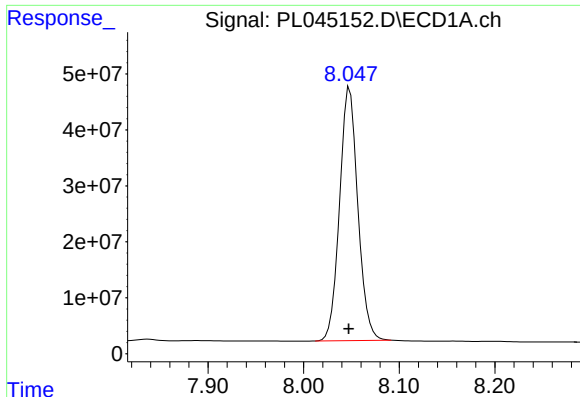

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 602437591
Conc: 73.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

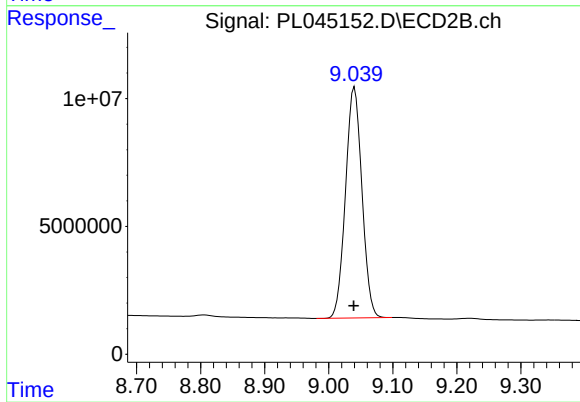

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 160717829
Conc: 72.97 ng/ml