

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 14:40
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 16:51:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 16:50:41 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	365.8E6	105.8E6	50.000	50.000
28)	SA Decachlor...	8.047	9.039	407.8E6	110.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.211	4.975	172.5E6	55912488	500.000	500.000
24)	Chlordane-2	4.704	5.443	191.7E6	59408882	500.000	500.000
25)	Chlordane-3	5.262	6.089	598.2E6	195.9E6	500.000	500.000
26)	Chlordane-4	5.317	6.162	546.8E6	233.7E6	500.000	500.000
27)	Chlordane-5	6.143	6.966	177.4E6	45677450	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 14:40
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 16:51:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 16:50:41 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

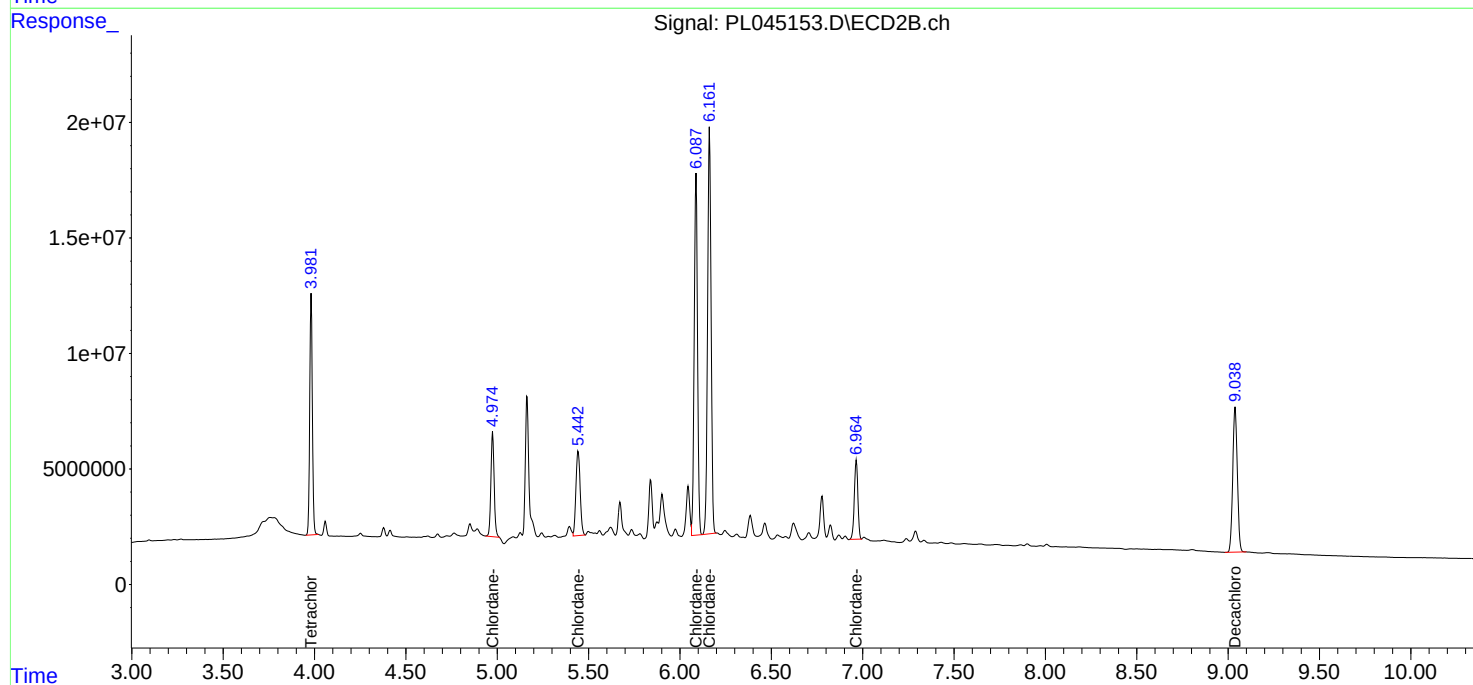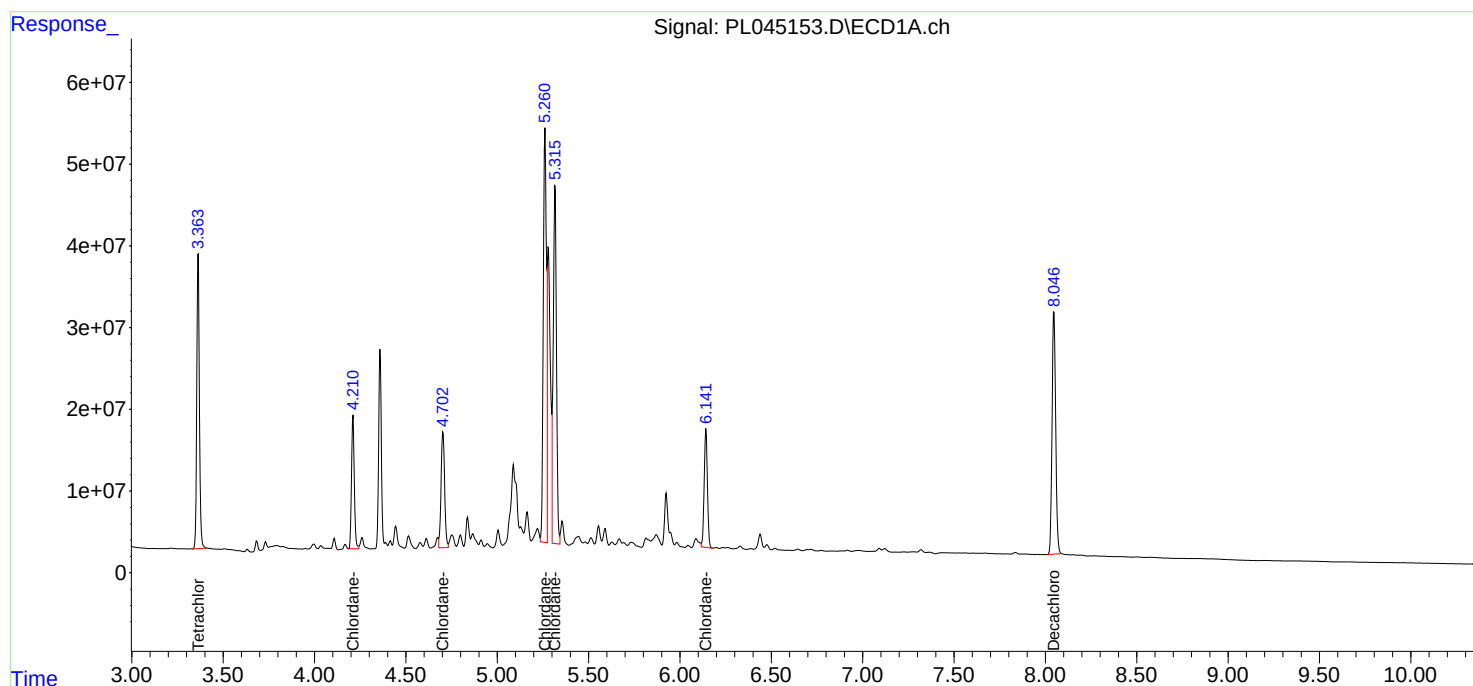


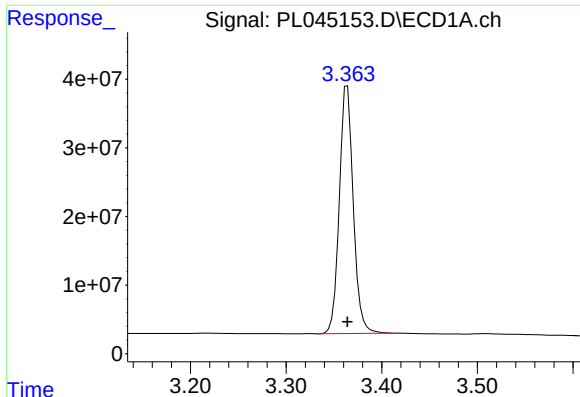

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 365792187
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

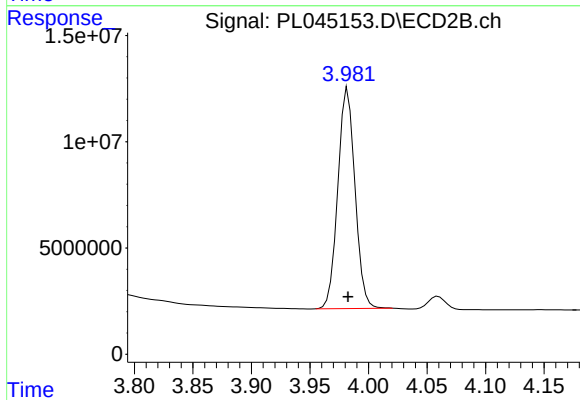


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 105807833
Conc: 50.00 ng/ml

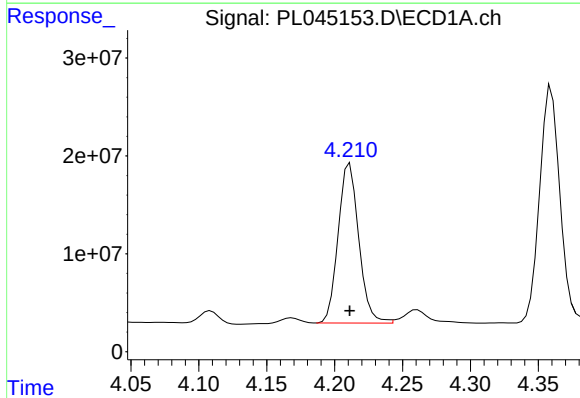


#23 Chlordane-1

R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 172522874
Conc: 500.00 ng/ml

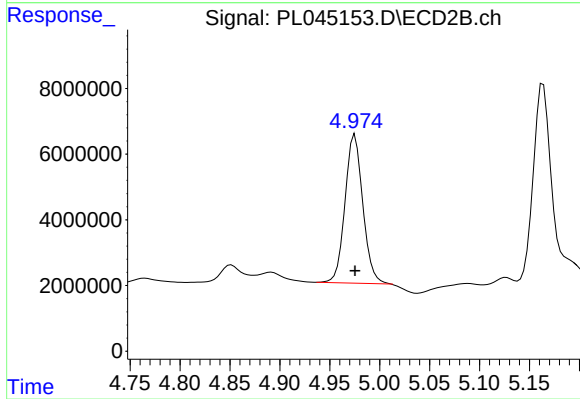

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 55912488
Conc: 500.00 ng/ml

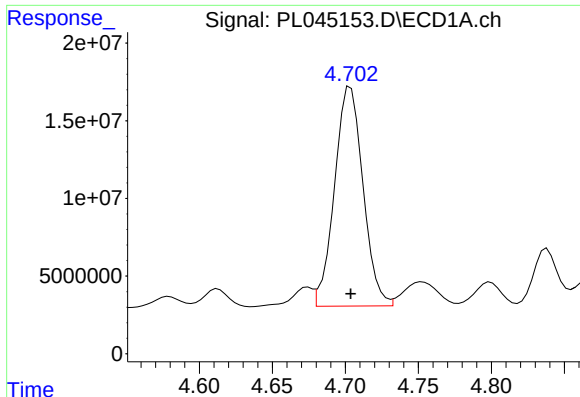

#24 Chlordane-2


R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 191724422
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

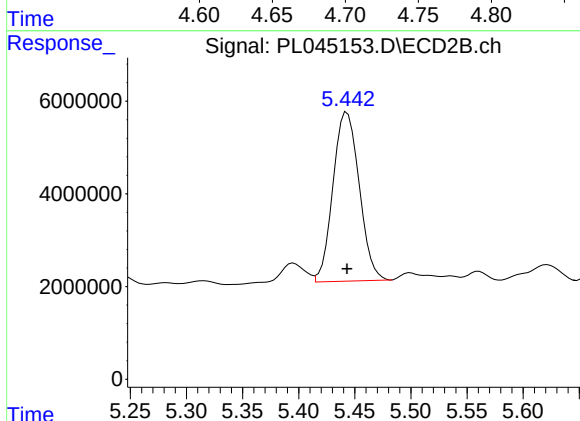


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 59408882
Conc: 500.00 ng/ml

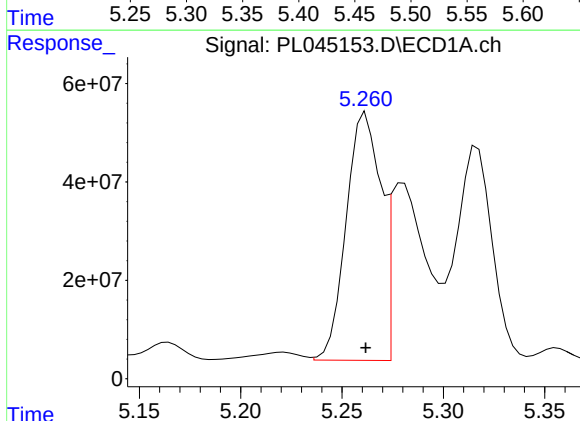


#25 Chlordane-3

R.T.: 5.262 min
Delta R.T.: 0.000 min
Response: 598228197
Conc: 500.00 ng/ml

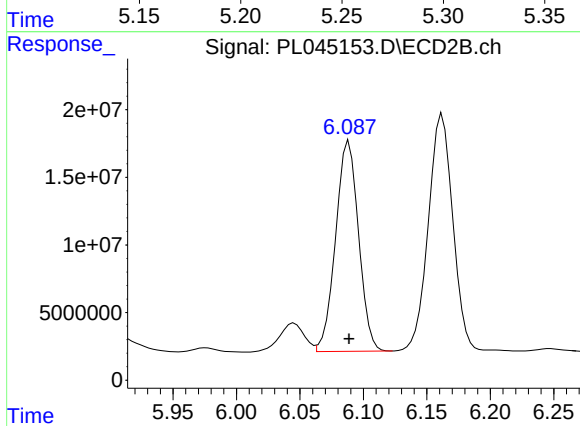

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 195900292
Conc: 500.00 ng/ml

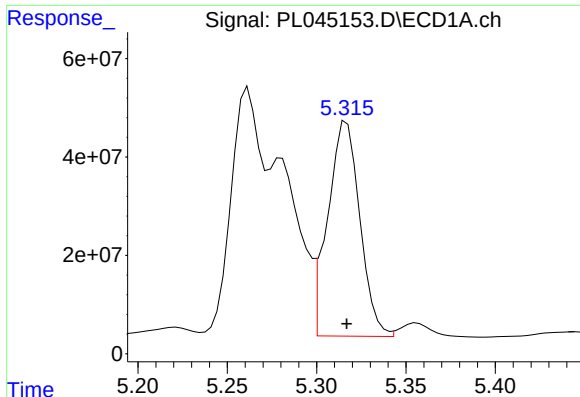

#26 Chlordane-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 546819633
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

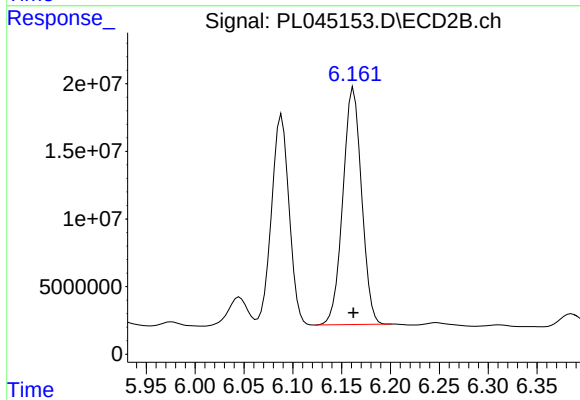


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 233651658
Conc: 500.00 ng/ml

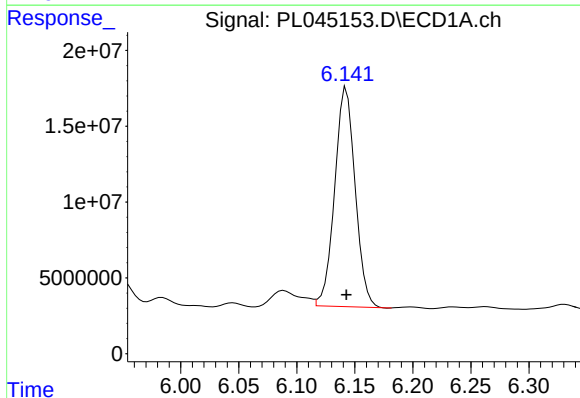


#27 Chlordane-5

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 177415543
Conc: 500.00 ng/ml

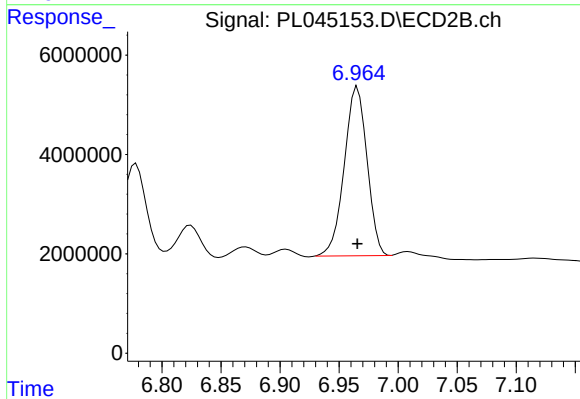

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 45677450
Conc: 500.00 ng/ml

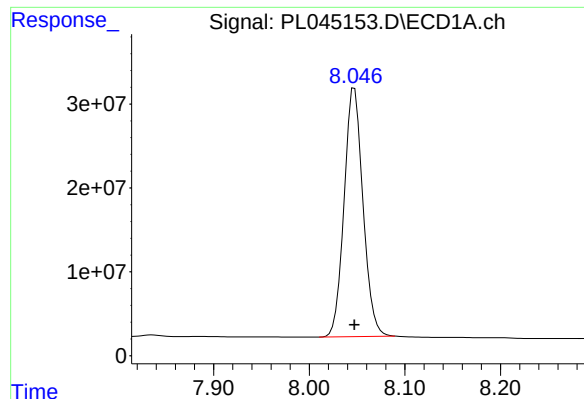

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 407812285
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

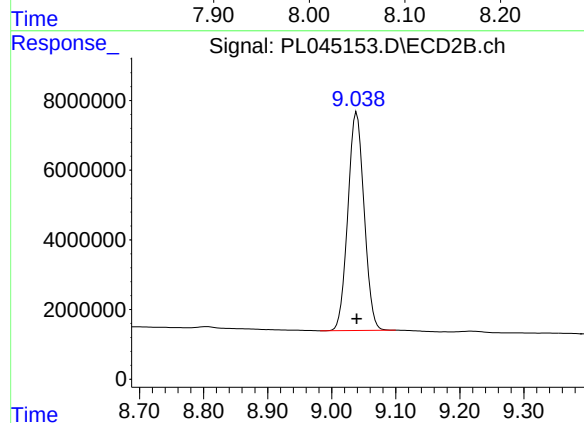

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 110127768
Conc: 50.00 ng/ml