

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 16:47
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL022719CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 16:58:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 16:55:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	365.8E6	106.4E6	51.198	50.962
28)	SA Decachlor...	8.048	9.039	403.5E6	109.2E6	48.325	48.627
Target Compounds							
23)	Chlordane-1	4.211	4.975	173.0E6	55623039	513.512	493.279
24)	Chlordane-2	4.703	5.442	190.1E6	59437722	491.346	491.911
25)	Chlordane-3	5.262	6.088	599.2E6	195.2E6	522.425	501.034
26)	Chlordane-4	5.317	6.162	547.3E6	233.5E6	516.256	499.053
27)	Chlordane-5	6.143	6.966	175.7E6	45068339	508.754	496.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 16:47
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL022719CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 16:58:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 16:55:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

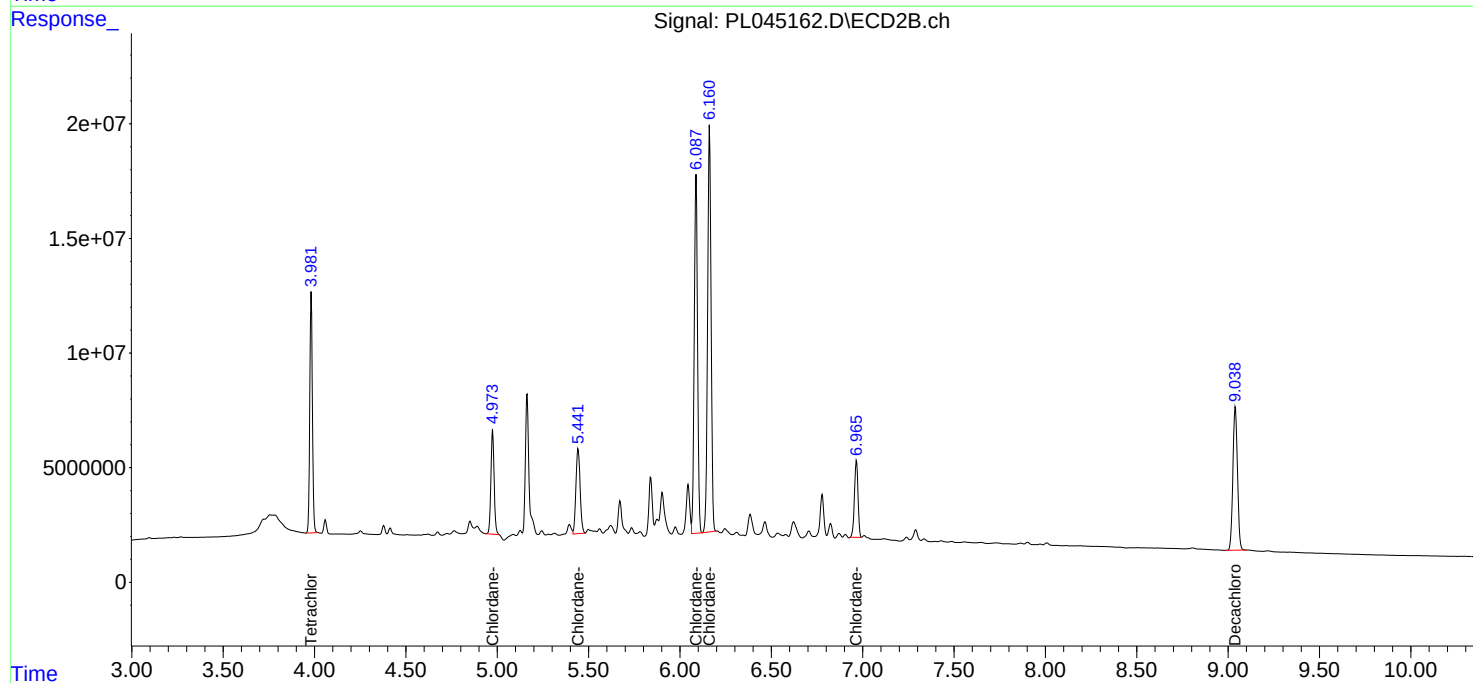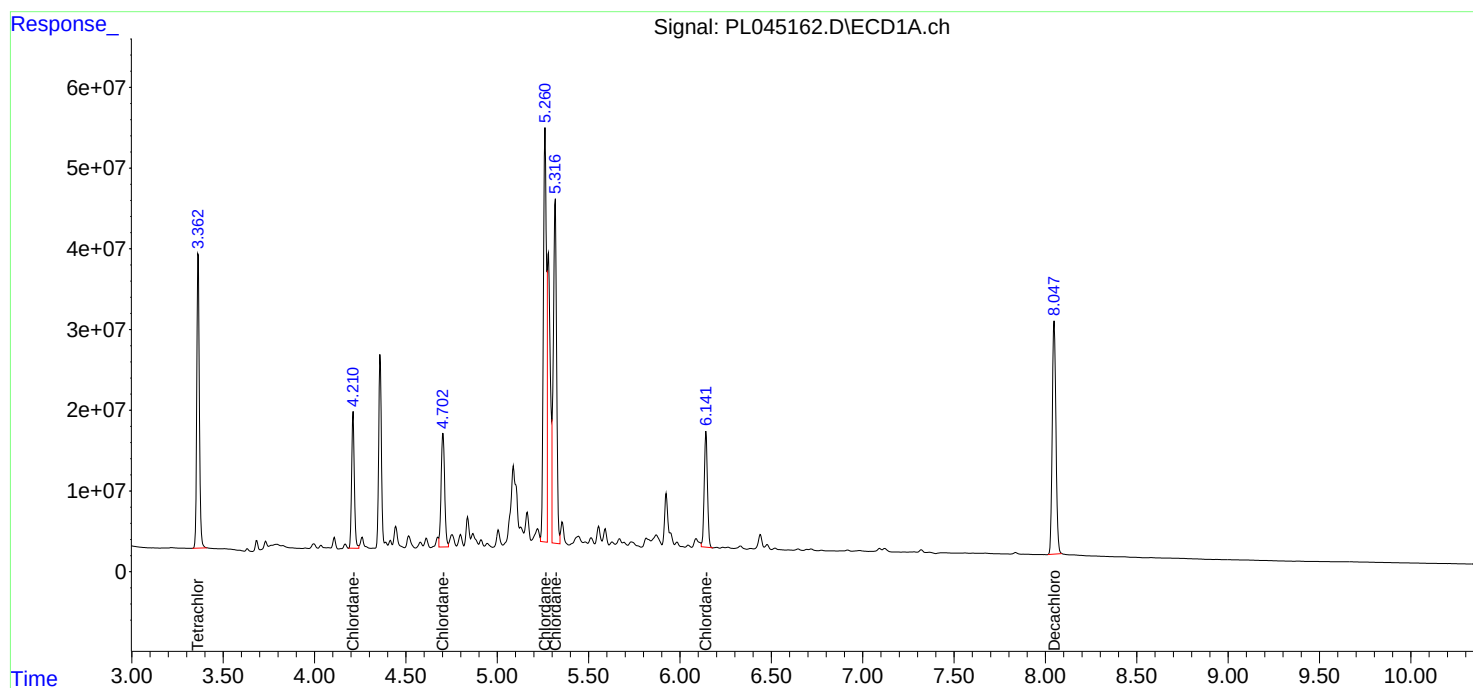


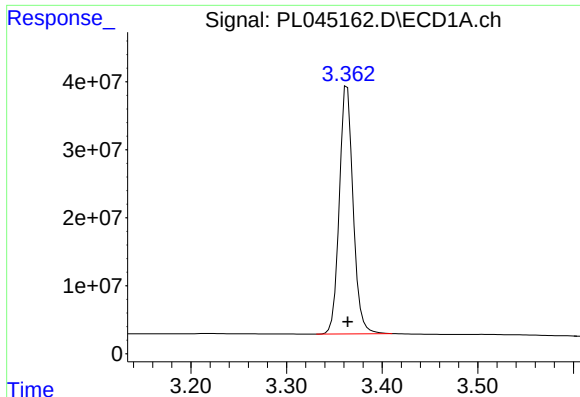

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 365754211
Conc: 51.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022719CHLOR

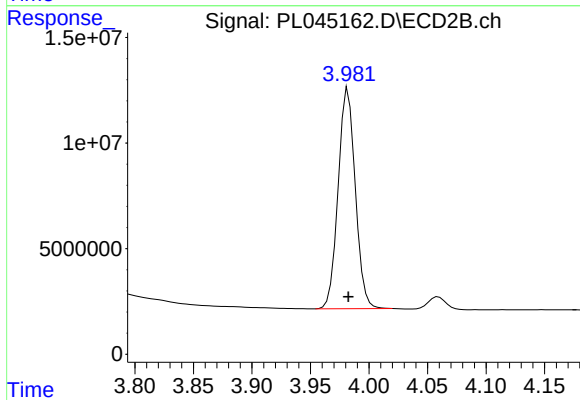


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 106398706
Conc: 50.96 ng/ml

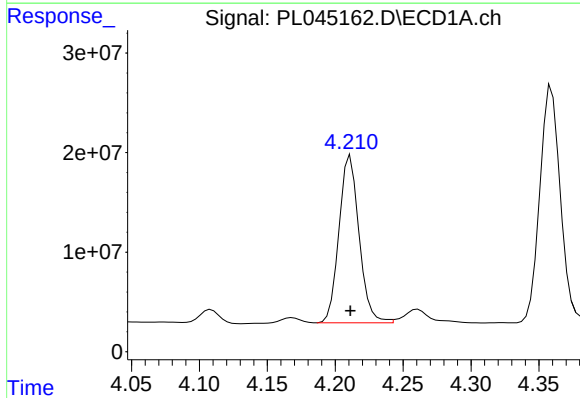


#23 Chlordane-1

R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 173022483
Conc: 513.51 ng/ml

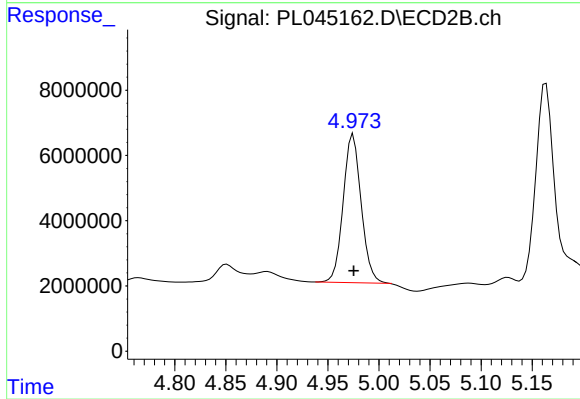

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 55623039
Conc: 493.28 ng/ml

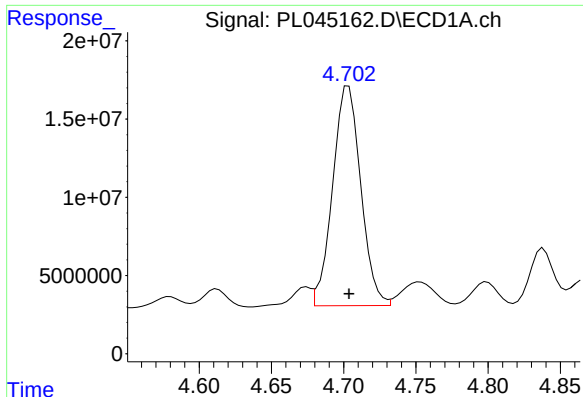

#24 Chlordane-2


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 190061034
Conc: 491.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022719CHLOR

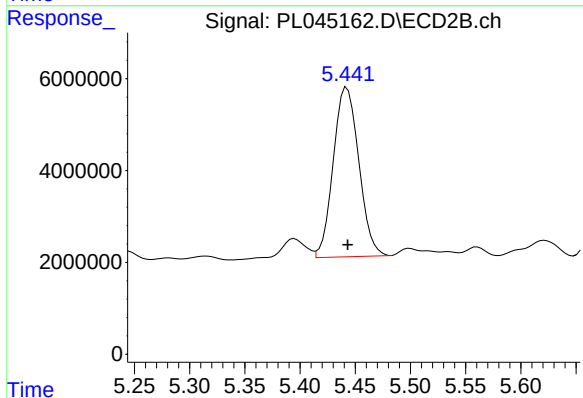


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 59437722
Conc: 491.91 ng/ml

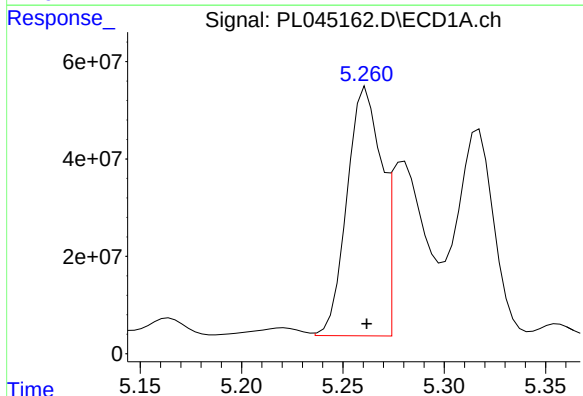


#25 Chlordane-3

R.T.: 5.262 min
Delta R.T.: 0.000 min
Response: 599232518
Conc: 522.42 ng/ml

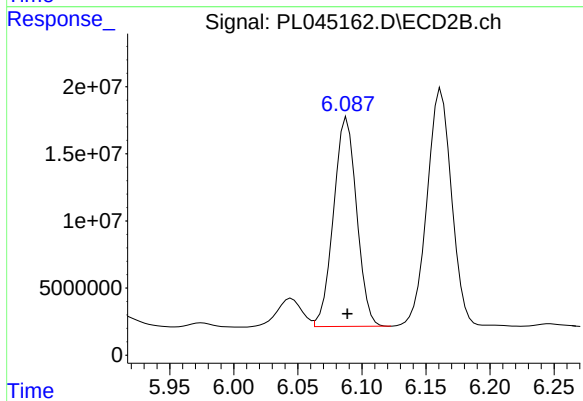

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 195218004
Conc: 501.03 ng/ml

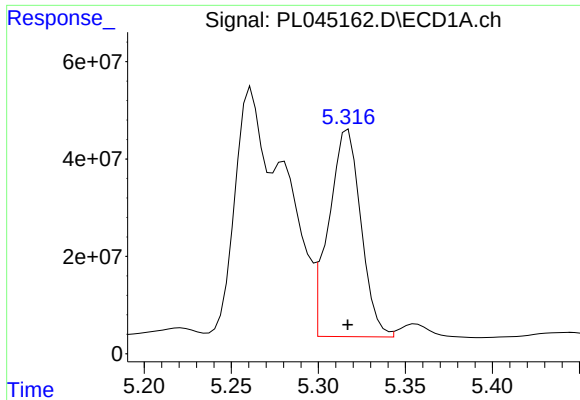

#26 Chlordane-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 547258702
Conc: 516.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022719CHLOR

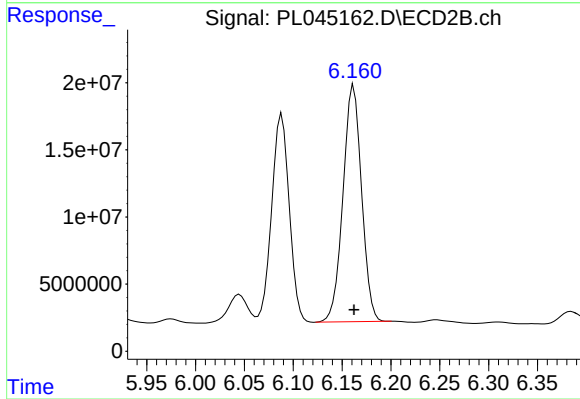


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 233469508
Conc: 499.05 ng/ml

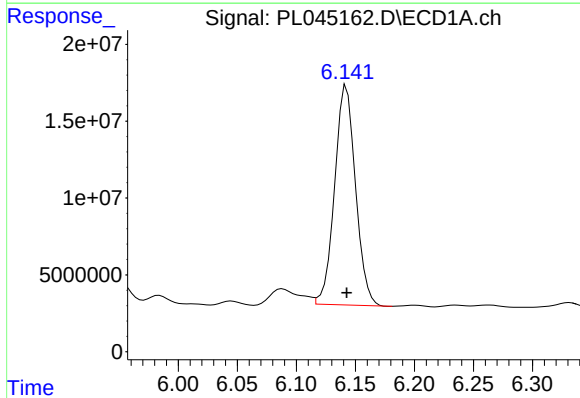


#27 Chlordane-5

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 175696383
Conc: 508.75 ng/ml

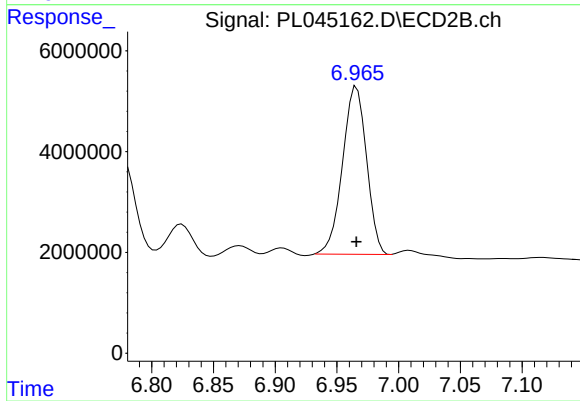

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 45068339
Conc: 496.14 ng/ml

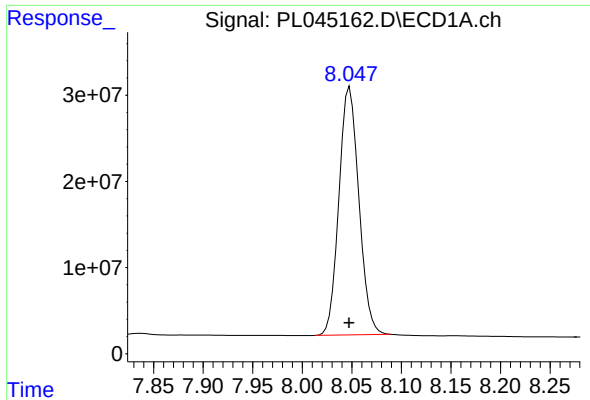

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 403538964
Conc: 48.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022719CHLOR

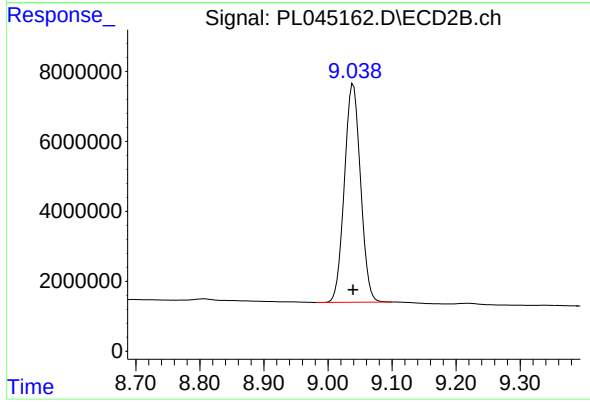

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 109180975
Conc: 48.63 ng/ml