

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022720\
 Data File : PL056864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 12:44
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 13:33:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:33:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	1029.8E6	269.1E6	50.000	50.000
28)	SA Decachlor...	8.254	9.097	1008.8E6	205.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.369	5.013	348.2E6	99090267	500.000	500.000
24)	Chlordane-2	4.871	5.482	388.2E6	104.2E6	500.000	500.000
25)	Chlordane-3	5.442	6.130	1164.6E6	381.0E6	500.000	500.000
26)	Chlordane-4	5.500	6.203	992.6E6	444.2E6	500.000	500.000
27)	Chlordane-5	6.337	7.010	414.1E6	85198568	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022720\
Data File : PL056864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 12:44
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 13:33:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:33:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

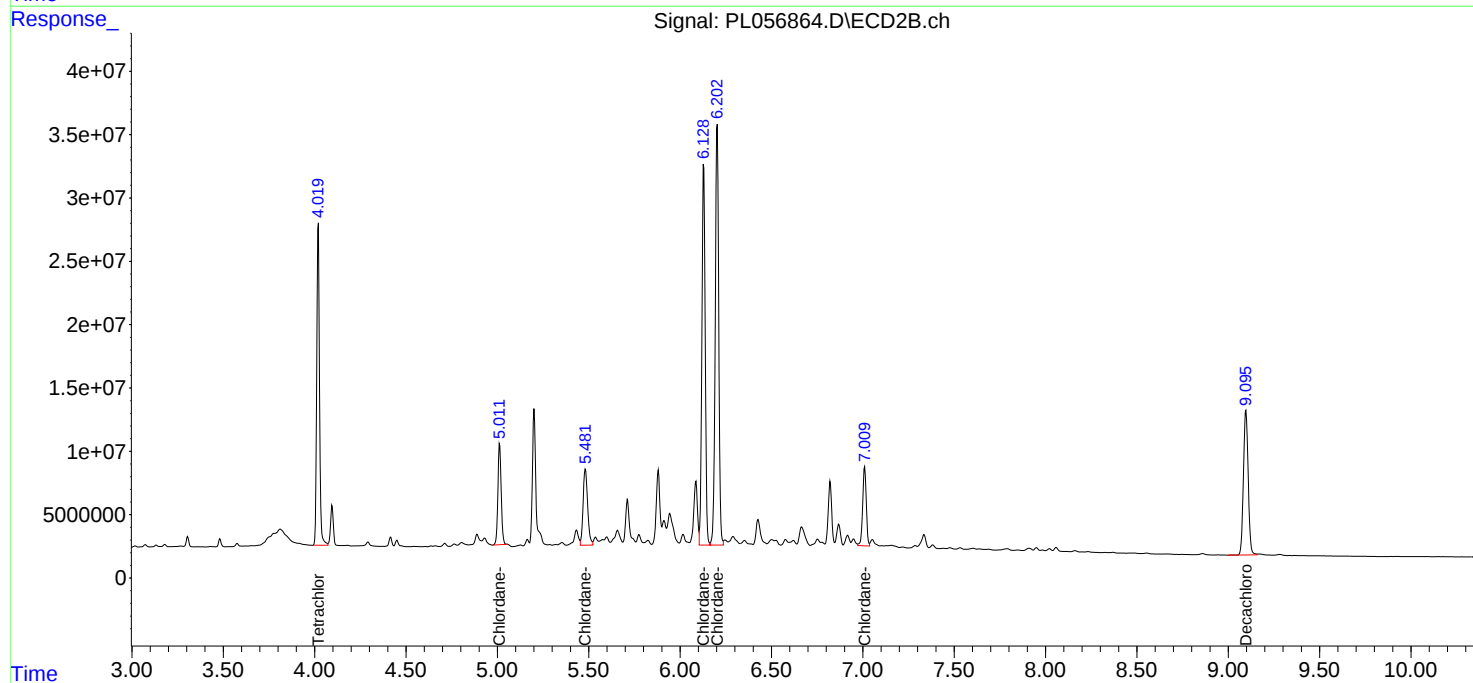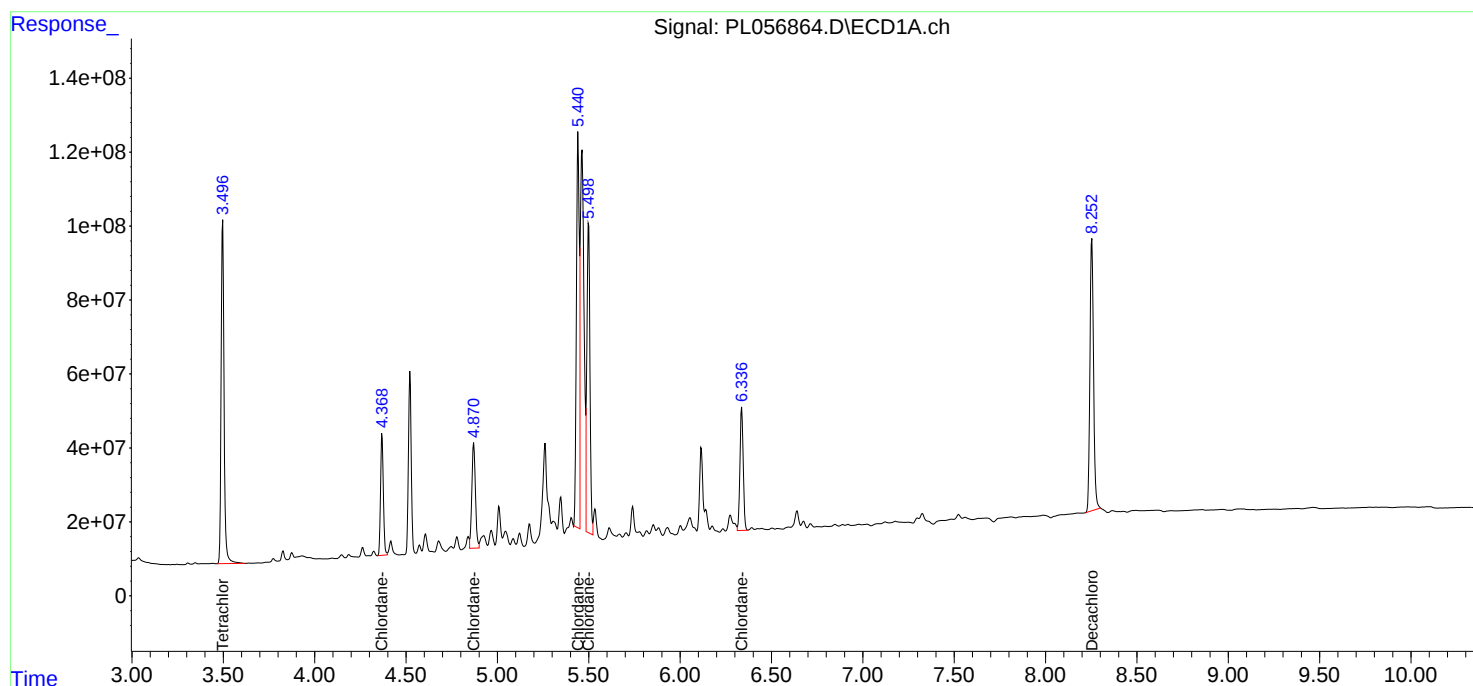


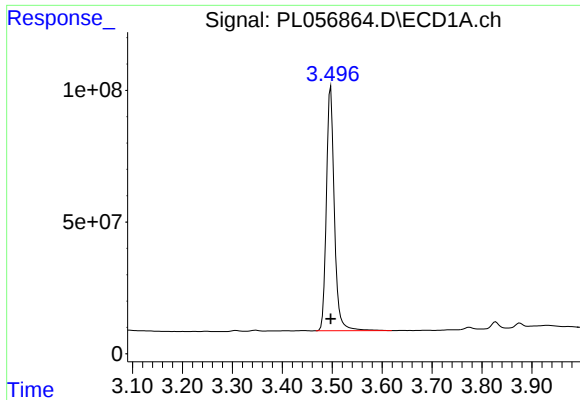

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 1029832378
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

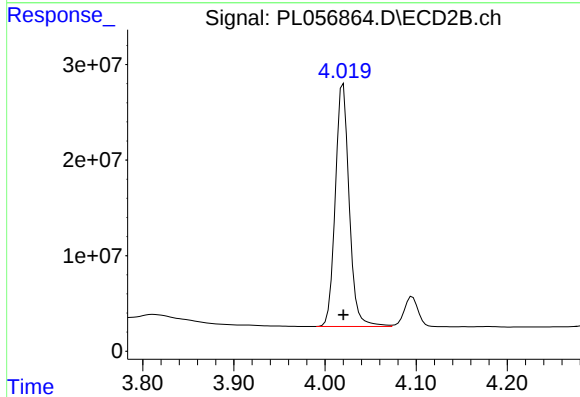


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 269087978
Conc: 50.00 ng/ml

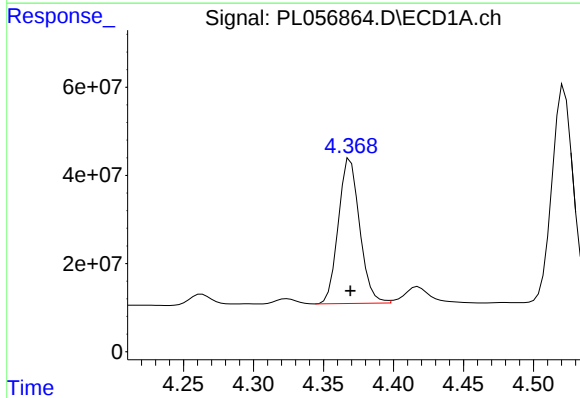


#23 Chlordane-1

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 348192537
Conc: 500.00 ng/ml

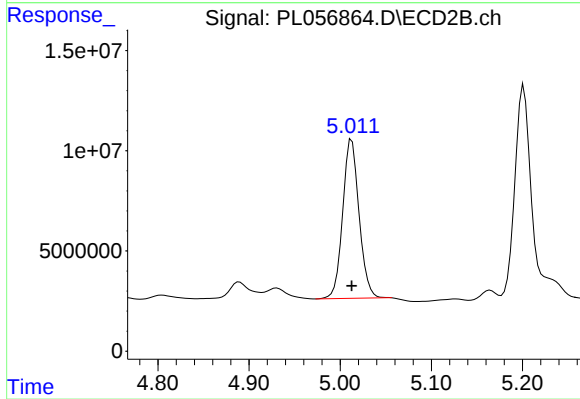

#23 Chlordane-1


R.T.: 5.013 min
Delta R.T.: 0.000 min
Response: 99090267
Conc: 500.00 ng/ml

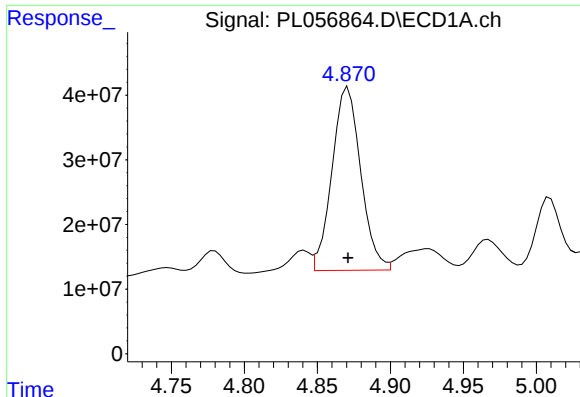

#24 Chlordane-2


R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 388221371
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

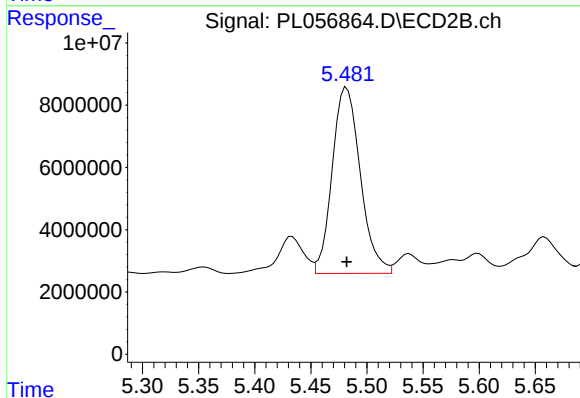


#24 Chlordane-2

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 104247406
Conc: 500.00 ng/ml

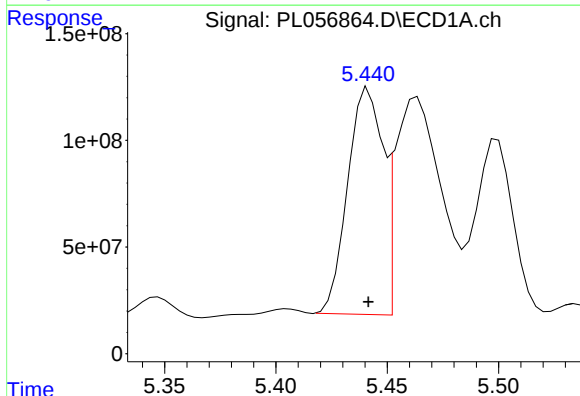


#25 Chlordane-3

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 1164573323
Conc: 500.00 ng/ml

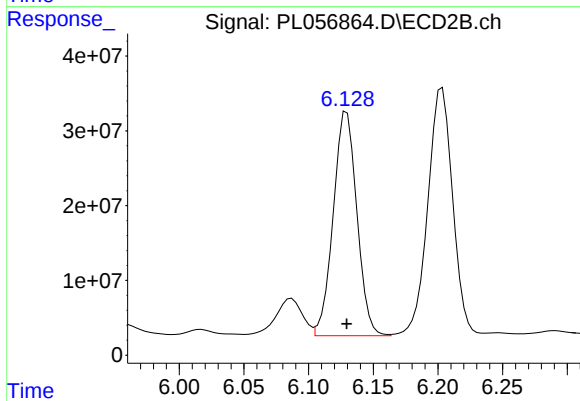

#25 Chlordane-3


R.T.: 6.130 min
Delta R.T.: 0.000 min
Response: 380963433
Conc: 500.00 ng/ml

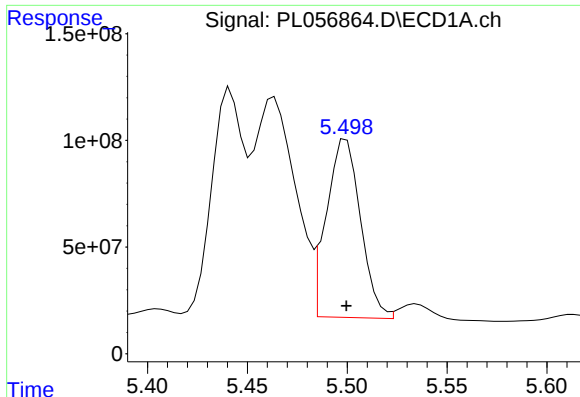

#26 Chlordane-4


R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 992620025
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

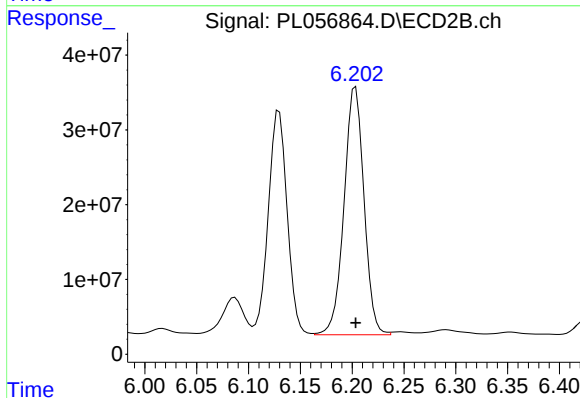


#26 Chlordane-4

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 444157411
Conc: 500.00 ng/ml

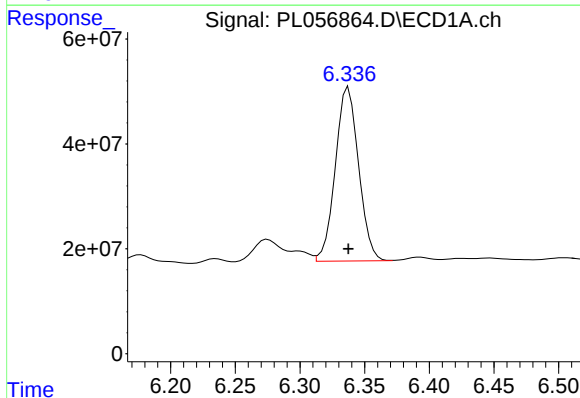


#27 Chlordane-5

R.T.: 6.337 min
Delta R.T.: 0.000 min
Response: 414123436
Conc: 500.00 ng/ml

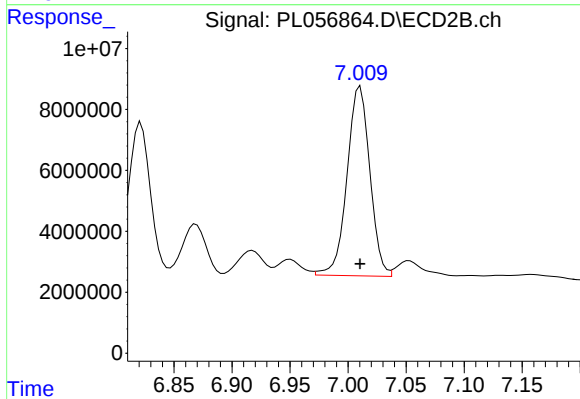

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 85198568
Conc: 500.00 ng/ml

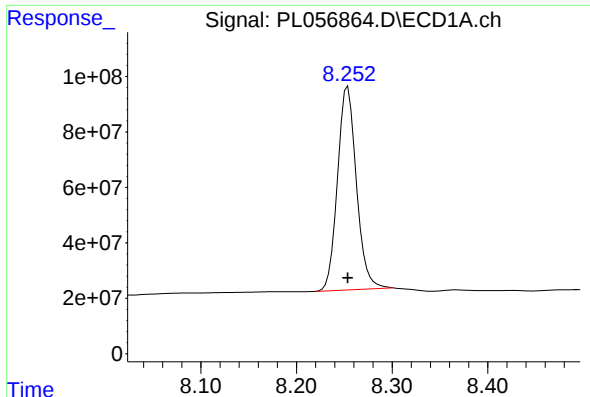

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 1008846395
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

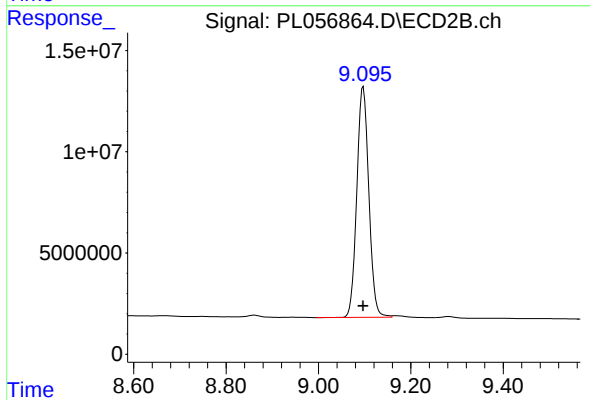

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 205758352
Conc: 50.00 ng/ml