

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022724\
 Data File : PL088315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 15:35
 Operator : AR\AJ
 Sample : P1583-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MANHOLE-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 10:08:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.644	2.855	54185415	26396508	19.727	18.821
28) SA Decachlor...	9.315	8.089	32819857	19611100	17.041	15.402
Target Compounds						
16) A 4,4'-DDD	6.870	5.936	6520631	5075087	2.514	3.715m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022724\
Data File : PL088315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 15:35
Operator : AR\AJ
Sample : P1583-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MANHOLE-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 10:08:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

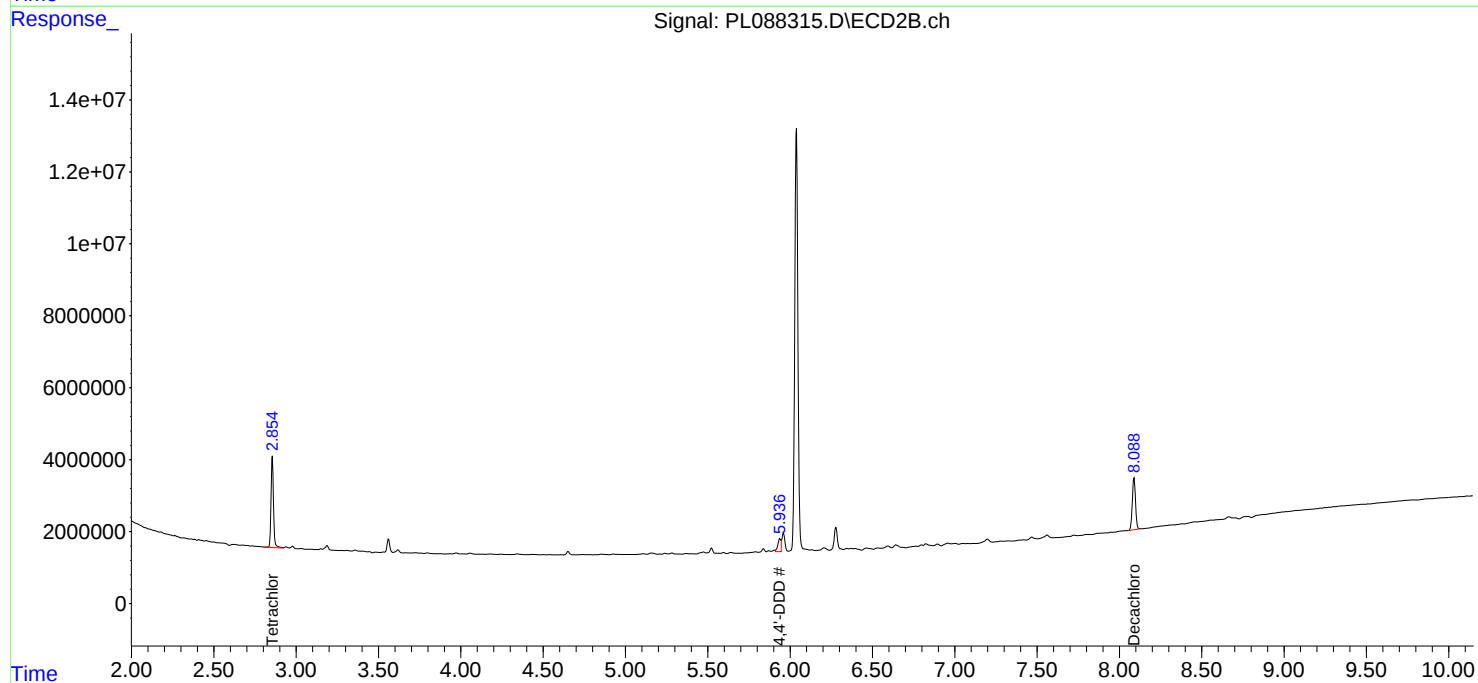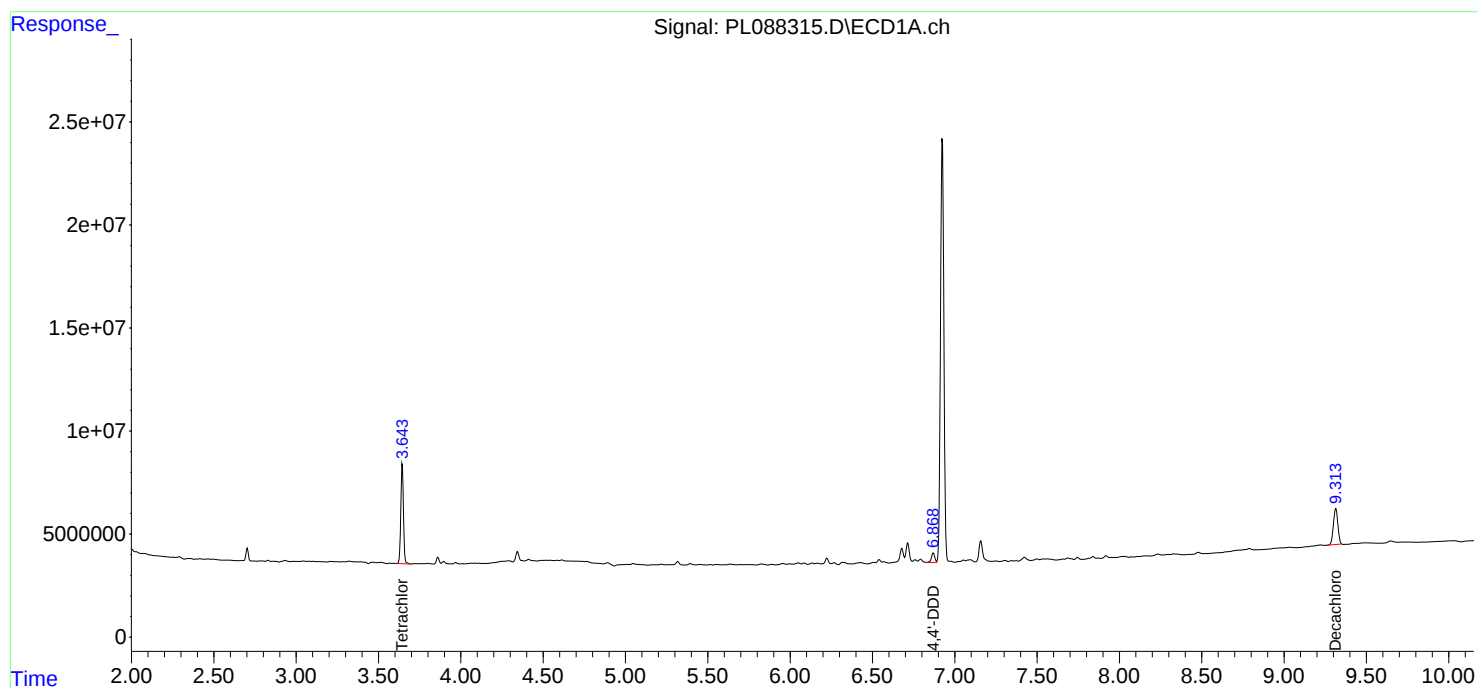


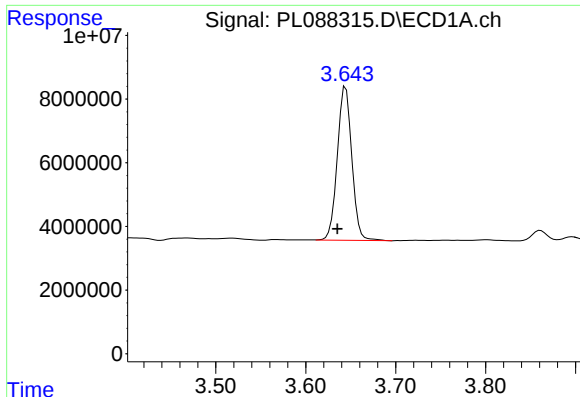

#1 Tetrachloro-m-xylene


R.T.: 3.644 min
Delta R.T.: 0.009 min
Response: 54185415
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-COMP

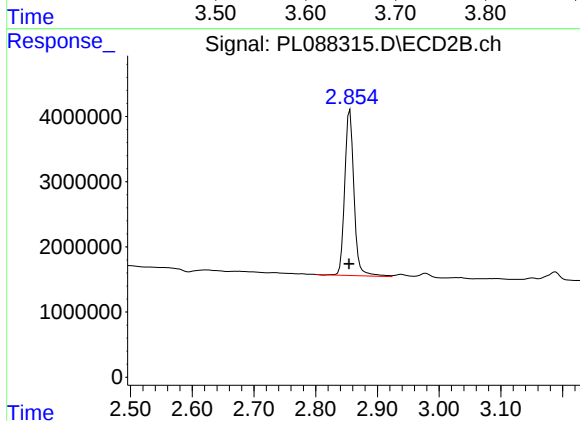


#1 Tetrachloro-m-xylene

R.T.: 2.855 min
Delta R.T.: 0.002 min
Response: 26396508
Conc: 18.82 ng/ml

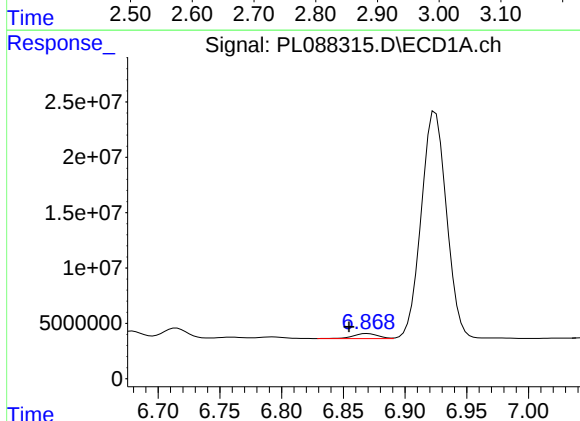


#16 4,4'-DDD

R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 6520631
Conc: 2.51 ng/ml

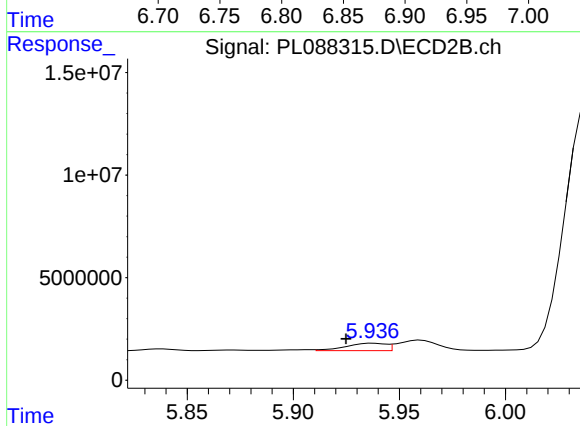

#16 4,4'-DDD


R.T.: 5.936 min
Delta R.T.: 0.011 min
Response: 5075087
Conc: 3.71 ng/ml m

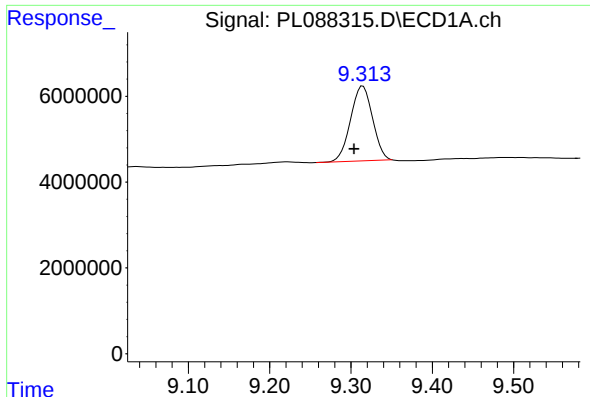

#28 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: 0.011 min
Response: 32819857
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-COMP

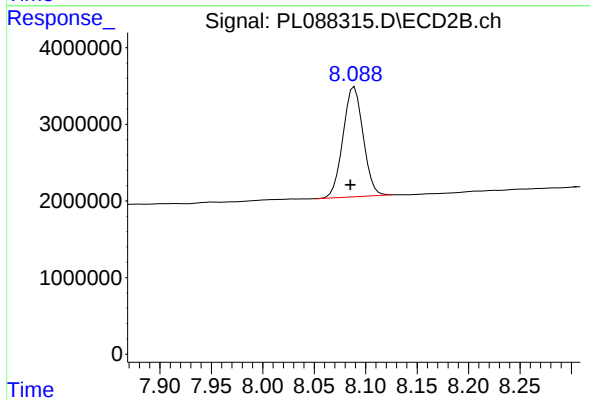

#28 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.004 min
Response: 19611100
Conc: 15.40 ng/ml