

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022724\
 Data File : PL088319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 16:30
 Operator : AR\AJ
 Sample : P1585-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-232

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:26:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.635	2.854	59869480	28977155	21.797	20.661
28)	SA Decachlor...	9.302	8.083	46038984	26827496	23.905	21.069
Target Compounds							
10)	B gamma-Chl...	6.075	5.105	406.4E6	126.2E6	119.578m	70.728 #
11)	B alpha-Chl...	6.160	5.169	674.1E6	185.7E6	197.535	104.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022724\
Data File : PL088319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 16:30
Operator : AR\AJ
Sample : P1585-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-232

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:26:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

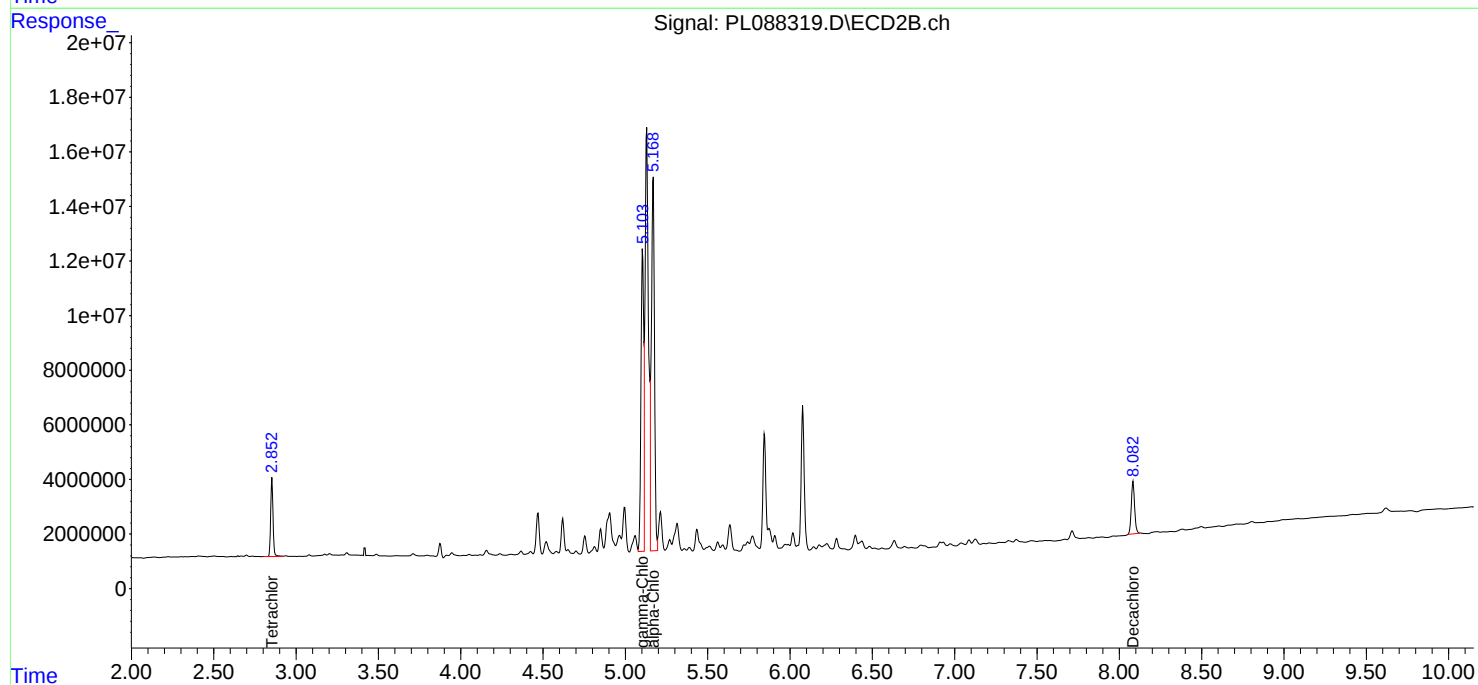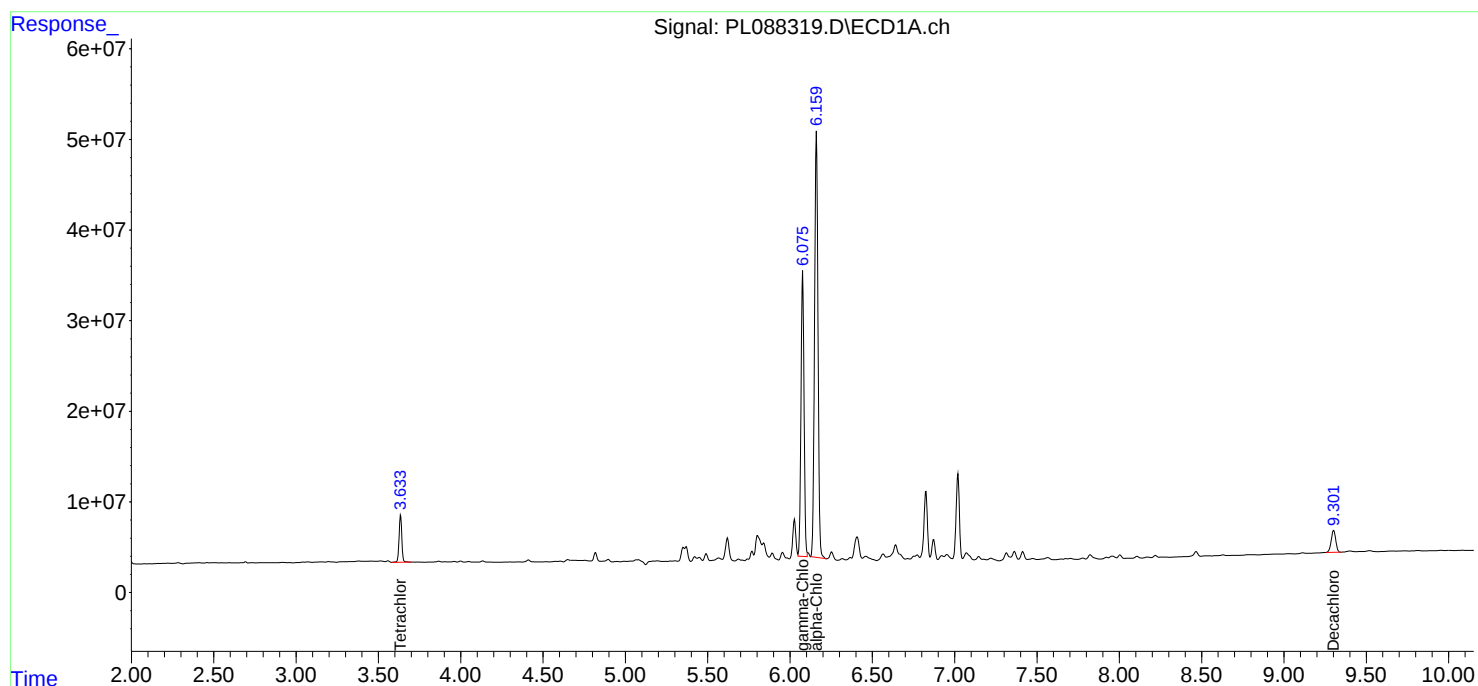


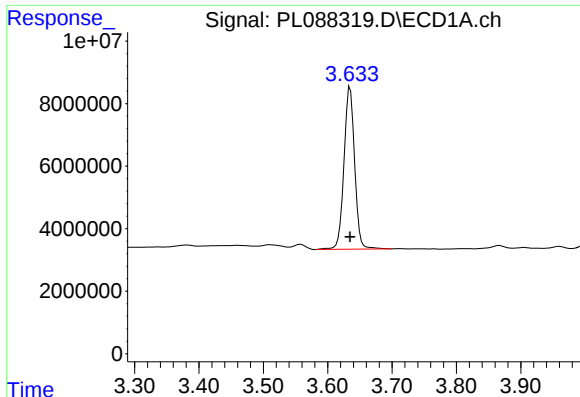

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 59869480
Conc: 21.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-232

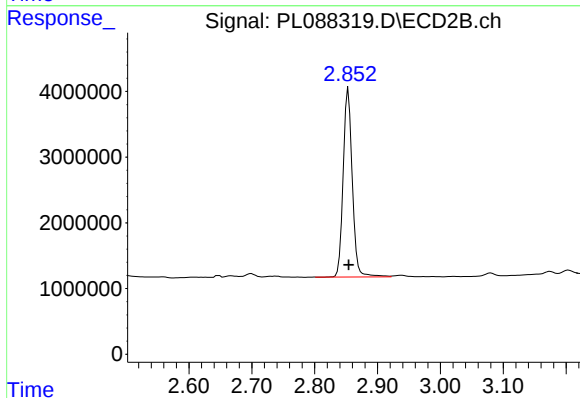


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 28977155
Conc: 20.66 ng/ml

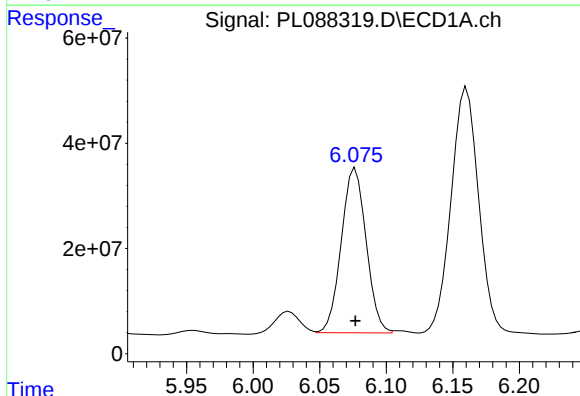


#10 gamma-Chlordane

R.T.: 6.075 min
Delta R.T.: -0.001 min
Response: 406365513
Conc: 119.58 ng/ml m

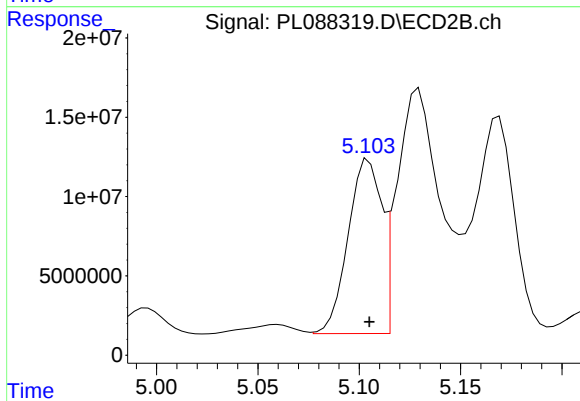

#10 gamma-Chlordane


R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 126163703
Conc: 70.73 ng/ml

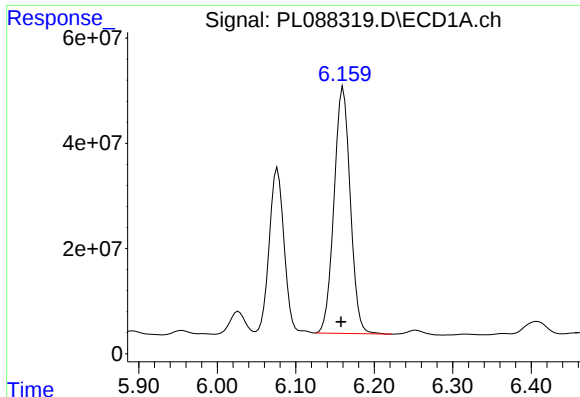

#11 alpha-Chlordane


R.T.: 6.160 min
Delta R.T.: 0.003 min
Response: 674138368
Conc: 197.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-232

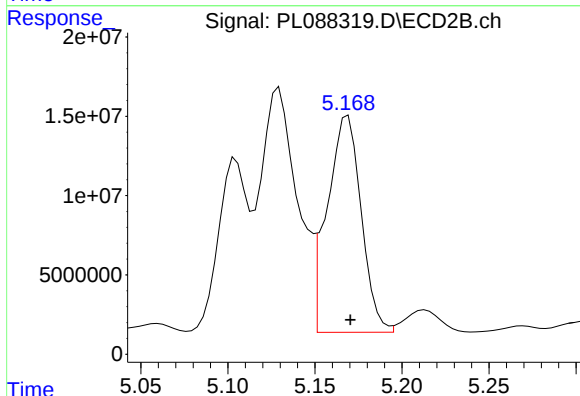


#11 alpha-Chlordane

R.T.: 5.169 min
Delta R.T.: -0.001 min
Response: 185693551
Conc: 104.24 ng/ml

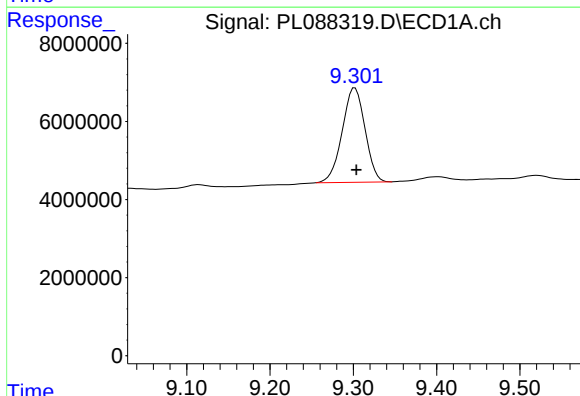

#28 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: -0.002 min
Response: 46038984
Conc: 23.90 ng/ml

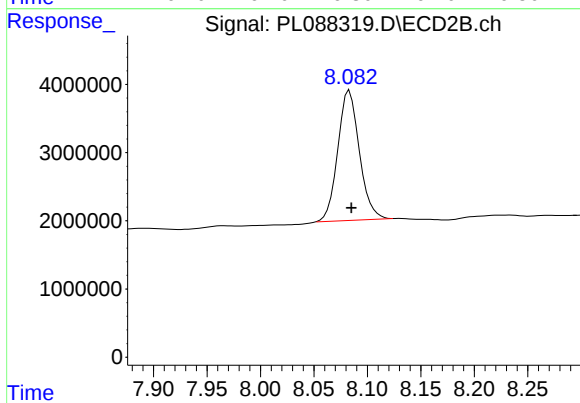

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 26827496
Conc: 21.07 ng/ml