

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL022819\  
 Data File : PL045220.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Feb 2019 10:00  
 Operator : AJ\SJ  
 Sample : K1350-13  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 EO-01-022619-B

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 01 00:02:07 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Feb 27 17:00:03 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|-------|---------|
| -----                       |                 |       |       |          |          |       |         |
| System Monitoring Compounds |                 |       |       |          |          |       |         |
| 1)                          | SA Tetrachlo... | 3.363 | 3.982 | 62632819 | 20404584 | 9.105 | 9.528   |
| 28)                         | SA Decachlor... | 8.047 | 9.040 | 79903127 | 25144318 | 9.549 | 11.004  |
| Target Compounds            |                 |       |       |          |          |       |         |
| 8)                          | B Heptachlo...  | 0.000 | 5.848 | 0        | 1359403  | N.D.  | 0.566 # |
| 11)                         | B alpha-Chl...  | 0.000 | 6.162 | 0        | 1574720  | N.D.  | 0.584 # |
| 12)                         | B 4,4'-DDE      | 0.000 | 6.318 | 0        | 1669056  | N.D.  | 0.715 # |
| 26)                         | Chlordane-4     | 0.000 | 6.162 | 0        | 1574720  | N.D.  | 3.366 # |
| -----                       |                 |       |       |          |          |       |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL022819\  
Data File : PL045220.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Feb 2019 10:00  
Operator : AJ\SJ  
Sample : K1350-13  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
EO-01-022619-B

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 01 00:02:07 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
Quant Title : GC Extractables  
QLast Update : Wed Feb 27 17:00:03 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

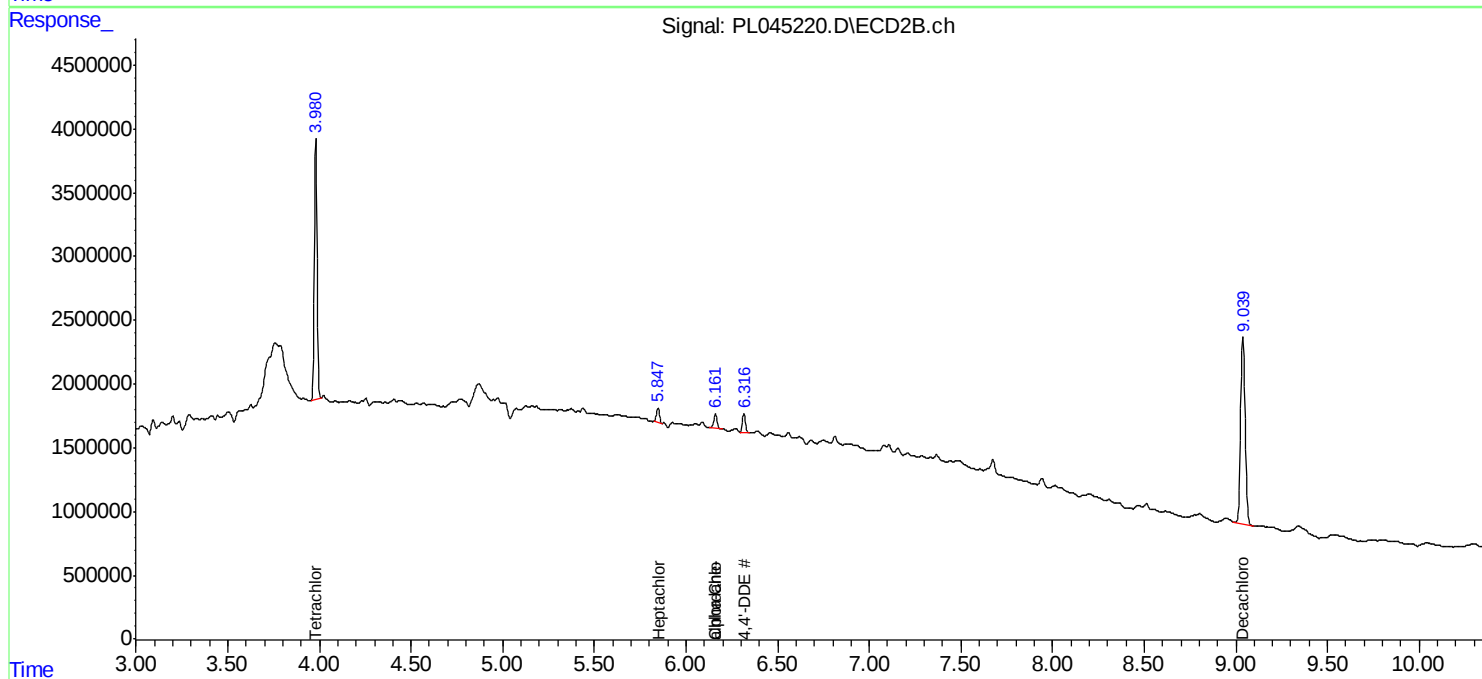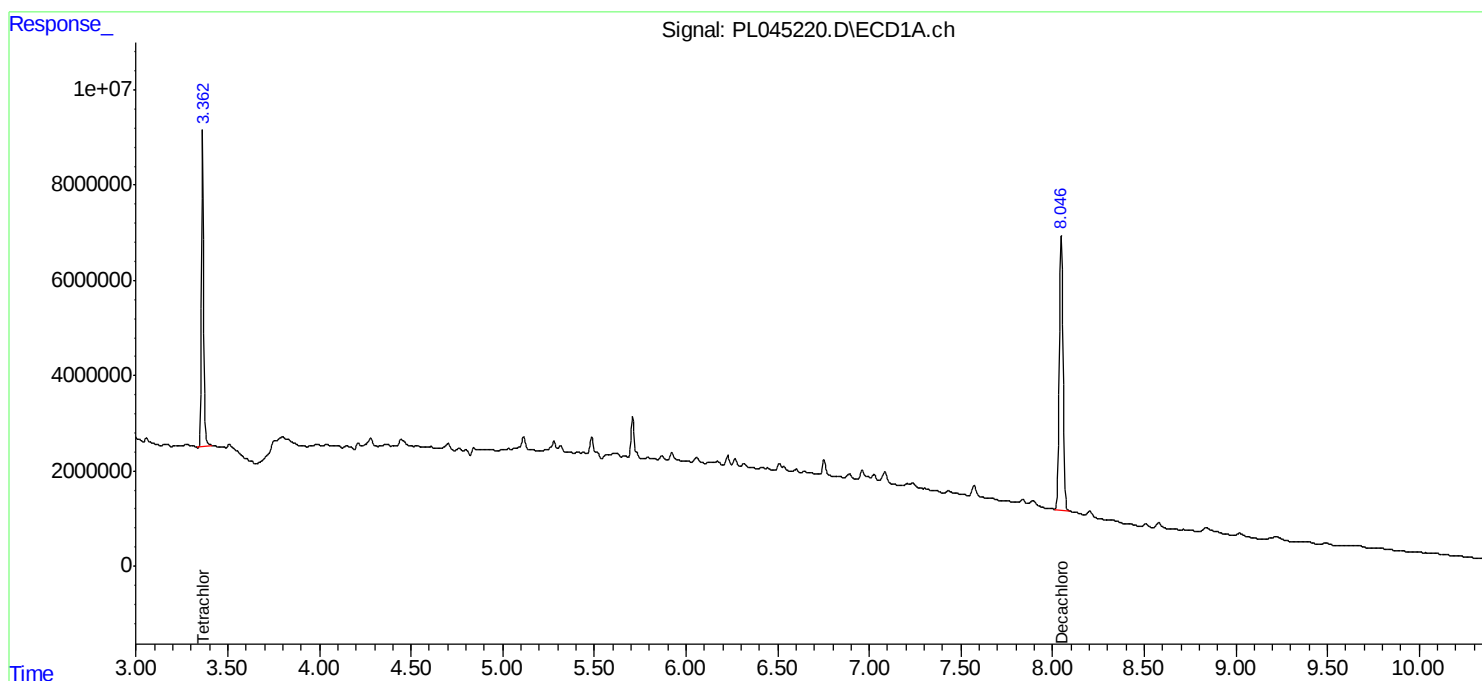


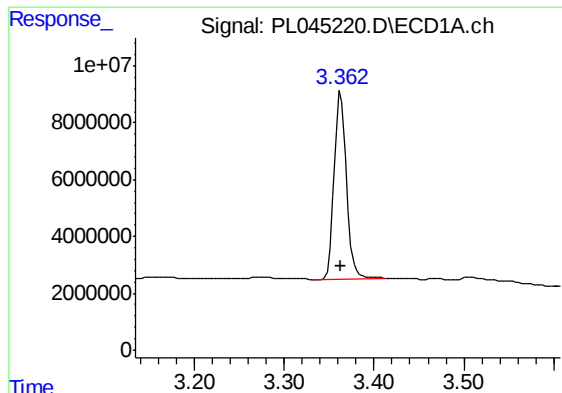

#1 Tetrachloro-m-xylene


R.T.: 3.363 min  
Delta R.T.: 0.000 min  
Response: 62632819  
Conc: 9.10 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
EO-01-022619-B

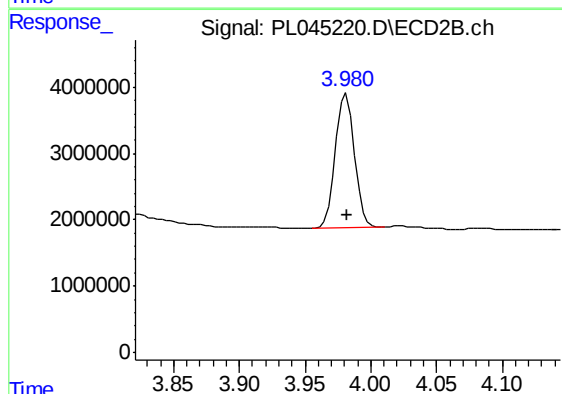


#1 Tetrachloro-m-xylene

R.T.: 3.982 min  
Delta R.T.: 0.000 min  
Response: 20404584  
Conc: 9.53 ng/ml

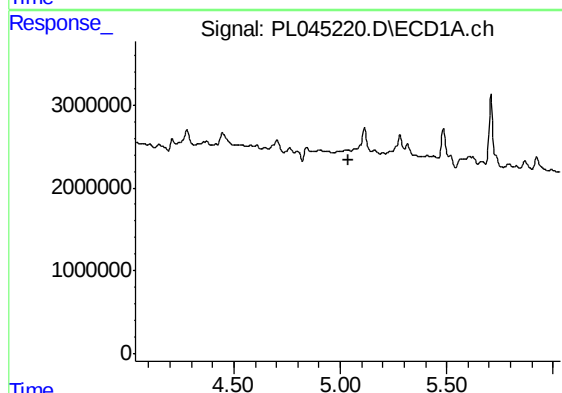


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T. : 5.037 min  
Response: 0  
Conc: N.D.

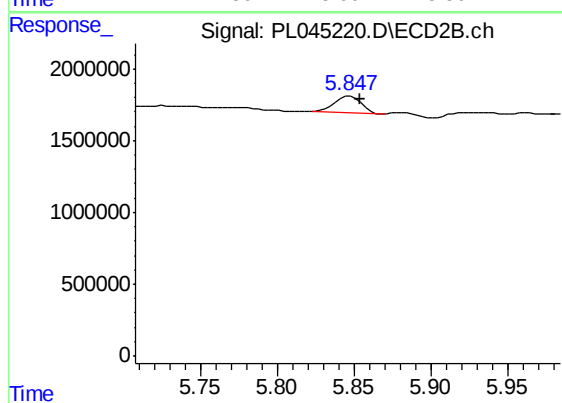

#8 Heptachlor epoxide


R.T.: 5.848 min  
Delta R.T.: -0.006 min  
Response: 1359403  
Conc: 0.57 ng/ml

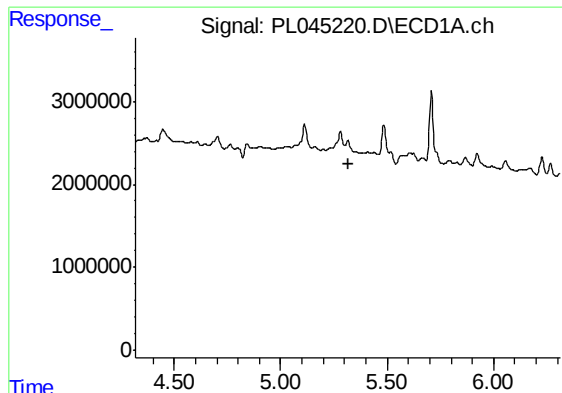

#11 alpha-Chlordane


R.T.: 0.000 min  
Exp R.T.: 5.317 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
EO-01-022619-B

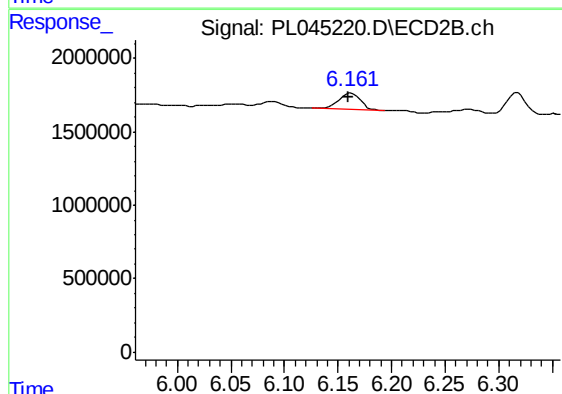


#11 alpha-Chlordane

R.T.: 6.162 min  
Delta R.T.: 0.002 min  
Response: 1574720  
Conc: 0.58 ng/ml

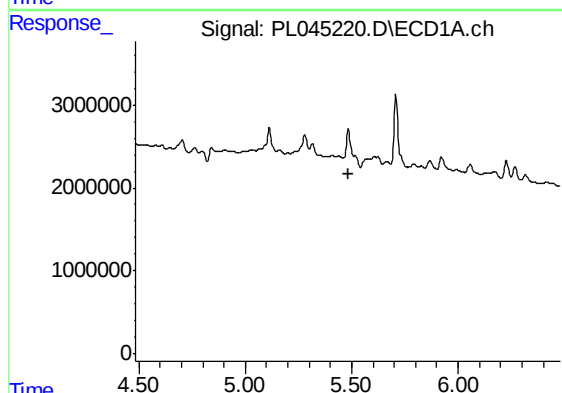


#12 4,4'-DDE

R.T.: 0.000 min  
Exp R.T.: 5.484 min  
Response: 0  
Conc: N.D.

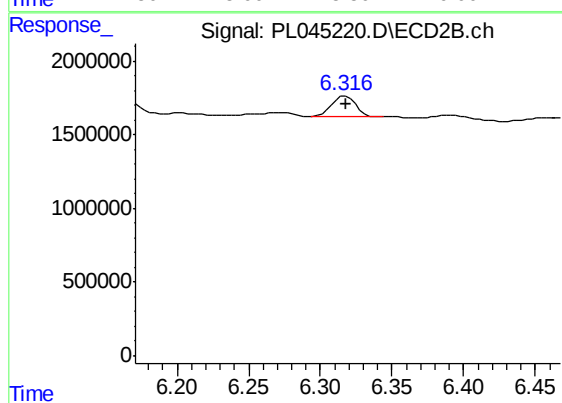

#12 4,4'-DDE


R.T.: 6.318 min  
Delta R.T.: 0.000 min  
Response: 1669056  
Conc: 0.71 ng/ml

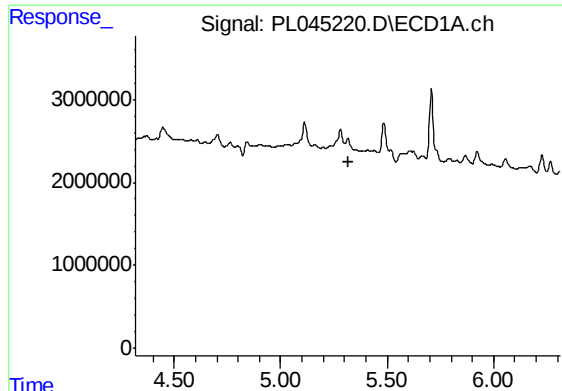

#26 Chlordane-4


R.T.: 0.000 min  
Exp R.T.: 5.317 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
EO-01-022619-B

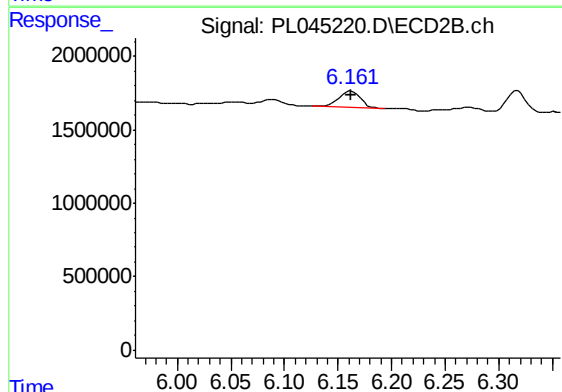


#26 Chlordane-4

R.T.: 6.162 min  
Delta R.T.: 0.000 min  
Response: 1574720  
Conc: 3.37 ng/ml

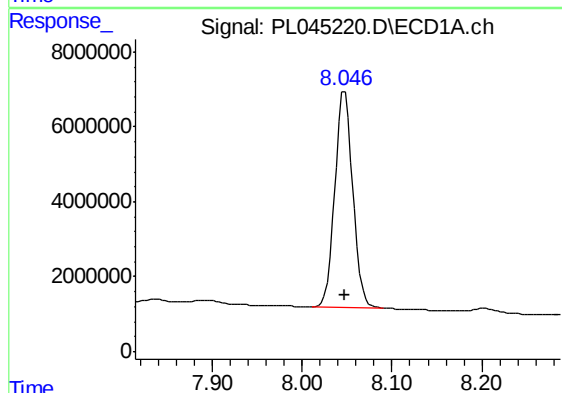

#28 Decachlorobiphenyl

R.T.: 8.047 min  
Delta R.T.: 0.000 min  
Response: 79903127  
Conc: 9.55 ng/ml

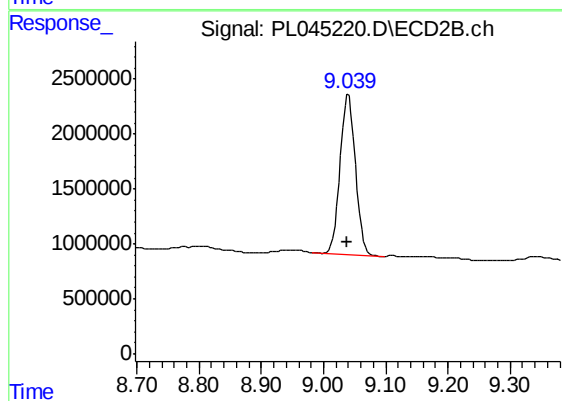

#28 Decachlorobiphenyl

R.T.: 9.040 min  
Delta R.T.: 0.001 min  
Response: 25144318  
Conc: 11.00 ng/ml