

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 11:39
 Operator : AJ\SJ
 Sample : K1627-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-01-(6-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:03:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	56702333	18483072	8.242	8.631
28)	SA Decachlor...	8.048	9.040	85106075	25424533	10.171	11.127
Target Compounds							
10)	B gamma-Chl...	5.281f	6.090	32434368	2267354	3.314	0.845 #
11)	B alpha-Chl...	5.317	6.163	9358731	10890634	0.965	4.037 #
12)	B 4,4'-DDE	5.486	6.319	844.6E6	212.3E6	96.217	90.873
14)	MA Endrin	5.867	6.713f	9277679	1931384	1.030	0.849
16)	A 4,4'-DDD	0.000	6.814	0	1955826	N.D.	1.017 #
17)	MA 4,4'-DDT	6.231	7.107	22175079	4820870	2.957	2.443
24)	Chlordane-2	4.708	0.000	5455594	0	14.104	N.D. #
25)	Chlordane-3	5.281f	6.090	32434368	2267354	28.277	5.819 #
26)	Chlordane-4	5.317	6.163	9358731	10890634	8.829	23.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 11:39
Operator : AJ\SJ
Sample : K1627-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-01-(6-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:03:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

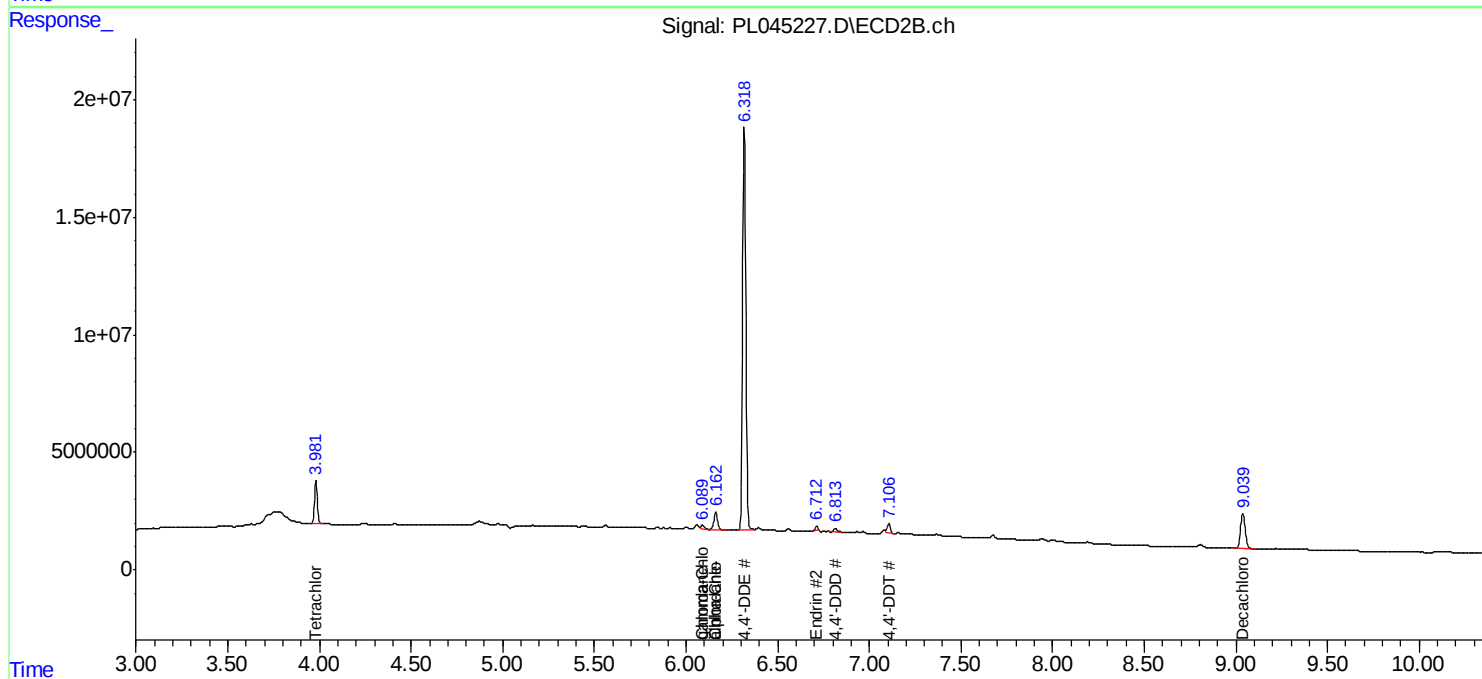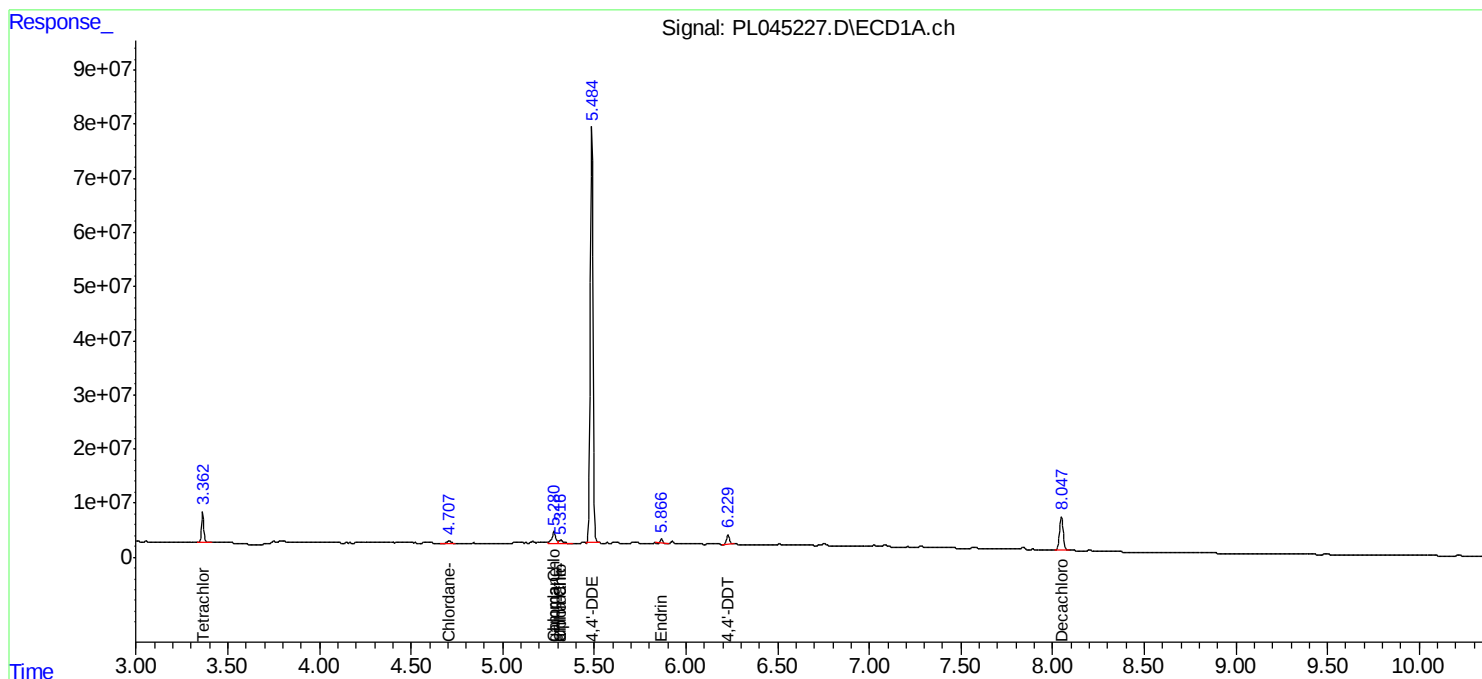


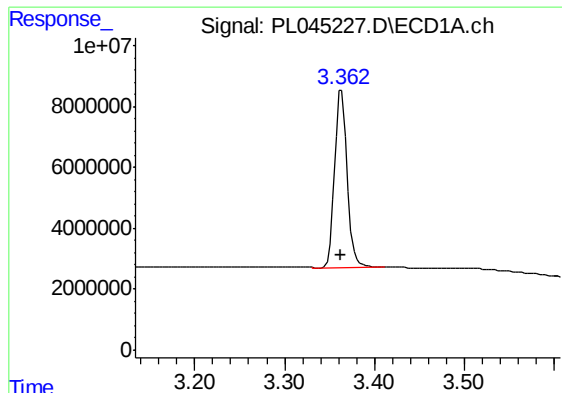

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 56702333
Conc: 8.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

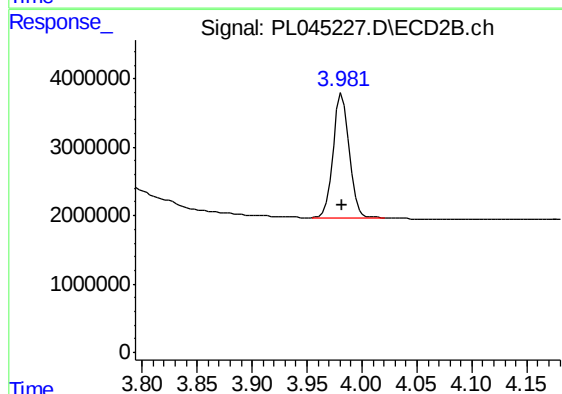


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 18483072
Conc: 8.63 ng/ml

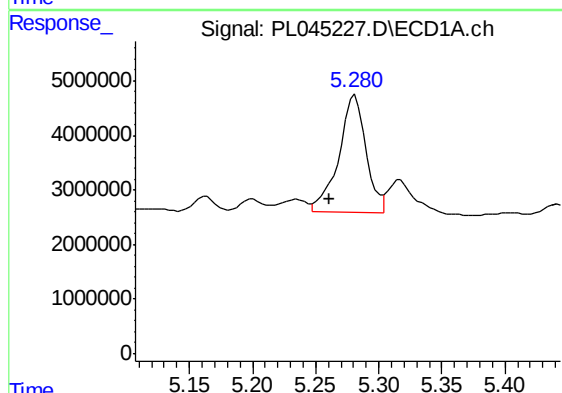


#10 gamma-Chlordane

R.T.: 5.281 min
Delta R.T.: 0.021 min
Response: 32434368
Conc: 3.31 ng/ml

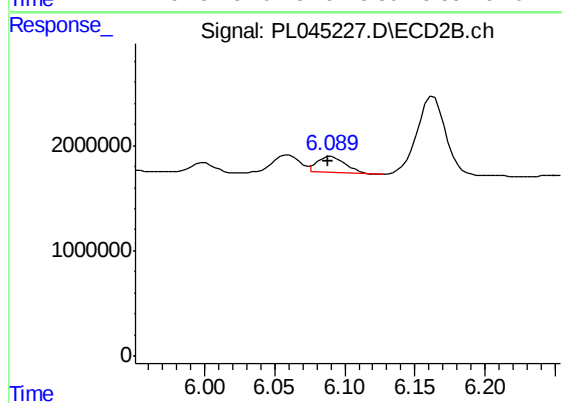

#10 gamma-Chlordane


R.T.: 6.090 min
Delta R.T.: 0.003 min
Response: 2267354
Conc: 0.85 ng/ml

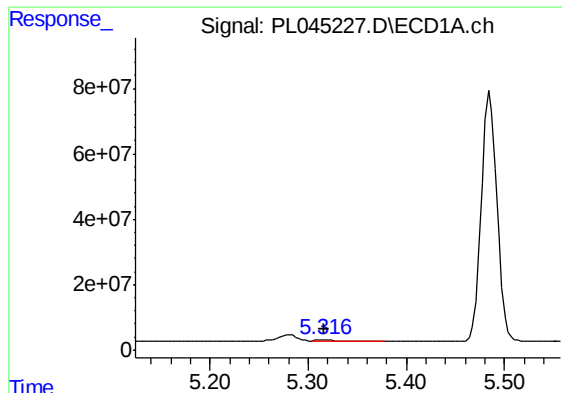

#11 alpha-Chlordane


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 9358731
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

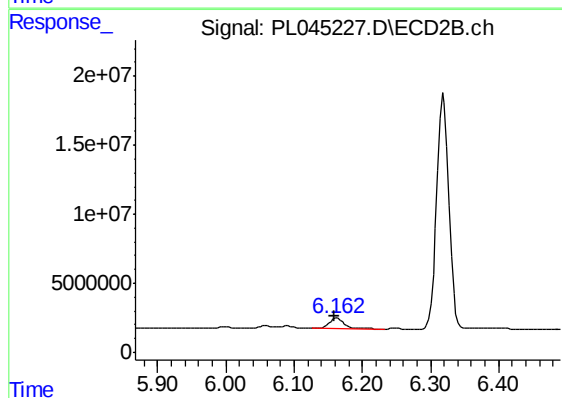


#11 alpha-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.003 min
Response: 10890634
Conc: 4.04 ng/ml

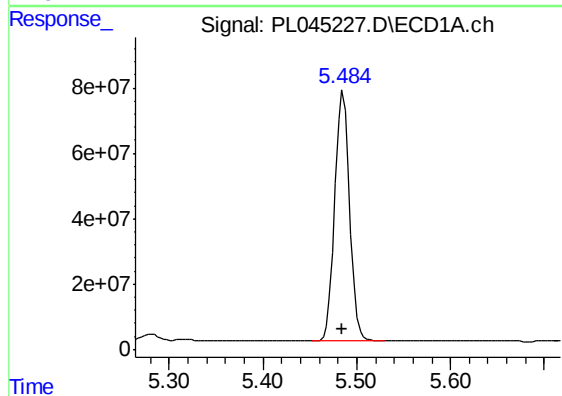


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: 0.002 min
Response: 844611193
Conc: 96.22 ng/ml

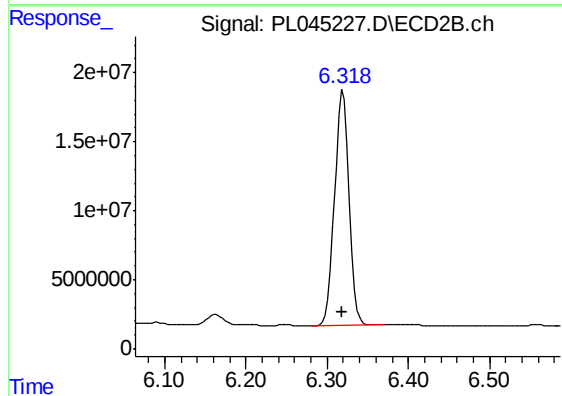

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.001 min
Response: 212271407
Conc: 90.87 ng/ml

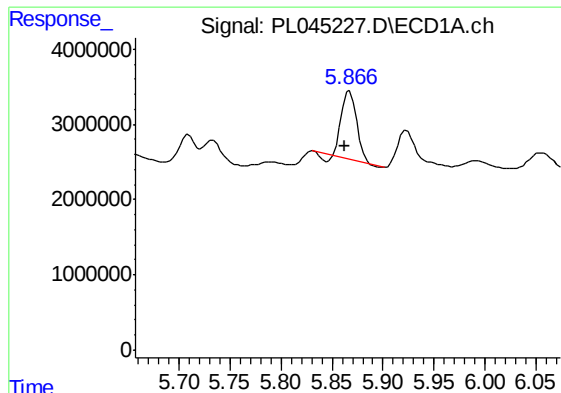

#14 Endrin


R.T.: 5.867 min
Delta R.T.: 0.005 min
Response: 9277679
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

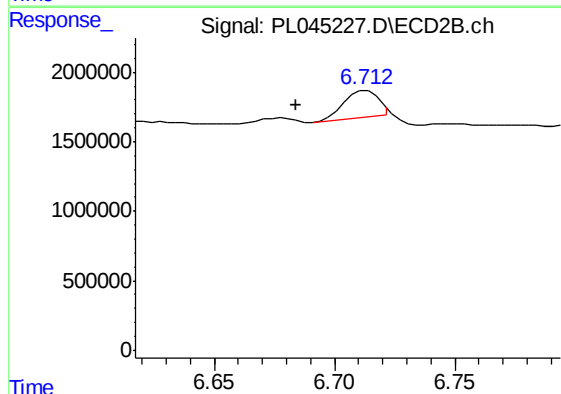


#14 Endrin

R.T.: 6.713 min
Delta R.T.: 0.029 min
Response: 1931384
Conc: 0.85 ng/ml

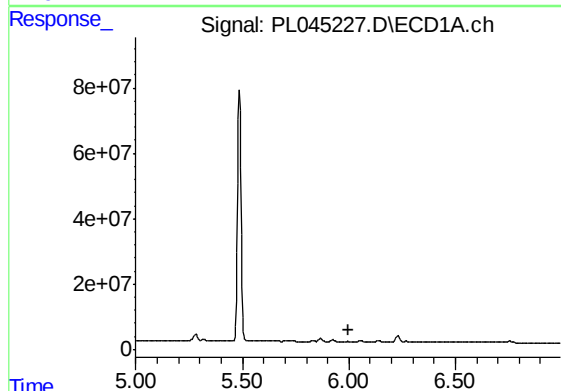


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

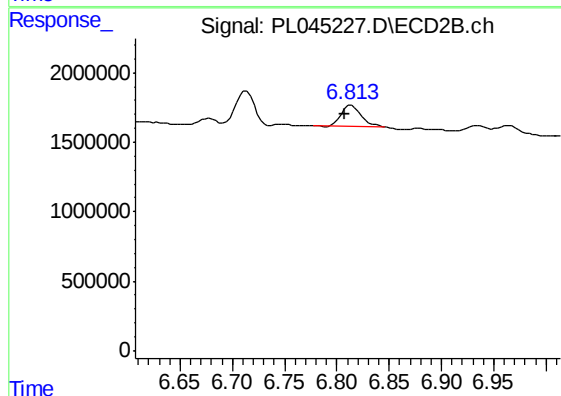

#16 4,4'-DDD


R.T.: 6.814 min
Delta R.T.: 0.006 min
Response: 1955826
Conc: 1.02 ng/ml

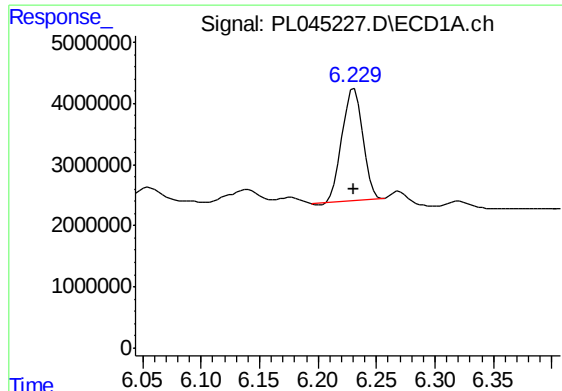

#17 4,4'-DDT


R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 22175079
Conc: 2.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

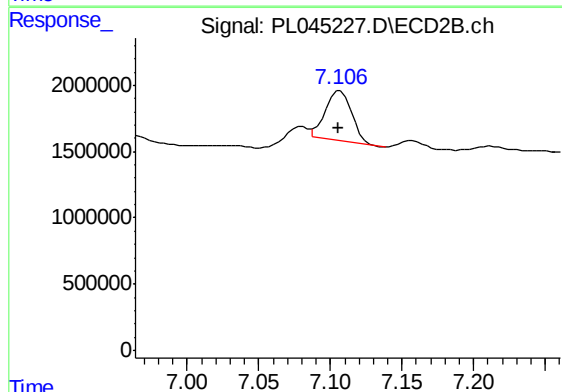


#17 4,4'-DDT

R.T.: 7.107 min
Delta R.T.: 0.001 min
Response: 4820870
Conc: 2.44 ng/ml

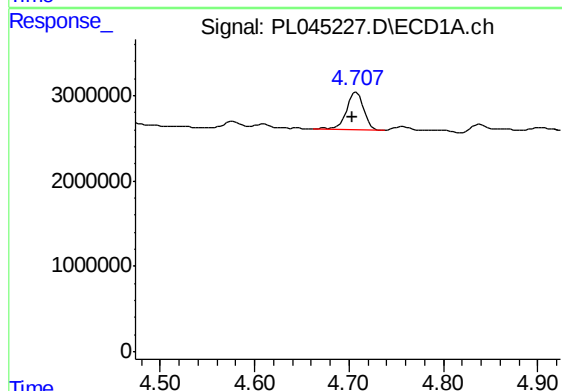


#24 Chlordane-2

R.T.: 4.708 min
Delta R.T.: 0.004 min
Response: 5455594
Conc: 14.10 ng/ml

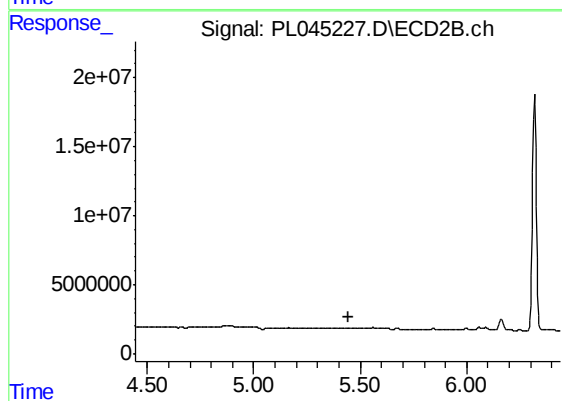

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

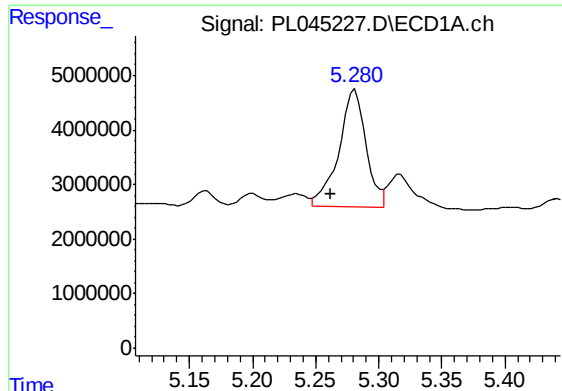

#25 Chlordane-3


R.T.: 5.281 min
Delta R.T.: 0.019 min
Response: 32434368
Conc: 28.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

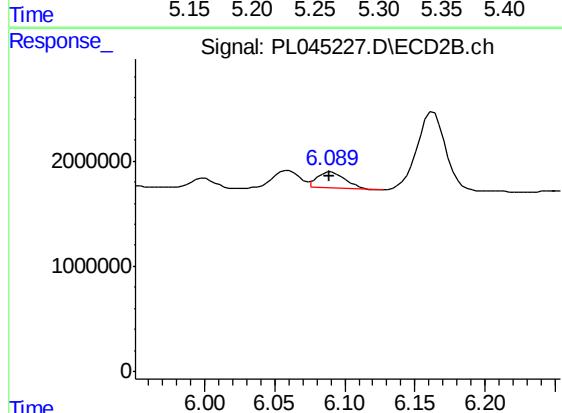


#25 Chlordane-3

R.T.: 6.090 min
Delta R.T.: 0.002 min
Response: 2267354
Conc: 5.82 ng/ml

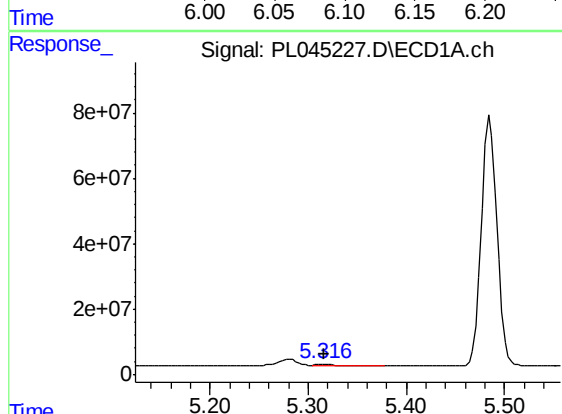


#26 Chlordane-4

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 9358731
Conc: 8.83 ng/ml

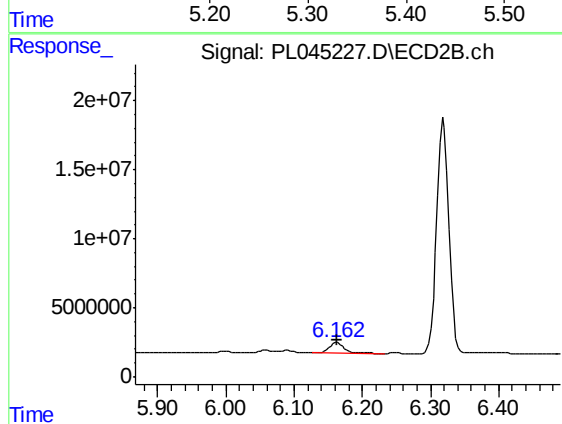

#26 Chlordane-4


R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 10890634
Conc: 23.28 ng/ml

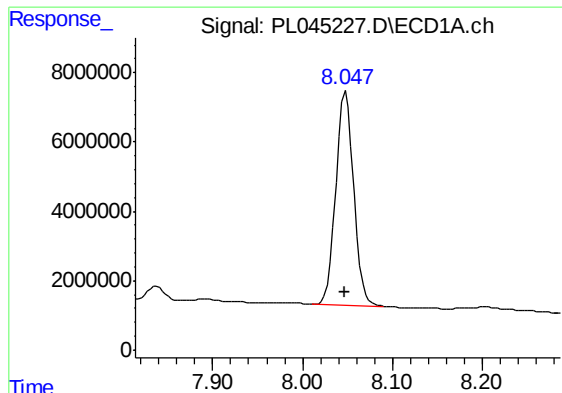

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.001 min
Response: 85106075
Conc: 10.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-(6-2)

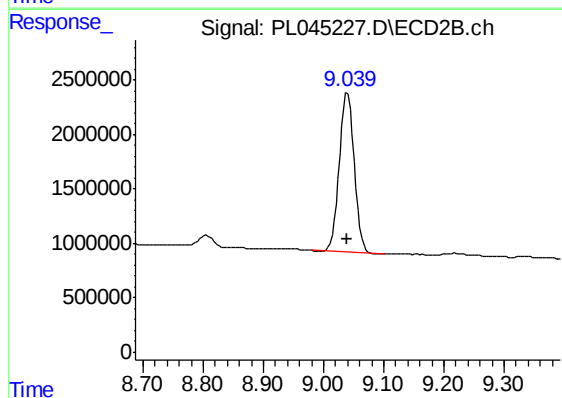

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 25424533
Conc: 11.13 ng/ml