

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 16:24
 Operator : AJ\SJ
 Sample : K1619-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OIL-WATER-SEPERATOR-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:08:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	160.5E6	48860841	23.336	22.816
28)	SA Decachlor...	8.048	9.039	117.0E6	33532540	13.981	14.676
Target Compounds							
5)	MB Aldrin	0.000	5.470	0	4499487	N.D.	1.666 #
11)	B alpha-Chl...	5.319	0.000	72168354	0	7.442	N.D. #
14)	MA Endrin	5.872	0.000	10981238	0	1.219	N.D. #
16)	A 4,4'-DDD	0.000	6.826f	0	2188561	N.D.	1.138 #
24)	Chlordane-2	0.000	5.470f	0	4499487	N.D.	37.238 #
26)	Chlordane-4	5.319	0.000	72168354	0	68.080	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 16:24
Operator : AJ\SJ
Sample : K1619-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:08:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

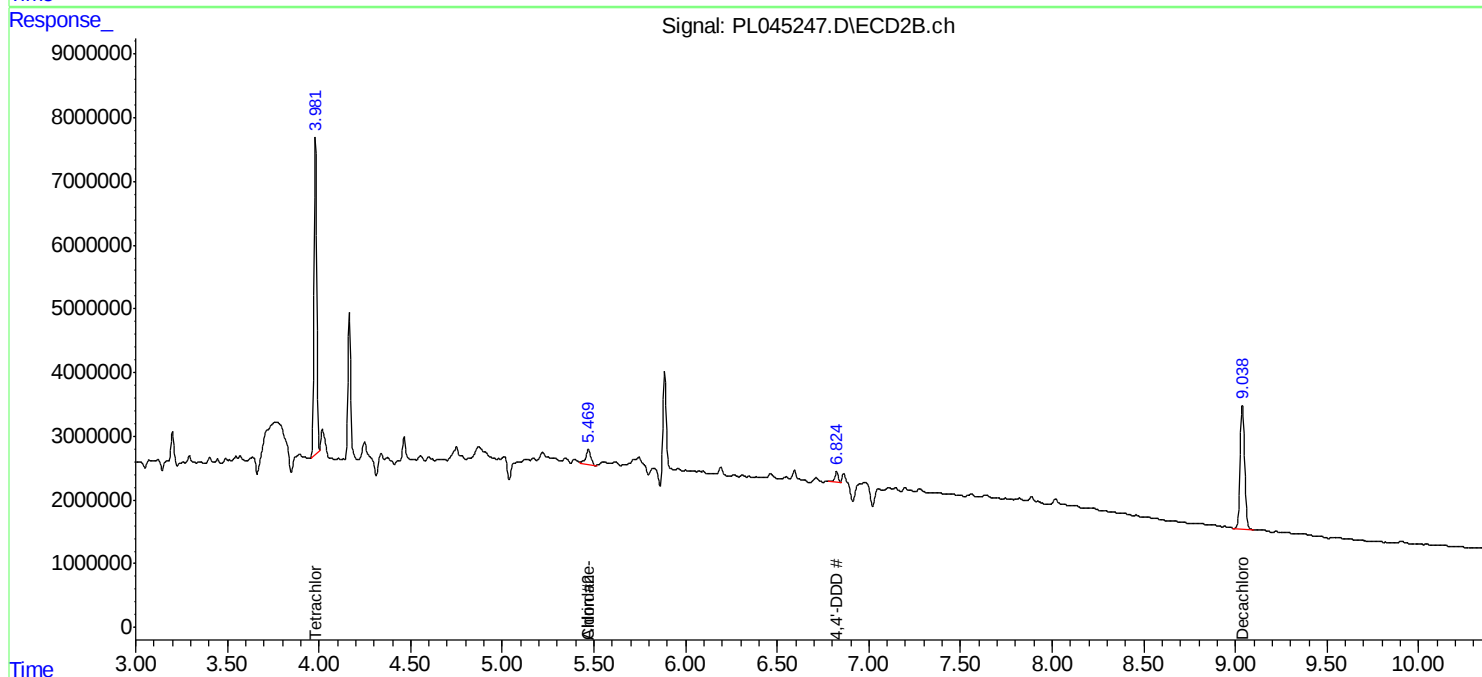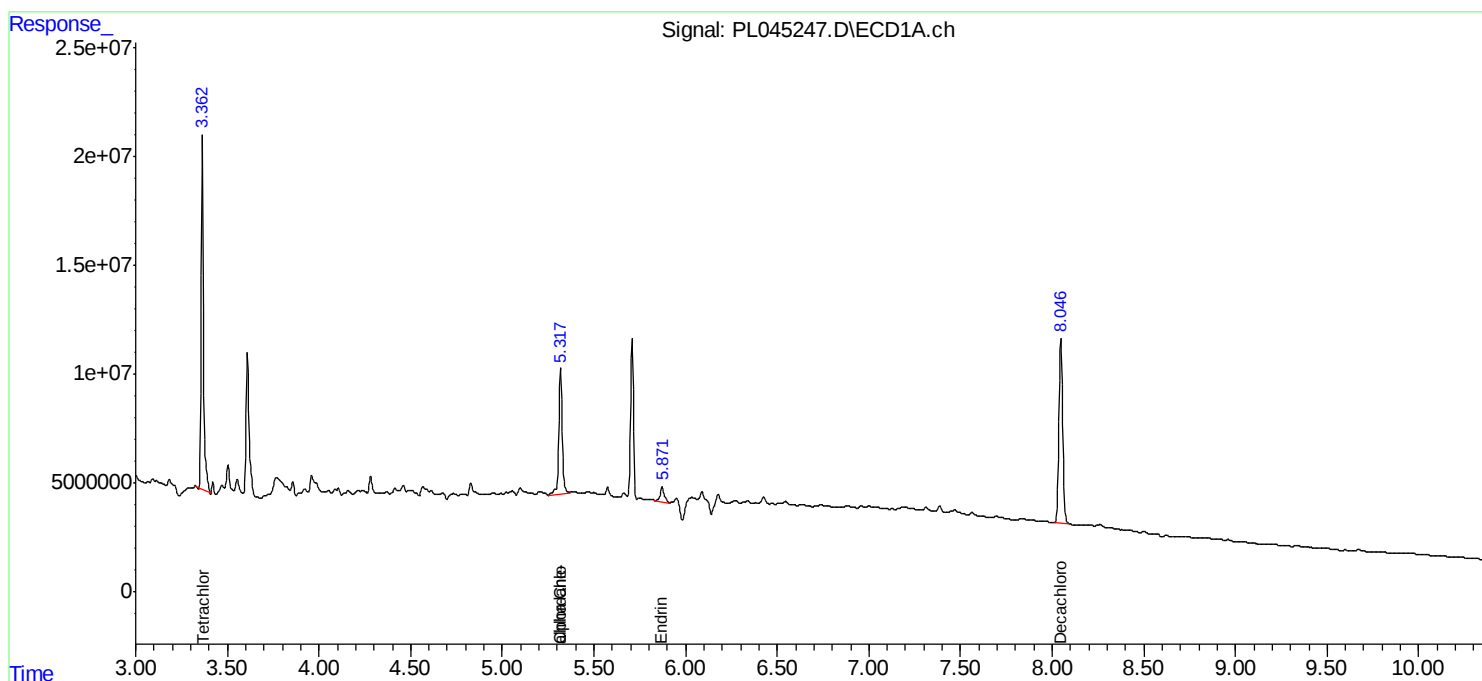


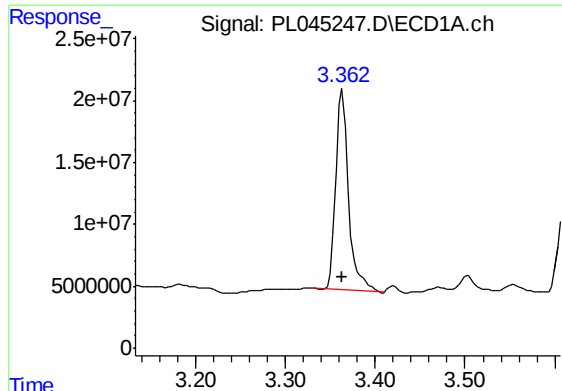

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 160533700
Conc: 23.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2

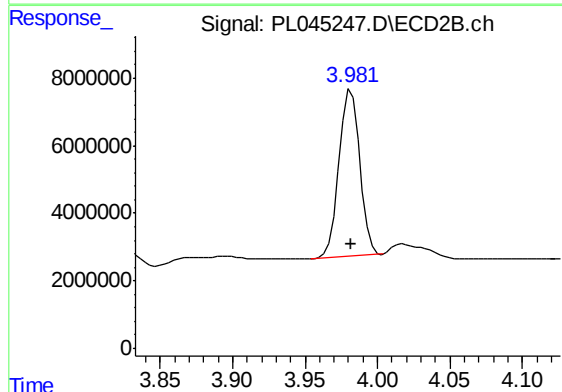


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 48860841
Conc: 22.82 ng/ml

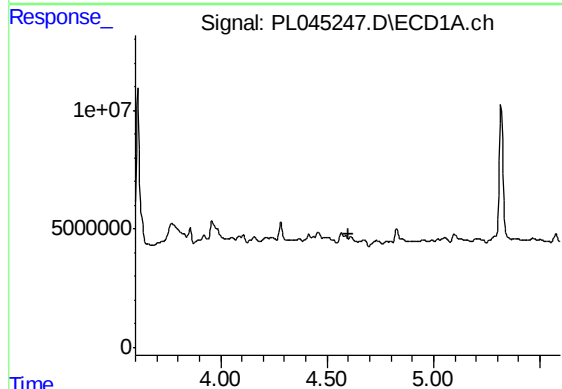


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.599 min
Response: 0
Conc: N.D.

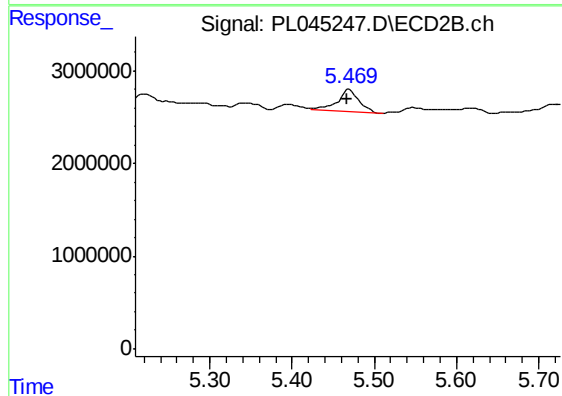

#5 Aldrin


R.T.: 5.470 min
Delta R.T.: 0.003 min
Response: 4499487
Conc: 1.67 ng/ml

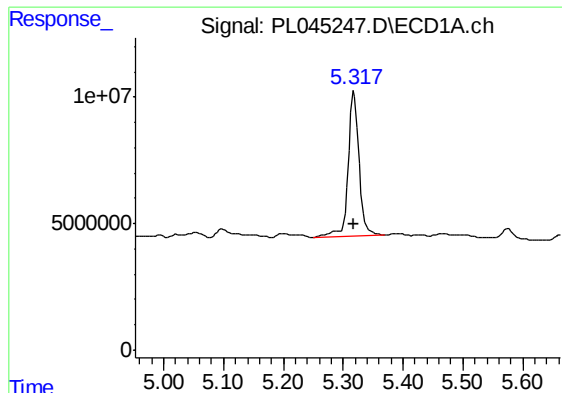

#11 alpha-Chlordane


R.T.: 5.319 min
Delta R.T.: 0.002 min
Response: 72168354
Conc: 7.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2

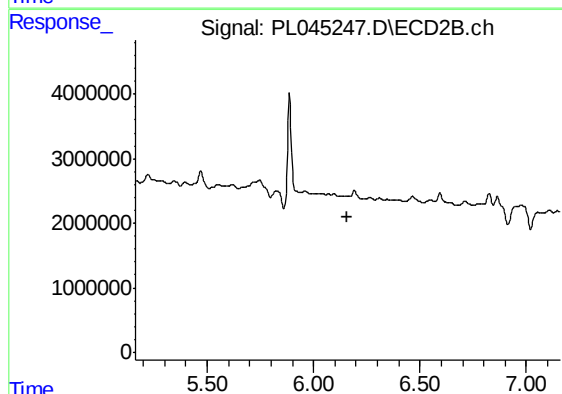


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

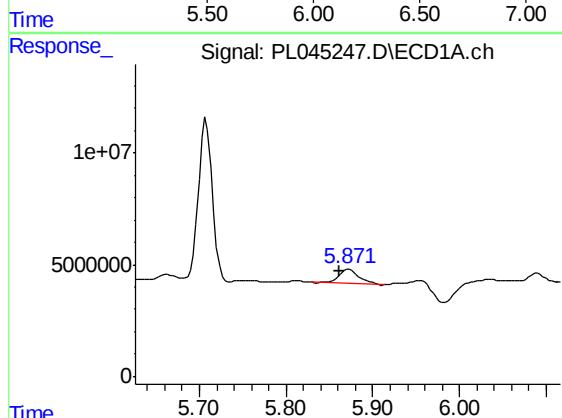


#14 Endrin

R.T.: 5.872 min
Delta R.T.: 0.010 min
Response: 10981238
Conc: 1.22 ng/ml

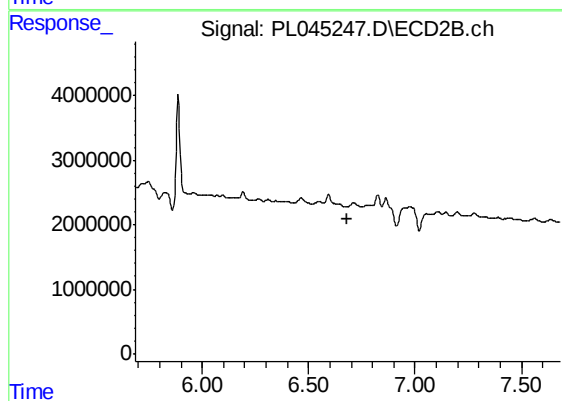

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.684 min
Response: 0
Conc: N.D.

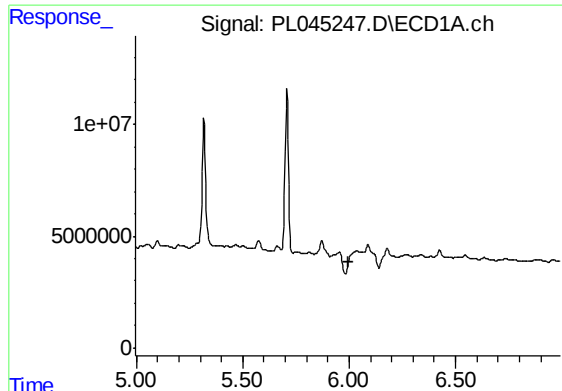

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2

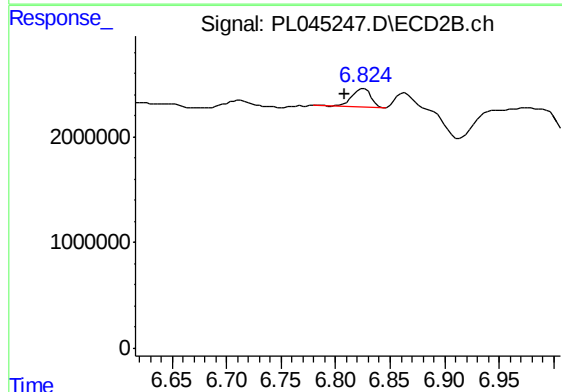


#16 4,4'-DDD

R.T.: 6.826 min
Delta R.T.: 0.018 min
Response: 2188561
Conc: 1.14 ng/ml

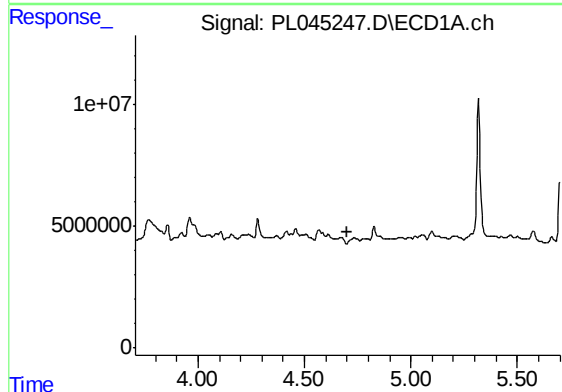


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

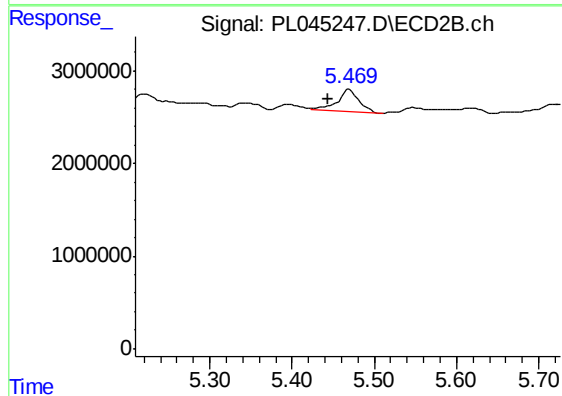

#24 Chlordane-2


R.T.: 5.470 min
Delta R.T.: 0.027 min
Response: 4499487
Conc: 37.24 ng/ml

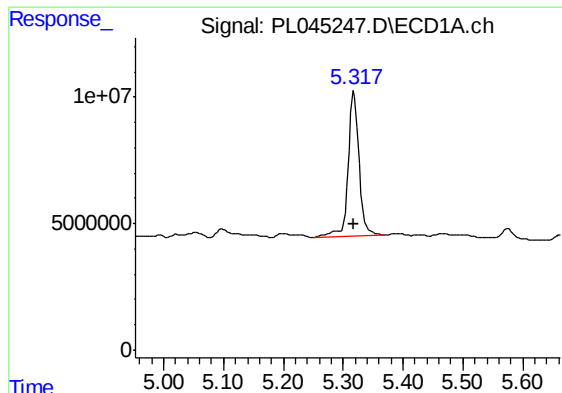

#26 Chlordane-4


R.T.: 5.319 min
Delta R.T.: 0.002 min
Response: 72168354
Conc: 68.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2

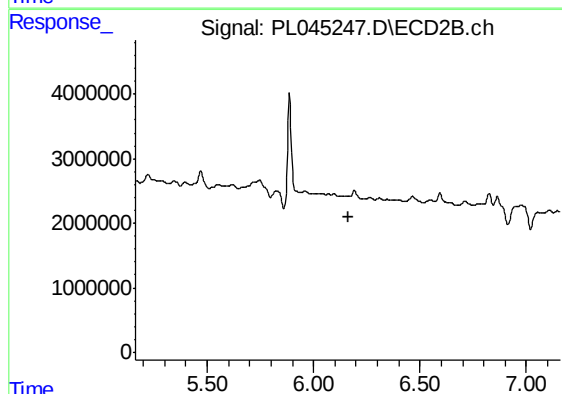


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

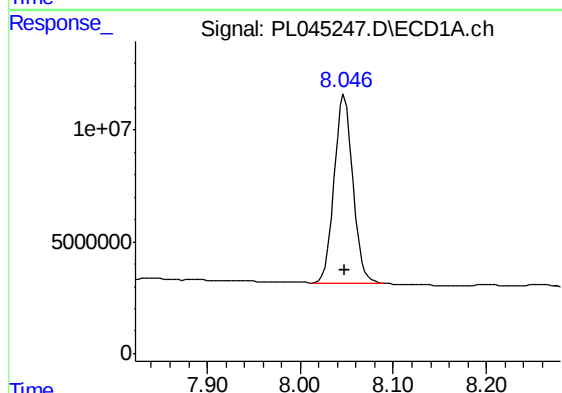

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 116988420
Conc: 13.98 ng/ml

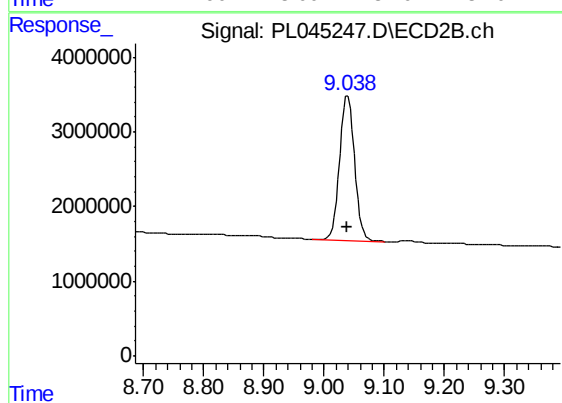

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 33532540
Conc: 14.68 ng/ml