

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 17:34
 Operator : AJ\SJ
 Sample : K1643-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FLOOR-SLAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:09:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	140.0E6	40460278	20.358	18.893
28)	SA Decachlor...	8.047	9.040	201.0E6	50451395	24.027	22.080
Target Compounds							
2)	A alpha-BHC	0.000	4.397f	0	1360851	N.D.	0.448 #
5)	MB Aldrin	4.613	5.454	23634138	4866325	2.430	1.802 #
8)	B Heptachlo...	0.000	5.846	0	2758848	N.D.	1.149 #
10)	B gamma-Chl...	5.284f	0.000	5615694	0	0.574	N.D. #
12)	B 4,4'-DDE	5.484	6.319	4107526	4086464	0.468	1.749 #
13)	MA Dieldrin	5.607	6.461	17652374	2252855	1.847	0.877 #
14)	MA Endrin	0.000	6.679	0	5218160	N.D.	2.293 #
15)	B Endosulfa...	6.124	0.000	6397624	0	0.738	N.D. #
16)	A 4,4'-DDD	0.000	6.815	0	5567709	N.D.	2.895 #
17)	MA 4,4'-DDT	6.226	7.079f	22952737	-444933	3.060	N.D. #
18)	B Endrin al...	6.318	0.000	8186897	0	1.120	N.D. #
19)	B Endosulfa...	6.510	0.000	5544678	0	0.682	N.D. #
20)	A Methoxychlor	6.755f	0.000	10860703	0	2.473	N.D. #
24)	Chlordane-2	4.679f	5.454	27932201	4866325	72.210	40.274 #
25)	Chlordane-3	5.284f	0.000	5615694	0	4.896	N.D. #
27)	Chlordane-5	6.124f	0.000	6397624	0	18.525	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 17:34
Operator : AJ\SJ
Sample : K1643-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:09:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

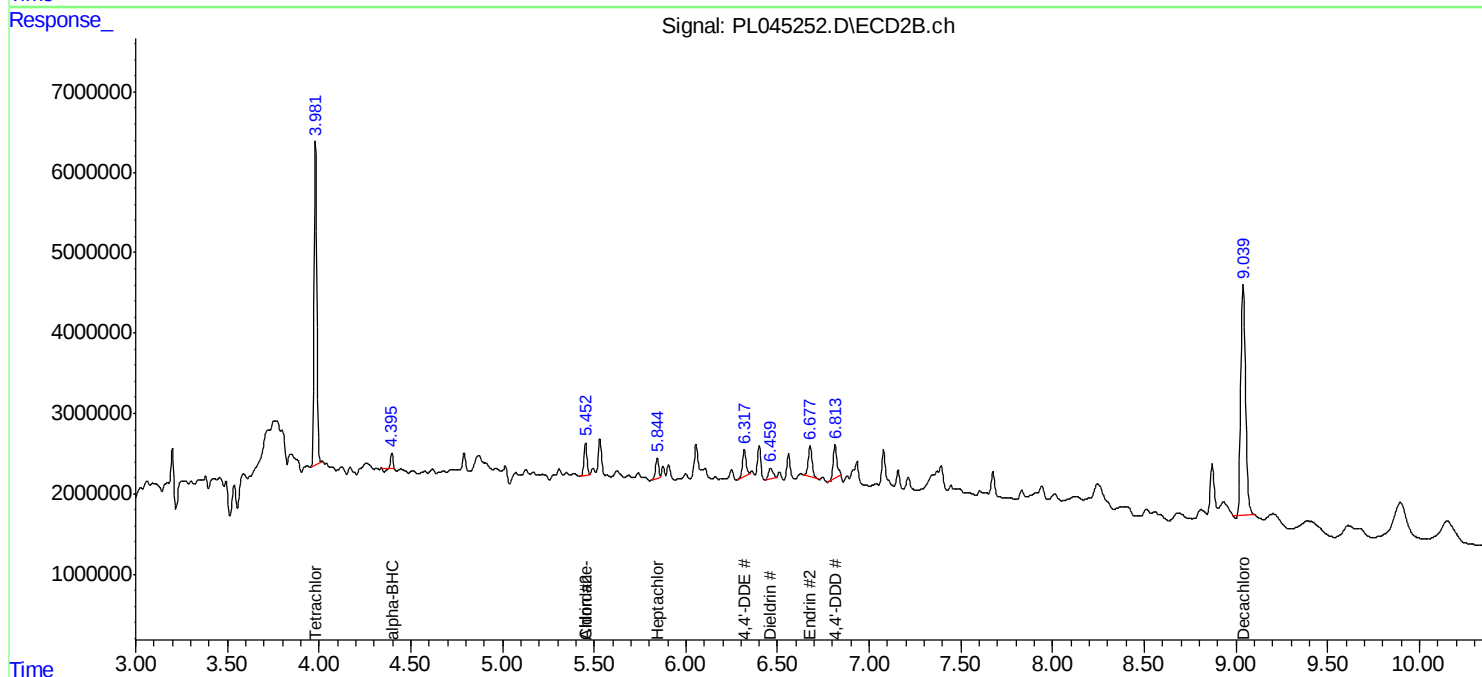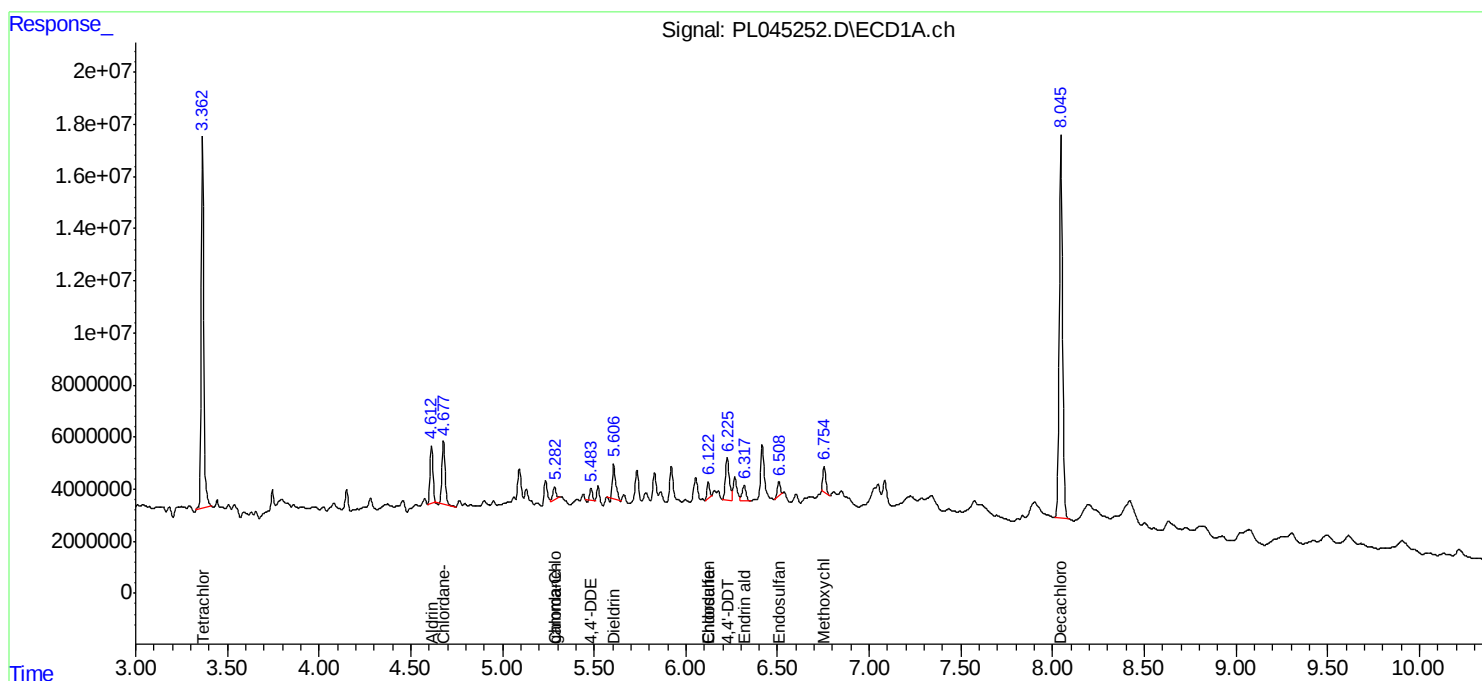


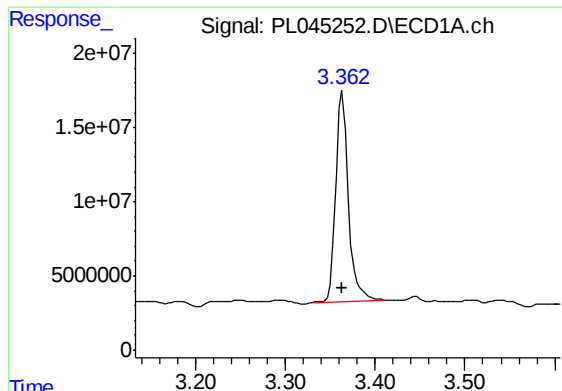

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 140045589
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

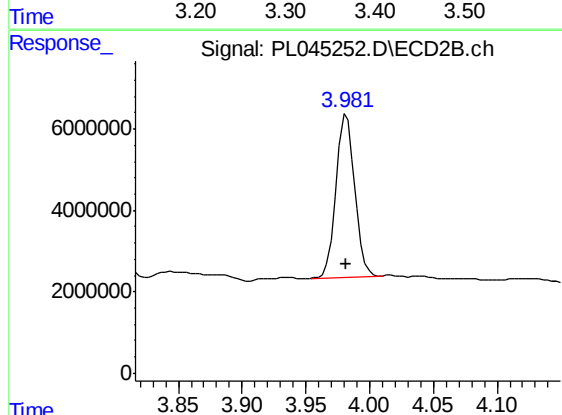


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 40460278
Conc: 18.89 ng/ml

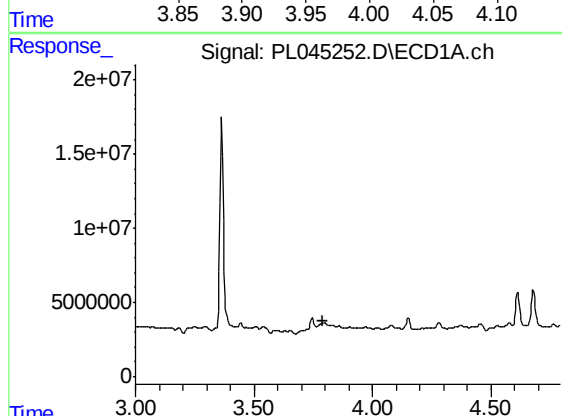


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.794 min
Response: 0
Conc: N.D.

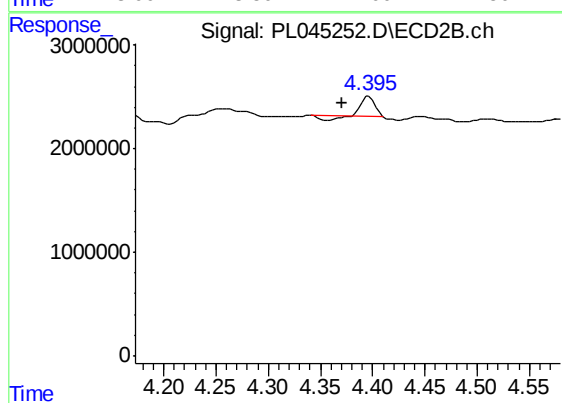

#2 alpha-BHC


R.T.: 4.397 min
Delta R.T.: 0.025 min
Response: 1360851
Conc: 0.45 ng/ml

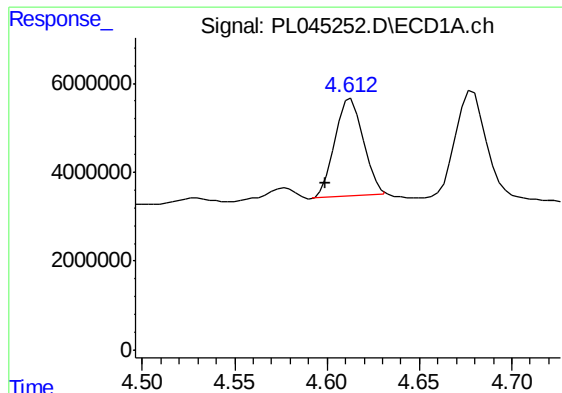

#5 Aldrin


R.T.: 4.613 min
Delta R.T.: 0.014 min
Response: 23634138
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

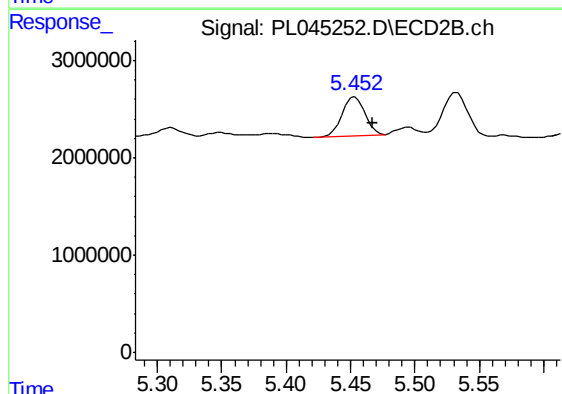


#5 Aldrin

R.T.: 5.454 min
Delta R.T.: -0.014 min
Response: 4866325
Conc: 1.80 ng/ml

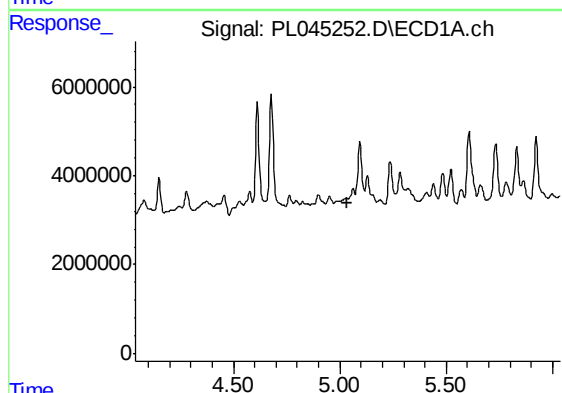


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

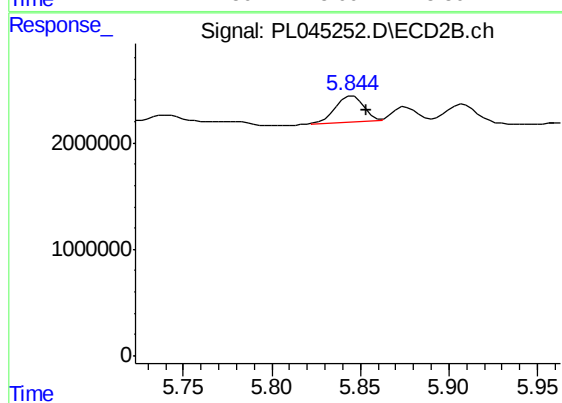

#8 Heptachlor epoxide


R.T.: 5.846 min
Delta R.T.: -0.008 min
Response: 2758848
Conc: 1.15 ng/ml

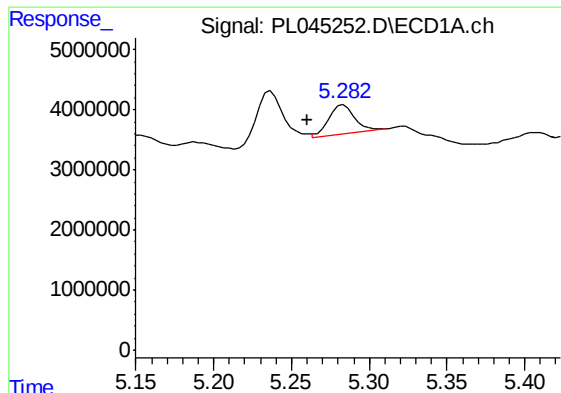

#10 gamma-Chlordane


R.T.: 5.284 min
Delta R.T.: 0.023 min
Response: 5615694
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

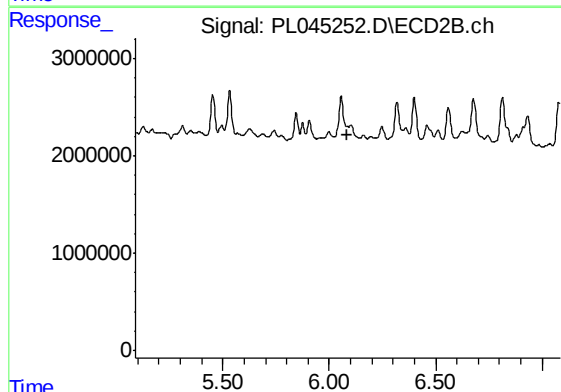


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

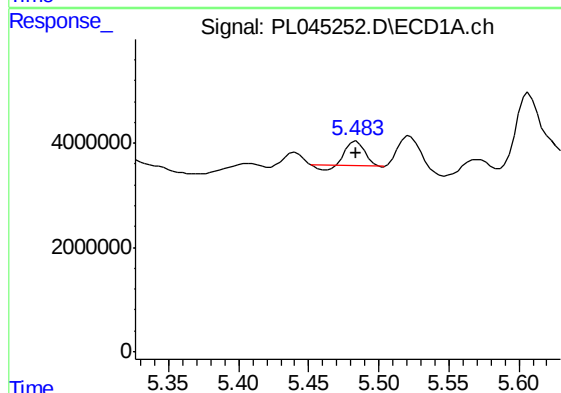


#12 4,4'-DDE

R.T.: 5.484 min
Delta R.T.: 0.000 min
Response: 4107526
Conc: 0.47 ng/ml

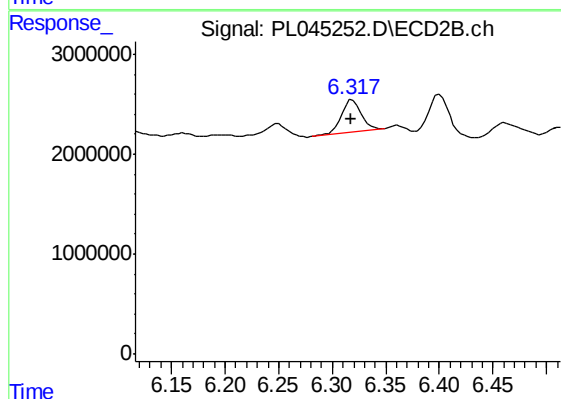

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 4086464
Conc: 1.75 ng/ml

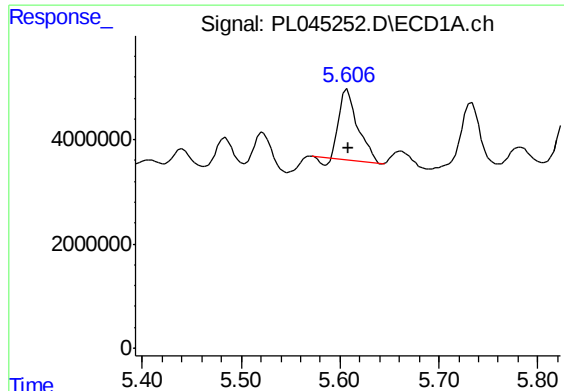

#13 Dieldrin


R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 17652374
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

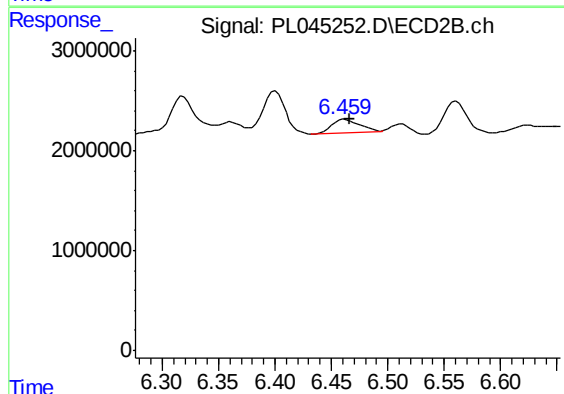


#13 Dieldrin

R.T.: 6.461 min
Delta R.T.: -0.006 min
Response: 2252855
Conc: 0.88 ng/ml

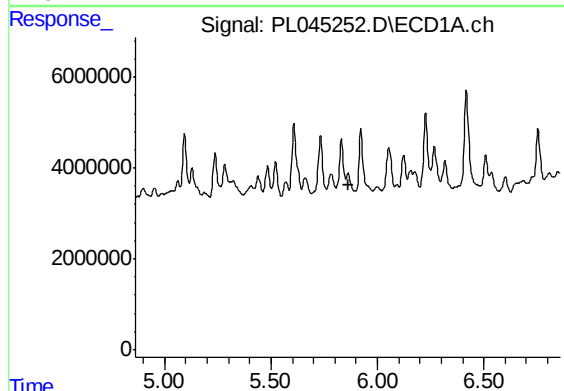


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.862 min
Response: 0
Conc: N.D.

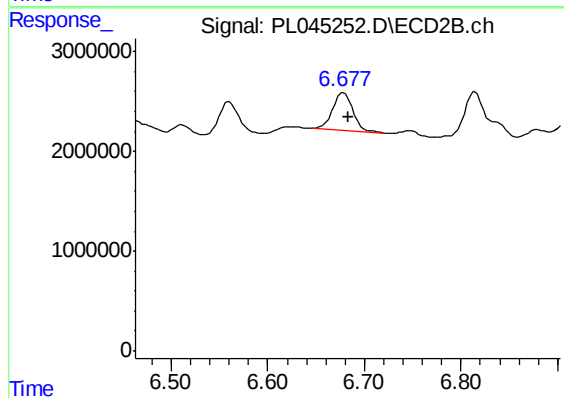

#14 Endrin


R.T.: 6.679 min
Delta R.T.: -0.005 min
Response: 5218160
Conc: 2.29 ng/ml

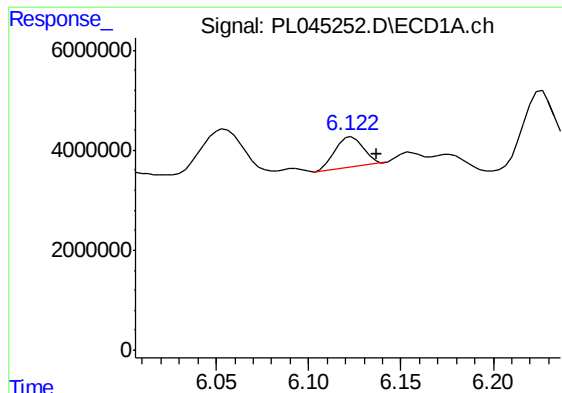

#15 Endosulfan II


R.T.: 6.124 min
Delta R.T.: -0.013 min
Response: 6397624
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

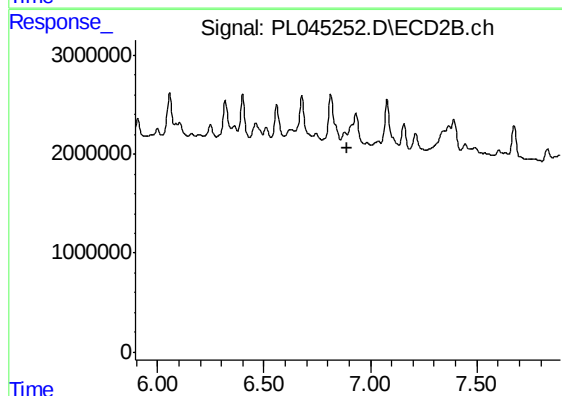


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.894 min
Response: 0
Conc: N.D.

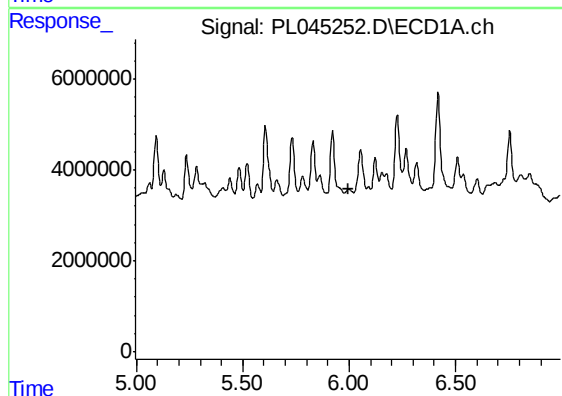


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

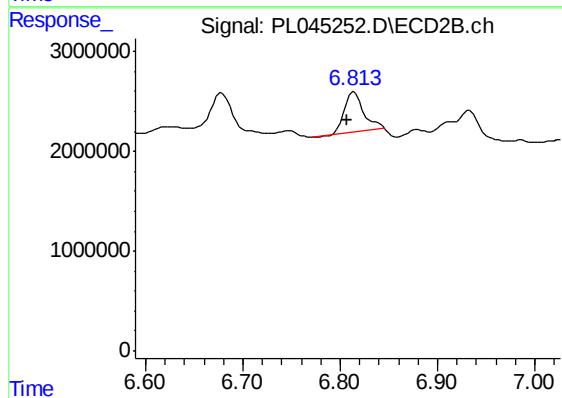

#16 4,4'-DDD


R.T.: 6.815 min
Delta R.T.: 0.007 min
Response: 5567709
Conc: 2.90 ng/ml

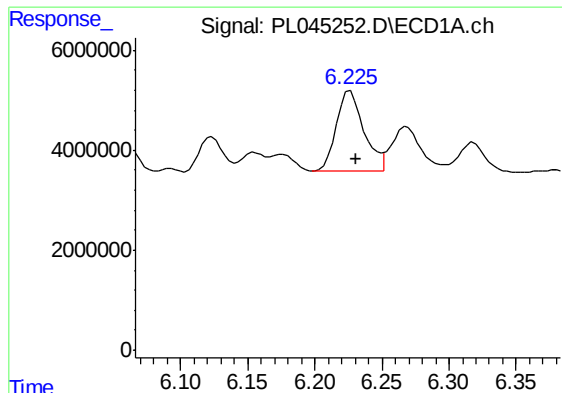

#17 4,4'-DDT


R.T.: 6.226 min
Delta R.T.: -0.004 min
Response: 22952737
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

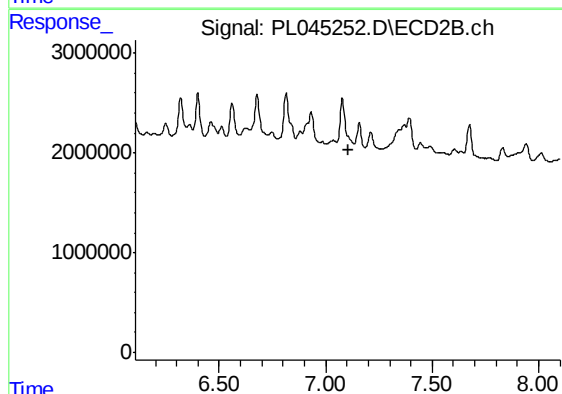


#17 4,4'-DDT

R.T.: 7.079 min
Delta R.T.: -0.027 min
Response: -444933
Conc: N.D.

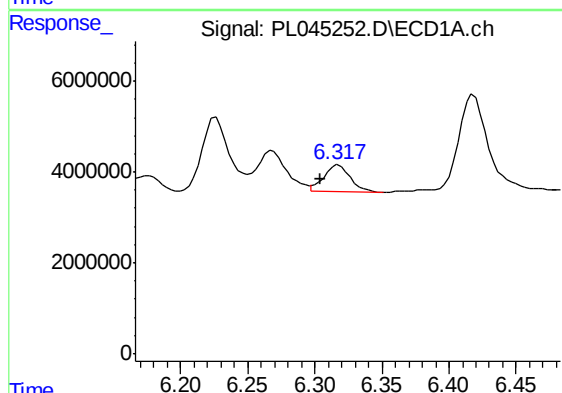


#18 Endrin aldehyde

R.T.: 6.318 min
Delta R.T.: 0.014 min
Response: 8186897
Conc: 1.12 ng/ml

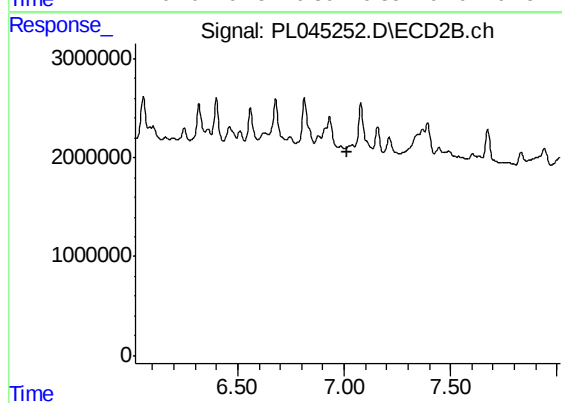

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

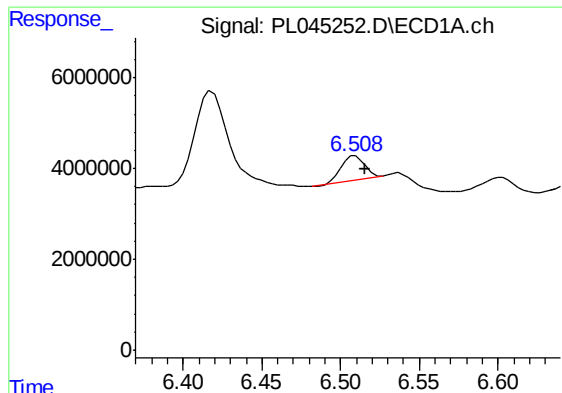

#19 Endosulfan Sulfate


R.T.: 6.510 min
Delta R.T.: -0.006 min
Response: 5544678
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

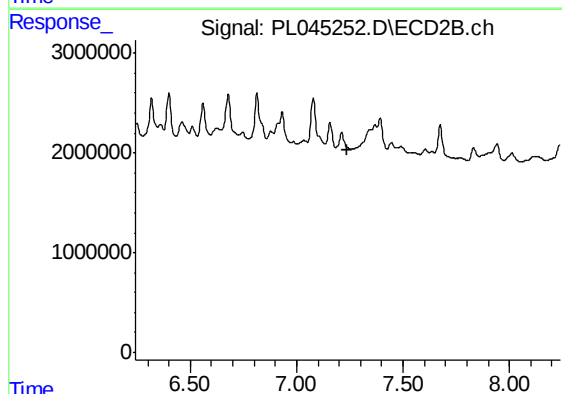


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

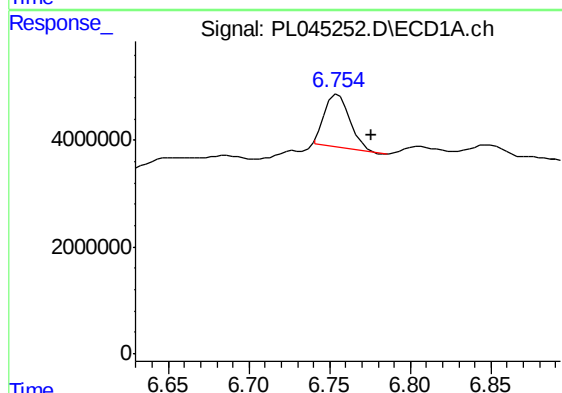


#20 Methoxychlor

R.T.: 6.755 min
Delta R.T.: -0.021 min
Response: 10860703
Conc: 2.47 ng/ml

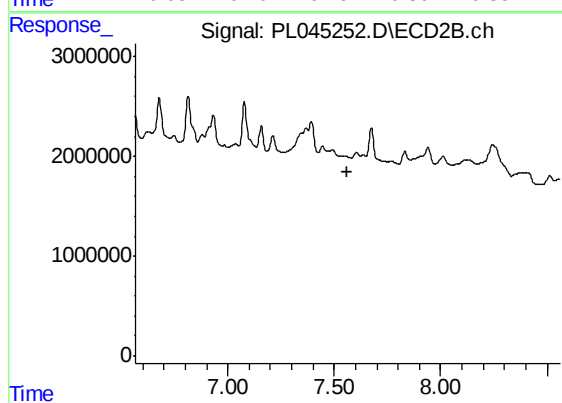

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

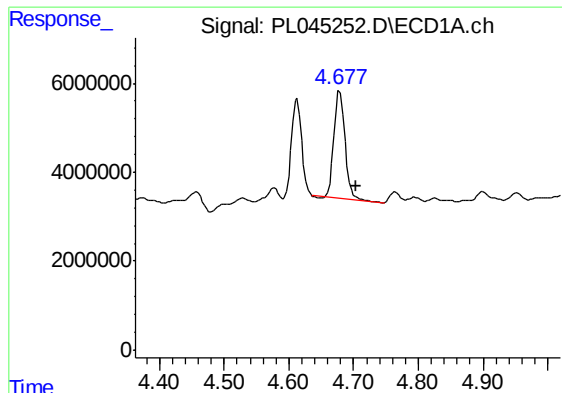

#24 Chlordane-2


R.T.: 4.679 min
Delta R.T.: -0.025 min
Response: 27932201
Conc: 72.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

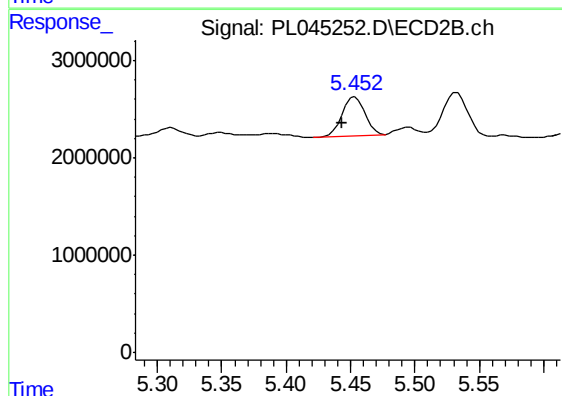


#24 Chlordane-2

R.T.: 5.454 min
Delta R.T.: 0.011 min
Response: 4866325
Conc: 40.27 ng/ml

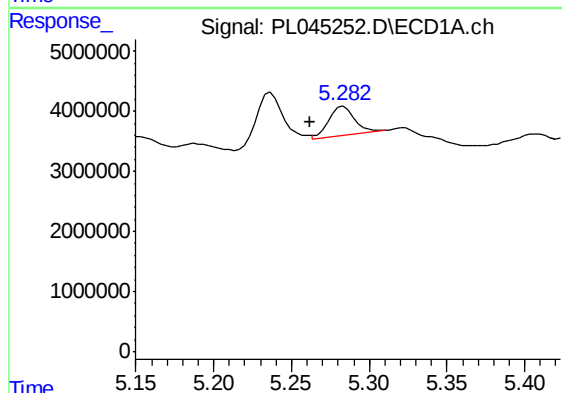


#25 Chlordane-3

R.T.: 5.284 min
Delta R.T.: 0.022 min
Response: 5615694
Conc: 4.90 ng/ml

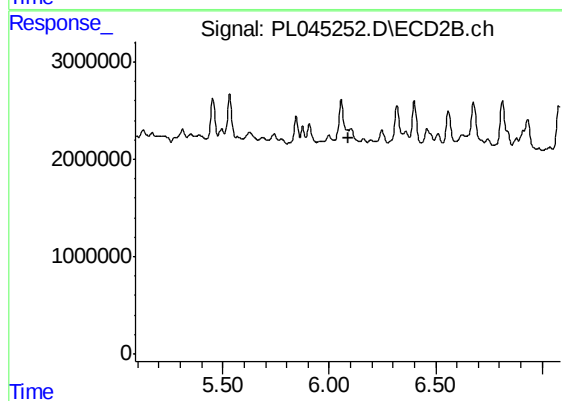

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

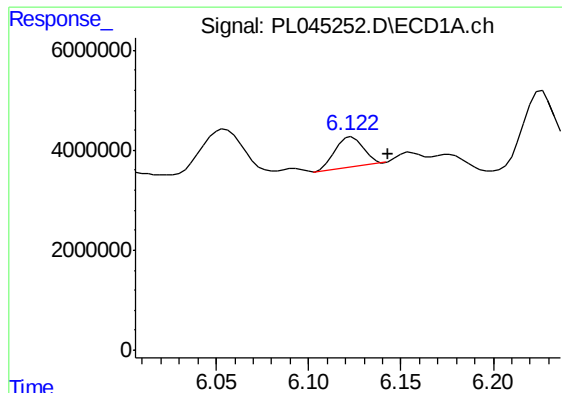

#27 Chlordane-5


R.T.: 6.124 min
Delta R.T.: -0.019 min
Response: 6397624
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOOR-SLAB

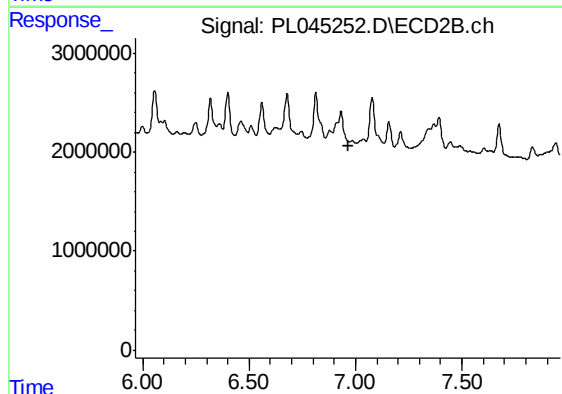


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.966 min
Response: 0
Conc: N.D.

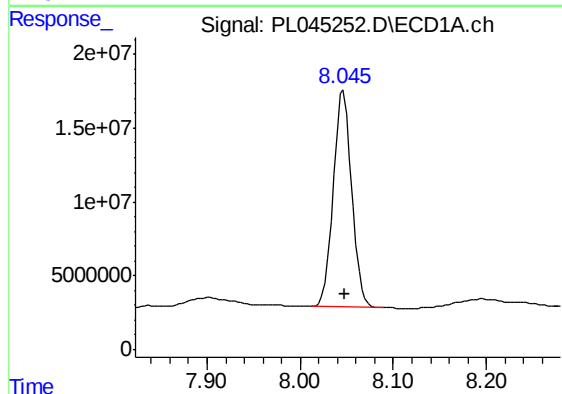

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 201044147
Conc: 24.03 ng/ml

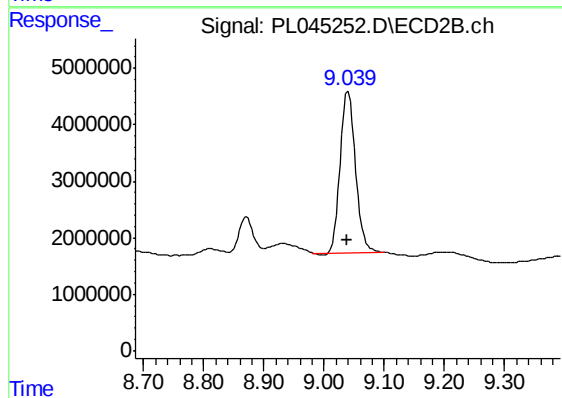

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 50451395
Conc: 22.08 ng/ml