

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 23:13
 Operator : AJ\SJ
 Sample : K1643-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INTERIOR-WALL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:15:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	157.2E6	47602784	22.847	22.228
28)	SA Decachlor...	8.046	9.038	187.5E6	55590123	22.411	24.329
Target Compounds							
4)	MA Heptachlor	0.000	5.140f	0	13471960	N.D.	4.528 #
8)	B Heptachlo...	0.000	5.841	0	2967959	N.D.	1.236 #
11)	B alpha-Chl...	5.312	0.000	15236797	0	1.571	N.D. #
14)	MA Endrin	0.000	6.672	0	3005098	N.D.	1.321 #
15)	B Endosulfa...	0.000	6.901	0	742628	N.D.	0.316 #
16)	A 4,4'-DDD	6.010	0.000	10204597	0	1.394	N.D. #
17)	MA 4,4'-DDT	0.000	7.127f	0	3722222	N.D.	1.886 #
18)	B Endrin al...	0.000	7.046f	0	2381006	N.D.	1.165 #
26)	Chlordane-4	5.312	0.000	15236797	0	14.374	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 23:13
Operator : AJ\SJ
Sample : K1643-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:15:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

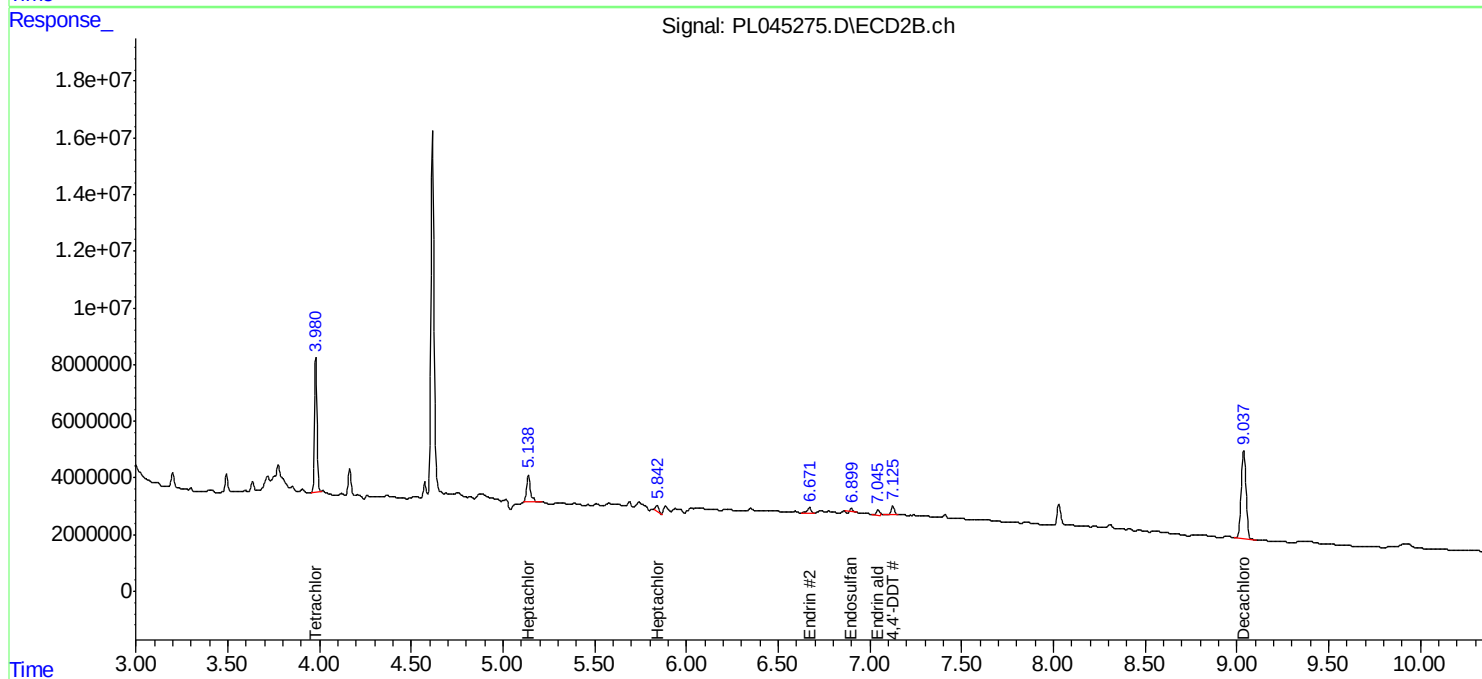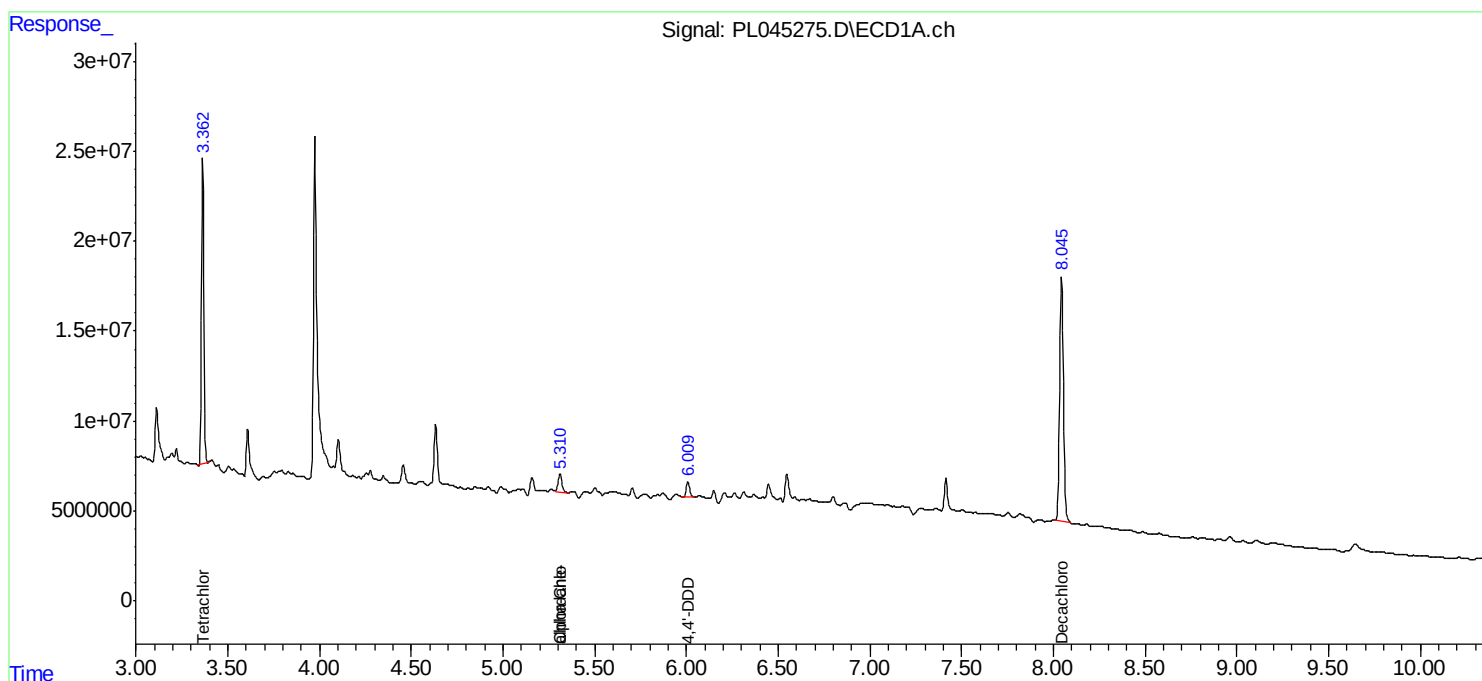


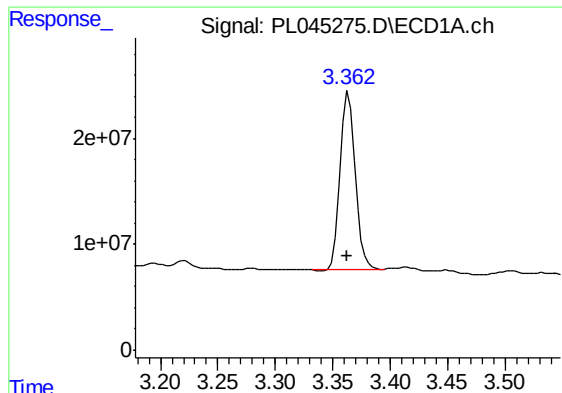

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 157172475
Conc: 22.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

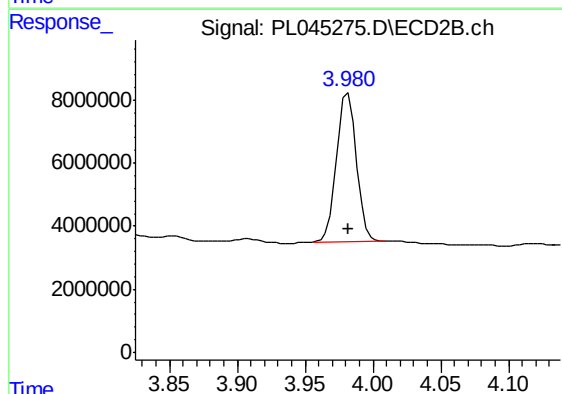


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 47602784
Conc: 22.23 ng/ml

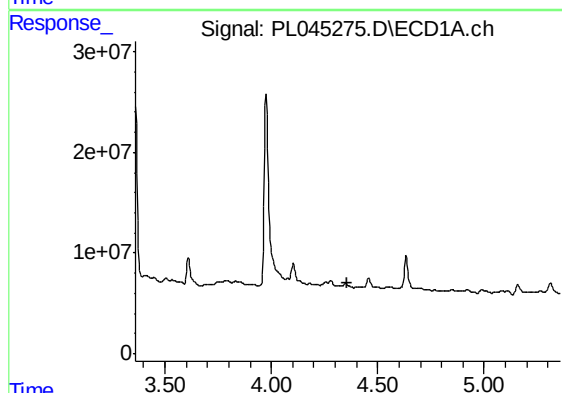


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.358 min
Response: 0
Conc: N.D.

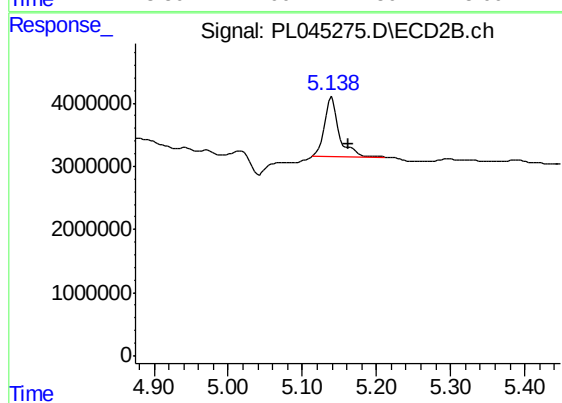

#4 Heptachlor


R.T.: 5.140 min
Delta R.T.: -0.024 min
Response: 13471960
Conc: 4.53 ng/ml

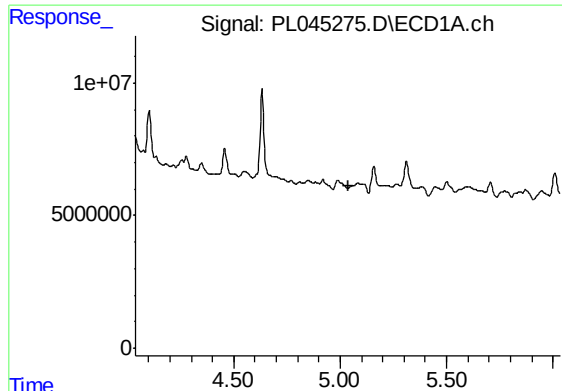

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

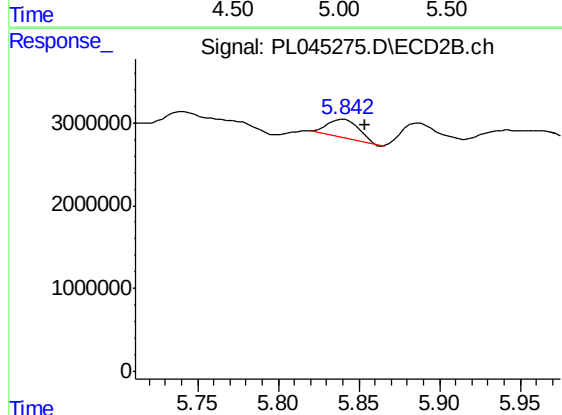


#8 Heptachlor epoxide

R.T.: 5.841 min
Delta R.T.: -0.013 min
Response: 2967959
Conc: 1.24 ng/ml

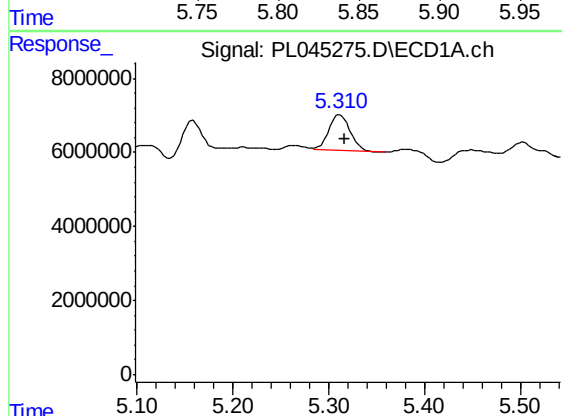


#11 alpha-Chlordane

R.T.: 5.312 min
Delta R.T.: -0.005 min
Response: 15236797
Conc: 1.57 ng/ml

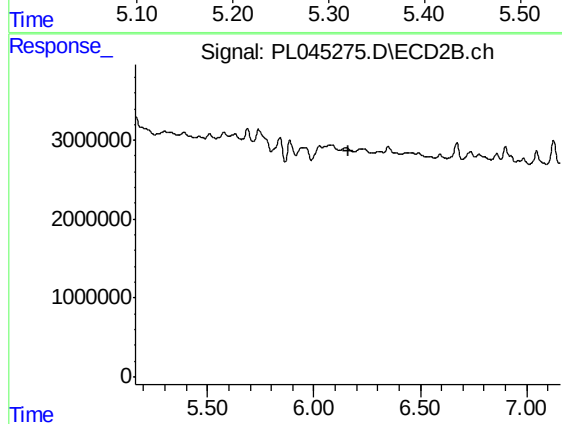

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

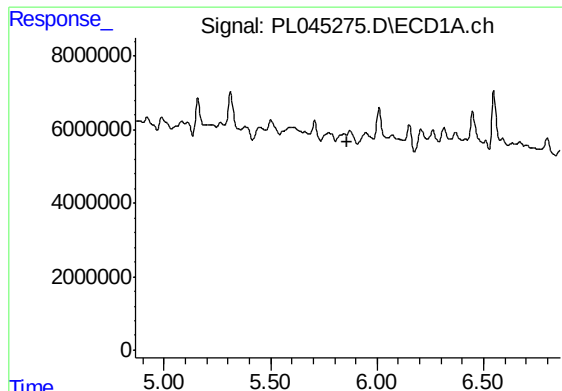

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

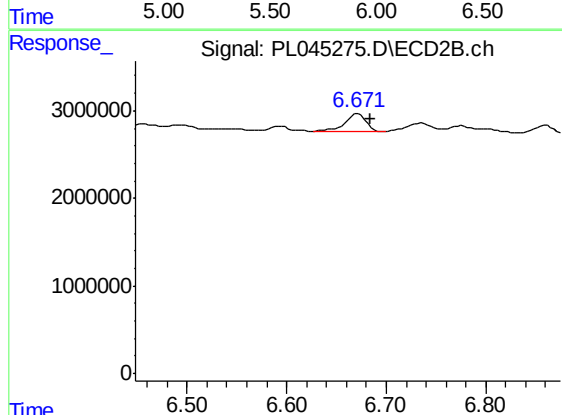


#14 Endrin

R.T.: 6.672 min
Delta R.T.: -0.012 min
Response: 3005098
Conc: 1.32 ng/ml

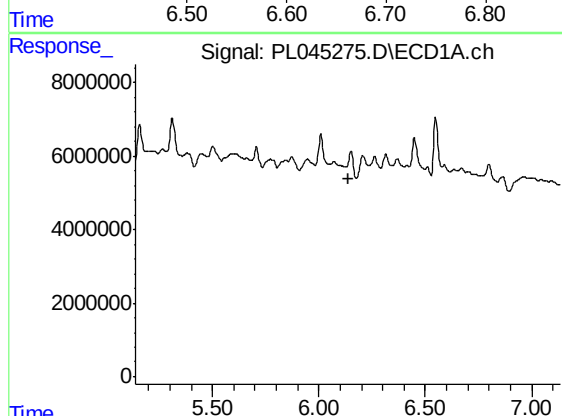


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

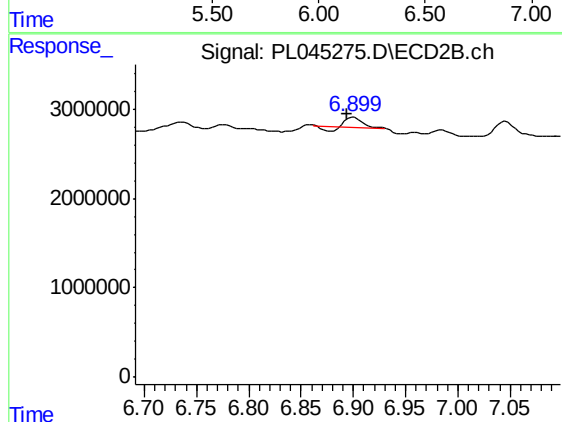

#15 Endosulfan II


R.T.: 6.901 min
Delta R.T.: 0.007 min
Response: 742628
Conc: 0.32 ng/ml

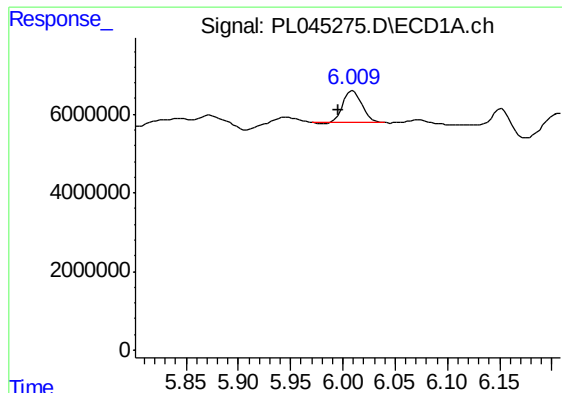

#16 4,4'-DDD


R.T.: 6.010 min
Delta R.T.: 0.014 min
Response: 10204597
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

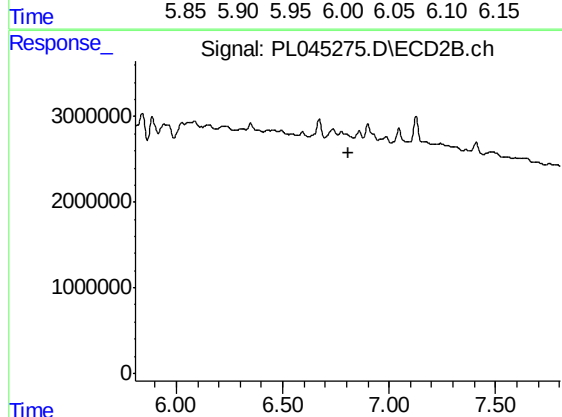


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

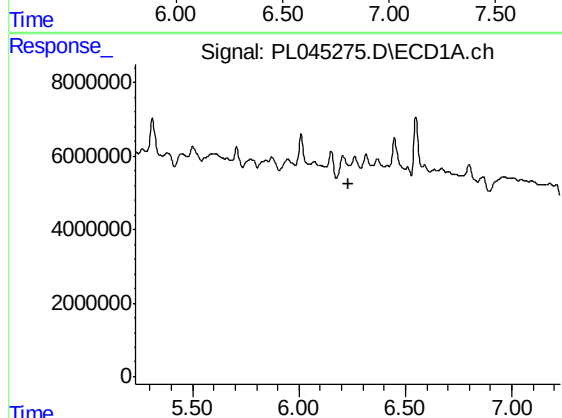


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

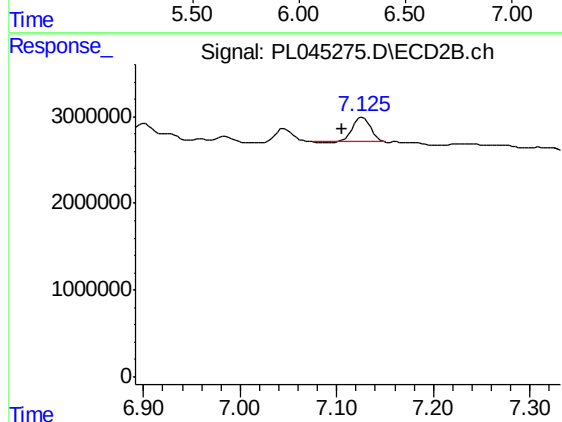

#17 4,4'-DDT


R.T.: 7.127 min
Delta R.T.: 0.021 min
Response: 3722222
Conc: 1.89 ng/ml

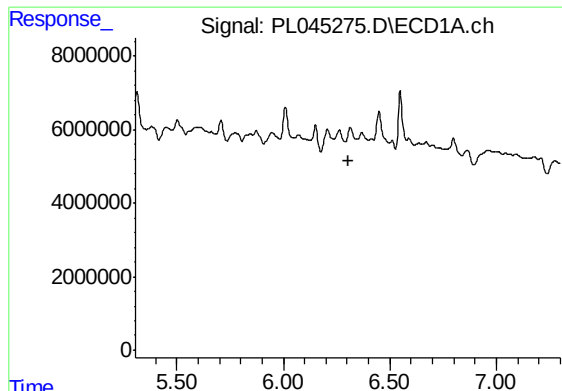

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.304 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

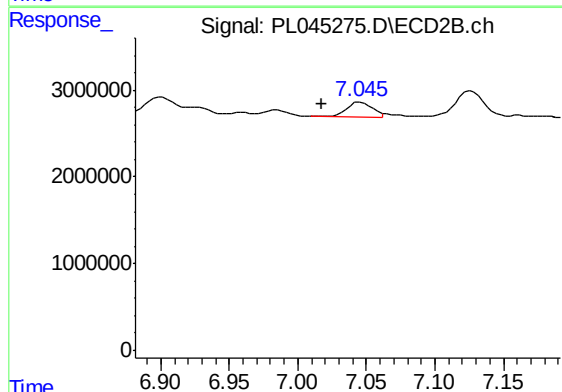


#18 Endrin aldehyde

R.T.: 7.046 min
Delta R.T.: 0.028 min
Response: 2381006
Conc: 1.16 ng/ml

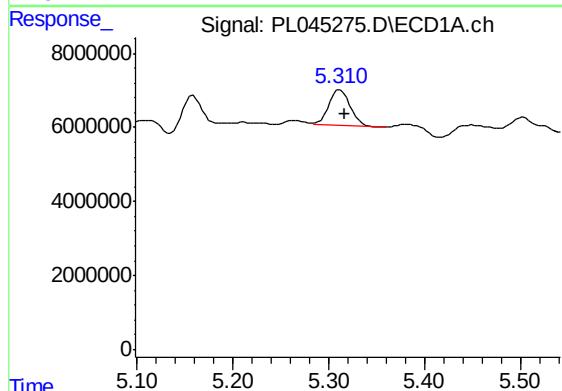


#26 Chlordane-4

R.T.: 5.312 min
Delta R.T.: -0.005 min
Response: 15236797
Conc: 14.37 ng/ml

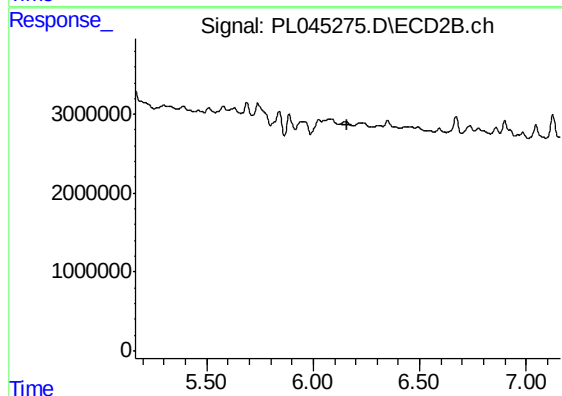

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

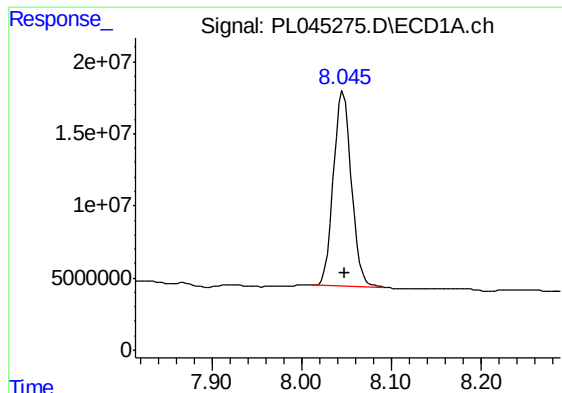

#28 Decachlorobiphenyl

R.T.: 8.046 min
Delta R.T.: 0.000 min
Response: 187520281
Conc: 22.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

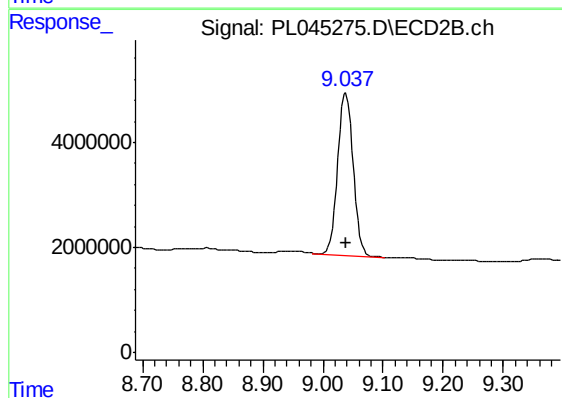

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 55590123
Conc: 24.33 ng/ml