

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 20:09
 Operator : AJ\SJ
 Sample : K1649-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TRE-FLOOR-SLAB

Manual Integrations
 APPROVED

Sohil
 3/1/2019 12:19:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:12:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.362	3.982	119.7E6	40769089	17.406m	19.037
28) SA Decachlor...	8.045	9.038	165.7E6	44543748	19.806m	19.495m
Target Compounds						
12) B 4,4'-DDE	5.483	6.317	43214454	20763350	4.923m	8.889m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 20:09
Operator : AJ\SJ
Sample : K1649-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TRE-FLOOR-SLAB


Manual Integrations
APPROVED

Sohil
3/1/2019 12:19:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:12:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

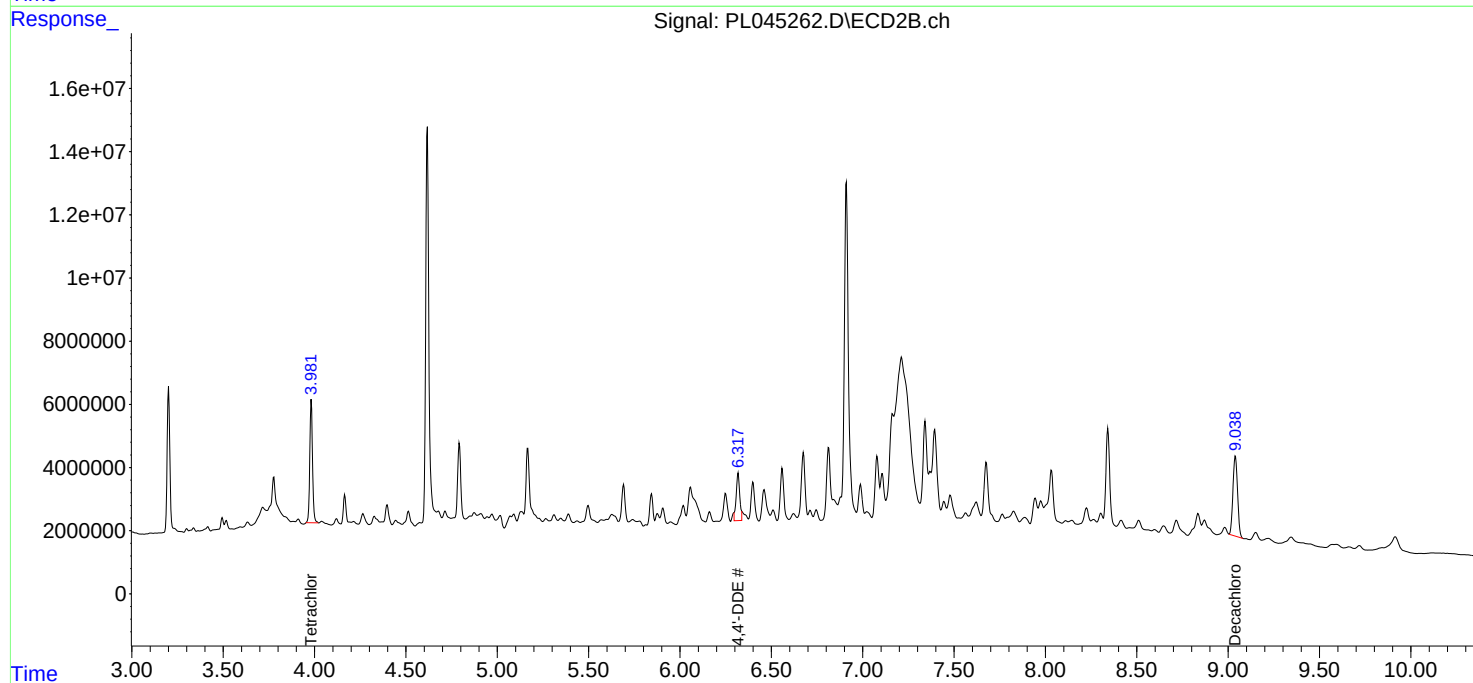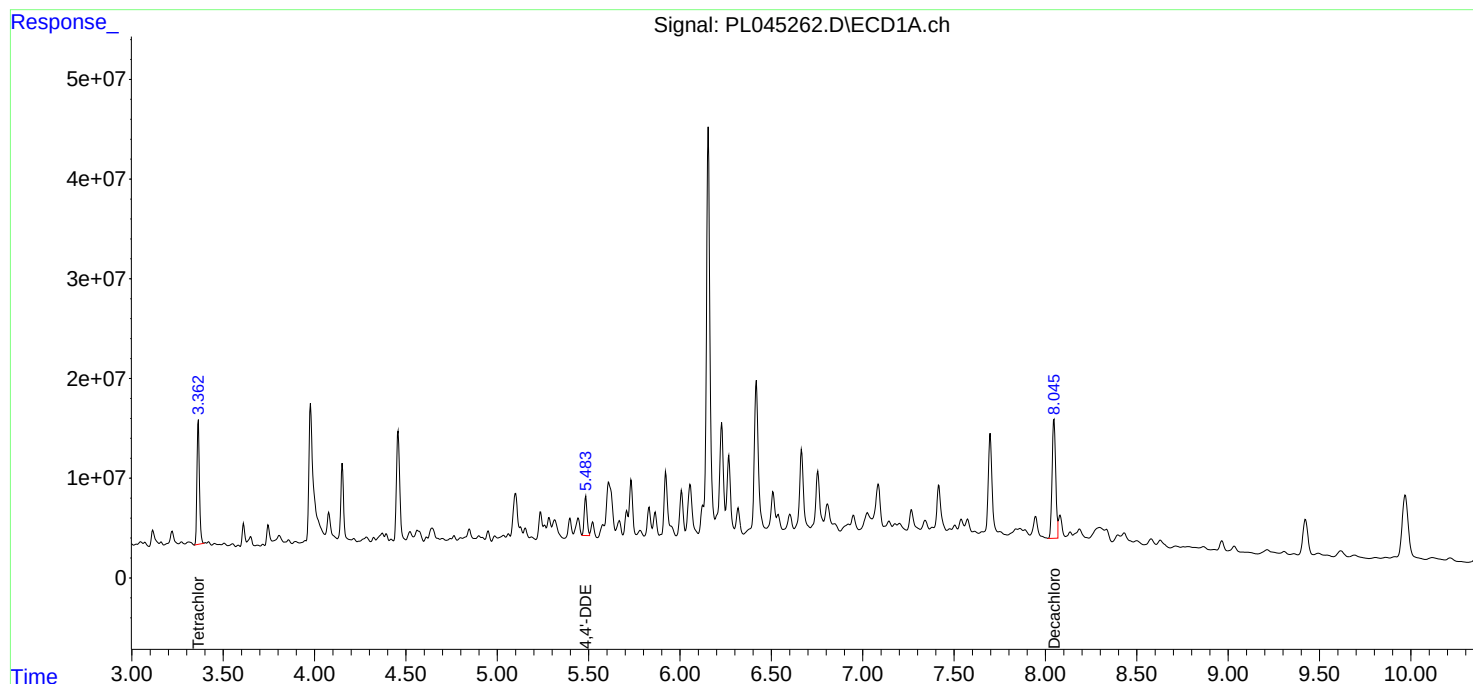

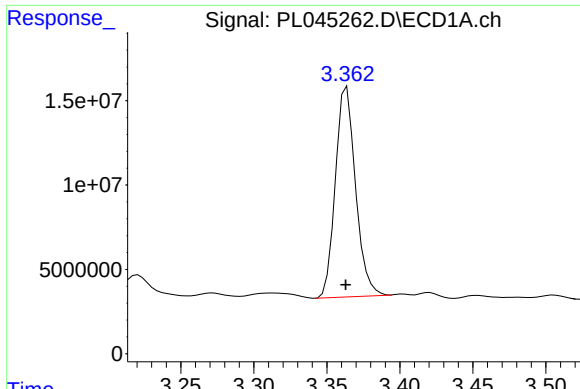


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 119740359
Conc: 17.41 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TRE-FLOOR-SLAB


Manual Integrations
APPROVED

Sohil
3/1/2019 12:19:43 PM

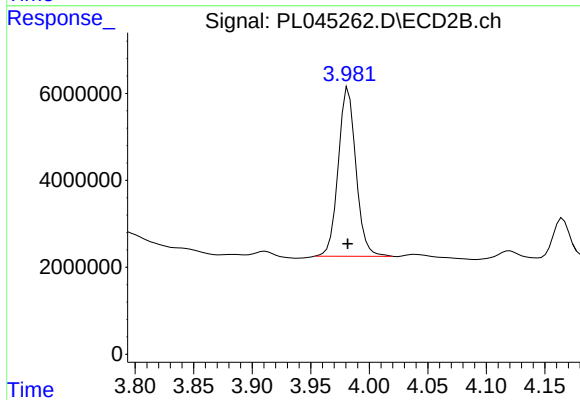


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 40769089
Conc: 19.04 ng/ml

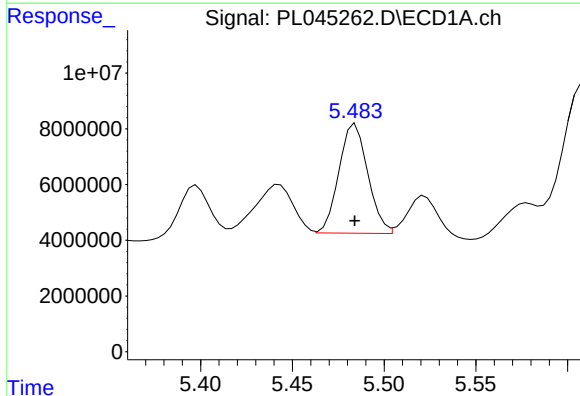


#12 4,4'-DDE

R.T.: 5.483 min
Delta R.T.: -0.001 min
Response: 43214454
Conc: 4.92 ng/ml m

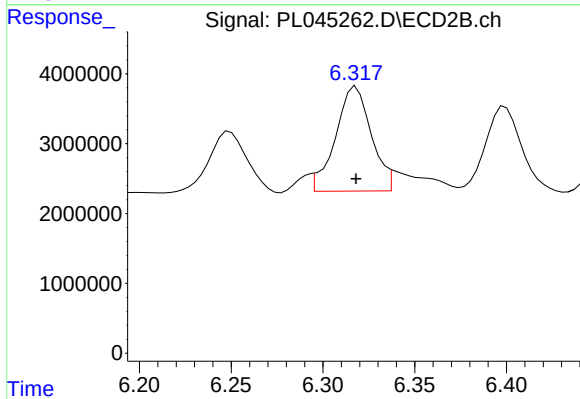

#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: -0.001 min
Response: 20763350
Conc: 8.89 ng/ml m

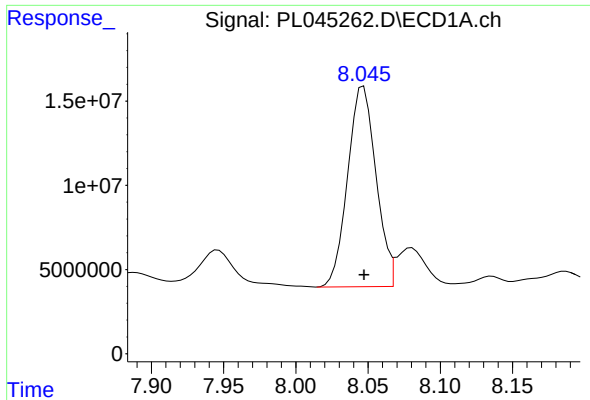


#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.002 min
Response: 165729998
Conc: 19.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TRE-FLOOR-SLAB

Manual Integrations
APPROVED

Sohil
3/1/2019 12:19:43 PM

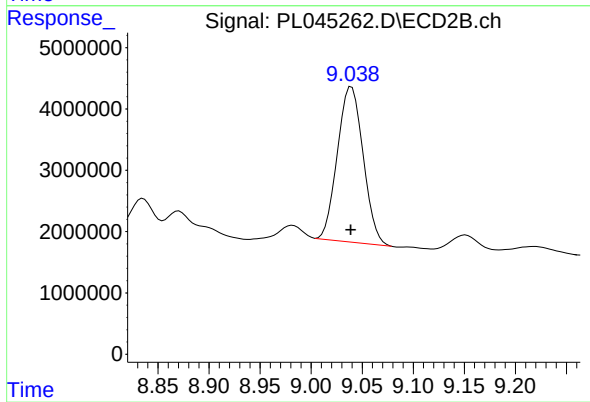

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 44543748
Conc: 19.49 ng/ml m