

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
 Data File : PL045275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 23:13
 Operator : AJ\SJ
 Sample : K1643-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INTERIOR-WALL

Manual Integrations
 APPROVED

Sohil
 3/1/2019 12:19:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:15:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.982	158.9E6	47602784	23.102m	22.228
28)	SA Decachlor...	8.046	9.038	187.5E6	55590123	22.411	24.329

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022819\
Data File : PL045275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 23:13
Operator : AJ\SJ
Sample : K1643-02
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
INTERIOR-WALL


Manual Integrations
APPROVED

Sohil
3/1/2019 12:19:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:15:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

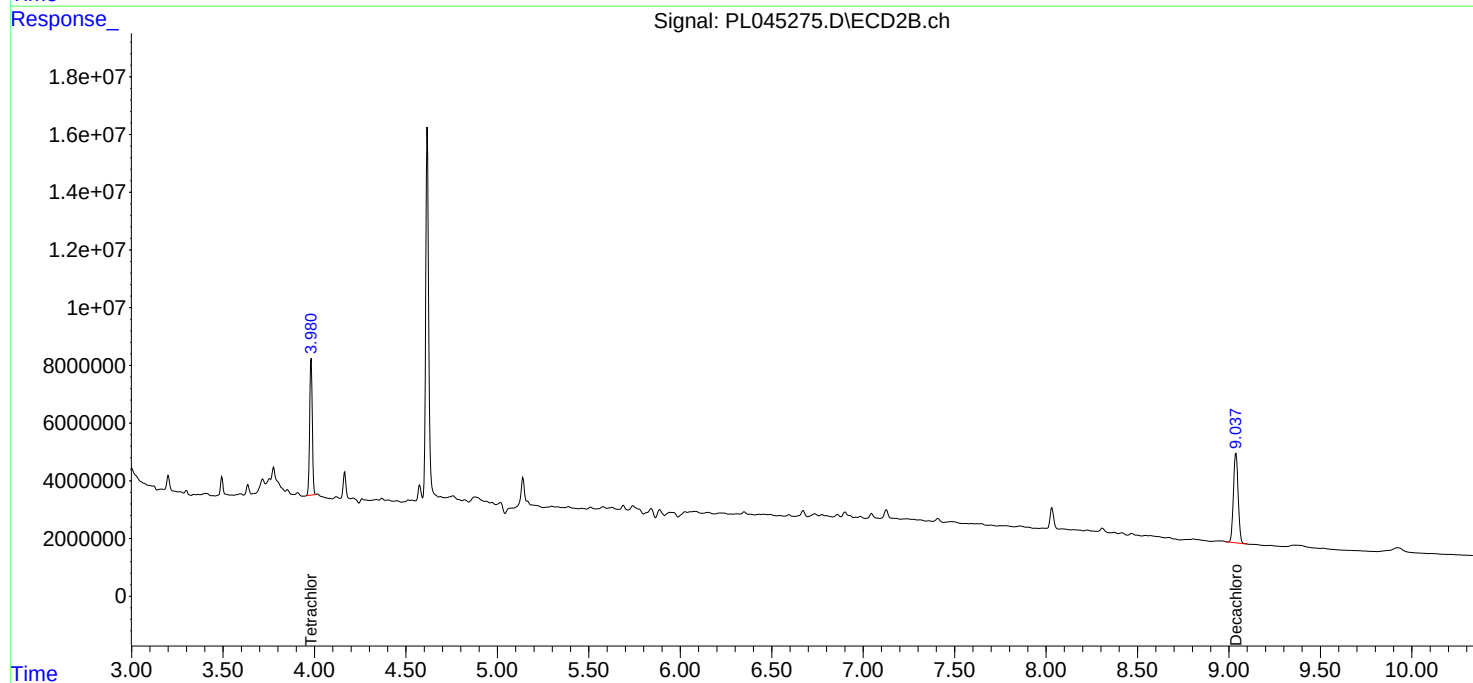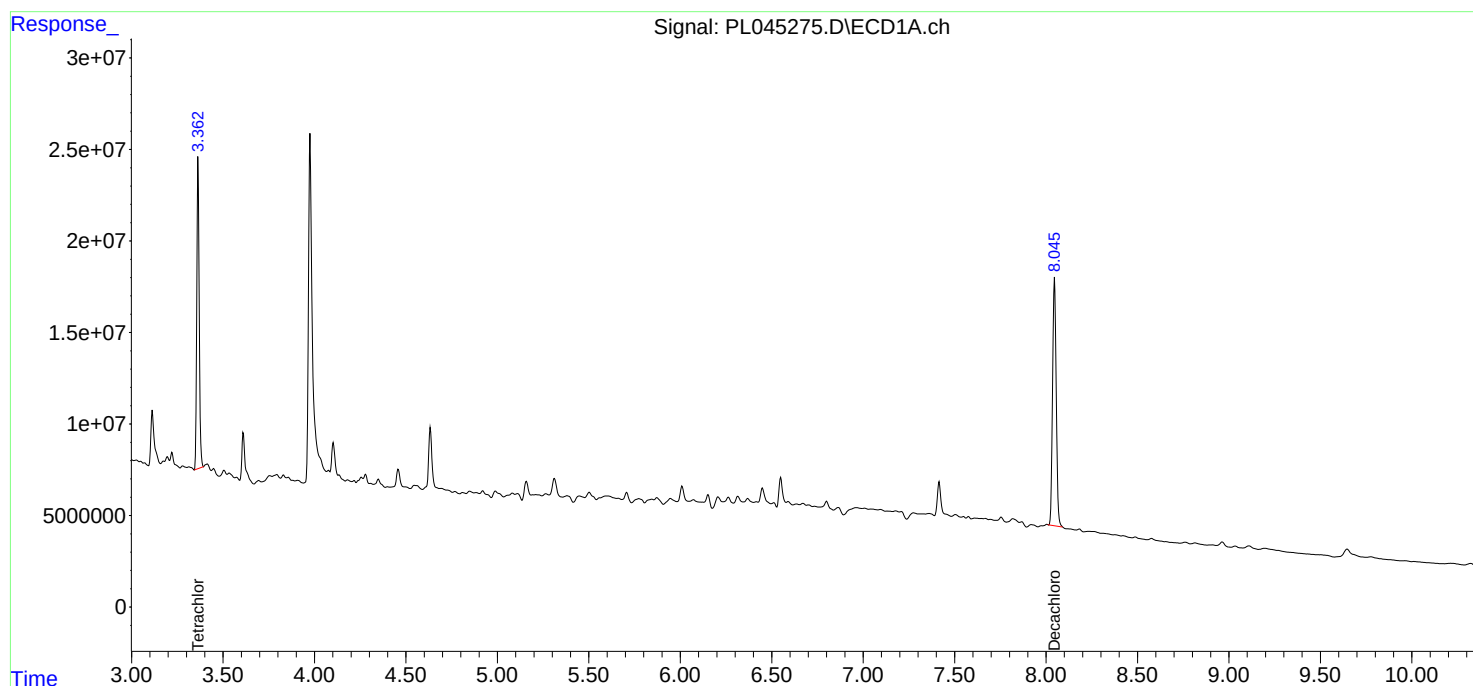

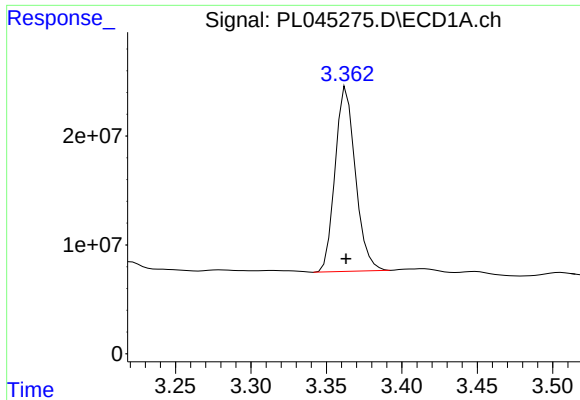

#1 Tetrachloro-m-xylene

R.T.: 3.362 min

Delta R.T.: 0.000 min


Response: 158924366

Conc: 23.10 ng/ml m

Instrument :
ECD_L
ClientSampleId :
INTERIOR-WALL

Manual Integrations
APPROVED

Sohil
3/1/2019 12:19:49 PM

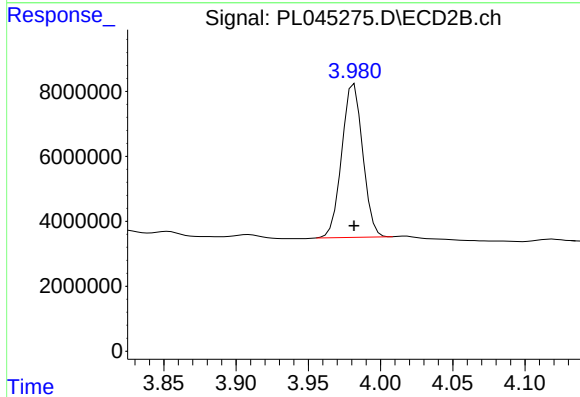


#1 Tetrachloro-m-xylene

R.T.: 3.982 min

Delta R.T.: 0.000 min

Response: 47602784

Conc: 22.23 ng/ml

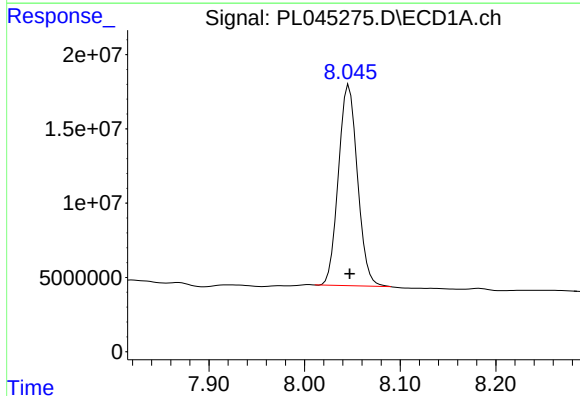


#28 Decachlorobiphenyl

R.T.: 8.046 min

Delta R.T.: 0.000 min

Response: 187520281

Conc: 22.41 ng/ml

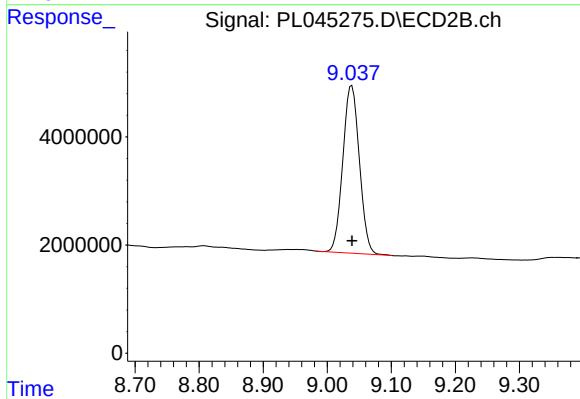

#28 Decachlorobiphenyl

R.T.: 9.038 min

Delta R.T.: 0.000 min

Response: 55590123

Conc: 24.33 ng/ml