

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022820\
 Data File : PL056896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 15:43
 Operator : AJ\MA
 Sample : L1718-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 03:38:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.002	163.4E6	56664594	9.135	10.574
28)	SA Decachlor...	8.254	9.068	210.8E6	57803684	10.611	13.658 #
Target Compounds							
4)	MA Heptachlor	0.000	5.203	0	342116	N.D.	0.053 #
6)	B beta-BHC	0.000	4.886f	0	3828314	N.D.	1.148 #
7)	B delta-BHC	4.675	0.000	1623976	0	0.058	N.D. #
10)	B gamma-Chl...	0.000	6.083f	0	719701	N.D.	0.120 #
11)	B alpha-Chl...	5.492	0.000	4955213	0	0.185	N.D. #
19)	B Endosulfa...	0.000	7.296	0	4163081	N.D.	0.862 #
23)	Chlordane-1	0.000	5.035f	0	2763377	N.D.	13.944 #
26)	Chlordane-4	5.492	0.000	4955213	0	2.496	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022820\
Data File : PL056896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 15:43
Operator : AJ\MA
Sample : L1718-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 03:38:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

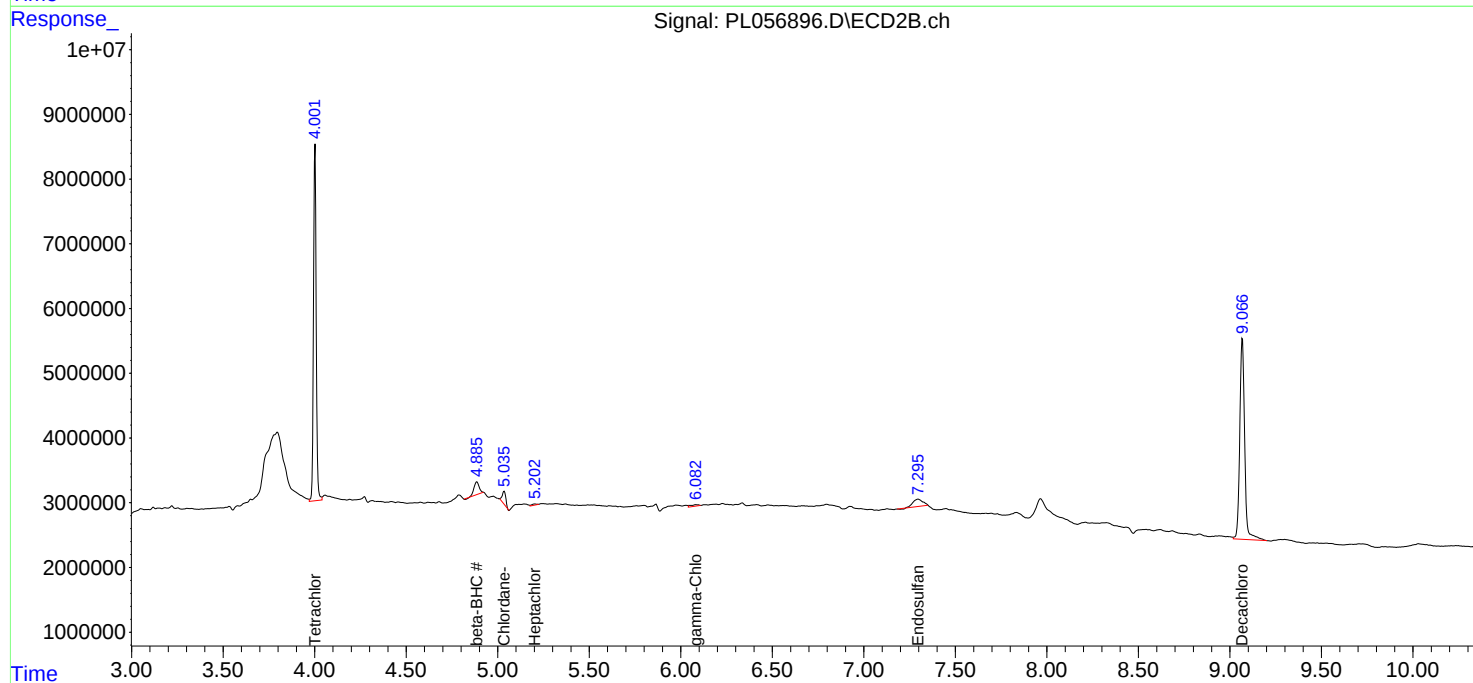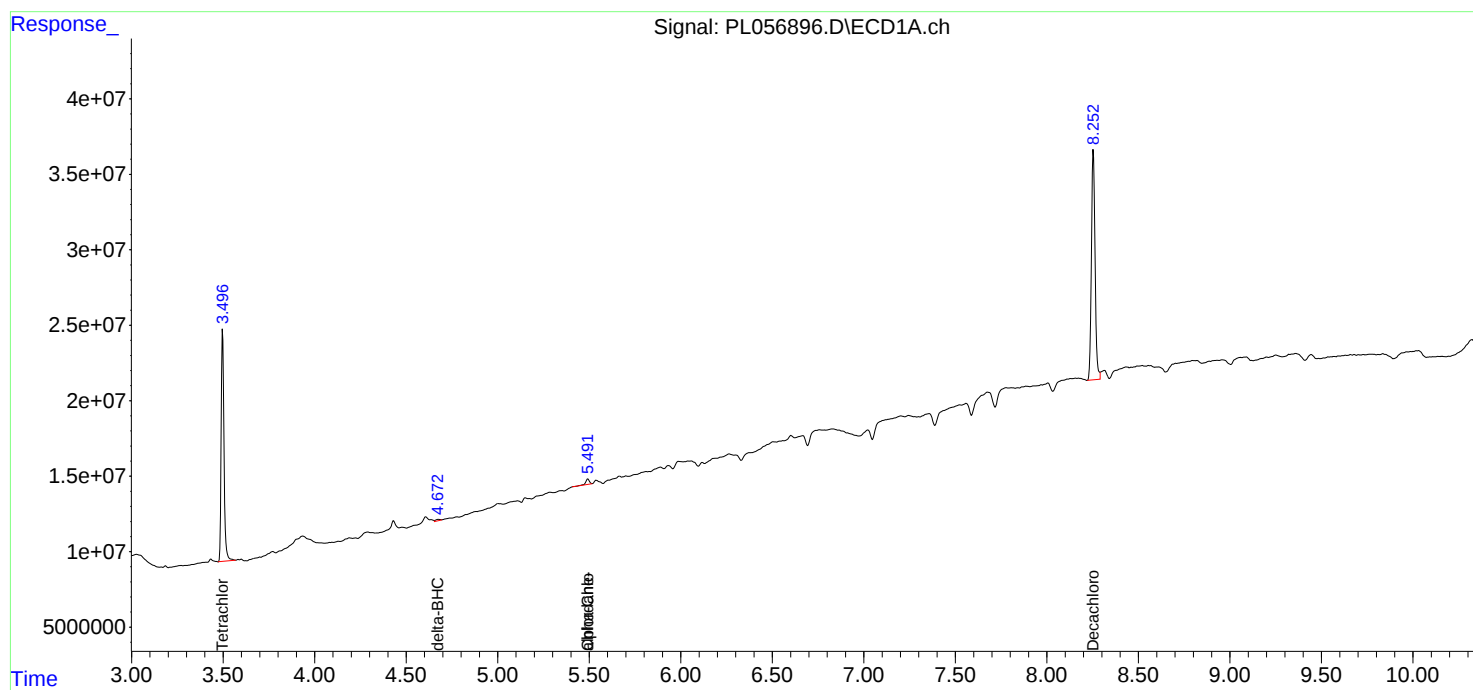


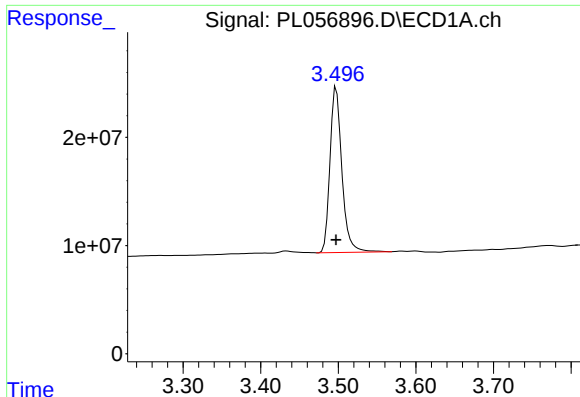

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 163365861
Conc: 9.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

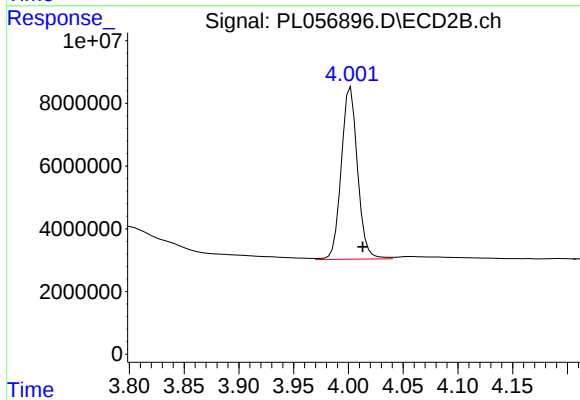


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.011 min
Response: 56664594
Conc: 10.57 ng/ml

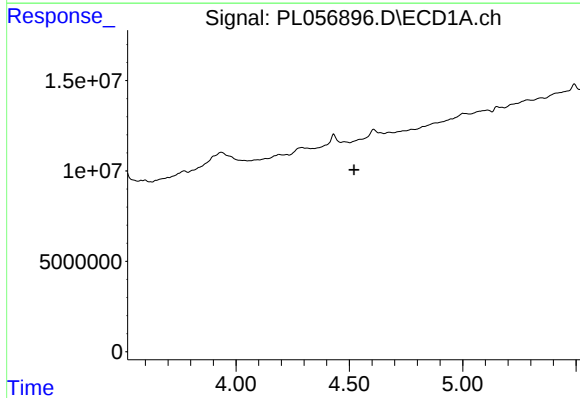


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.521 min
Response: 0
Conc: N.D.

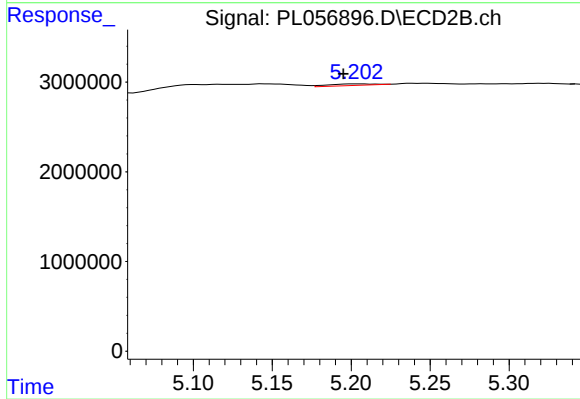

#4 Heptachlor


R.T.: 5.203 min
Delta R.T.: 0.008 min
Response: 342116
Conc: 0.05 ng/ml

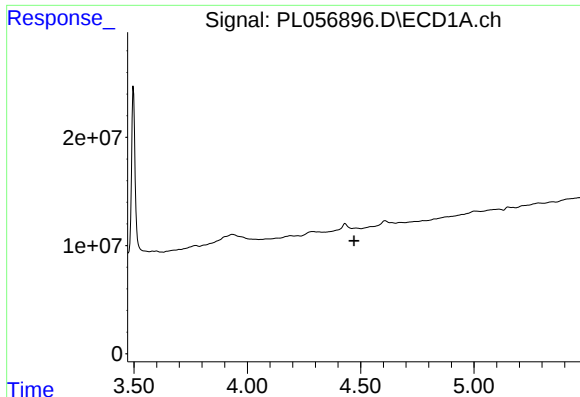

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

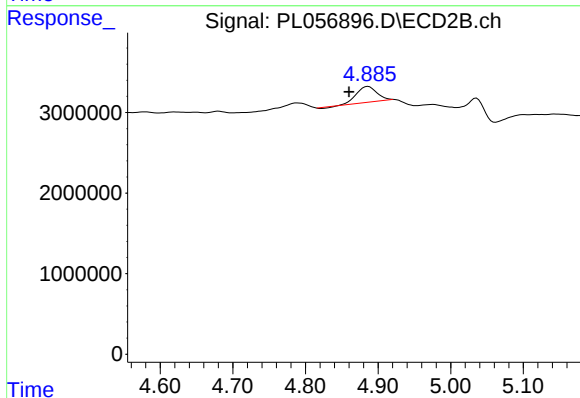


#6 beta-BHC

R.T.: 4.886 min
Delta R.T.: 0.026 min
Response: 3828314
Conc: 1.15 ng/ml

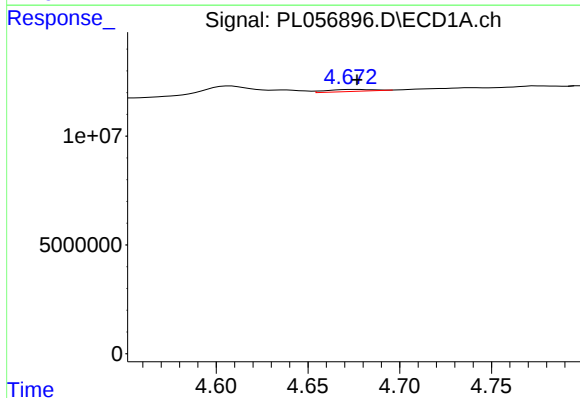


#7 delta-BHC

R.T.: 4.675 min
Delta R.T.: -0.002 min
Response: 1623976
Conc: 0.06 ng/ml

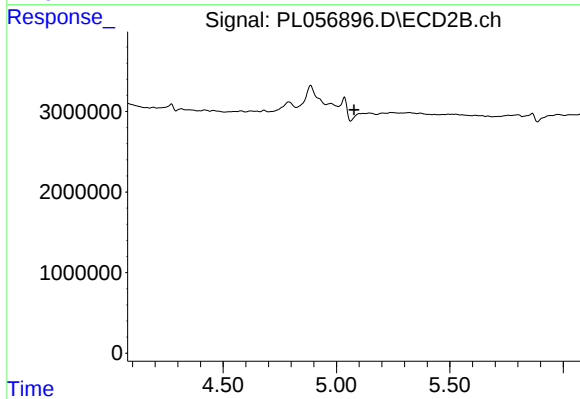

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.078 min
Response: 0
Conc: N.D.

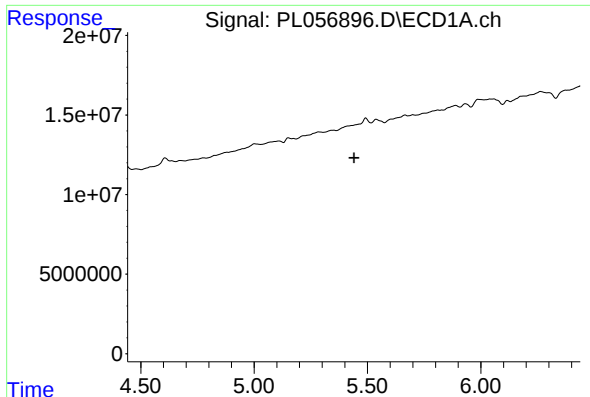

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

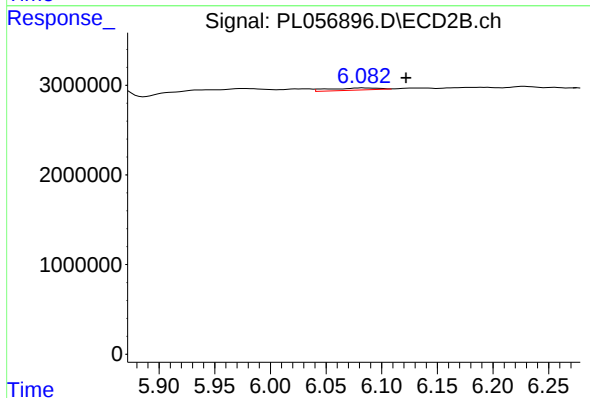


#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: -0.039 min
Response: 719701
Conc: 0.12 ng/ml

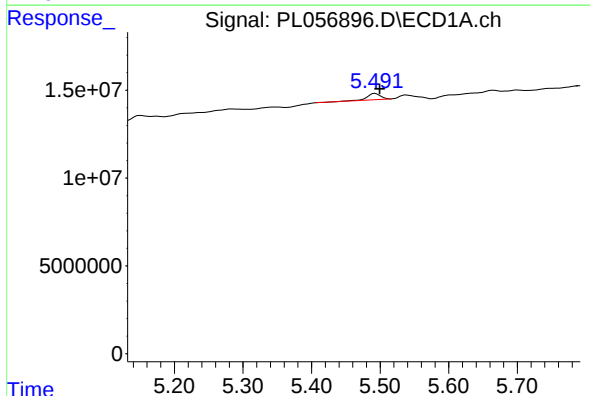


#11 alpha-Chlordane

R.T.: 5.492 min
Delta R.T.: -0.007 min
Response: 4955213
Conc: 0.18 ng/ml

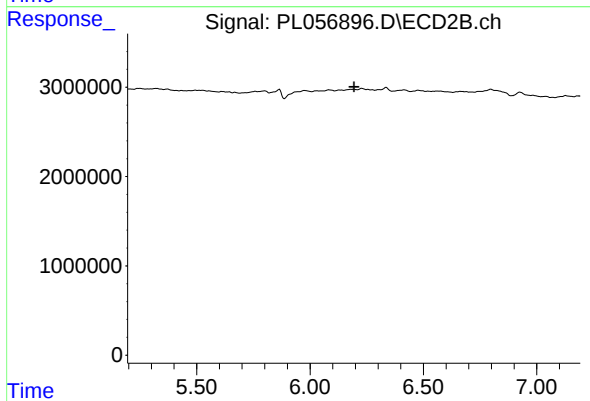

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.194 min
Response: 0
Conc: N.D.

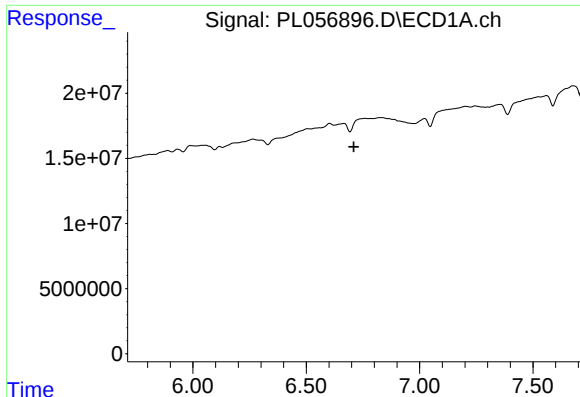

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

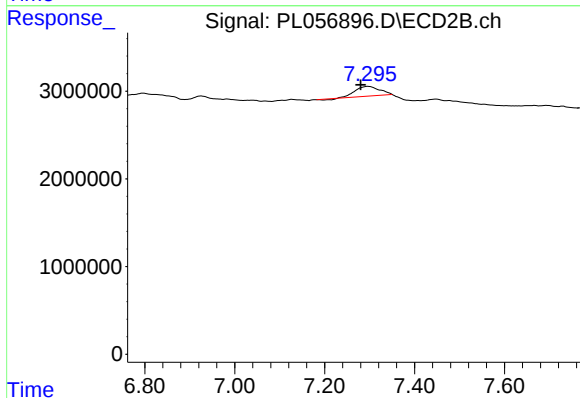


#19 Endosulfan Sulfate

R.T.: 7.296 min
Delta R.T.: 0.016 min
Response: 4163081
Conc: 0.86 ng/ml

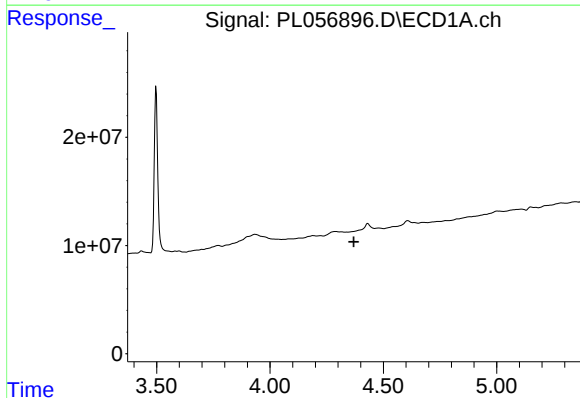


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.369 min
Response: 0
Conc: N.D.

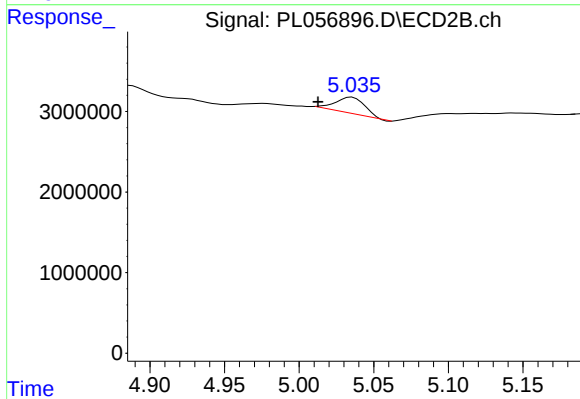

#23 Chlordane-1


R.T.: 5.035 min
Delta R.T.: 0.023 min
Response: 2763377
Conc: 13.94 ng/ml

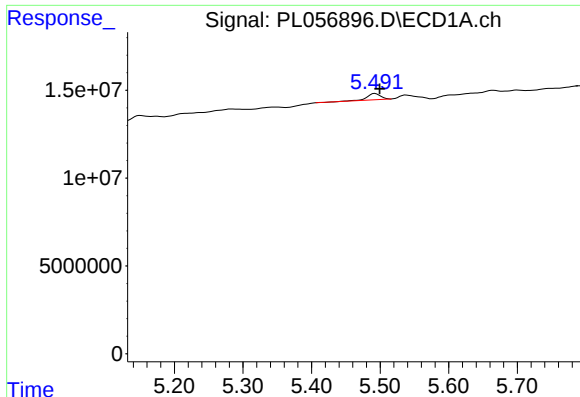

#26 Chlordane-4


R.T.: 5.492 min
Delta R.T.: -0.007 min
Response: 4955213
Conc: 2.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

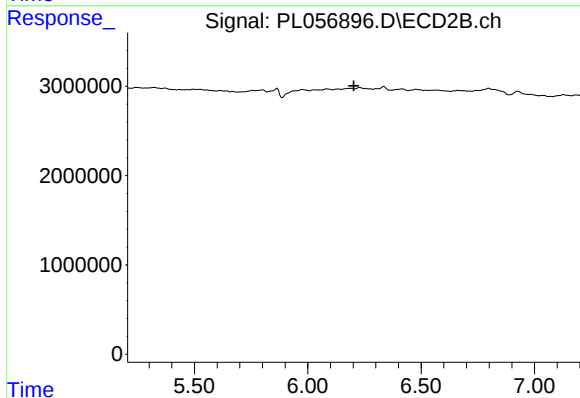


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

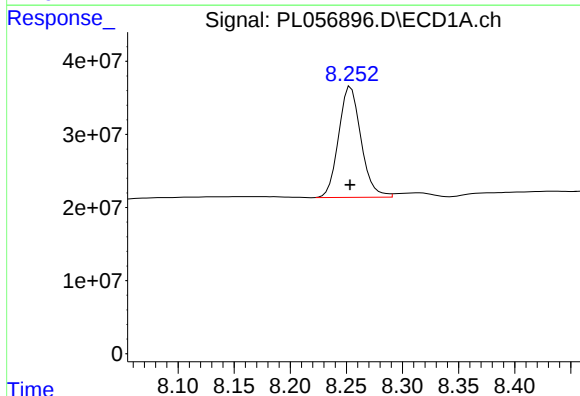

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 210767169
Conc: 10.61 ng/ml

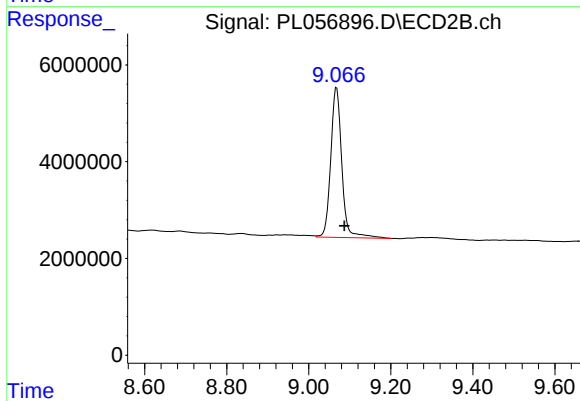

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.019 min
Response: 57803684
Conc: 13.66 ng/ml