

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
 Data File : PL073058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 21:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:33:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.648	5.490	6667003	30998921	20.805	21.361
2)	SA Decachlor...	10.426	11.327	10227236	34401778	21.850	21.807
Target Compounds							
2)	A alpha-BHC	5.382f	0.000	26946	0	0.064	N.D. #
5)	MB Aldrin	6.501f	0.000	7267	0	0.016	N.D. #
6)	B beta-BHC	0.000	6.678	0	560032	N.D.	0.621 #
7)	B delta-BHC	6.413	6.956	1773	2099239	0.004	1.109 #
8)	B Heptachlo...	0.000	7.925	0	280454	N.D.	0.159 #
9)	A Endosulfan I	7.525f	0.000	14211	0	0.032	N.D. #
10)	B gamma-Chl...	7.387	0.000	18077	0	0.038	N.D. #
11)	B alpha-Chl...	7.442	0.000	13143	0	0.027	N.D. #
13)	MA Dieldrin	7.786	0.000	76335	0	0.170	N.D. #
14)	MA Endrin	8.098f	0.000	115806	0	0.292	N.D. #
15)	B Endosulfa...	8.387	9.051f	129240	705968	0.298	0.510 #
20)	A Methoxychlor	9.101	0.000	18896	0	0.076	N.D. #
24)	Chlordane-2	6.653f	0.000	47129	0	2.377	N.D. #
25)	Chlordane-3	7.387	0.000	18077	0	0.366	N.D. #
26)	Chlordane-4	7.442	0.000	13143	0	0.248	N.D. #
27)	Chlordane-5	8.387	9.141	129240	18157	6.422	0.338 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
Data File : PL073058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 21:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:33:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

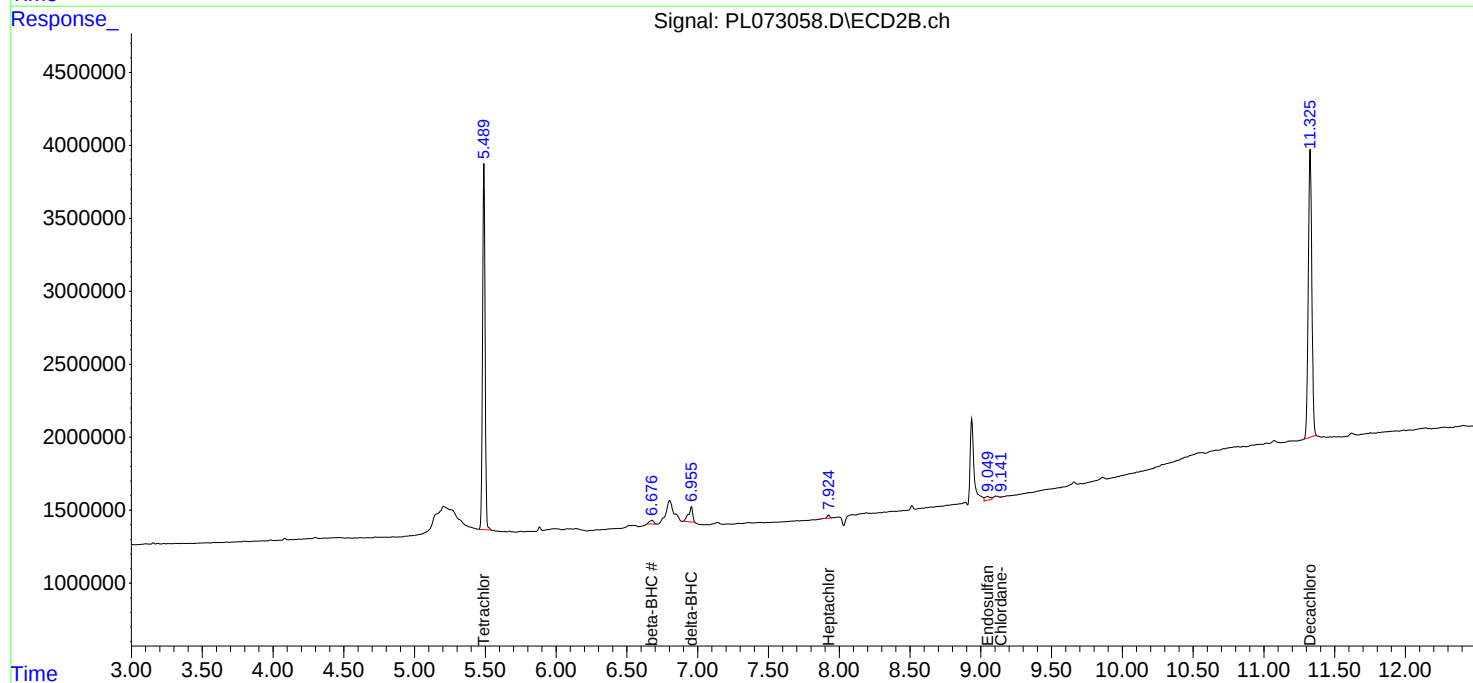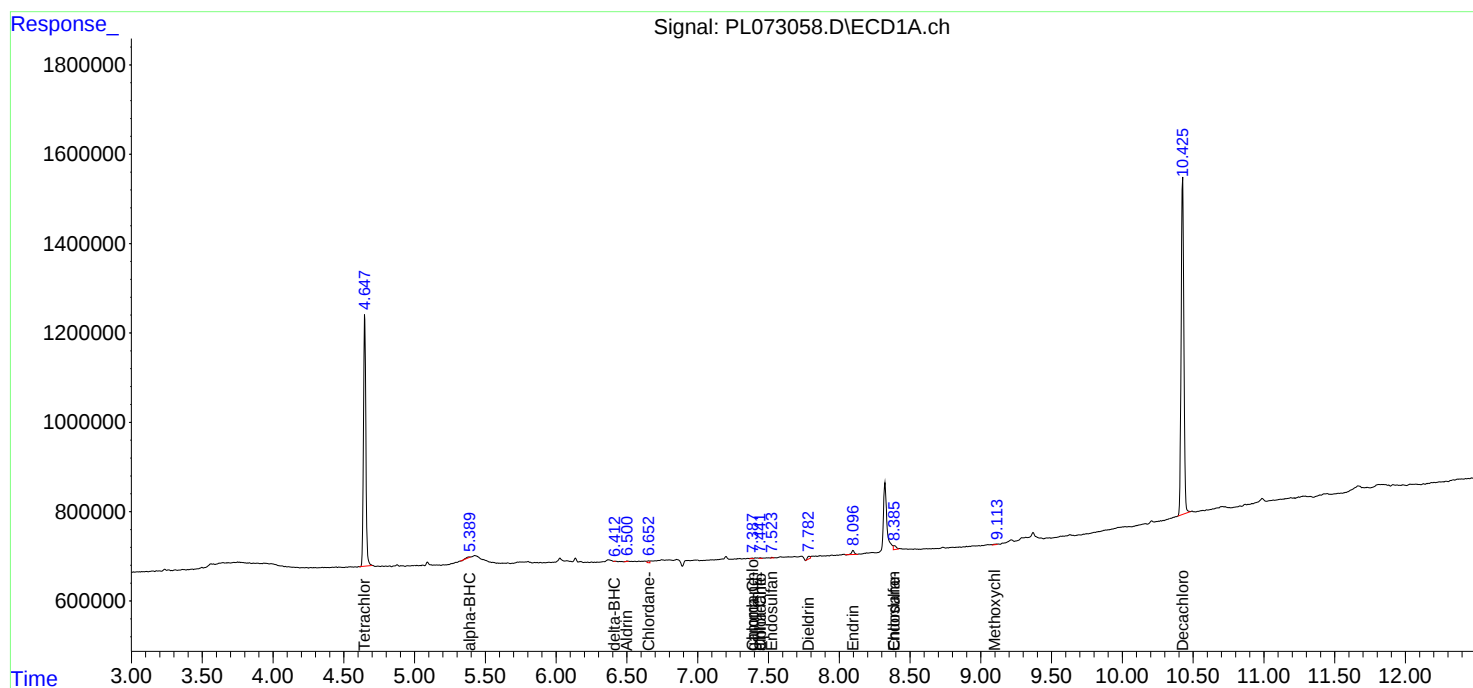


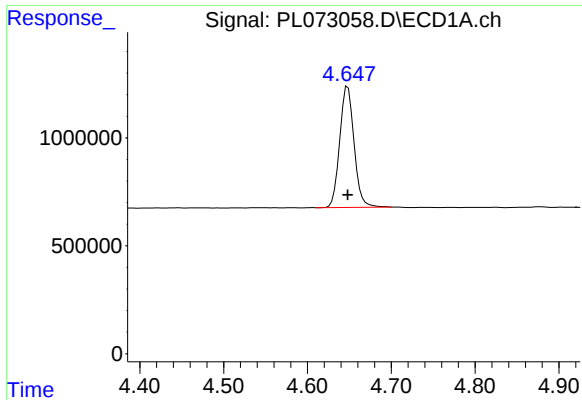

#1 Tetrachloro-m-xylene


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 6667003
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

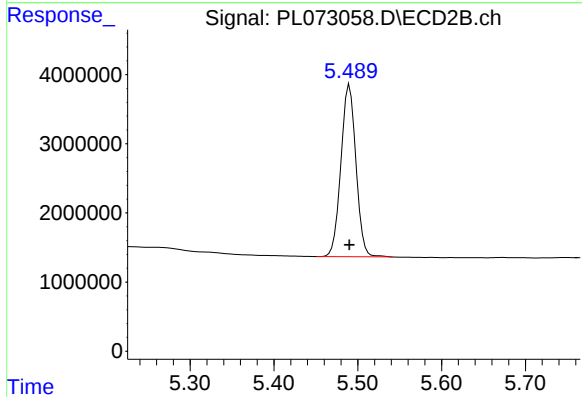


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 30998921
Conc: 21.36 ng/ml

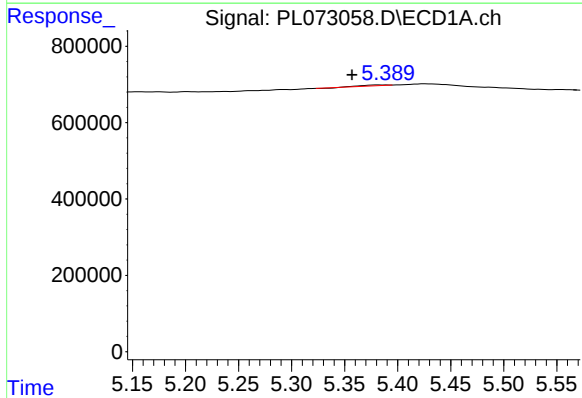


#2 alpha-BHC

R.T.: 5.382 min
Delta R.T.: 0.025 min
Response: 26946
Conc: 0.06 ng/ml

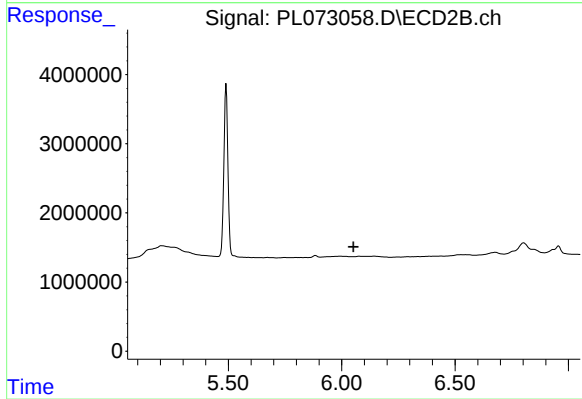

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

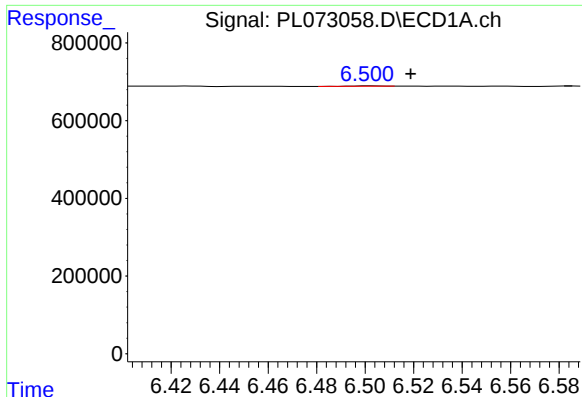

#5 Aldrin


R.T.: 6.501 min
Delta R.T.: -0.018 min
Response: 7267
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

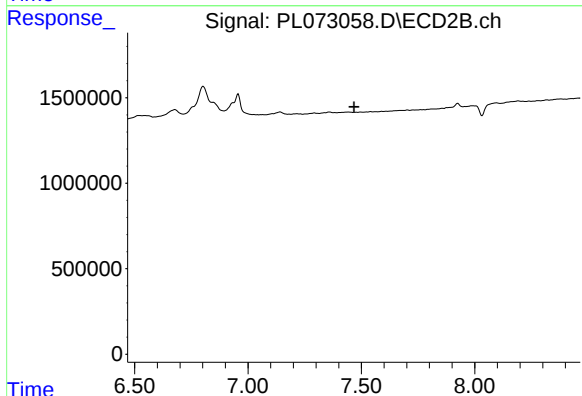


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.468 min
Response: 0
Conc: N.D.

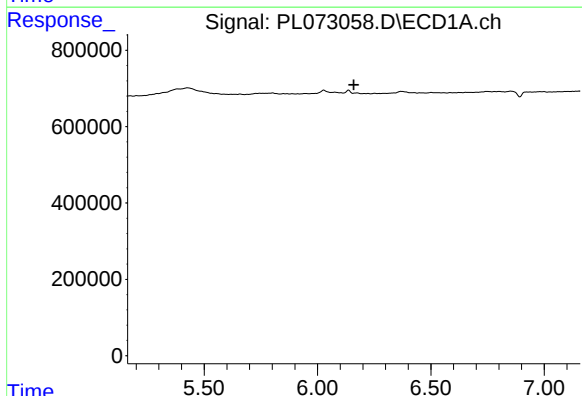


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

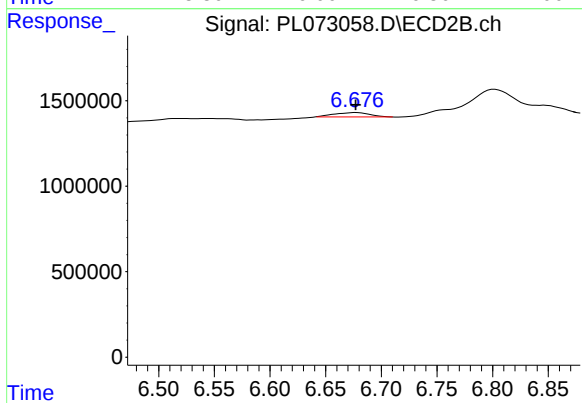

#6 beta-BHC


R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 560032
Conc: 0.62 ng/ml

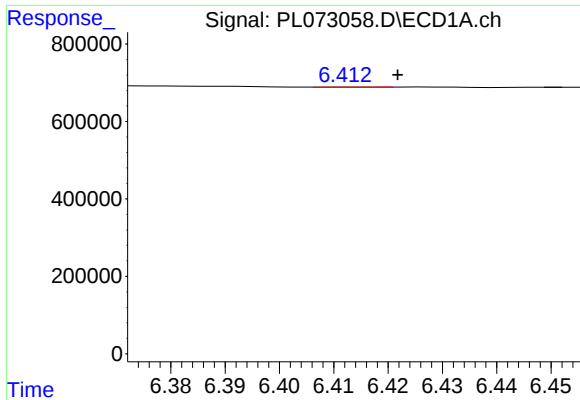

#7 delta-BHC


R.T.: 6.413 min
Delta R.T.: -0.009 min
Response: 1773
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

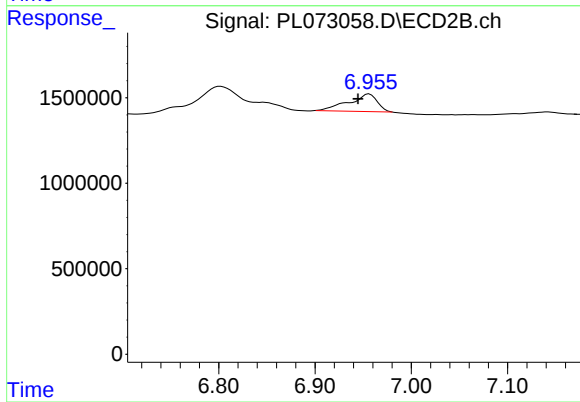


#7 delta-BHC

R.T.: 6.956 min
Delta R.T.: 0.011 min
Response: 2099239
Conc: 1.11 ng/ml

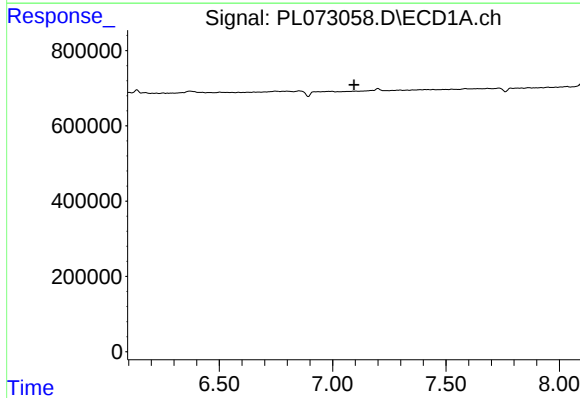


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.095 min
Response: 0
Conc: N.D.

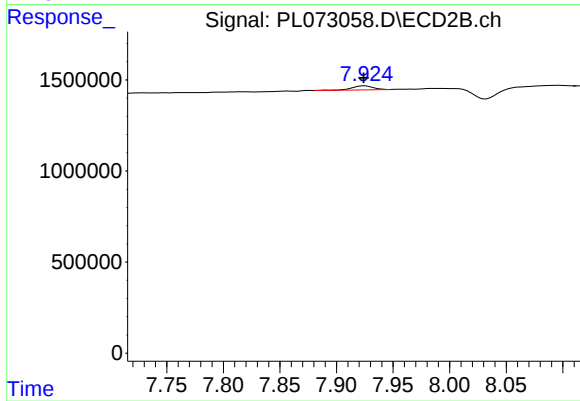

#8 Heptachlor epoxide


R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 280454
Conc: 0.16 ng/ml

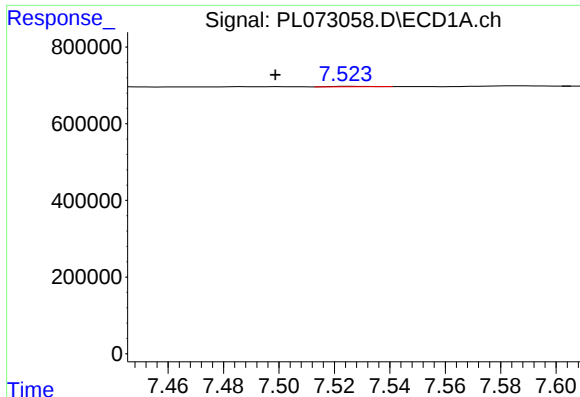

#9 Endosulfan I


R.T.: 7.525 min
Delta R.T.: 0.026 min
Response: 14211
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

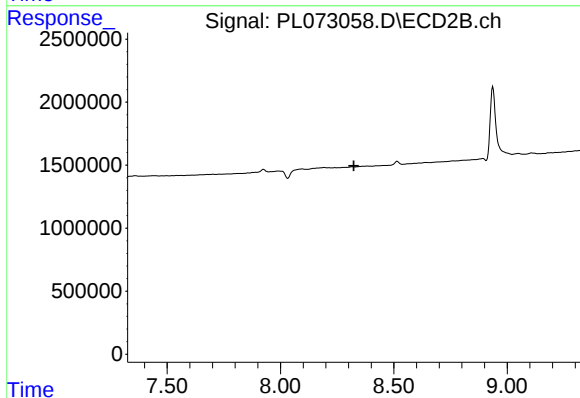


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.324 min
Response: 0
Conc: N.D.

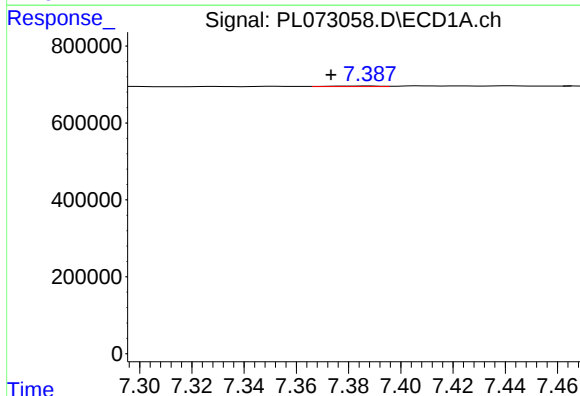


#10 gamma-Chlordane

R.T.: 7.387 min
Delta R.T.: 0.014 min
Response: 18077
Conc: 0.04 ng/ml

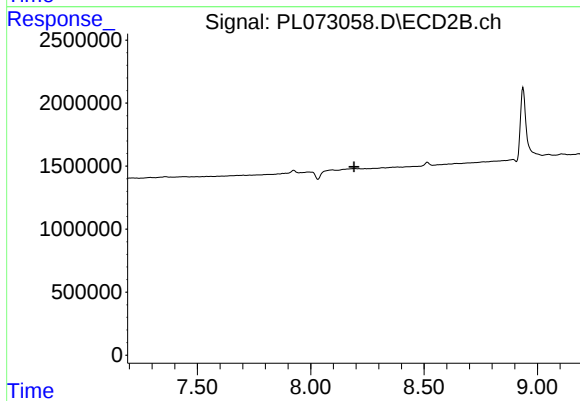

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

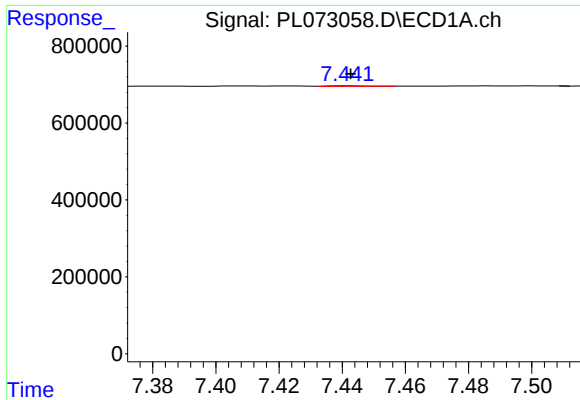

#11 alpha-Chlordane


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 13143
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

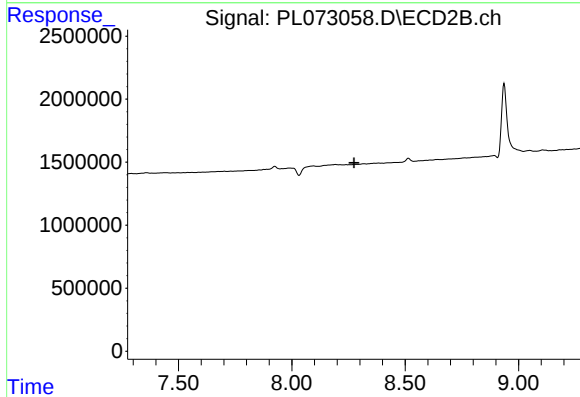


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.274 min
Response: 0
Conc: N.D.

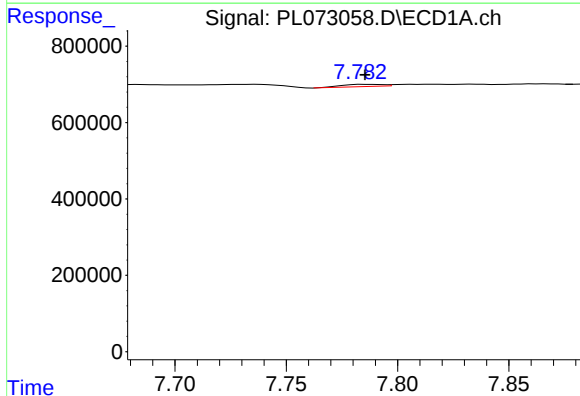


#13 Dieldrin

R.T.: 7.786 min
Delta R.T.: 0.000 min
Response: 76335
Conc: 0.17 ng/ml

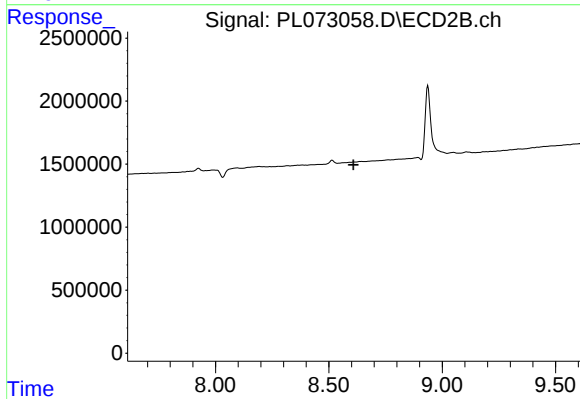

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.609 min
Response: 0
Conc: N.D.

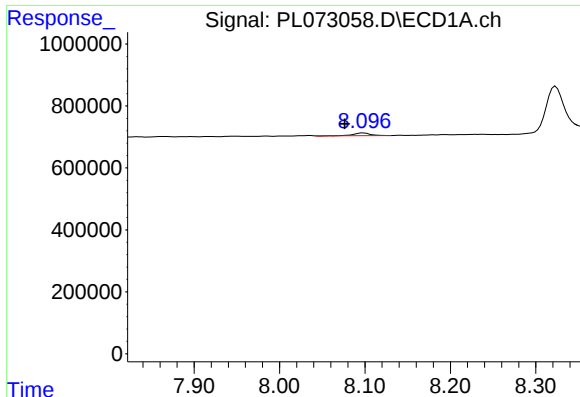

#14 Endrin


R.T.: 8.098 min
Delta R.T.: 0.022 min
Response: 115806
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

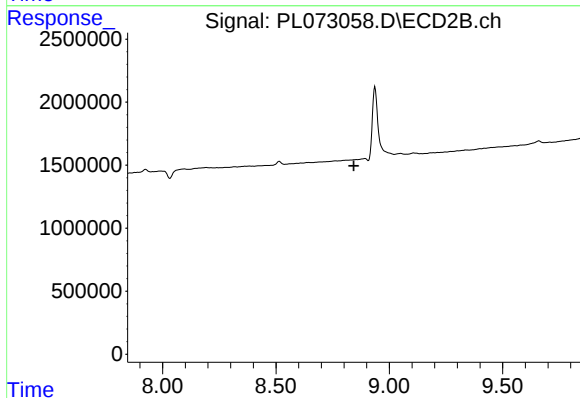


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

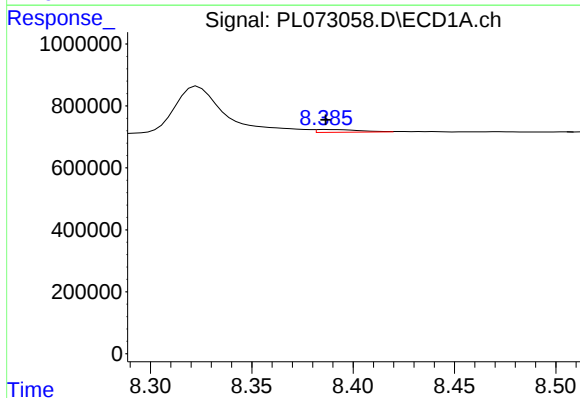


#15 Endosulfan II

R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 129240
Conc: 0.30 ng/ml

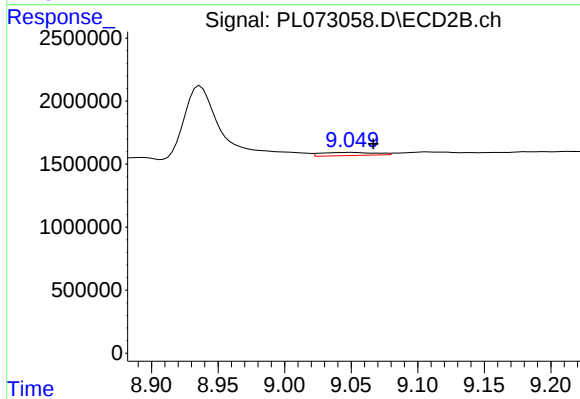

#15 Endosulfan II


R.T.: 9.051 min
Delta R.T.: -0.016 min
Response: 705968
Conc: 0.51 ng/ml

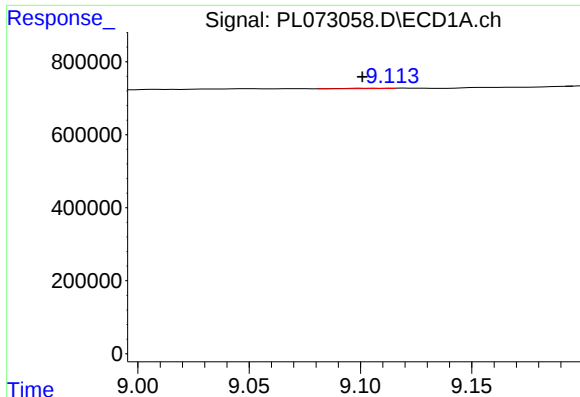

#20 Methoxychlor


R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 18896
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

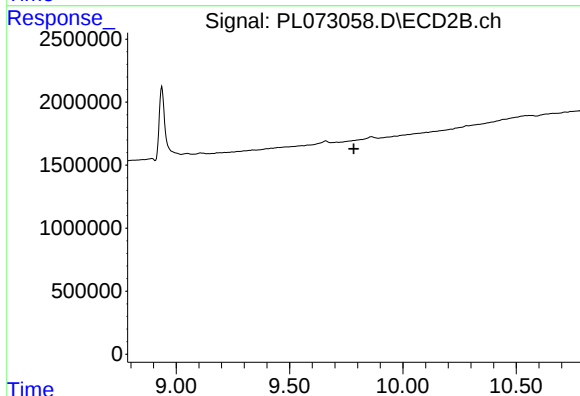


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.783 min
Response: 0
Conc: N.D.

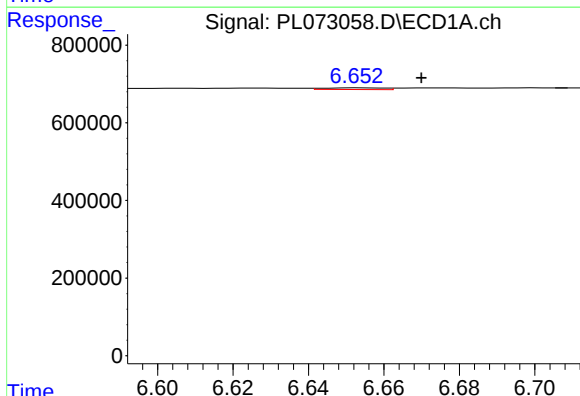


#24 Chlordane-2

R.T.: 6.653 min
Delta R.T.: -0.017 min
Response: 47129
Conc: 2.38 ng/ml

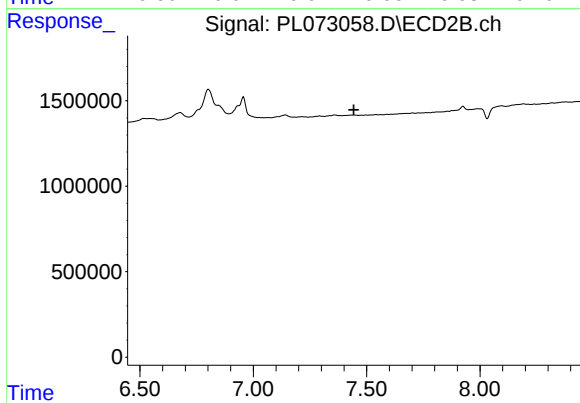

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.443 min
Response: 0
Conc: N.D.

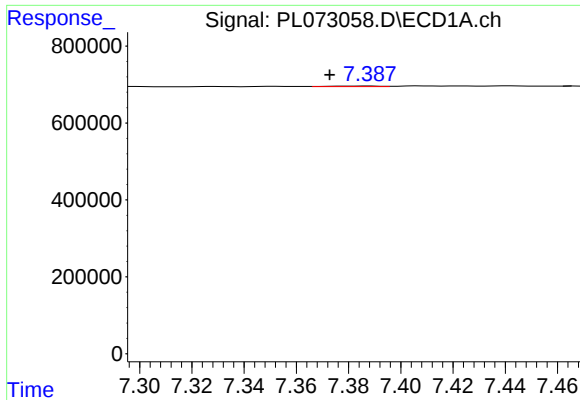

#25 Chlordane-3


R.T.: 7.387 min
Delta R.T.: 0.014 min
Response: 18077
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

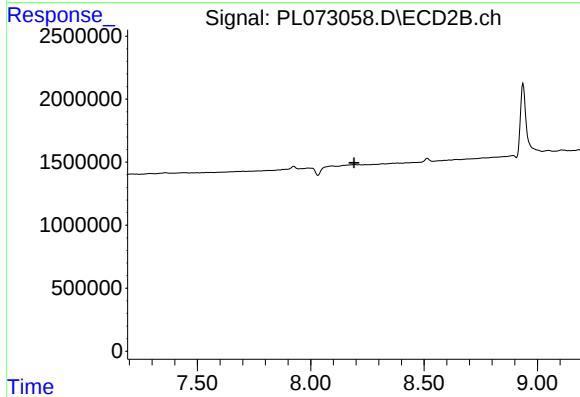


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

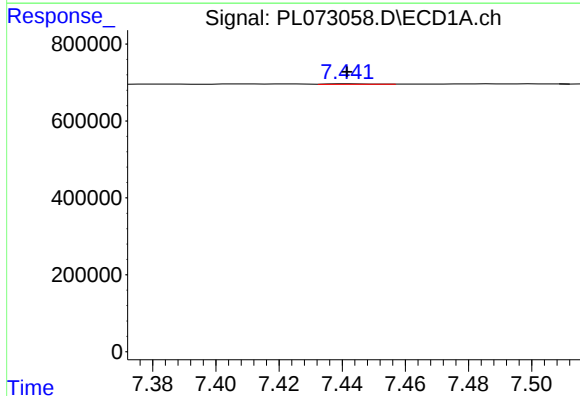


#26 Chlordane-4

R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 13143
Conc: 0.25 ng/ml

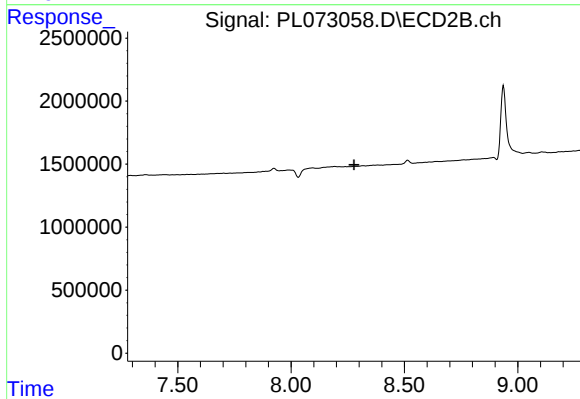

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.278 min
Response: 0
Conc: N.D.

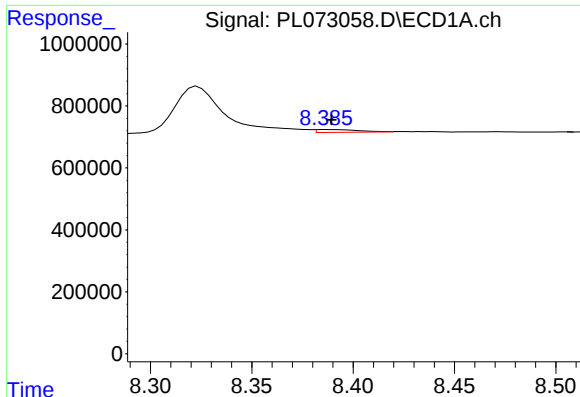

#27 Chlordane-5


R.T.: 8.387 min
Delta R.T.: -0.002 min
Response: 129240
Conc: 6.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

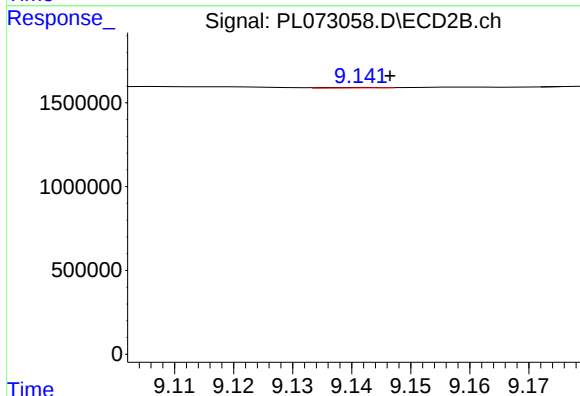


#27 Chlordane-5

R.T.: 9.141 min
Delta R.T.: -0.006 min
Response: 18157
Conc: 0.34 ng/ml

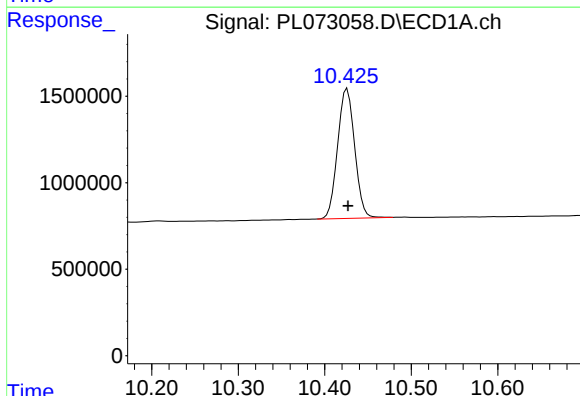

#28 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.001 min
Response: 10227236
Conc: 21.85 ng/ml

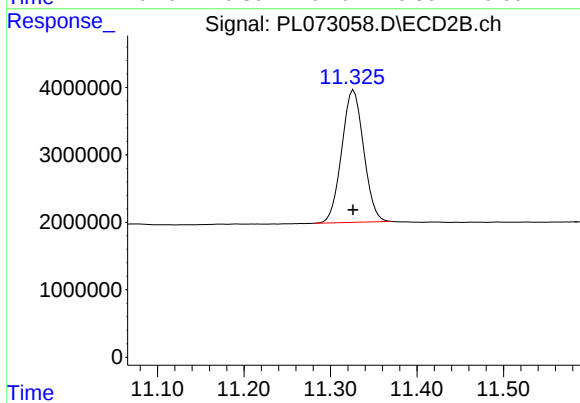

#28 Decachlorobiphenyl

R.T.: 11.327 min
Delta R.T.: 0.000 min
Response: 34401778
Conc: 21.81 ng/ml