

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
 Data File : PL073023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 11:59
 Operator : AR\AJ
 Sample : N1670-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-022422

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:20:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.648	5.488	733940	3065810	2.290	2.113m
28) SA Decachlor...	10.428	11.326	2625707	8428089	5.610	5.343
Target Compounds						
4) MA Heptachlor	6.194	7.098	1136489	4920093	2.476	2.461m
10) B gamma-Chl...	7.374	8.191	2136483	11794596	4.499	6.605m#
11) B alpha-Chl...	7.443	8.278	3438798	21482982	7.185	12.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
Data File : PL073023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 11:59
Operator : AR\AJ
Sample : N1670-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-03-022422

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:20:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

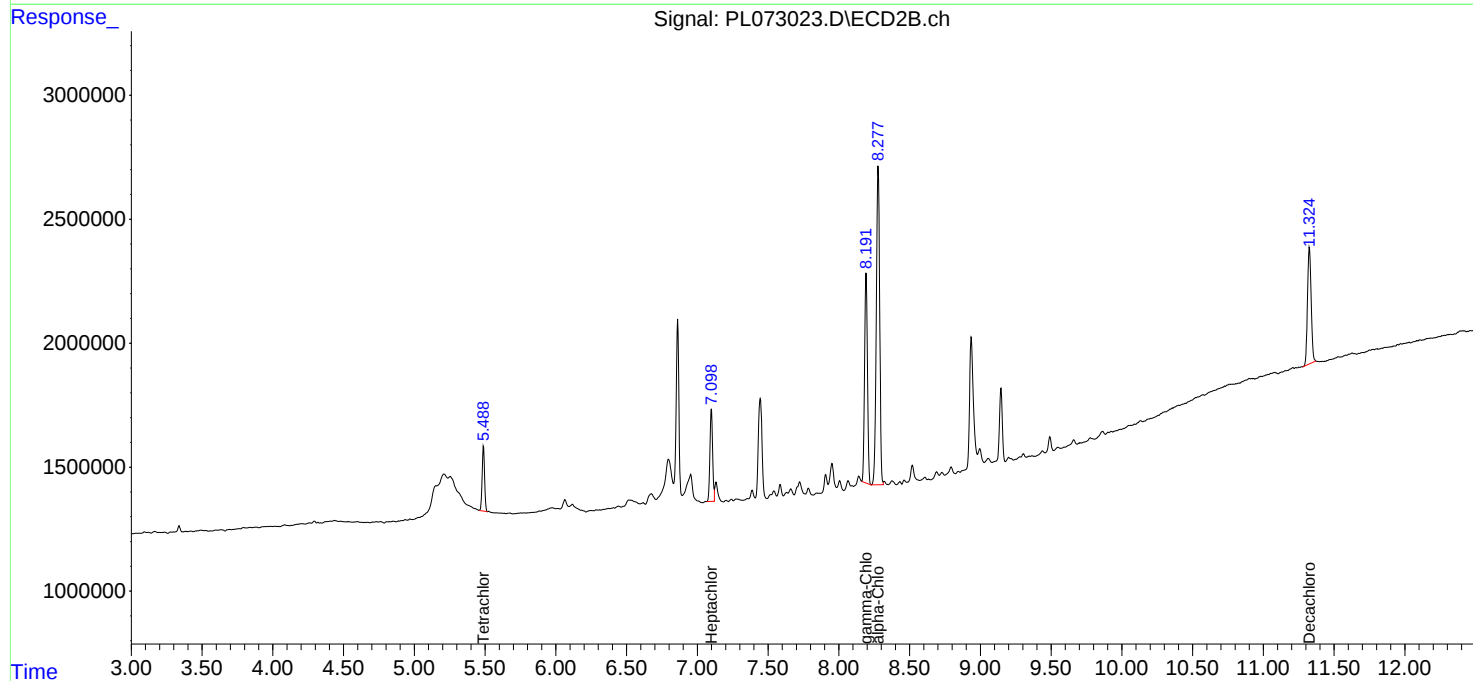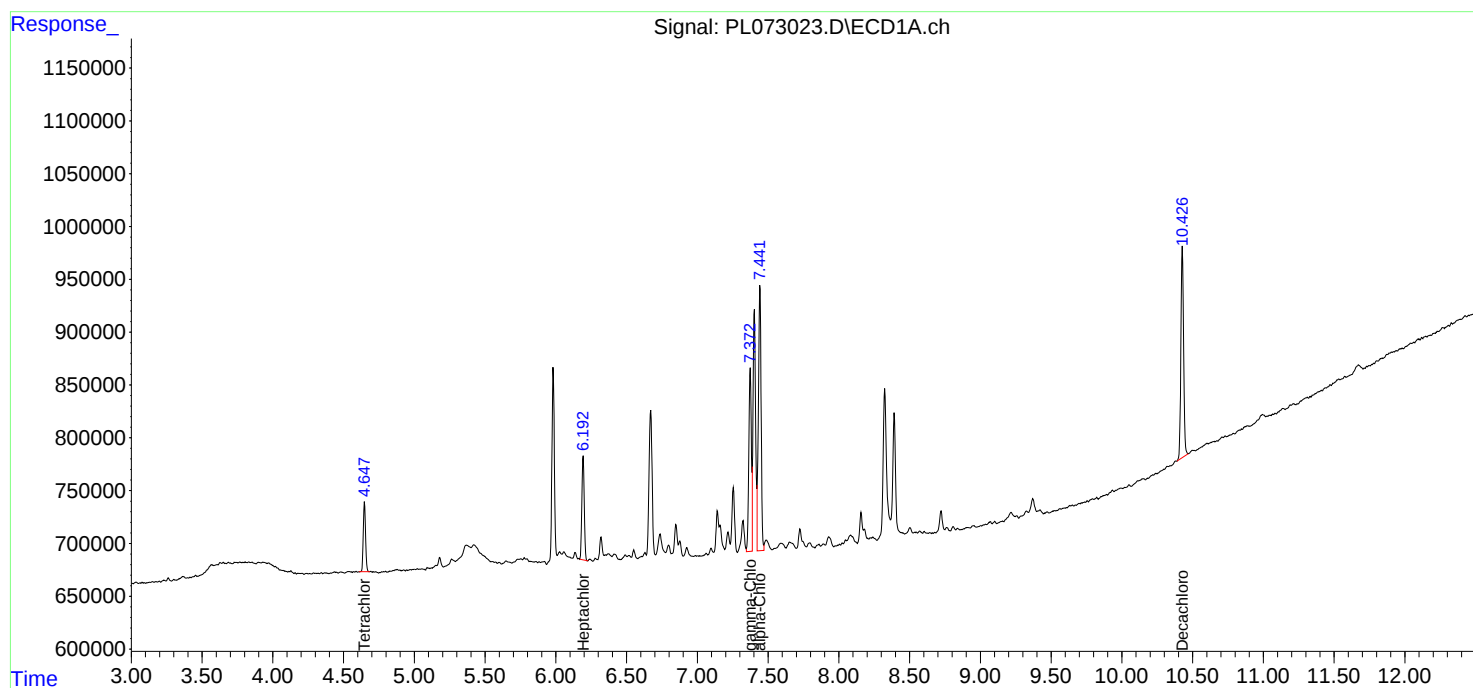


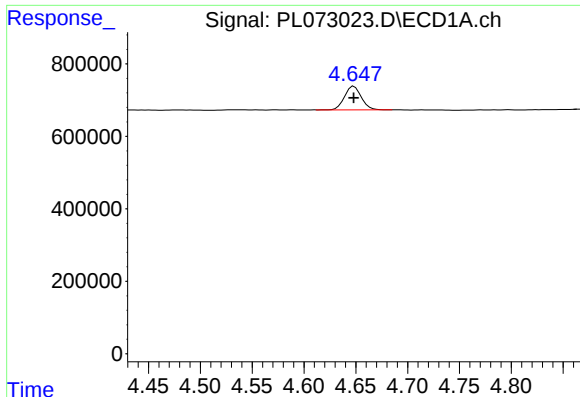

#1 Tetrachloro-m-xylene


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 733940
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-022422

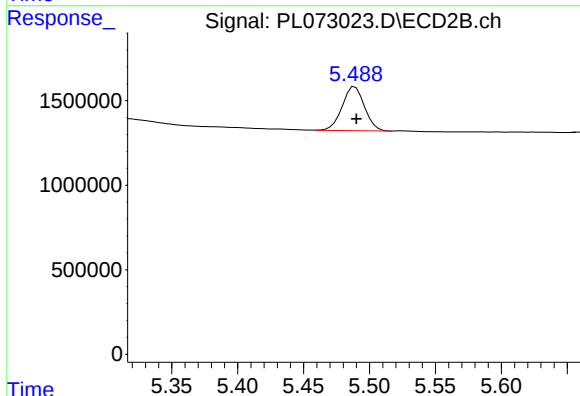


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.002 min
Response: 3065810
Conc: 2.11 ng/ml m

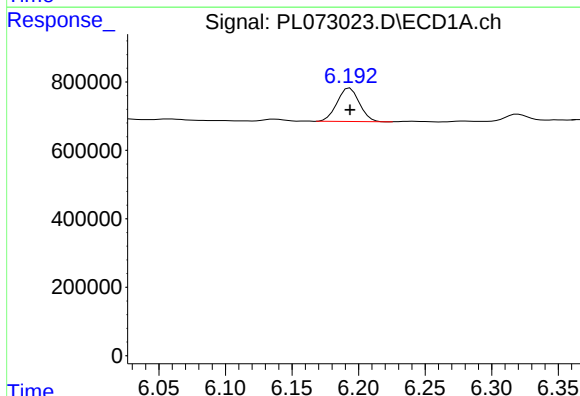


#4 Heptachlor

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1136489
Conc: 2.48 ng/ml

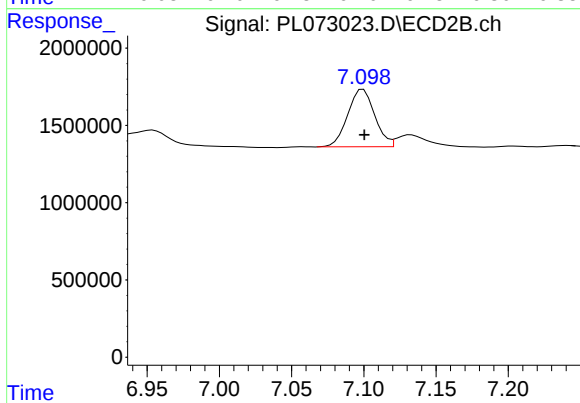

#4 Heptachlor


R.T.: 7.098 min
Delta R.T.: -0.002 min
Response: 4920093
Conc: 2.46 ng/ml m

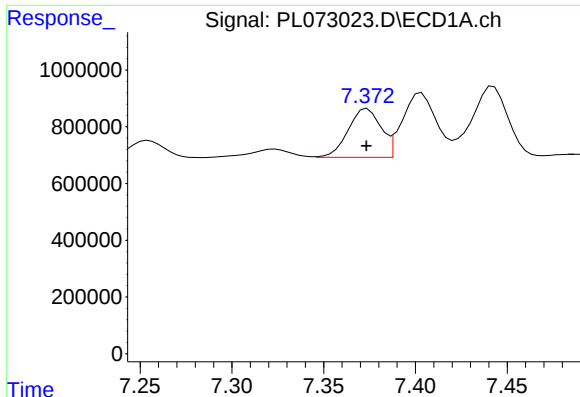

#10 gamma-Chlordane


R.T.: 7.374 min
Delta R.T.: 0.000 min
Response: 2136483
Conc: 4.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-022422

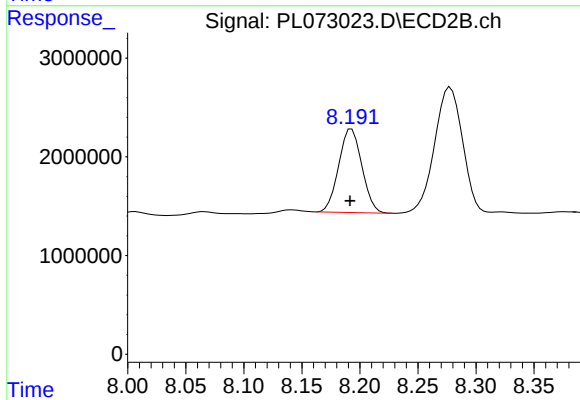


#10 gamma-Chlordane

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 11794596
Conc: 6.60 ng/ml m

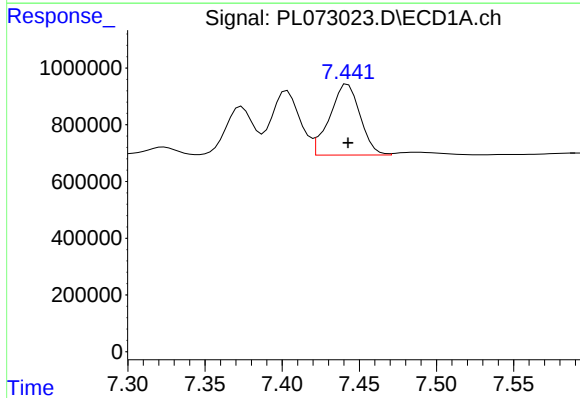


#11 alpha-Chlordane

R.T.: 7.443 min
Delta R.T.: 0.000 min
Response: 3438798
Conc: 7.18 ng/ml

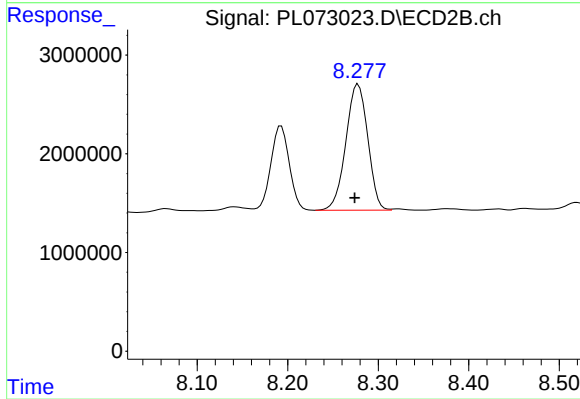

#11 alpha-Chlordane


R.T.: 8.278 min
Delta R.T.: 0.004 min
Response: 21482982
Conc: 12.20 ng/ml

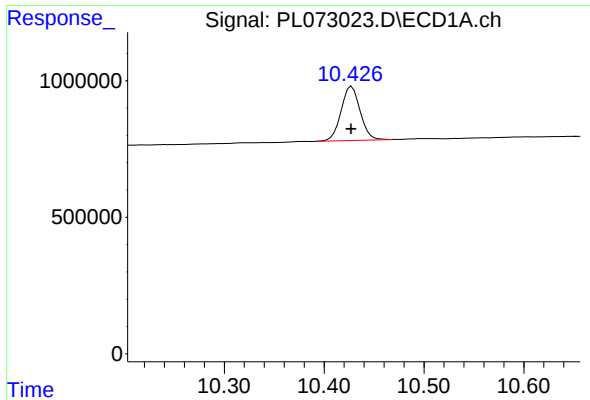

#28 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.000 min
Response: 2625707
Conc: 5.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-022422

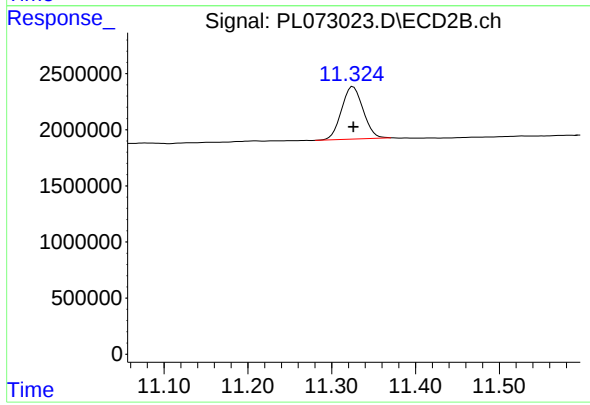

#28 Decachlorobiphenyl

R.T.: 11.326 min
Delta R.T.: 0.000 min
Response: 8428089
Conc: 5.34 ng/ml