

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
 Data File : PL073028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 13:23
 Operator : AR\AJ
 Sample : N1654-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220091-BERKELEY-3-ELUTRIATE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/01/2022
 Supervised By :Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 04:18:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.645	5.488	5225605	26696545	16.307	18.396m
28) SA Decachlor...	10.425	11.325	5471307	18588762	11.689	11.783

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
Data File : PL073028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 13:23
Operator : AR\AJ
Sample : N1654-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20220091-BERKELEY-3-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/01/2022
Supervised By : Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 04:18:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

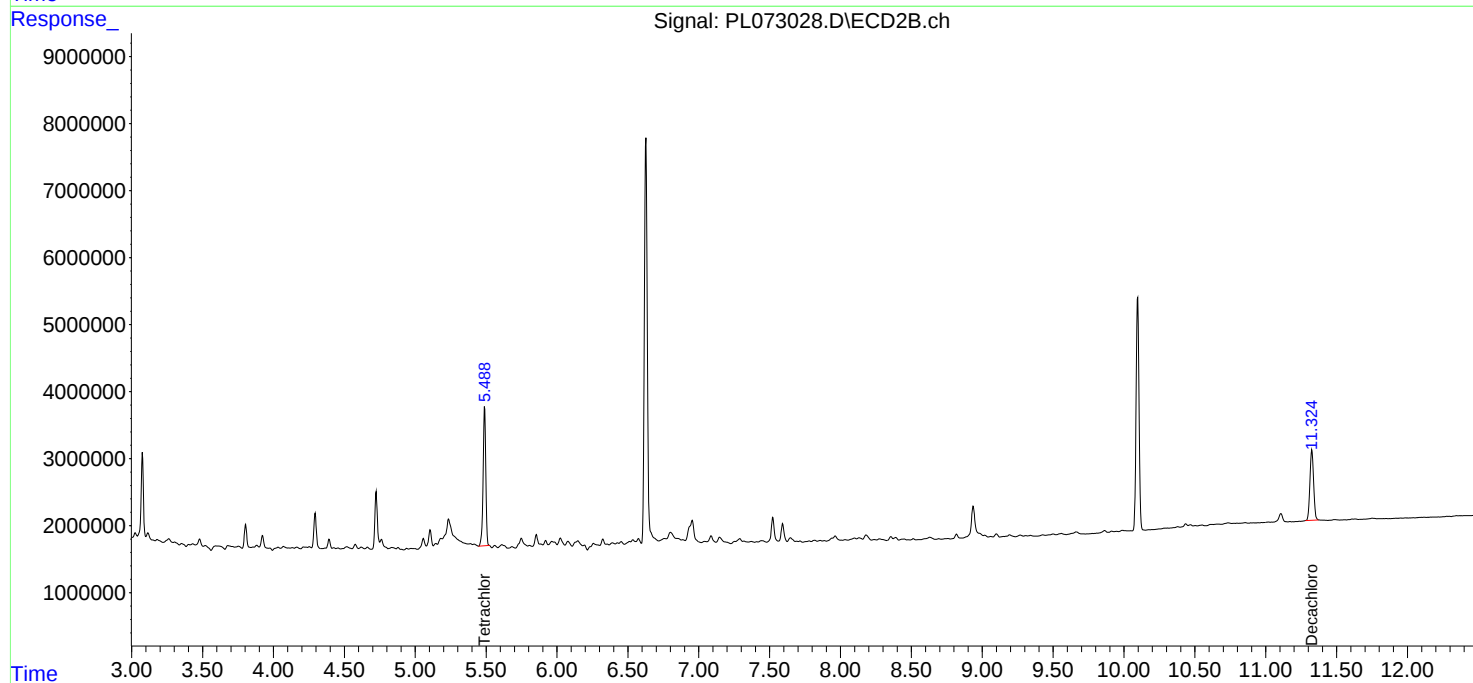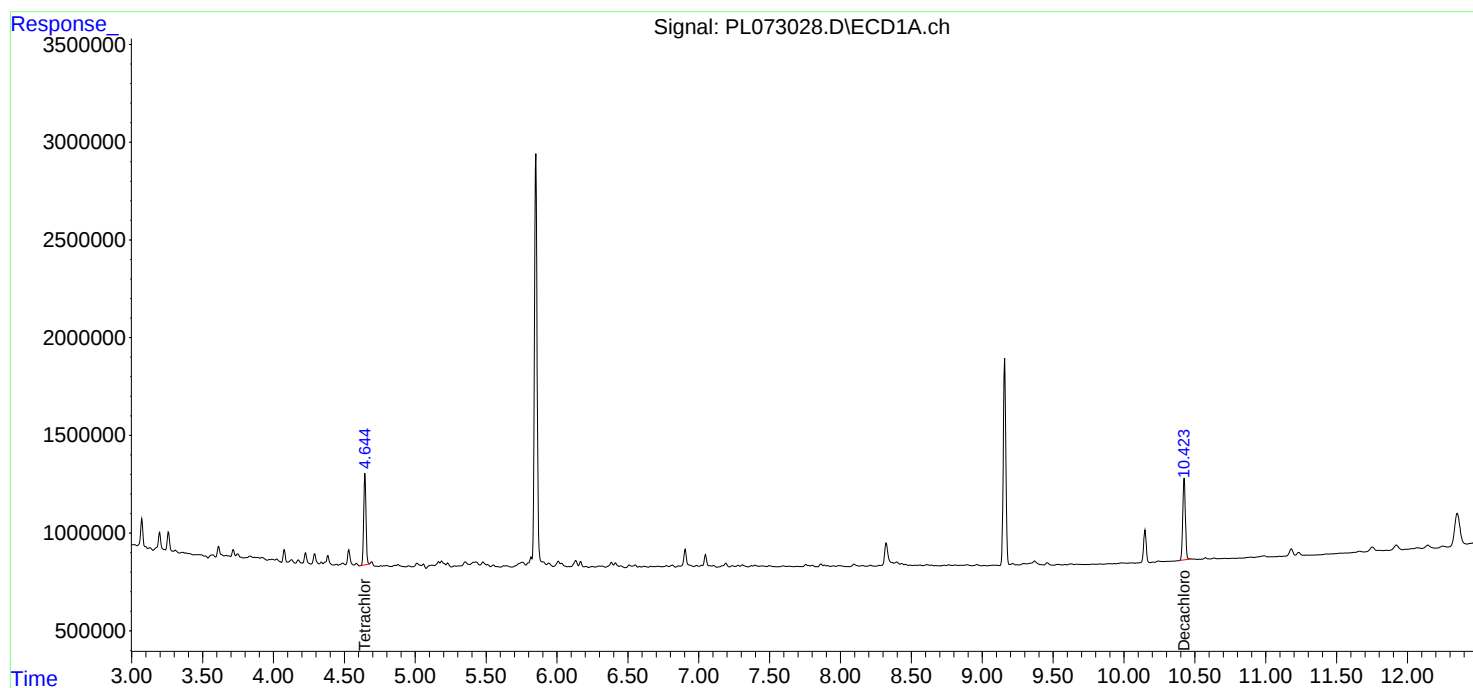

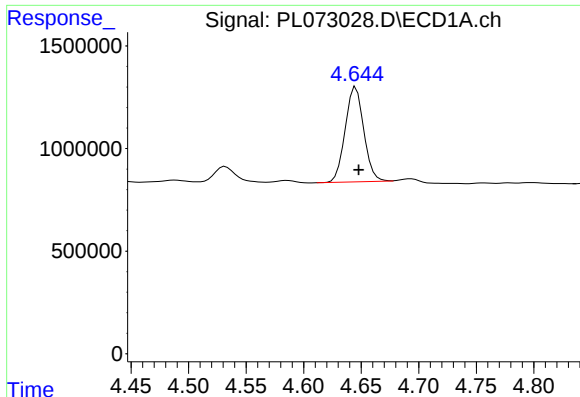


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.003 min
Response: 5225605
Conc: 16.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220091-BERKELEY-3-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

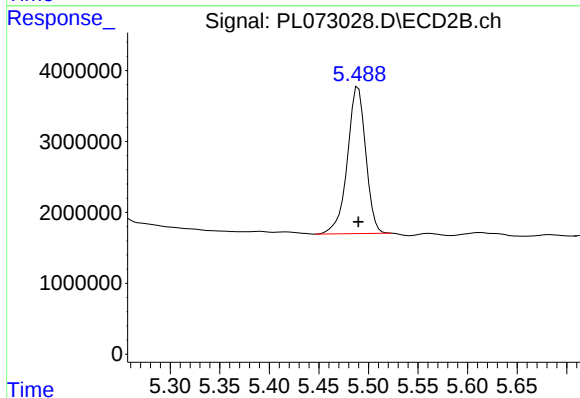


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.002 min
Response: 26696545
Conc: 18.40 ng/ml m

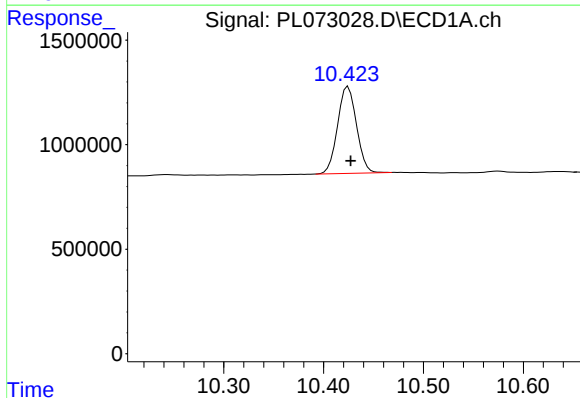

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.003 min
Response: 5471307
Conc: 11.69 ng/ml

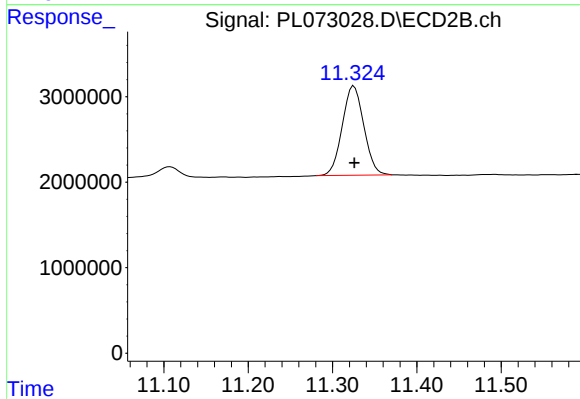

#28 Decachlorobiphenyl

R.T.: 11.325 min
Delta R.T.: 0.000 min
Response: 18588762
Conc: 11.78 ng/ml