

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
 Data File : PL073052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 20:08
 Operator : AR\AJ
 Sample : N1681-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-1-8FT

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/01/2022
 Supervised By : Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:31:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.490	3989570	17979894	12.450	12.390
28)	SA Decachlor...	10.427	11.326	314.8E6	1127.3E6	672.485	714.564
Target Compounds							
11)	B alpha-Chl...	7.439	8.279	197778	1199700	0.413m	0.681 #
12)	B 4,4'-DDE	7.656	8.459	5835374	23227898	15.013	14.856
16)	A 4,4'-DDD	8.241	8.990	331141	2563344	0.951m	1.928m#
17)	MA 4,4'-DDT	8.504	9.304	9334901	34008408	24.530	24.793

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022822\
Data File : PL073052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 20:08
Operator : AR\AJ
Sample : N1681-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1-1-8FT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/01/2022
Supervised By : Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:31:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

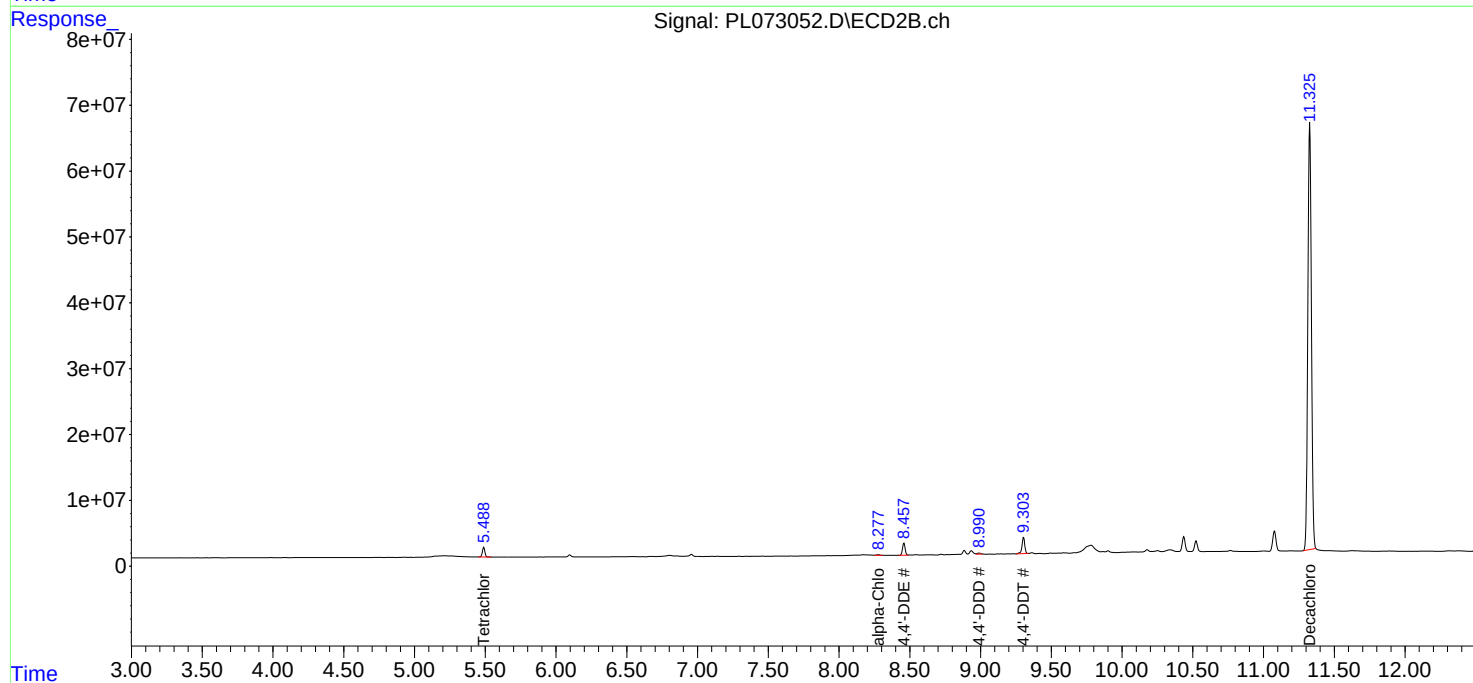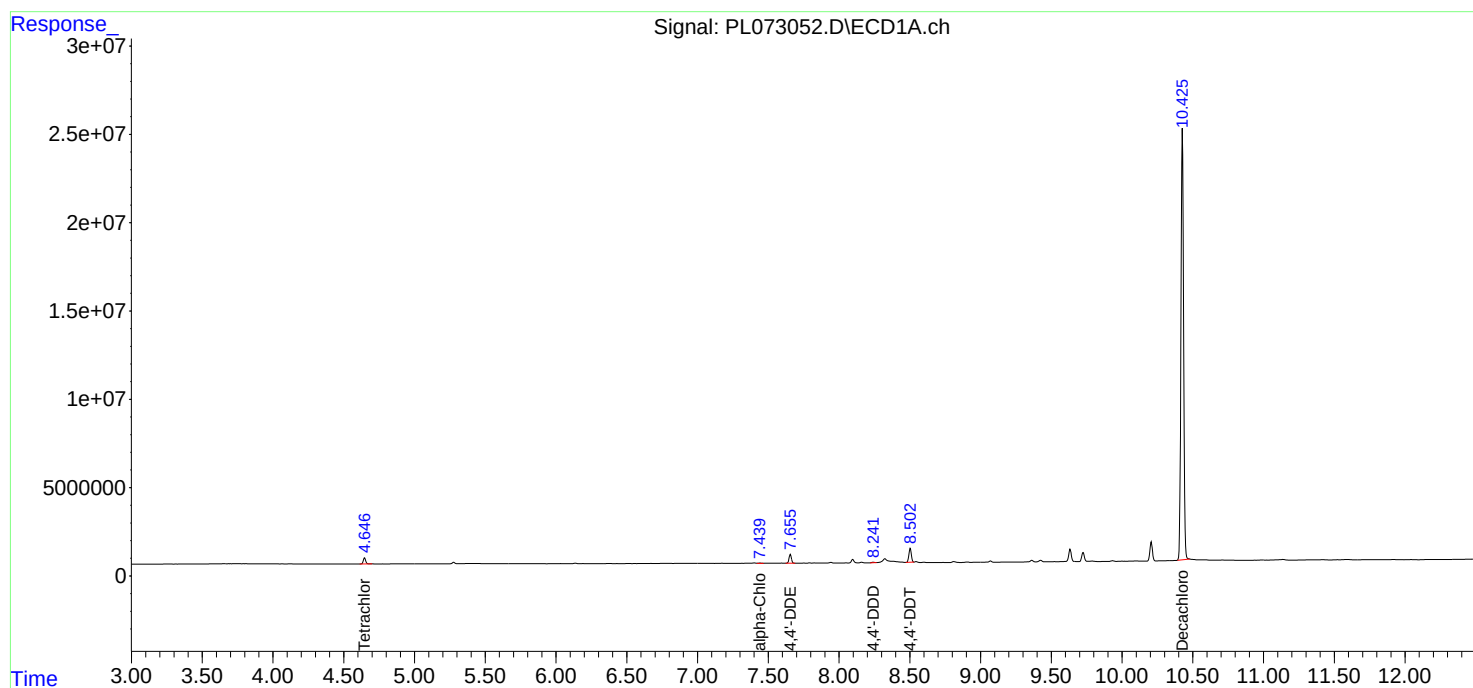

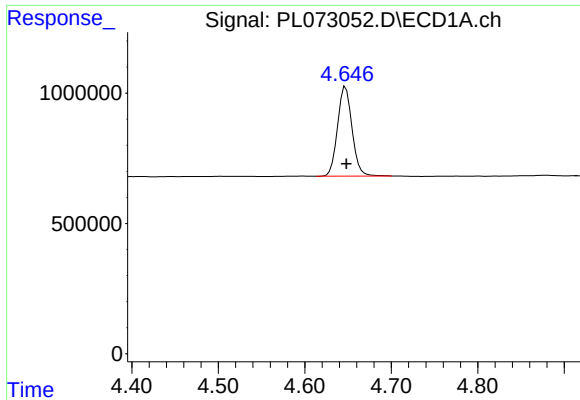


#1 Tetrachloro-m-xylene

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 3989570
Conc: 12.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-1-8FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

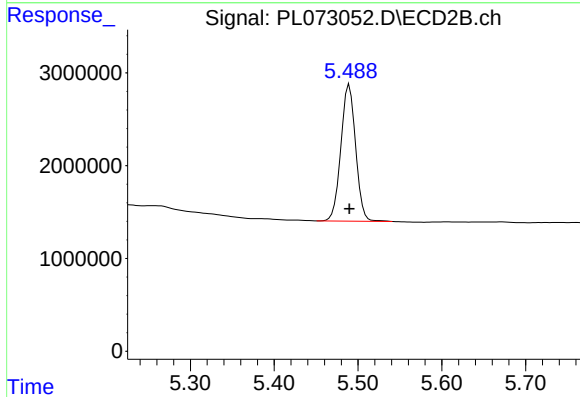


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 17979894
Conc: 12.39 ng/ml

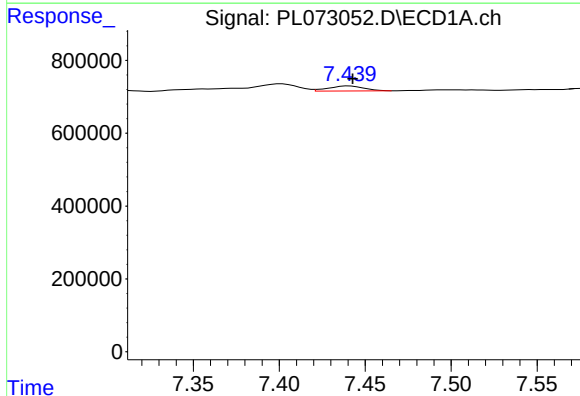


#11 alpha-Chlordane

R.T.: 7.439 min
Delta R.T.: -0.003 min
Response: 197778
Conc: 0.41 ng/ml m

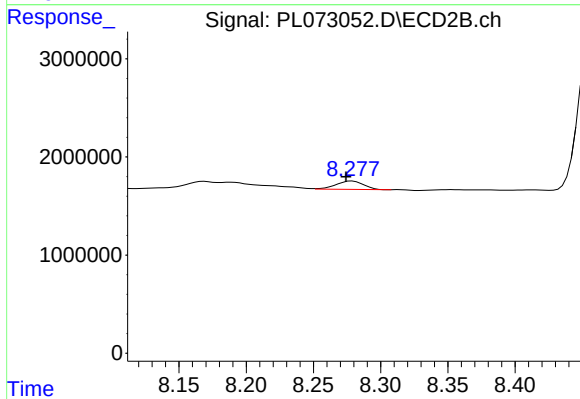

#11 alpha-Chlordane

R.T.: 8.279 min
Delta R.T.: 0.005 min
Response: 1199700
Conc: 0.68 ng/ml

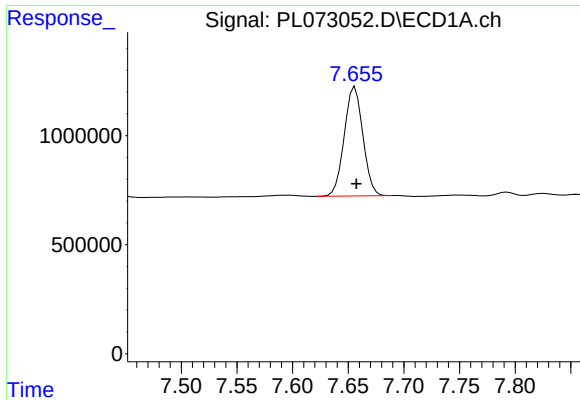


#12 4,4'-DDE

R.T.: 7.656 min
Delta R.T.: -0.001 min
Response: 5835374
Conc: 15.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-1-8FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

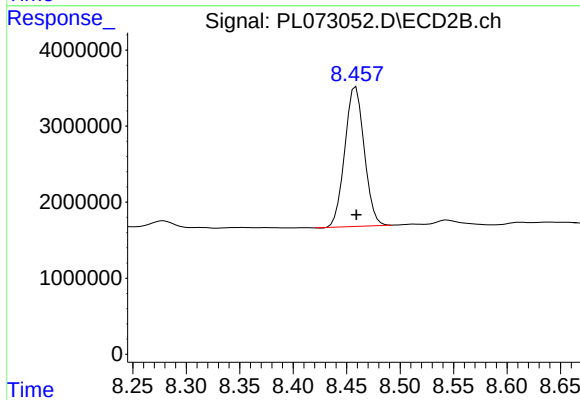


#12 4,4'-DDE

R.T.: 8.459 min
Delta R.T.: 0.000 min
Response: 23227898
Conc: 14.86 ng/ml

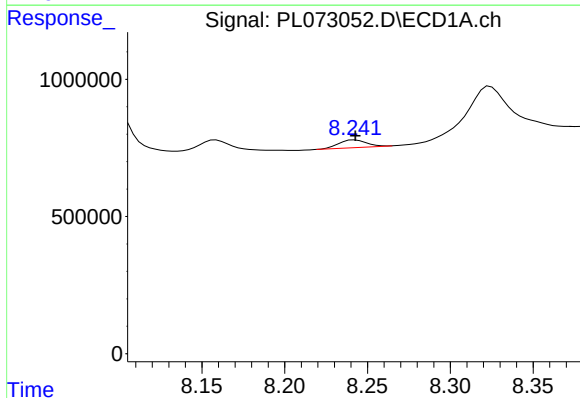


#16 4,4'-DDD

R.T.: 8.241 min
Delta R.T.: -0.002 min
Response: 331141
Conc: 0.95 ng/ml m

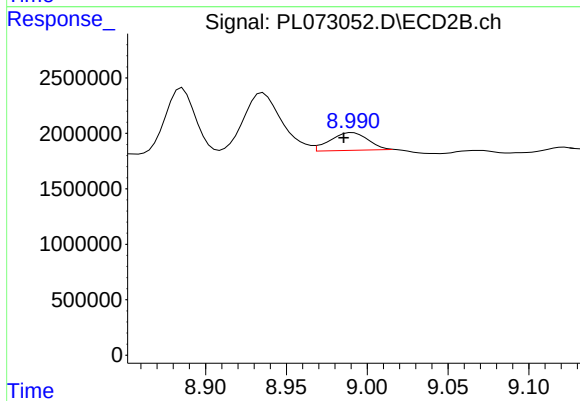

#16 4,4'-DDD

R.T.: 8.990 min
Delta R.T.: 0.004 min
Response: 2563344
Conc: 1.93 ng/ml m

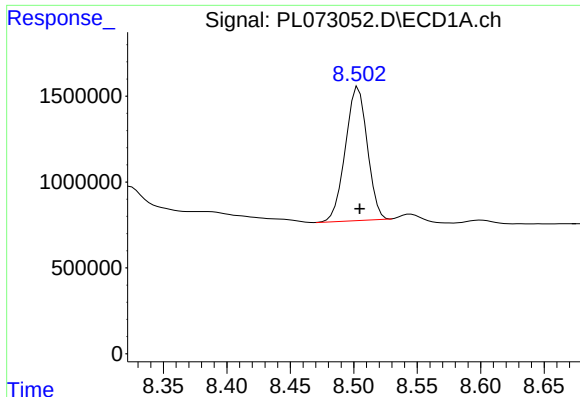


#17 4,4'-DDT

R.T.: 8.504 min
Delta R.T.: -0.001 min
Response: 9334901
Conc: 24.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-1-8FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

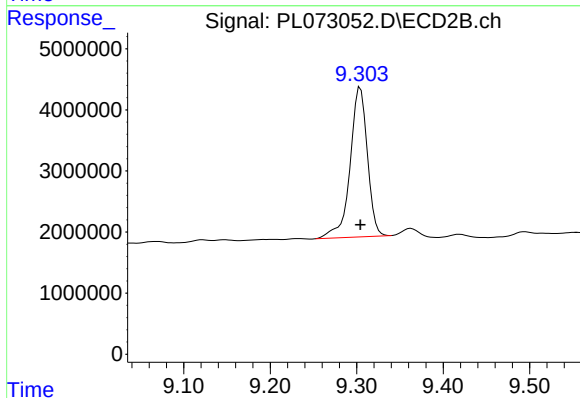


#17 4,4'-DDT

R.T.: 9.304 min
Delta R.T.: 0.000 min
Response: 34008408
Conc: 24.79 ng/ml

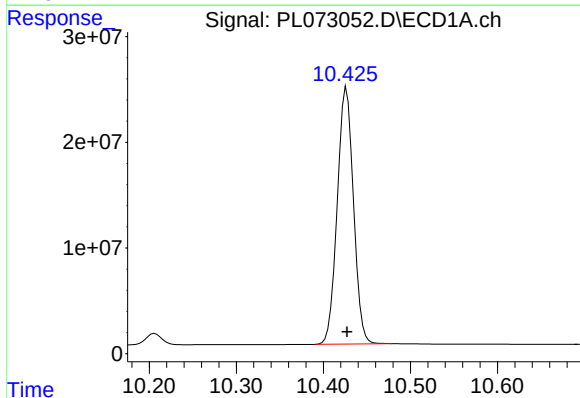

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 314769471
Conc: 672.49 ng/ml

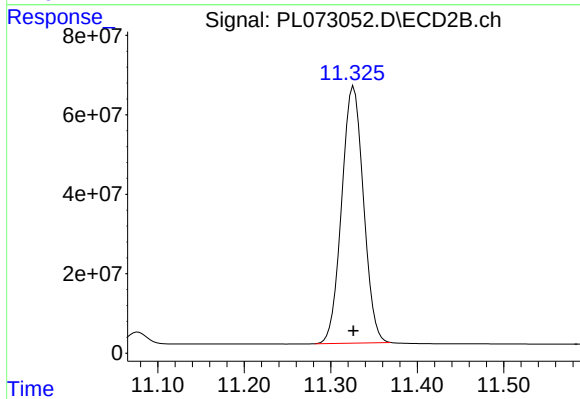

#28 Decachlorobiphenyl

R.T.: 11.326 min
Delta R.T.: 0.000 min
Response: 1127252176
Conc: 714.56 ng/ml