

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
 Data File : PL081129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 09:28
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 14:31:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 13:01:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	8.761	0.000	5099736	0	5.325	N.D. #
Target Compounds							
3)	MA gamma-BHC...	4.117	0.000	164448	0	0.091	N.D. #
6)	B beta-BHC	0.000	3.788	0	65739	N.D.	0.074 #
9)	A Endosulfan I	5.825f	0.000	641025	0	0.529	N.D. #
11)	B alpha-Chl...	5.825f	0.000	641025	0	0.504	N.D. #
15)	B Endosulfa...	6.604f	5.815	22578321	6448188	19.784	5.580 #
16)	A 4,4'-DDD	6.505	0.000	2197778	0	2.296	N.D. #
17)	MA 4,4'-DDT	6.780f	0.000	1785934	0	1.996	N.D. #
19)	B Endosulfa...	6.947	0.000	315959	0	0.306	N.D. #
20)	A Methoxychlor	7.302	0.000	2754174	0	5.929	N.D. #
21)	B Endrin ke...	7.421	0.000	4232471	0	3.688	N.D. #
22)	Mirex	7.868	0.000	8017681	0	9.287	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
Data File : PL081129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 09:28
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 14:31:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 13:01:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

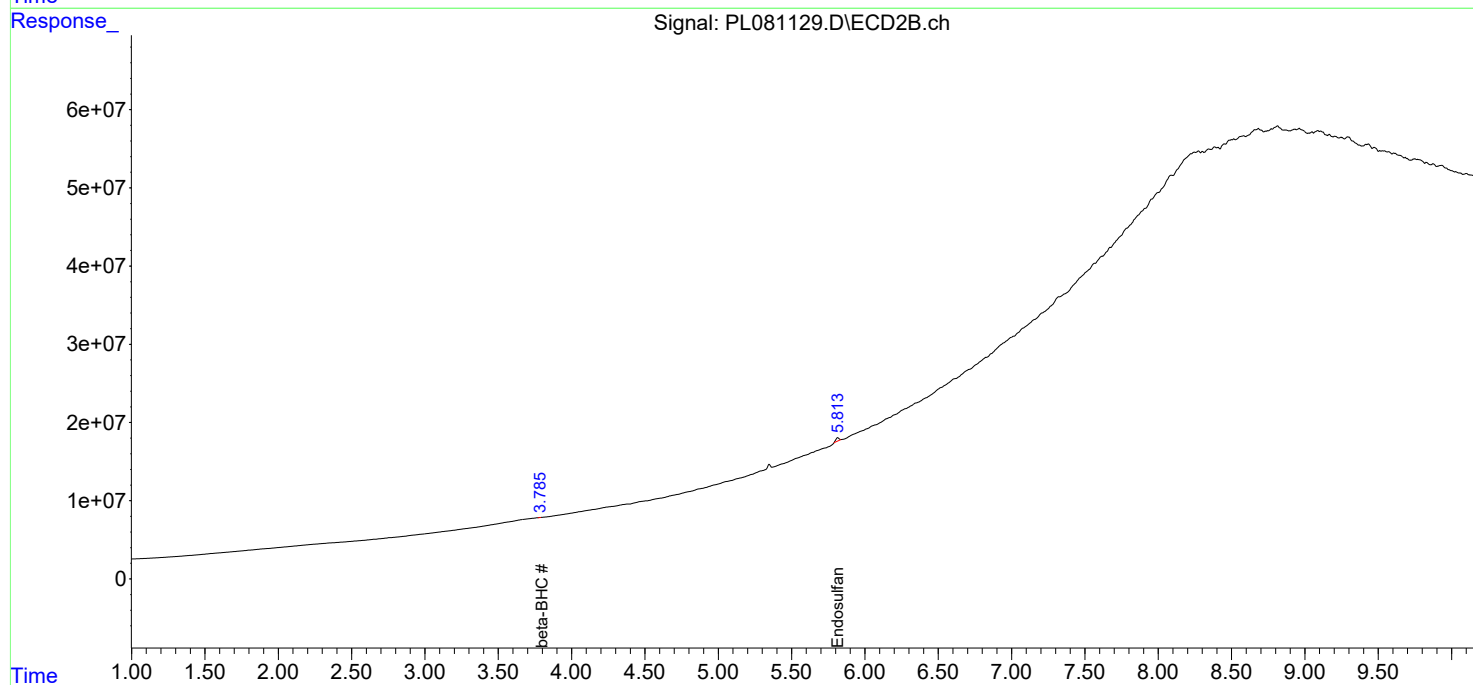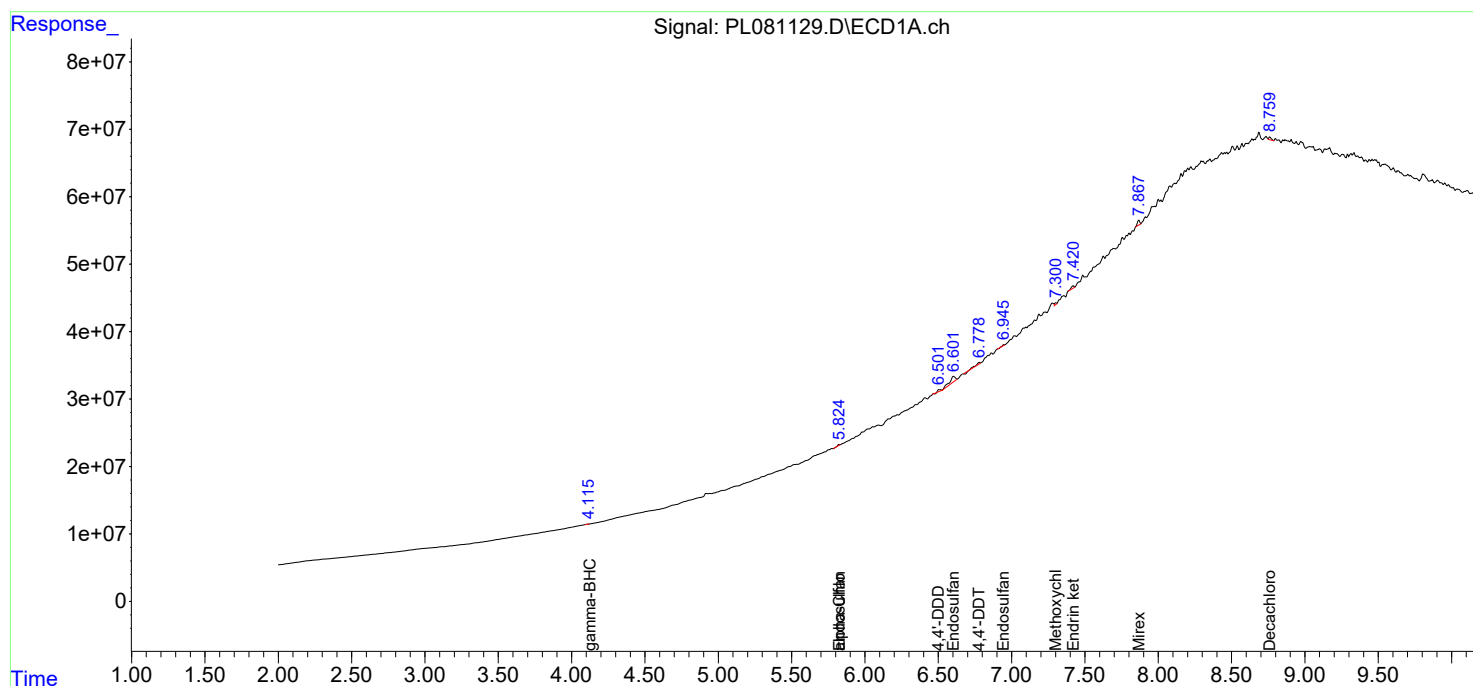


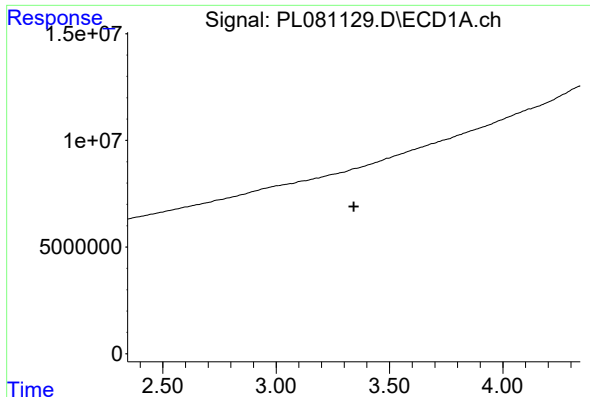

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

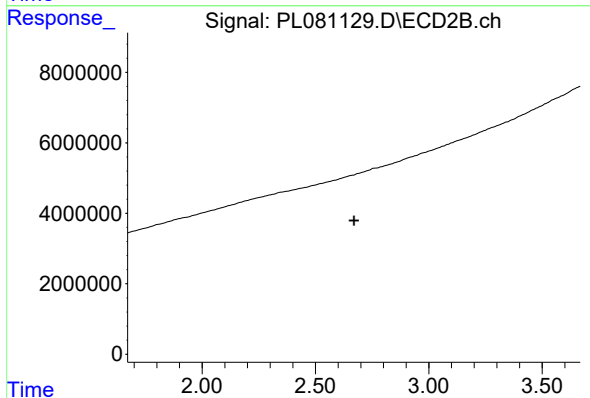


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

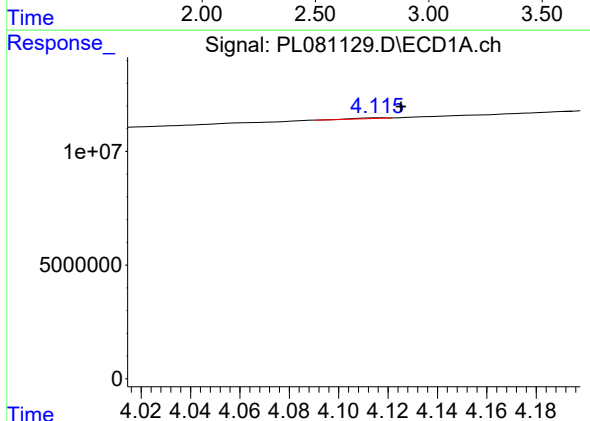


#3 gamma-BHC (Lindane)

R.T.: 4.117 min
Delta R.T.: -0.008 min
Response: 164448
Conc: 0.09 ng/ml

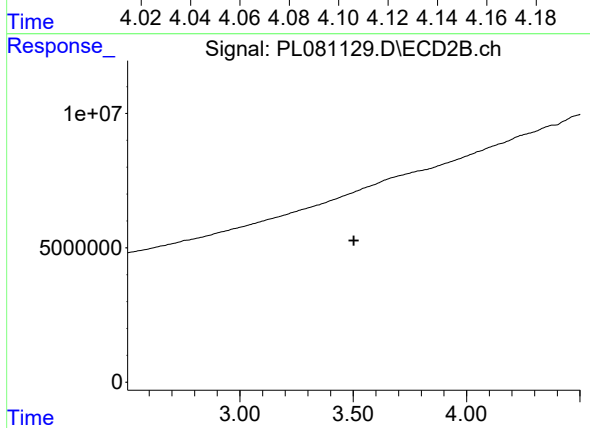

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.503 min
Response: 0
Conc: N.D.

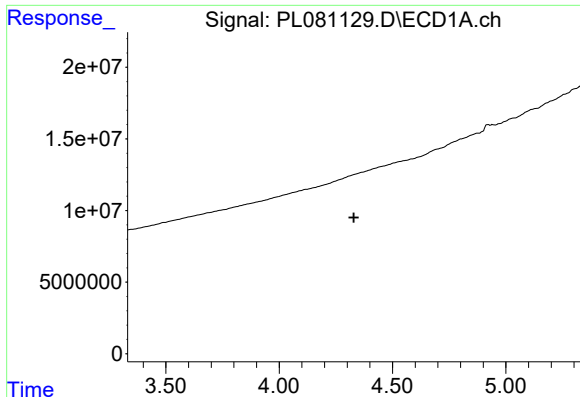

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

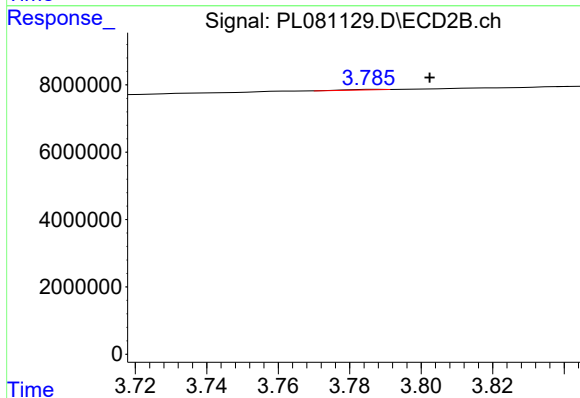


#6 beta-BHC

R.T.: 3.788 min
Delta R.T.: -0.014 min
Response: 65739
Conc: 0.07 ng/ml

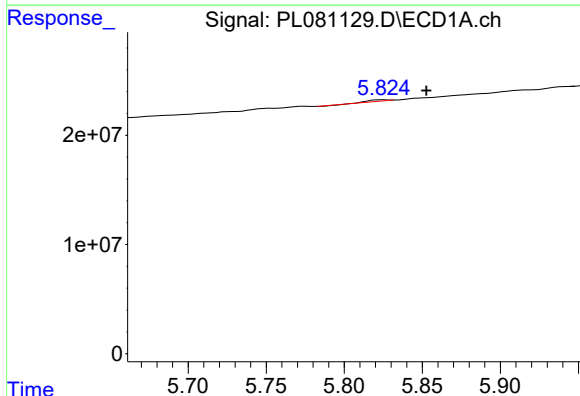


#9 Endosulfan I

R.T.: 5.825 min
Delta R.T.: -0.028 min
Response: 641025
Conc: 0.53 ng/ml

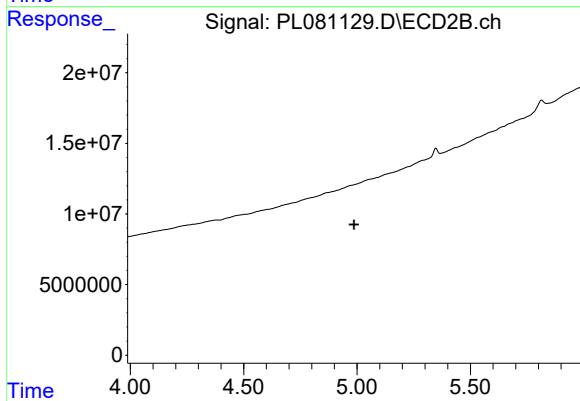

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 4.987 min
Response: 0
Conc: N.D.

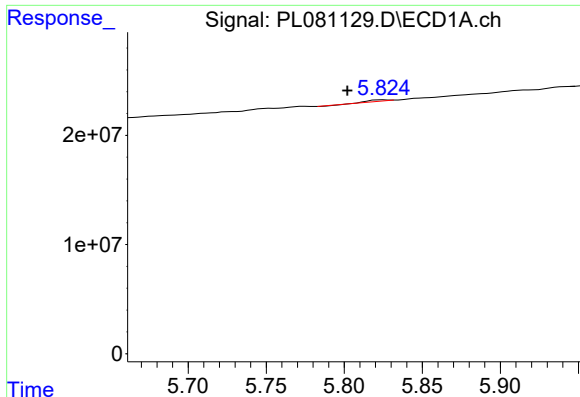

#11 alpha-Chlordane


R.T.: 5.825 min
Delta R.T.: 0.023 min
Response: 641025
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

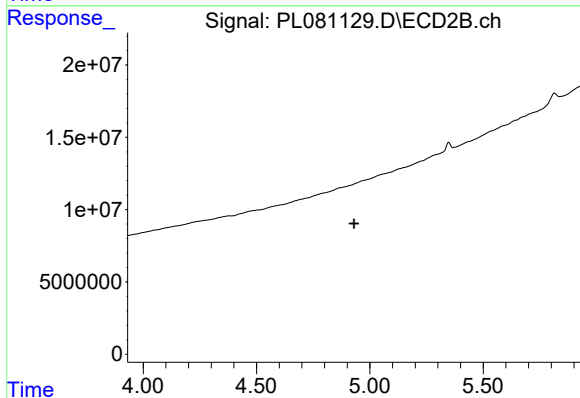


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.931 min
Response: 0
Conc: N.D.

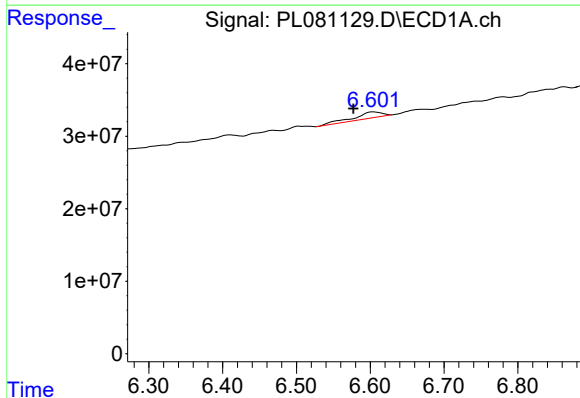


#15 Endosulfan II

R.T.: 6.604 min
Delta R.T.: 0.027 min
Response: 22578321
Conc: 19.78 ng/ml

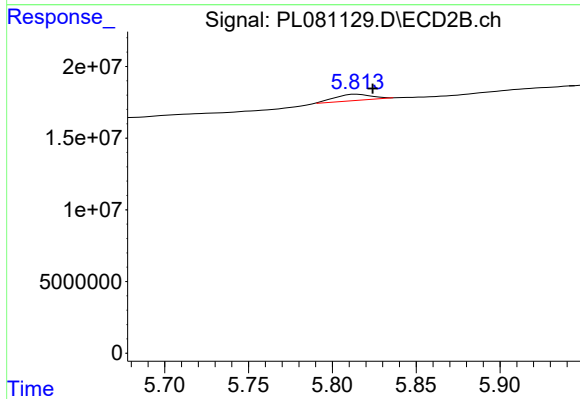

#15 Endosulfan II


R.T.: 5.815 min
Delta R.T.: -0.009 min
Response: 6448188
Conc: 5.58 ng/ml

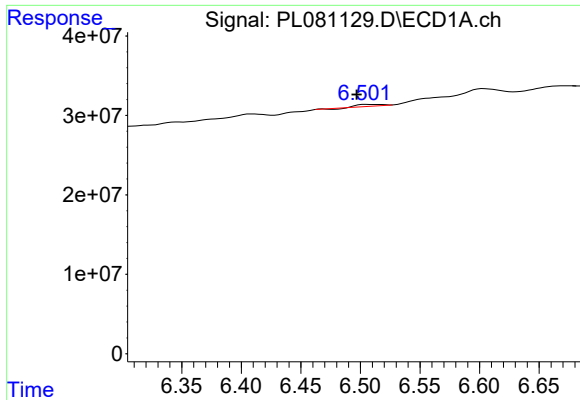

#16 4,4'-DDD


R.T.: 6.505 min
Delta R.T.: 0.008 min
Response: 2197778
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

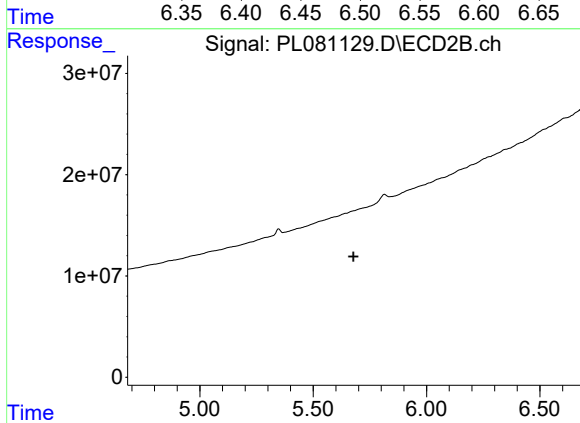


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.678 min
Response: 0
Conc: N.D.

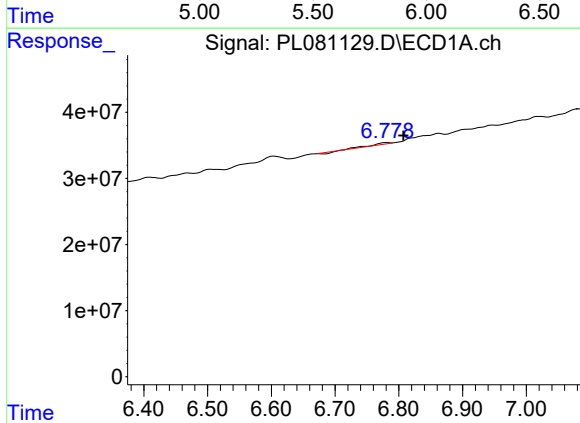


#17 4,4'-DDT

R.T.: 6.780 min
Delta R.T.: -0.027 min
Response: 1785934
Conc: 2.00 ng/ml

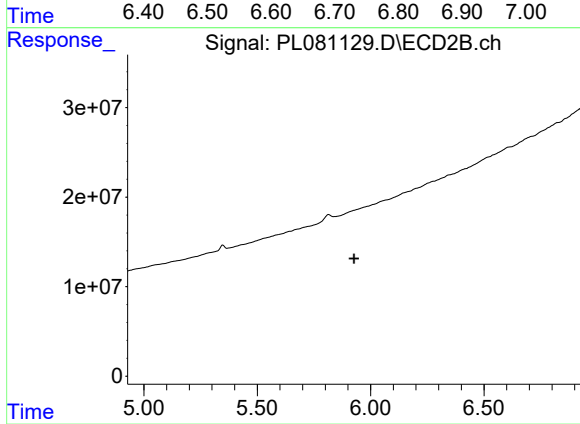

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.927 min
Response: 0
Conc: N.D.

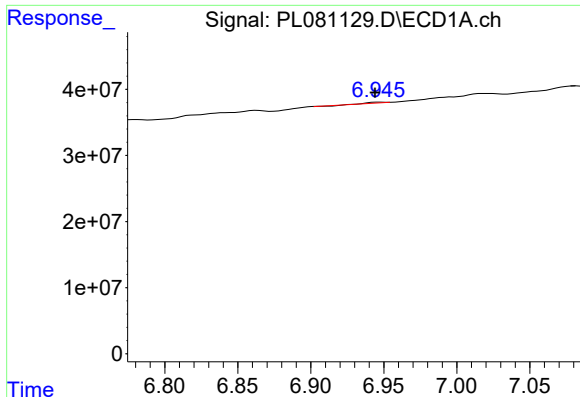

#19 Endosulfan Sulfate


R.T.: 6.947 min
Delta R.T.: 0.003 min
Response: 315959
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

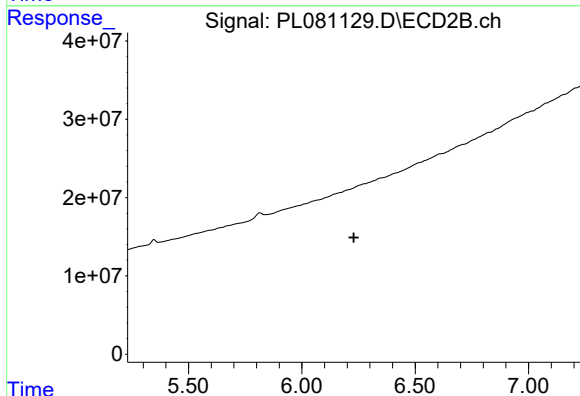


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.229 min
Response: 0
Conc: N.D.

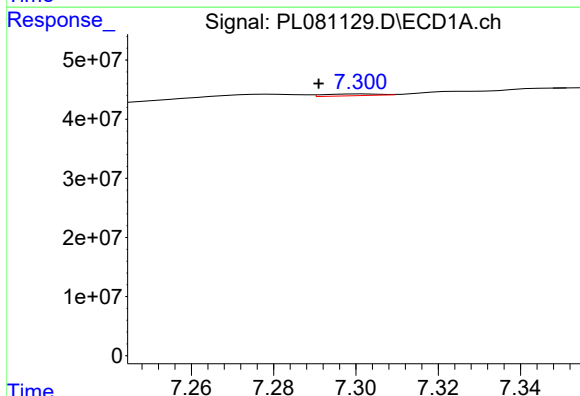


#20 Methoxychlor

R.T.: 7.302 min
Delta R.T.: 0.011 min
Response: 2754174
Conc: 5.93 ng/ml

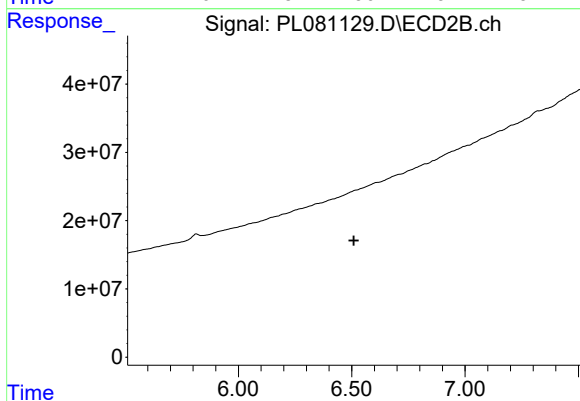

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

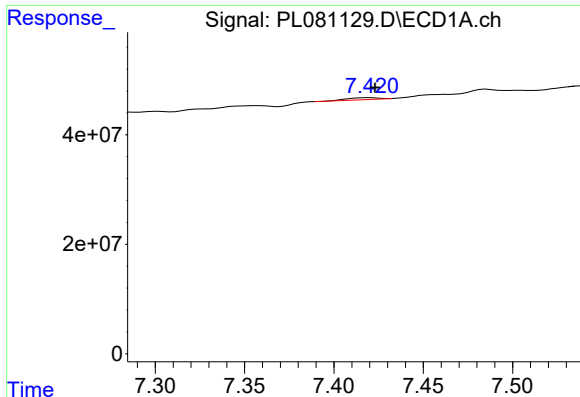

#21 Endrin ketone


R.T.: 7.421 min
Delta R.T.: -0.002 min
Response: 4232471
Conc: 3.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

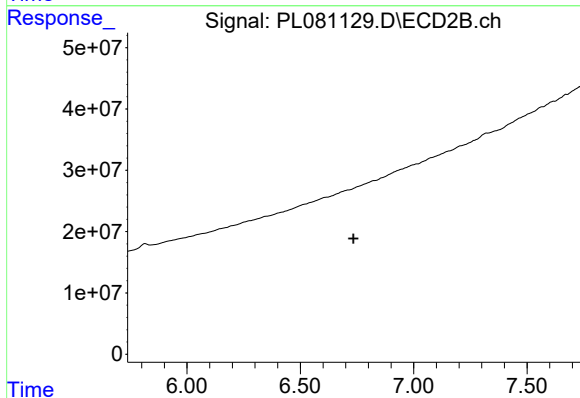


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.735 min
Response: 0
Conc: N.D.

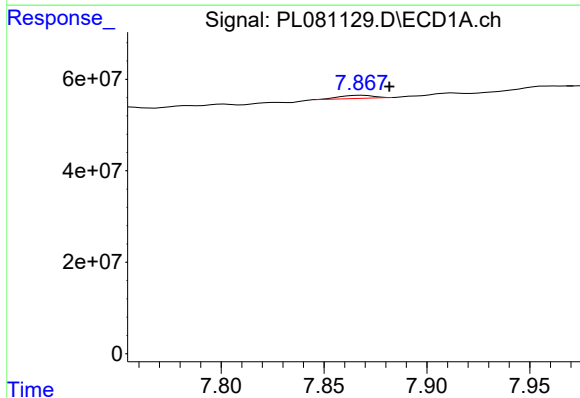


#22 Mirex

R.T.: 7.868 min
Delta R.T.: -0.014 min
Response: 8017681
Conc: 9.29 ng/ml

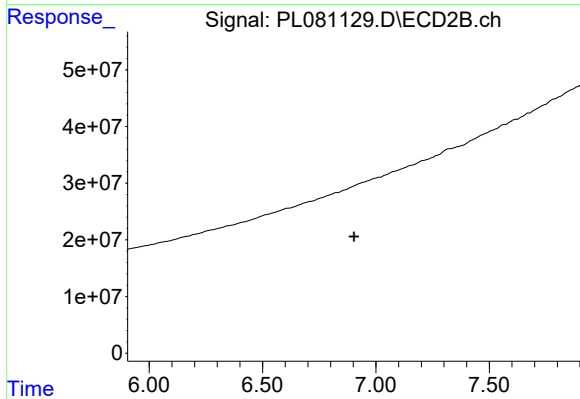

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 6.904 min
Response: 0
Conc: N.D.

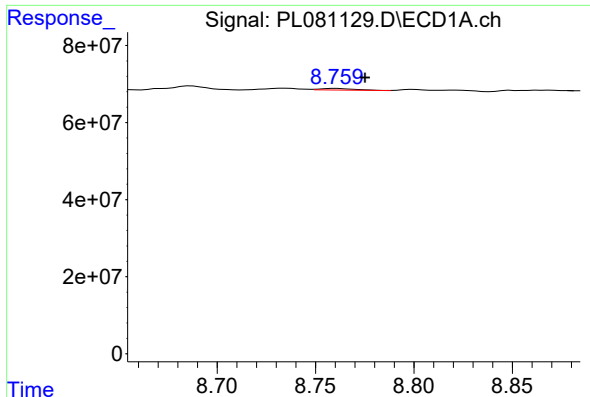

#28 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.014 min
Response: 5099736
Conc: 5.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

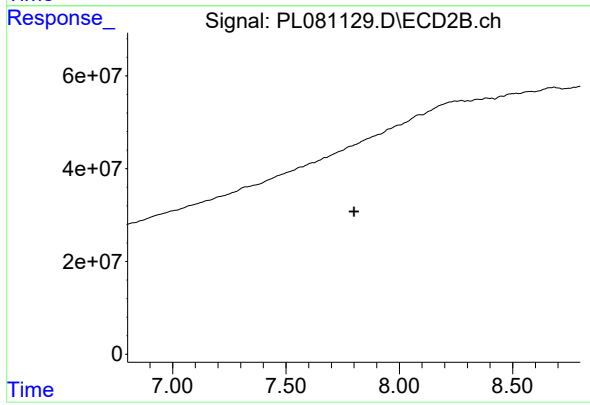

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.800 min
Response: 0
Conc: N.D.