

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
 Data File : PL081141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 12:14
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 12:53:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 12:53:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	2.670	78171940	105.8E6	50.000	50.000
28)	SA Decachlor...	8.773	7.799	49813206	61403694	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.488	3.662	31518809	35098223	500.000	500.000
24)	Chlordane-2	5.016	4.238	32125299	41216401	500.000	500.000
25)	Chlordane-3	5.722	4.867	112.8E6	107.1E6	500.000	500.000
26)	Chlordane-4	5.803	4.928	135.1E6	110.1E6	500.000	500.000
27)	Chlordane-5	6.645	5.596	21783929	25248875	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
Data File : PL081141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 12:14
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 12:53:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 12:53:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

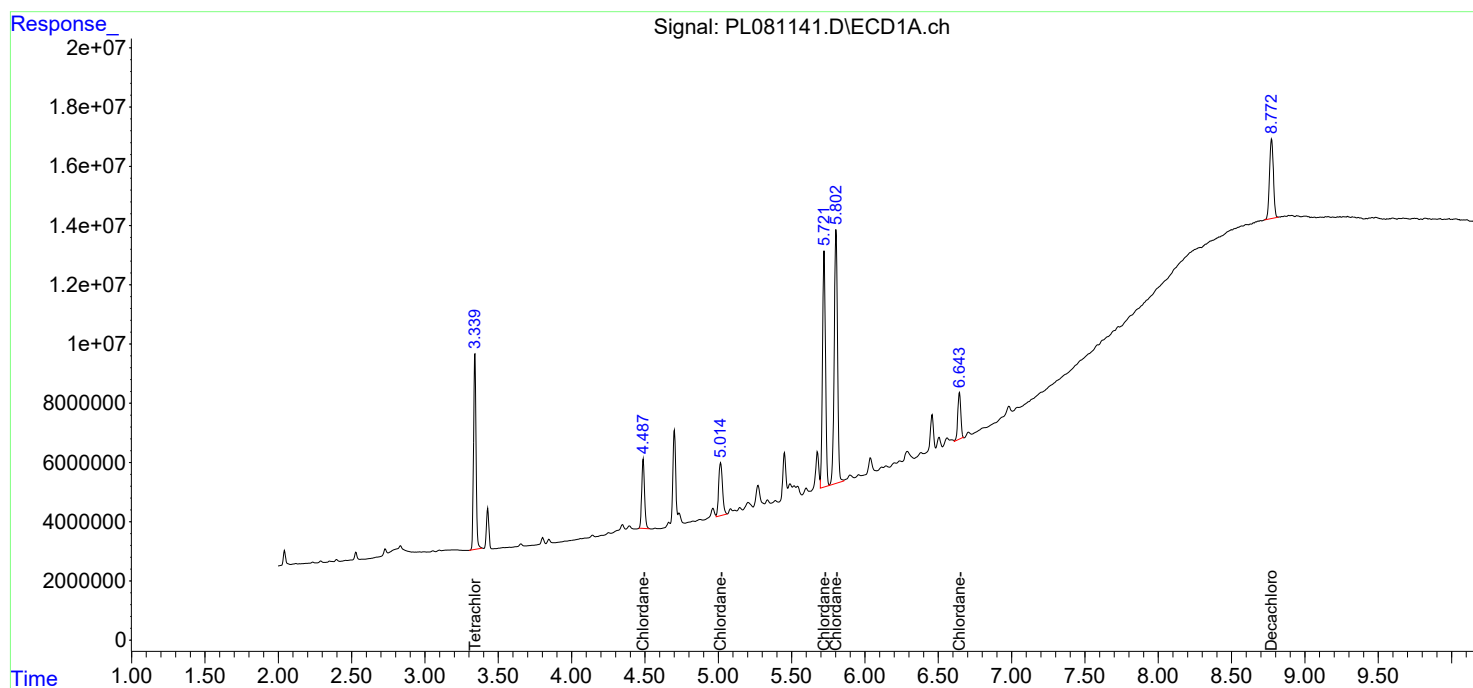


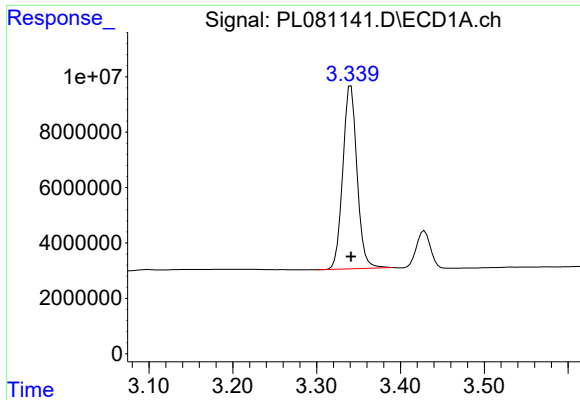

#1 Tetrachloro-m-xylene


R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 78171940
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

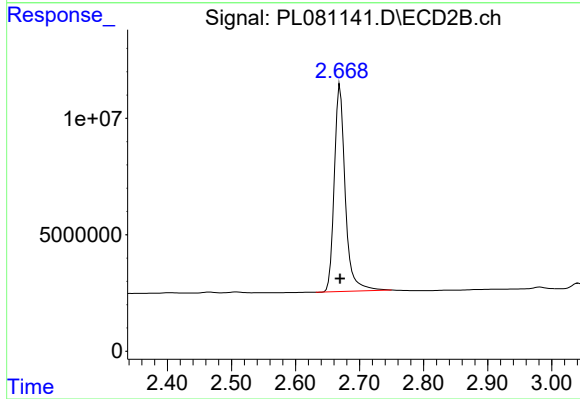


#1 Tetrachloro-m-xylene

R.T.: 2.670 min
Delta R.T.: 0.000 min
Response: 105800448
Conc: 50.00 ng/ml

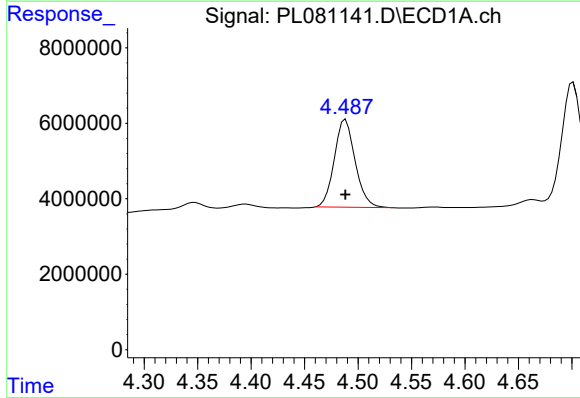


#23 Chlordane-1

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 31518809
Conc: 500.00 ng/ml

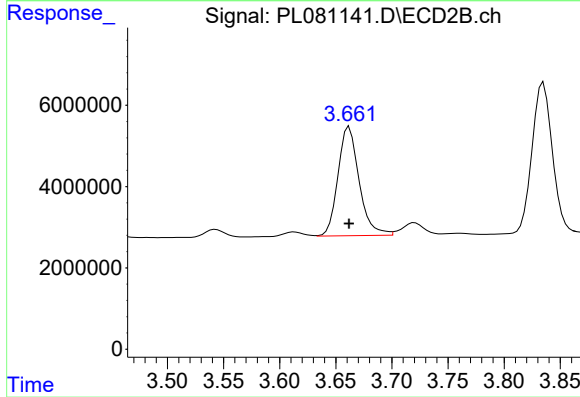

#23 Chlordane-1


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 35098223
Conc: 500.00 ng/ml

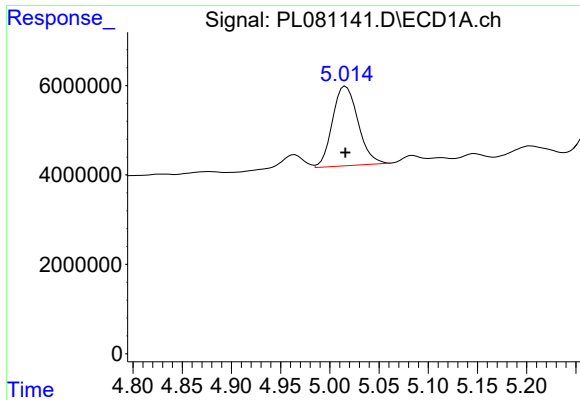

#24 Chlordane-2


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 32125299
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

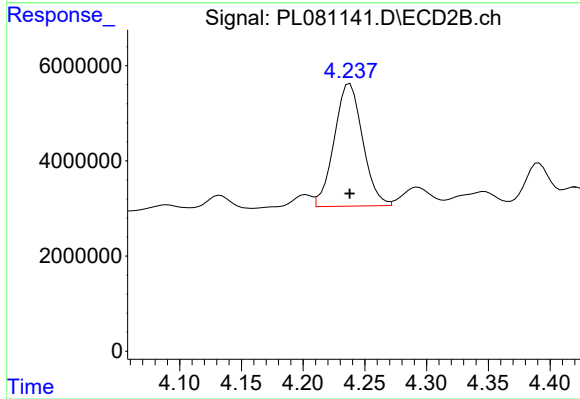


#24 Chlordane-2

R.T.: 4.238 min
Delta R.T.: 0.000 min
Response: 41216401
Conc: 500.00 ng/ml

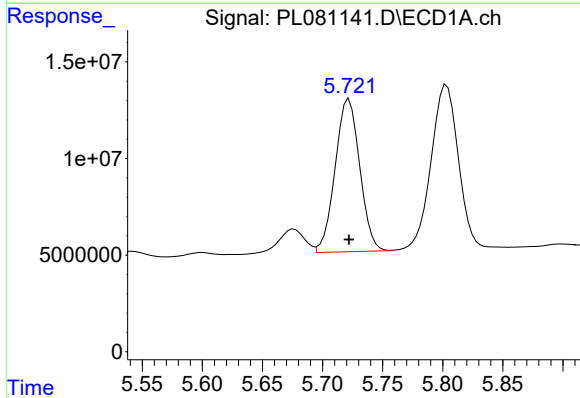


#25 Chlordane-3

R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 112775786
Conc: 500.00 ng/ml

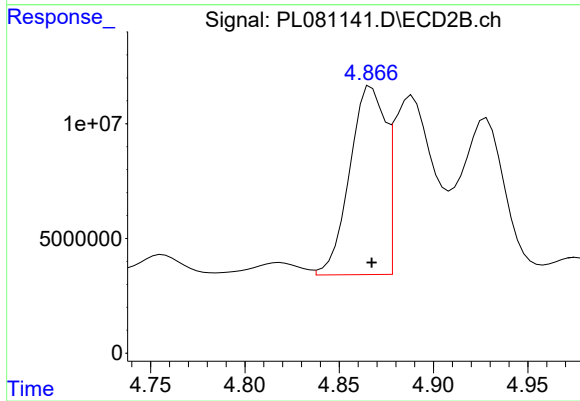

#25 Chlordane-3


R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 107123432
Conc: 500.00 ng/ml

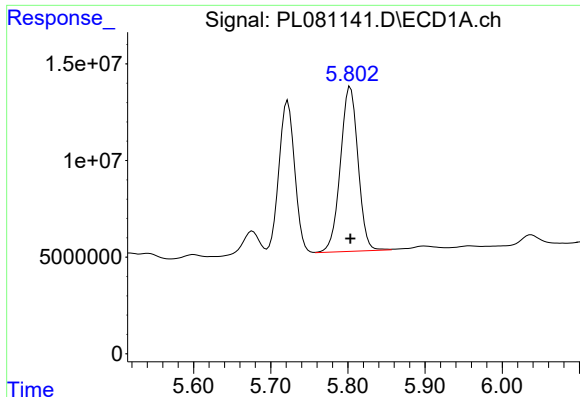

#26 Chlordane-4


R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 135117326
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

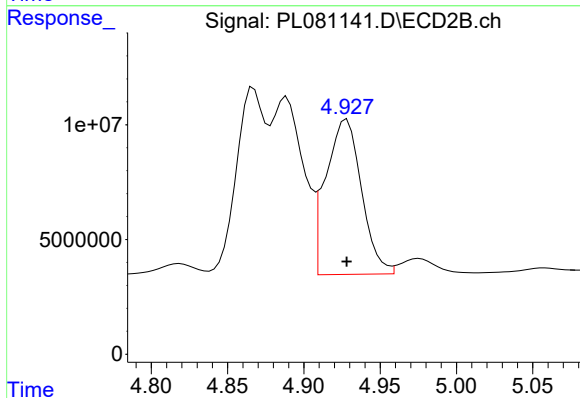


#26 Chlordane-4

R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 110084682
Conc: 500.00 ng/ml

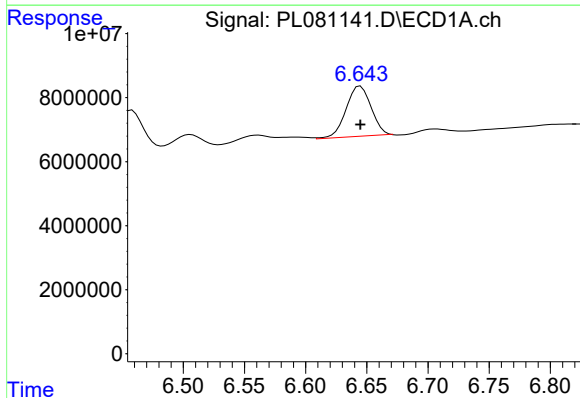


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 21783929
Conc: 500.00 ng/ml

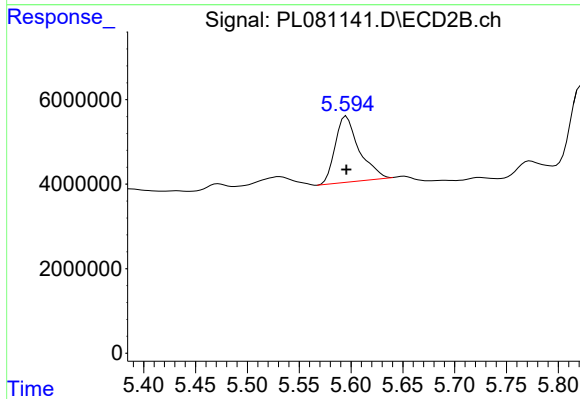

#27 Chlordane-5

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 25248875
Conc: 500.00 ng/ml

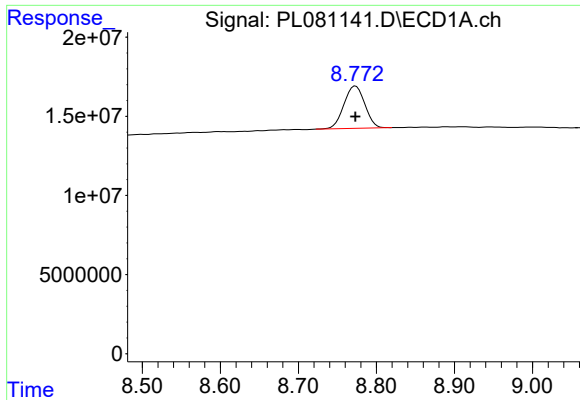

#28 Decachlorobiphenyl


R.T.: 8.773 min

Delta R.T.: 0.000 min

Response: 49813206

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

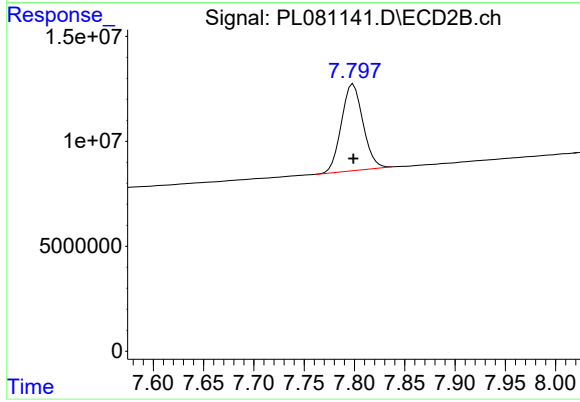

#28 Decachlorobiphenyl

R.T.: 7.799 min

Delta R.T.: 0.000 min

Response: 61403694

Conc: 50.00 ng/ml