

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
 Data File : PL081142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 12:28
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 12:54:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 12:53:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	2.669	39180769	52075394	25.061	24.610
28)	SA Decachlor...	8.774	7.800	26195288	30337861	26.294	24.704
Target Compounds							
23)	Chlordane-1	4.488	3.662	15853128	17525734	251.487	249.667
24)	Chlordane-2	5.017	4.238	16435321	21058744	255.800	255.466
25)	Chlordane-3	5.722	4.867	55063922	51636773	244.130	241.015
26)	Chlordane-4	5.803	4.928	66457414	53738917	245.925	244.080
27)	Chlordane-5	6.645	5.596	11379667	11961134	261.194	236.865


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
Data File : PL081142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 12:28
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 12:54:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 12:53:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

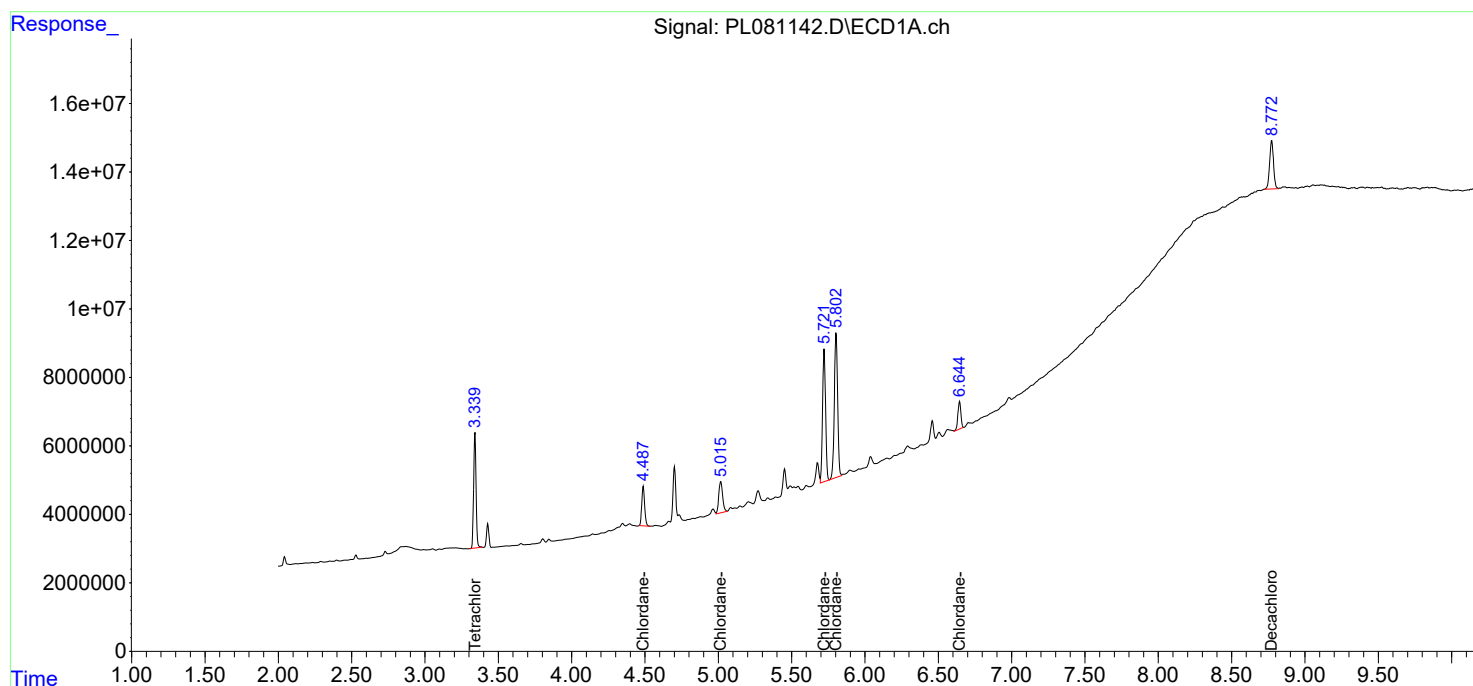


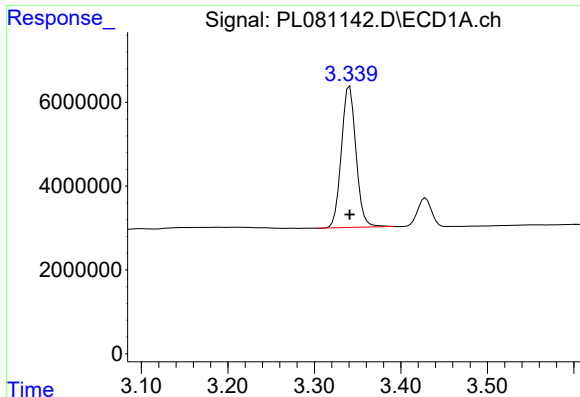

#1 Tetrachloro-m-xylene


R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 39180769
Conc: 25.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

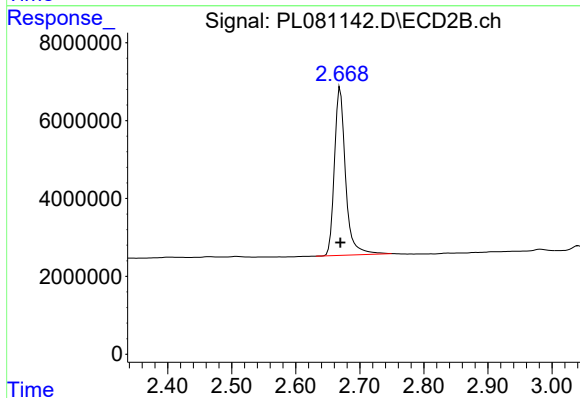


#1 Tetrachloro-m-xylene

R.T.: 2.669 min
Delta R.T.: 0.000 min
Response: 52075394
Conc: 24.61 ng/ml

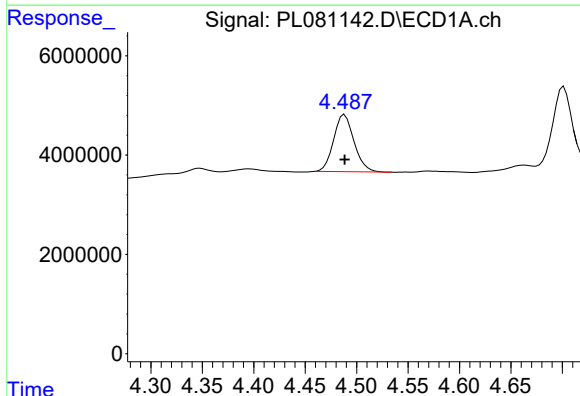


#23 Chlordane-1

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 15853128
Conc: 251.49 ng/ml

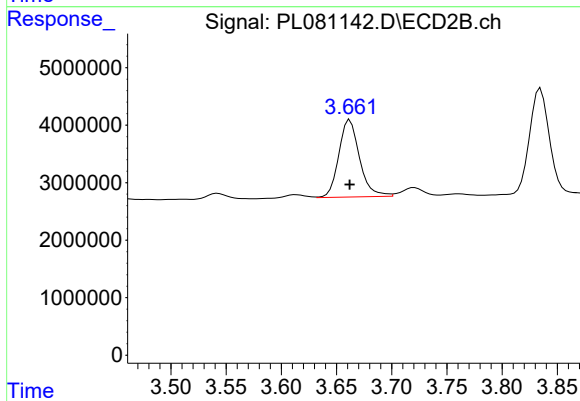

#23 Chlordane-1


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 17525734
Conc: 249.67 ng/ml

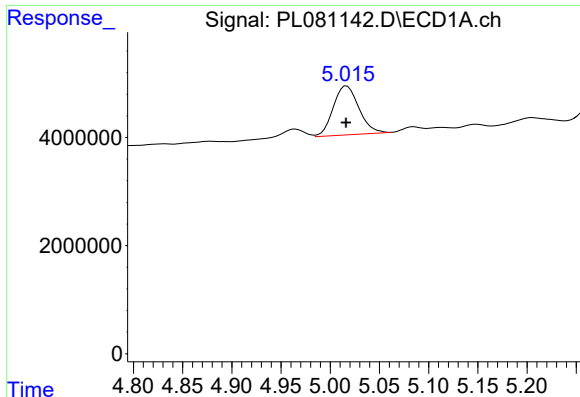

#24 Chlordane-2


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 16435321
Conc: 255.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

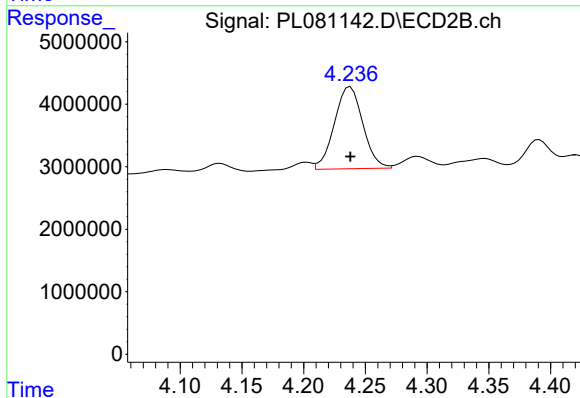


#24 Chlordane-2

R.T.: 4.238 min
Delta R.T.: 0.000 min
Response: 21058744
Conc: 255.47 ng/ml

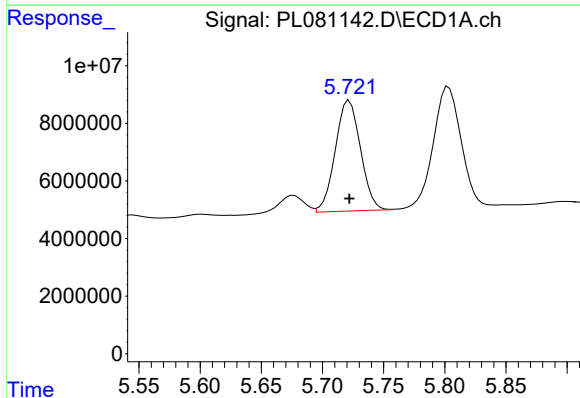


#25 Chlordane-3

R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 55063922
Conc: 244.13 ng/ml

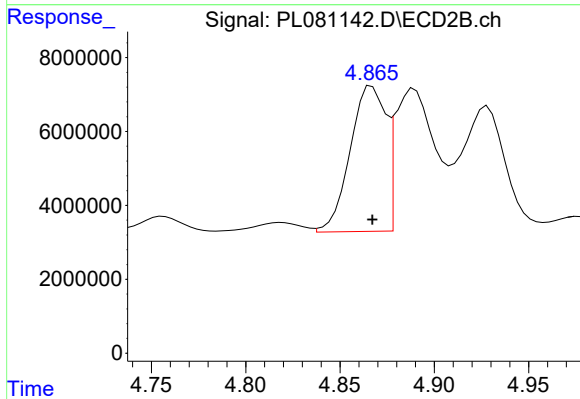

#25 Chlordane-3


R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 51636773
Conc: 241.02 ng/ml

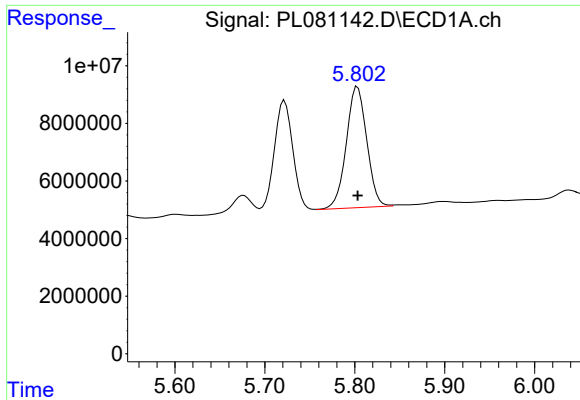

#26 Chlordane-4


R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 66457414
Conc: 245.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

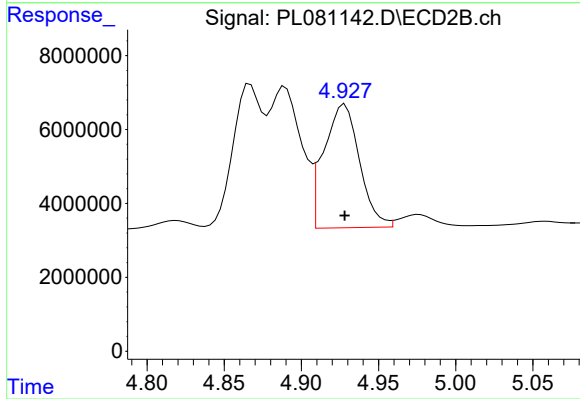


#26 Chlordane-4

R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 53738917
Conc: 244.08 ng/ml

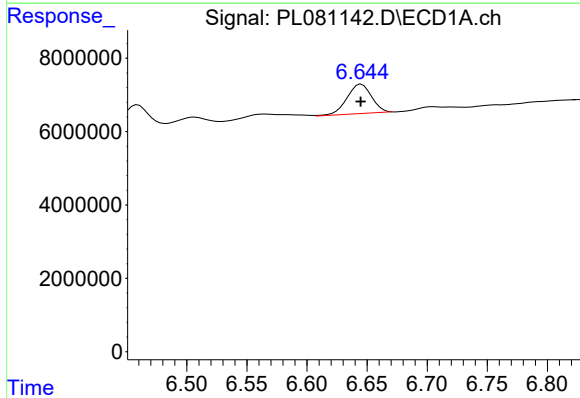


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 11379667
Conc: 261.19 ng/ml

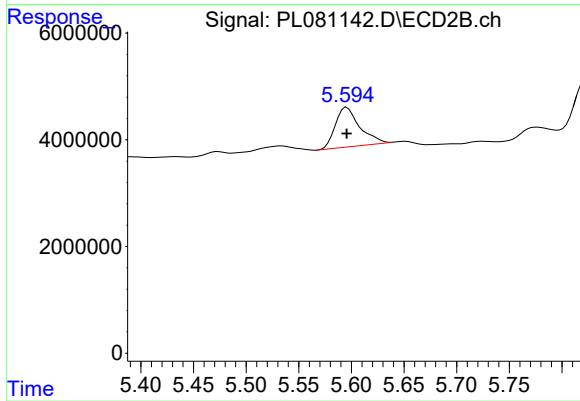

#27 Chlordane-5


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 11961134
Conc: 236.86 ng/ml

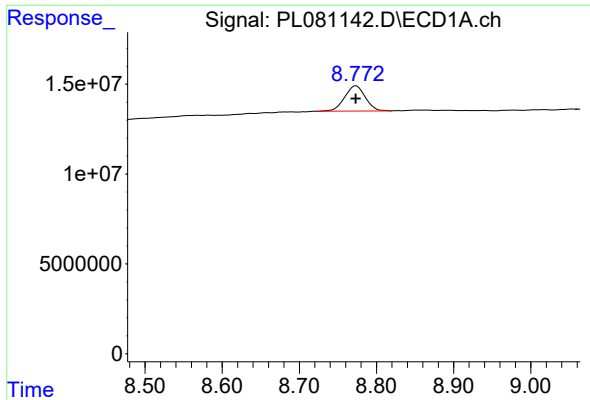

#28 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.000 min
Response: 26195288
Conc: 26.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

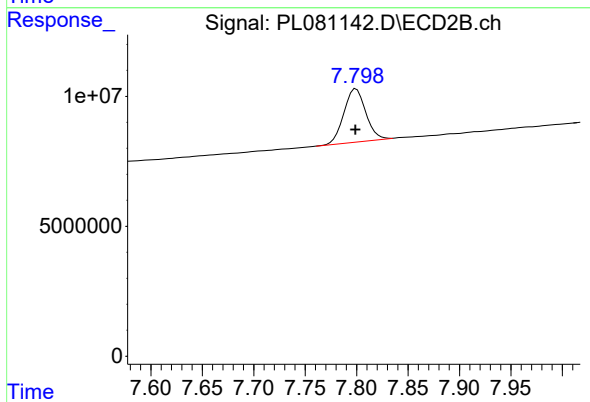

#28 Decachlorobiphenyl

R.T.: 7.800 min
Delta R.T.: 0.000 min
Response: 30337861
Conc: 24.70 ng/ml