

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
 Data File : PL081151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 14:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 15:12:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 15:11:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	2.668	85223011	110.2E6	54.682	52.475
28)	SA Decachlor...	8.770	7.797	51606802	66582491	52.349	55.464
Target Compounds							
23)	Chlordane-1	4.486	3.660	33926618	36477980	540.420	523.452
24)	Chlordane-2	5.014	4.236	36565074	43271231	576.966	529.800
25)	Chlordane-3	5.720	4.865	122.8E6	112.4E6	552.091	533.744
26)	Chlordane-4	5.801	4.926	147.5E6	116.7E6	553.464	531.314
27)	Chlordane-5	6.643	5.594	23598622	27577676	527.639	569.587



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022823\
Data File : PL081151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 14:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 15:12:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 15:11:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

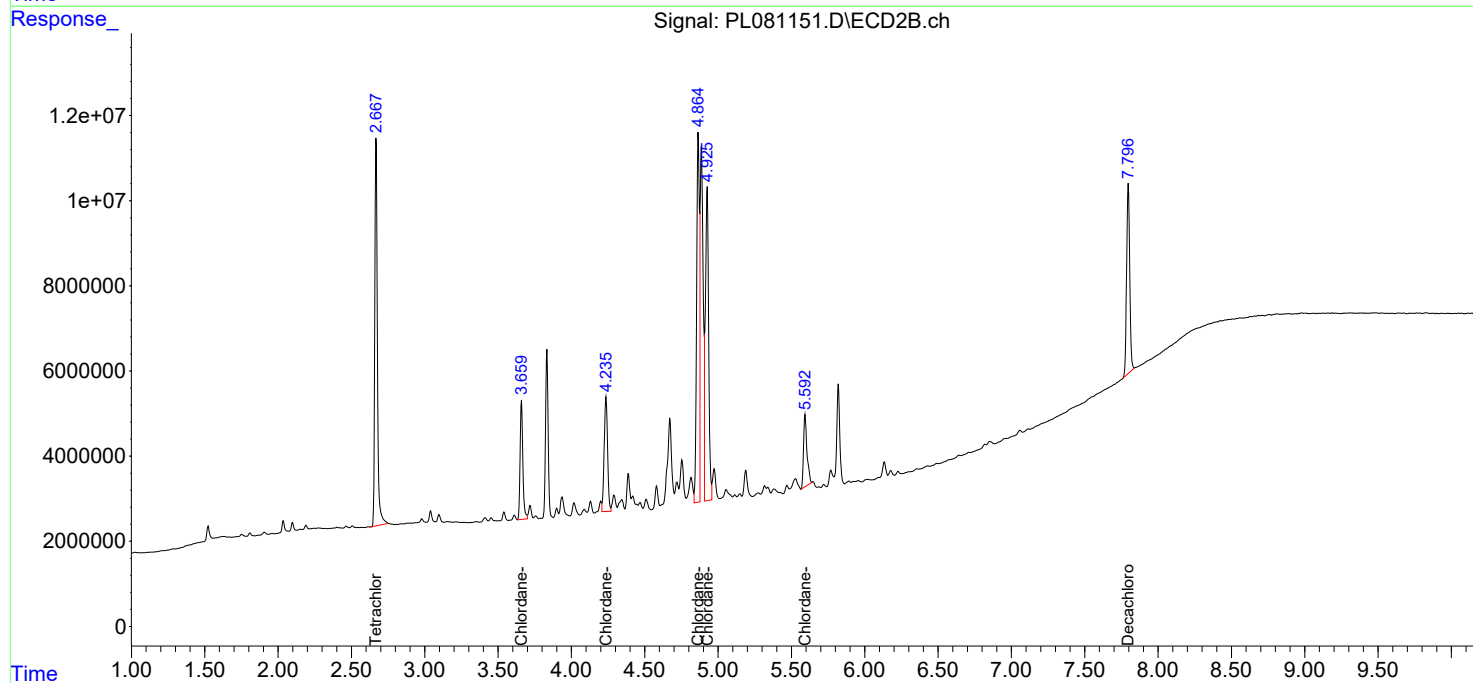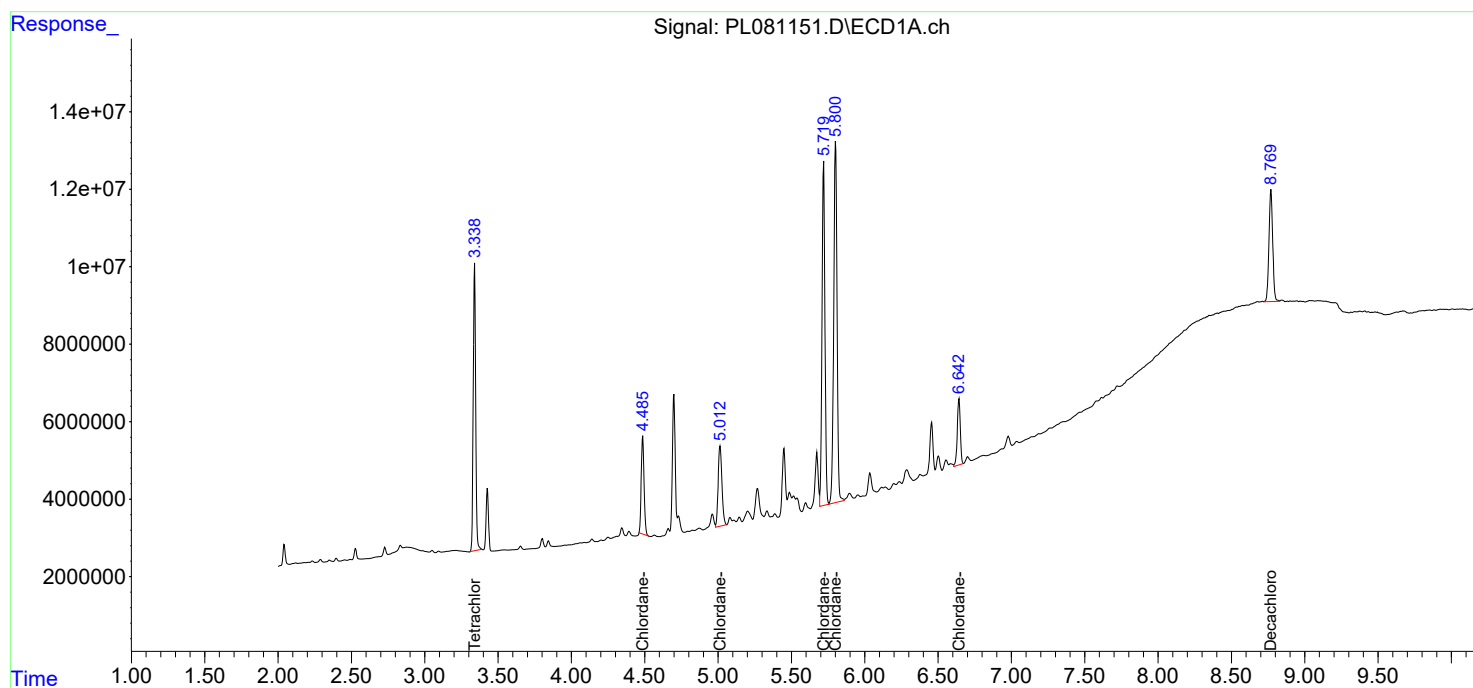


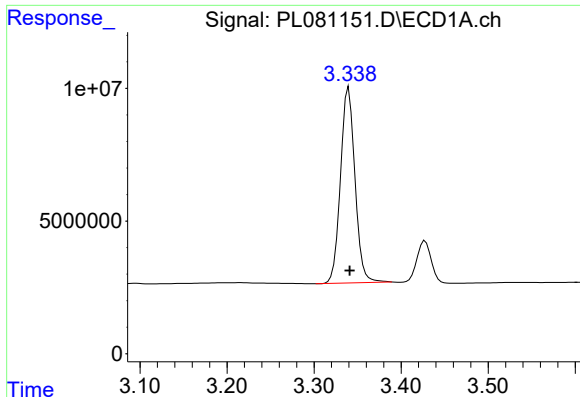

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 85223011
Conc: 54.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

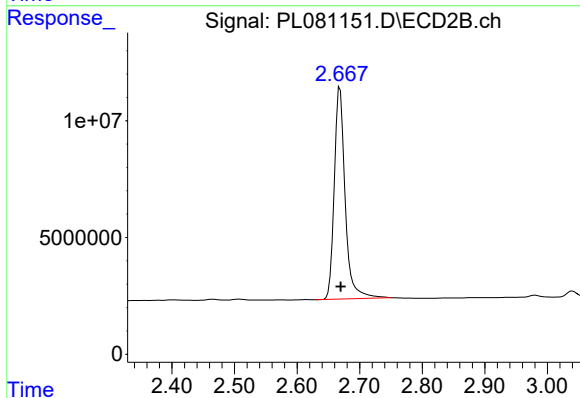


#1 Tetrachloro-m-xylene

R.T.: 2.668 min
Delta R.T.: -0.001 min
Response: 110201863
Conc: 52.48 ng/ml

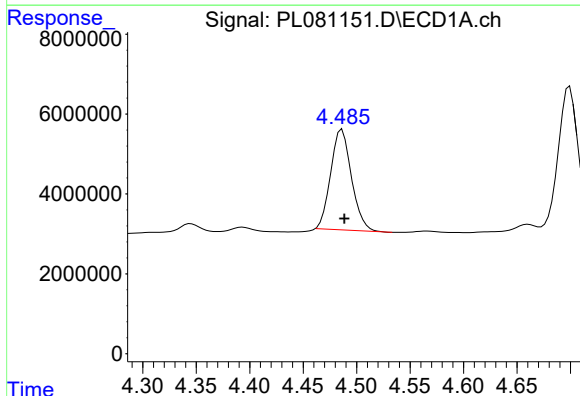


#23 Chlordane-1

R.T.: 4.486 min
Delta R.T.: -0.002 min
Response: 33926618
Conc: 540.42 ng/ml

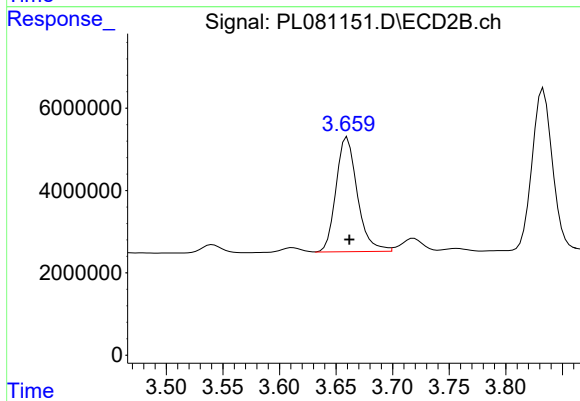

#23 Chlordane-1


R.T.: 3.660 min
Delta R.T.: -0.002 min
Response: 36477980
Conc: 523.45 ng/ml

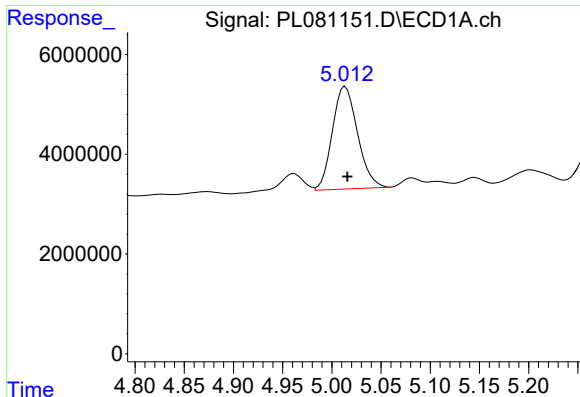

#24 Chlordane-2


R.T.: 5.014 min
Delta R.T.: -0.002 min
Response: 36565074
Conc: 576.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

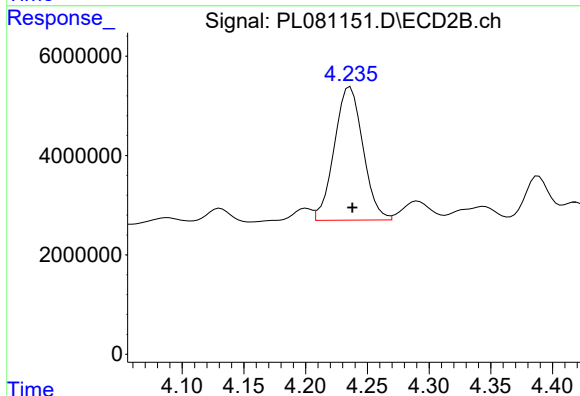


#24 Chlordane-2

R.T.: 4.236 min
Delta R.T.: -0.002 min
Response: 43271231
Conc: 529.80 ng/ml

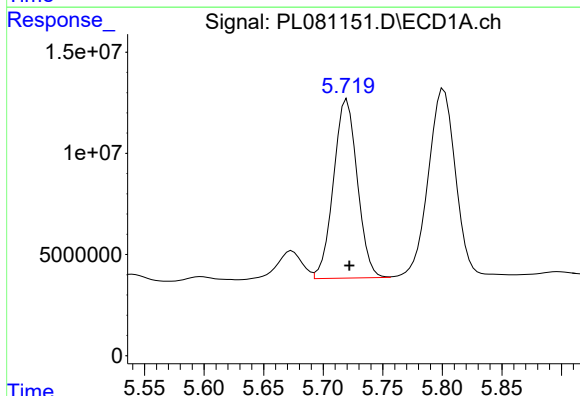


#25 Chlordane-3

R.T.: 5.720 min
Delta R.T.: -0.002 min
Response: 122841982
Conc: 552.09 ng/ml

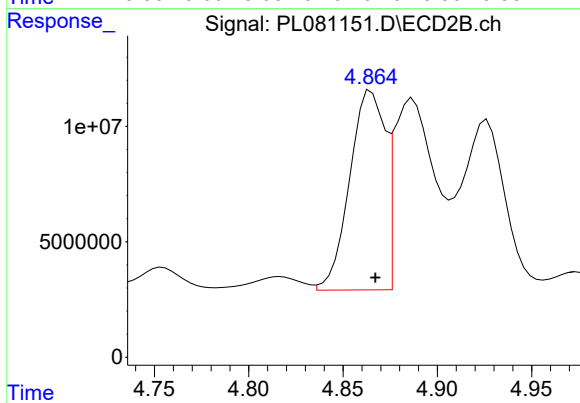

#25 Chlordane-3


R.T.: 4.865 min
Delta R.T.: -0.002 min
Response: 112410388
Conc: 533.74 ng/ml

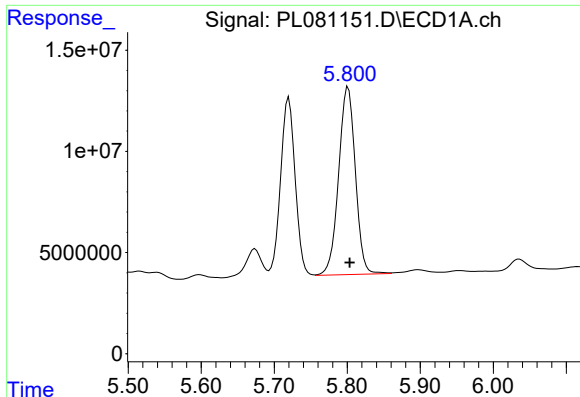

#26 Chlordane-4


R.T.: 5.801 min
Delta R.T.: -0.002 min
Response: 147528411
Conc: 553.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

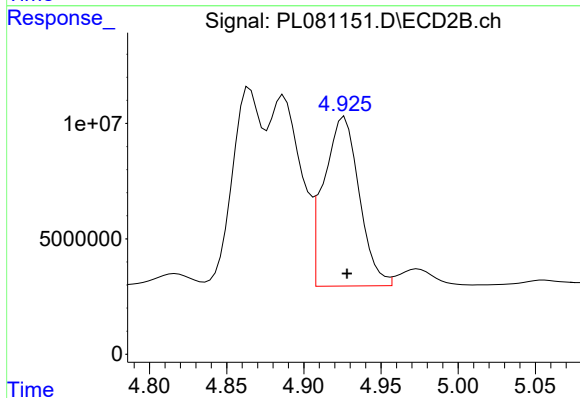


#26 Chlordane-4

R.T.: 4.926 min
Delta R.T.: -0.002 min
Response: 116707588
Conc: 531.31 ng/ml

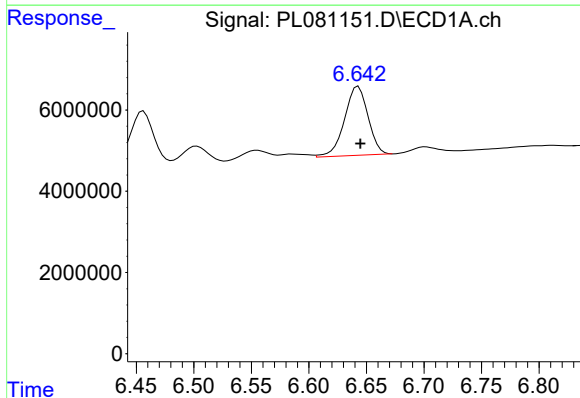


#27 Chlordane-5

R.T.: 6.643 min
Delta R.T.: -0.002 min
Response: 23598622
Conc: 527.64 ng/ml

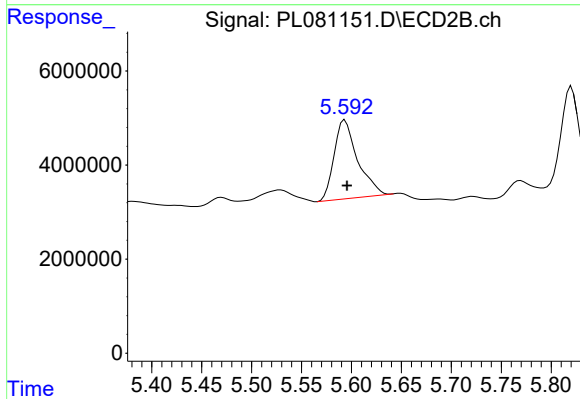

#27 Chlordane-5


R.T.: 5.594 min
Delta R.T.: -0.002 min
Response: 27577676
Conc: 569.59 ng/ml

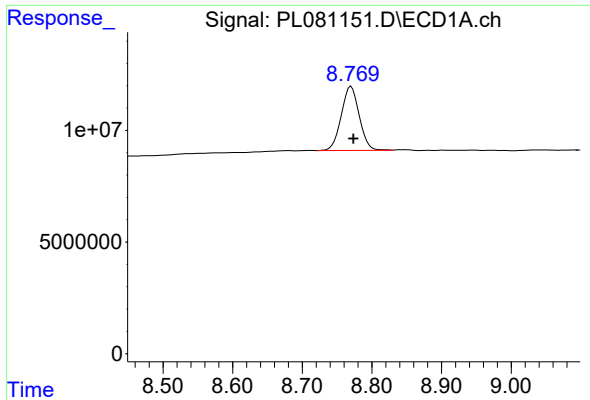

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.003 min
Response: 51606802
Conc: 52.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

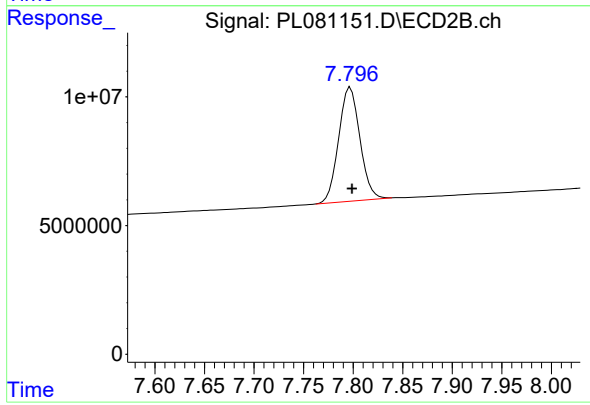

#28 Decachlorobiphenyl

R.T.: 7.797 min
Delta R.T.: -0.002 min
Response: 66582491
Conc: 55.46 ng/ml