

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022824\
 Data File : PL088335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 14:10
 Operator : AR\AJ
 Sample : PB159344BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159344BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/29/2024
 Supervised By : Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 01:21:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.646	2.855	56295604	27131408	20.496	19.345
2) SA Decachlor...	9.318	8.092	48693241	28132587	25.283m	22.094

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022824\
Data File : PL088335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 14:10
Operator : AR\AJ
Sample : PB159344BL
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB159344BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/29/2024
Supervised By : Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 01:21:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

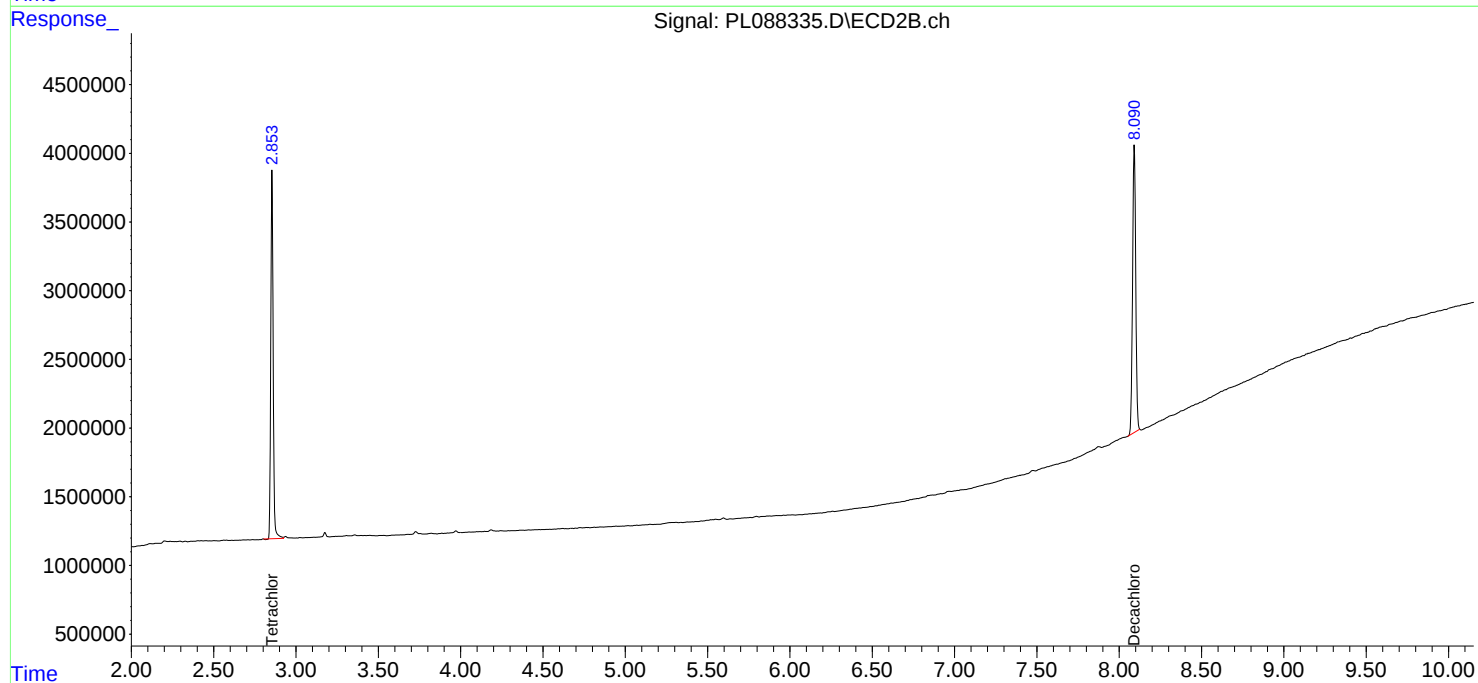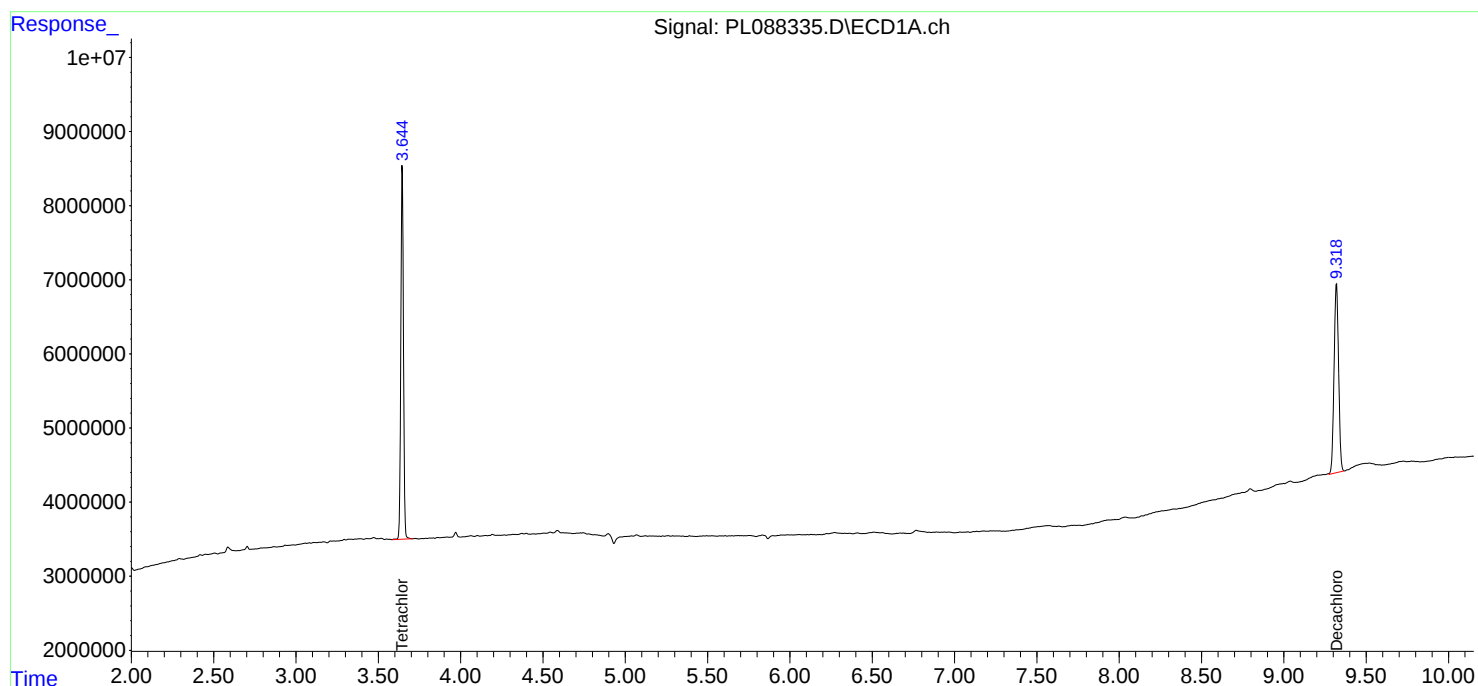

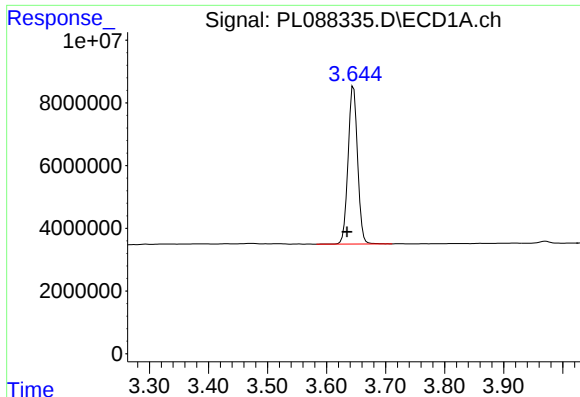


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.011 min
Response: 56295604
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159344BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/29/2024
Supervised By :Ankita Jodhani 02/29/2024

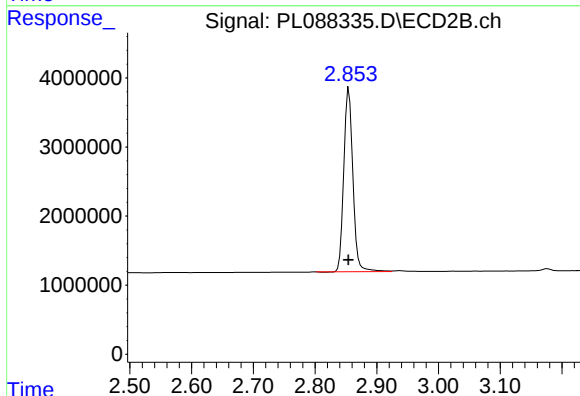


#1 Tetrachloro-m-xylene

R.T.: 2.855 min
Delta R.T.: 0.000 min
Response: 27131408
Conc: 19.34 ng/ml

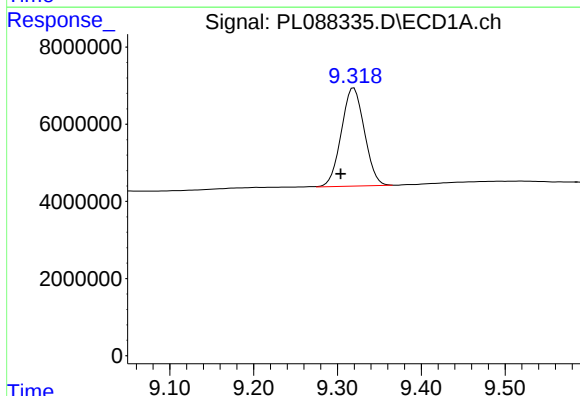

#28 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: 0.014 min
Response: 48693241
Conc: 25.28 ng/ml m

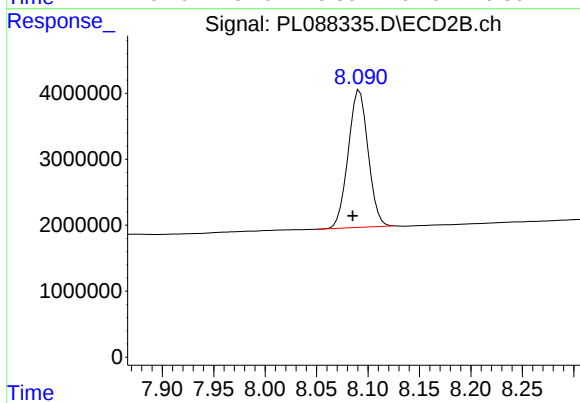

#28 Decachlorobiphenyl

R.T.: 8.092 min
Delta R.T.: 0.007 min
Response: 28132587
Conc: 22.09 ng/ml