

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022824\
 Data File : PL088340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 15:33
 Operator : AR\AJ
 Sample : P1611-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-022724

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/29/2024
 Supervised By : Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 01:22:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.853	24634620	14095597	8.969m	10.050m
28) SA Decachlor...	9.304	8.084	31810861	16200710	16.517	12.724

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022824\
Data File : PL088340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 15:33
Operator : AR\AJ
Sample : P1611-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-05-022724


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/29/2024
Supervised By : Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 01:22:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

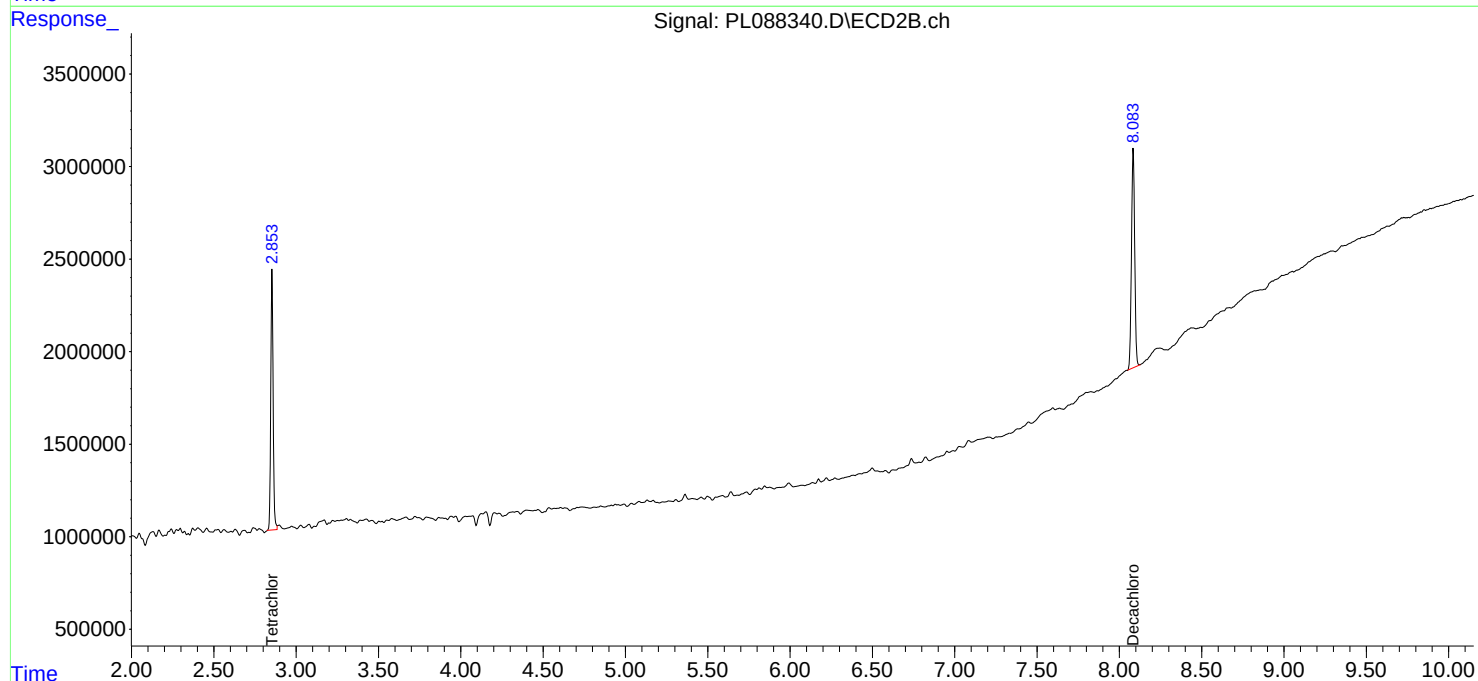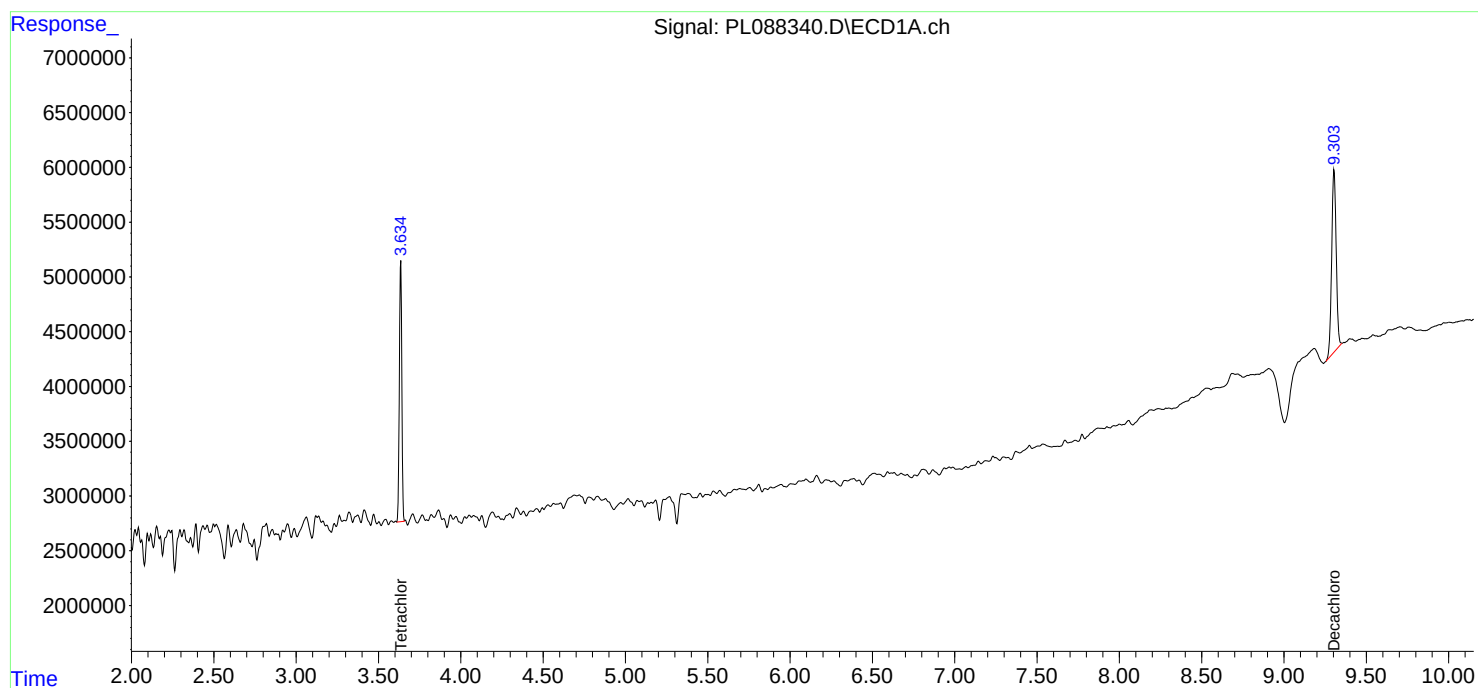

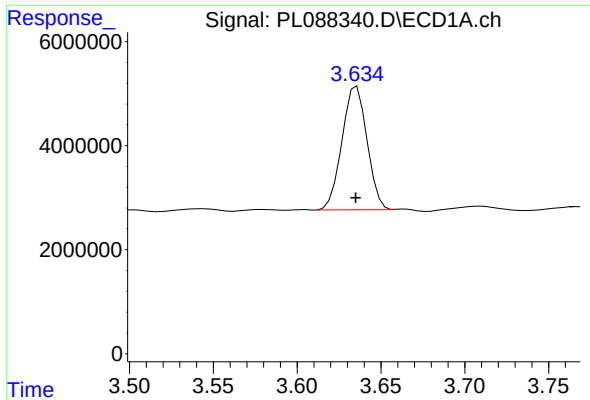


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 24634620
Conc: 8.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-022724


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/29/2024
Supervised By :Ankita Jodhani 02/29/2024

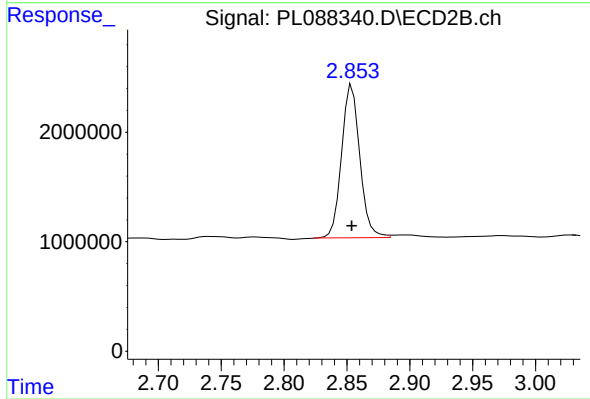


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: -0.001 min
Response: 14095597
Conc: 10.05 ng/ml m

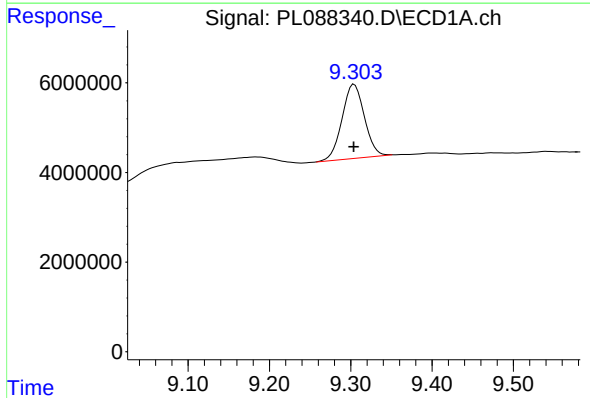

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: 0.000 min
Response: 31810861
Conc: 16.52 ng/ml

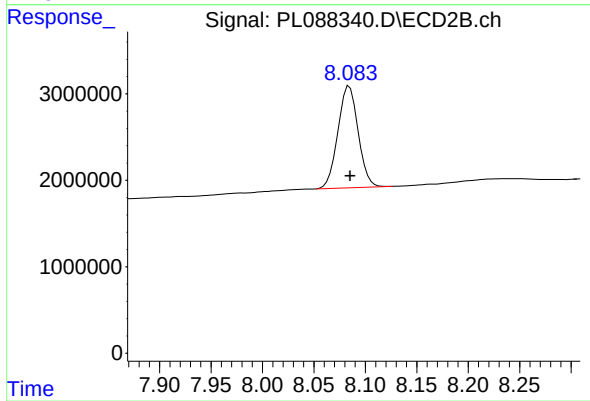

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 16200710
Conc: 12.72 ng/ml