

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022924\
 Data File : PL088362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Feb 2024 17:08
 Operator : AR\AJ
 Sample : P1628-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/01/2024
 Supervised By :Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:44:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.853	39250302	21329927	14.290m	15.208
28) SA Decachlor...	9.302	8.080	41605703	25900955	21.603	20.342m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022924\
Data File : PL088362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Feb 2024 17:08
Operator : AR\AJ
Sample : P1628-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2024
Supervised By :Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:44:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

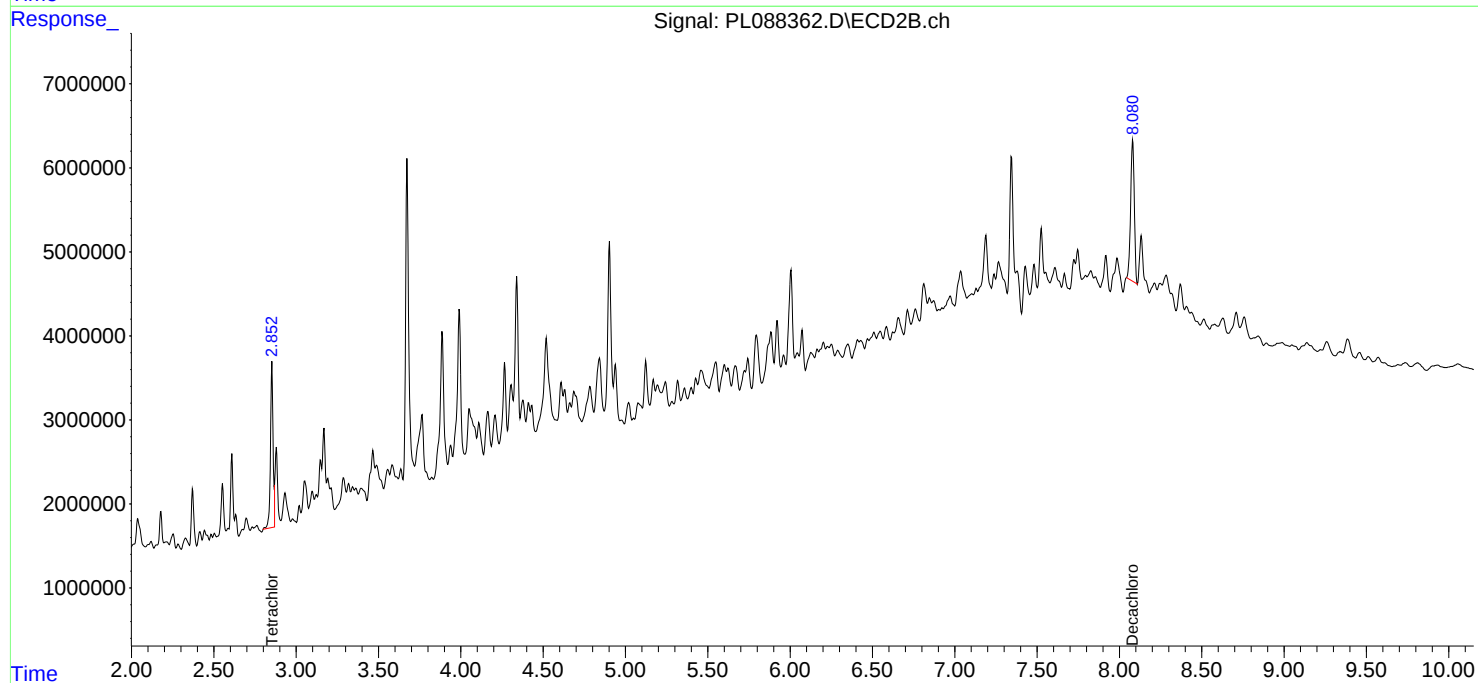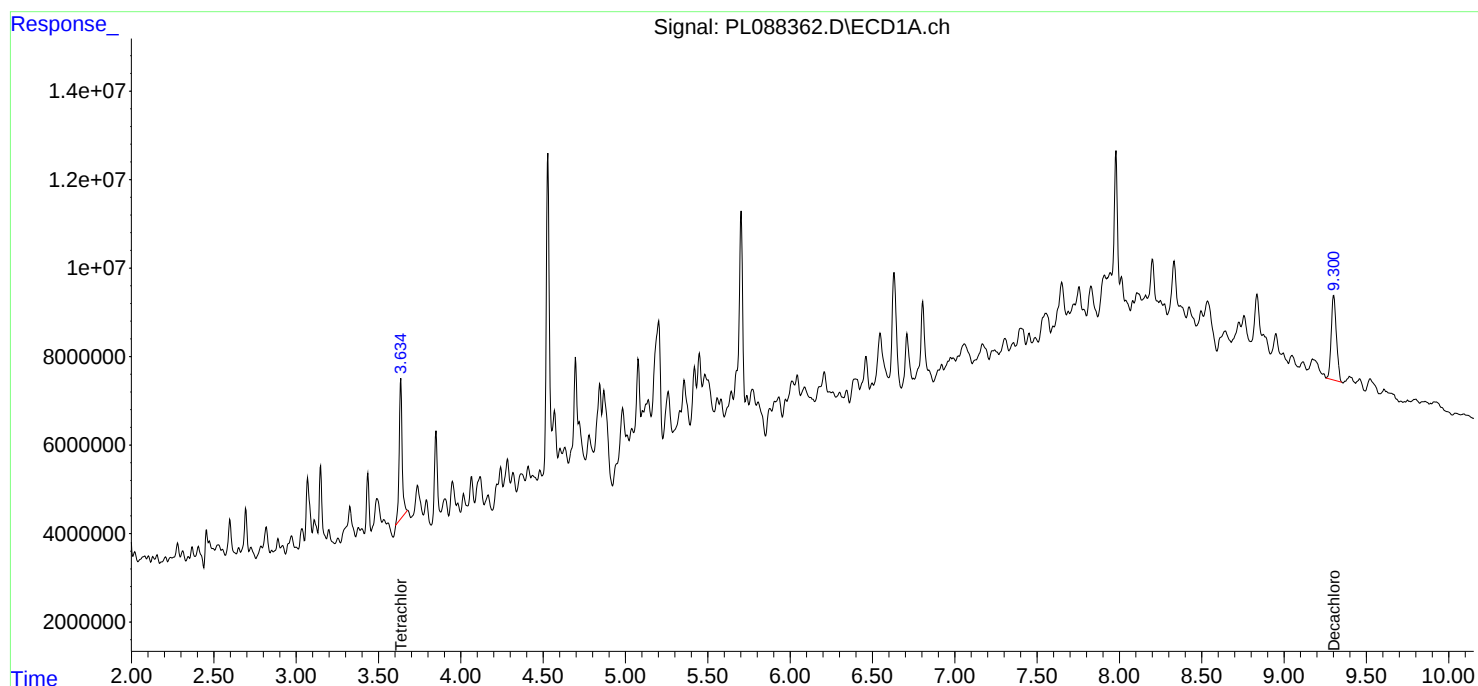

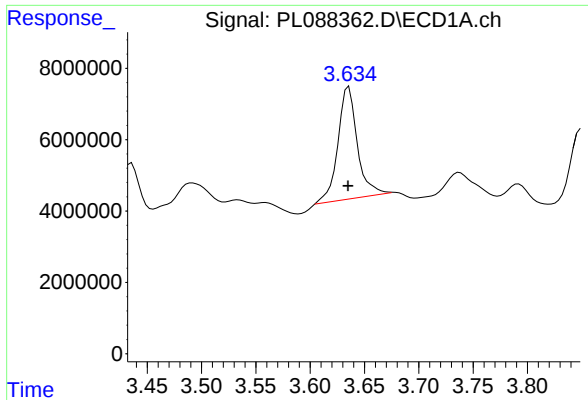


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 39250302
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/01/2024
Supervised By :Ankita Jodhani 03/01/2024

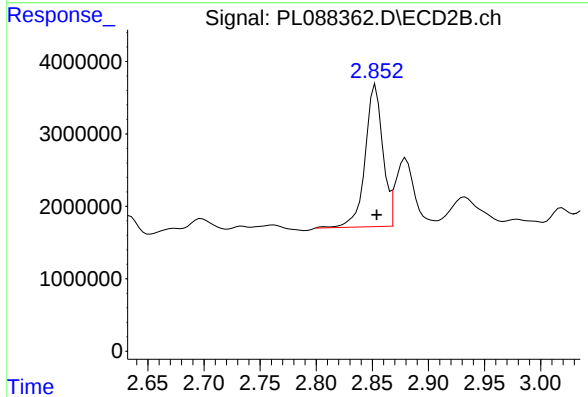


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 21329927
Conc: 15.21 ng/ml

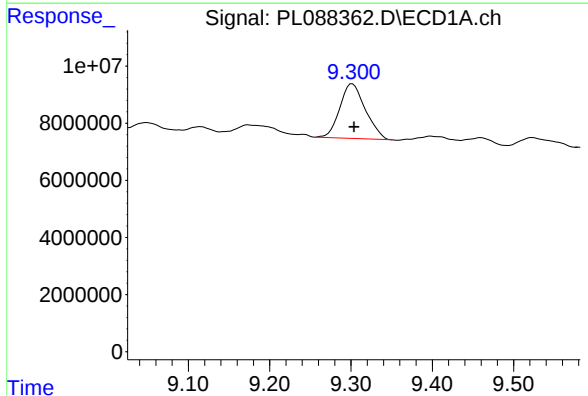

#28 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: -0.002 min
Response: 41605703
Conc: 21.60 ng/ml

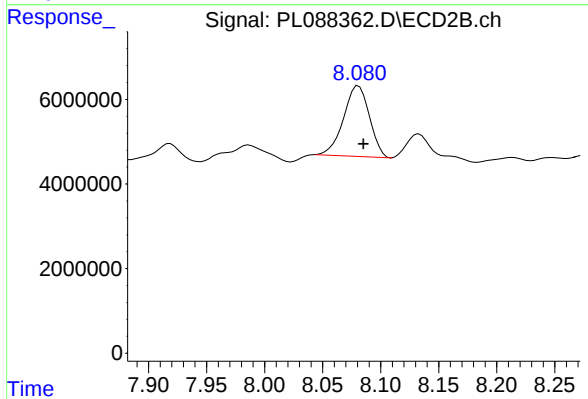

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: -0.006 min
Response: 25900955
Conc: 20.34 ng/ml m