

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030119\
 Data File : PL045308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2019 12:40
 Operator : AJ\SJ
 Sample : K1650-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-7(3.5-4.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 22:08:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	93457480	29971344	13.585	13.995
28)	SA Decachlor...	8.046	9.039	79651949	24474370	9.519	10.711
Target Compounds							
10)	B gamma-Chl...	5.261	6.088	-56265	2535680	N.D.	0.945
11)	B alpha-Chl...	0.000	6.162	0	4275460	N.D.	1.585 #
25)	Chlordane-3	5.261	6.088	-56265	2535680	N.D.	6.508
26)	Chlordane-4	0.000	6.162	0	4275460	N.D.	9.139 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030119\
Data File : PL045308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2019 12:40
Operator : AJ\SJ
Sample : K1650-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-7(3.5-4.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 22:08:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

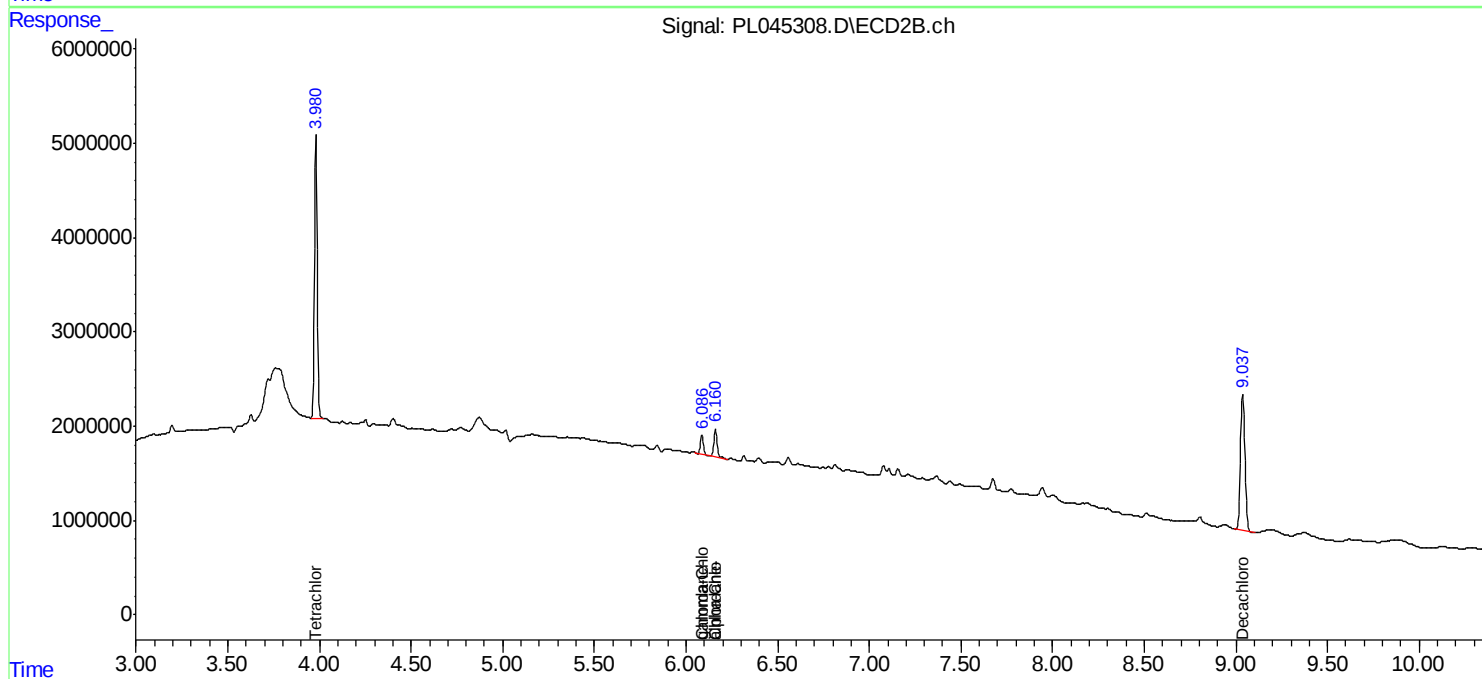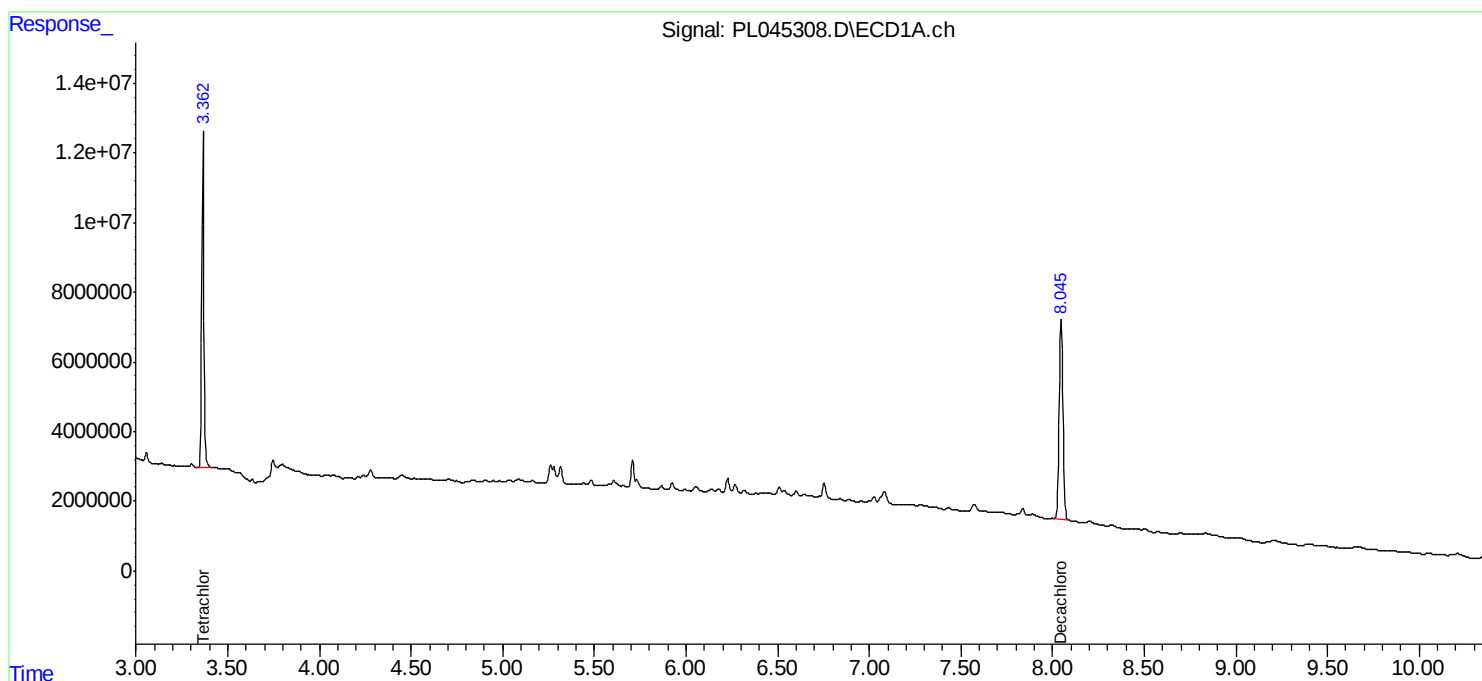


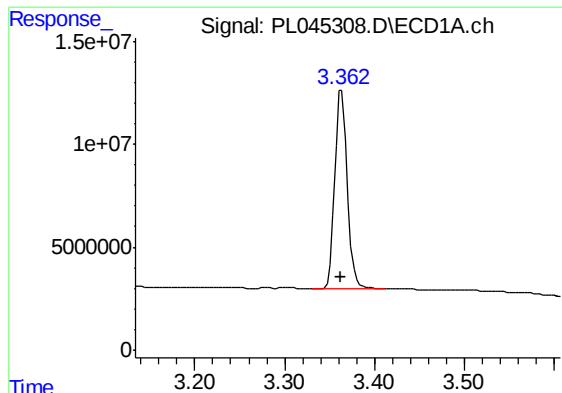

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 93457480
Conc: 13.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-7(3.5-4.5)

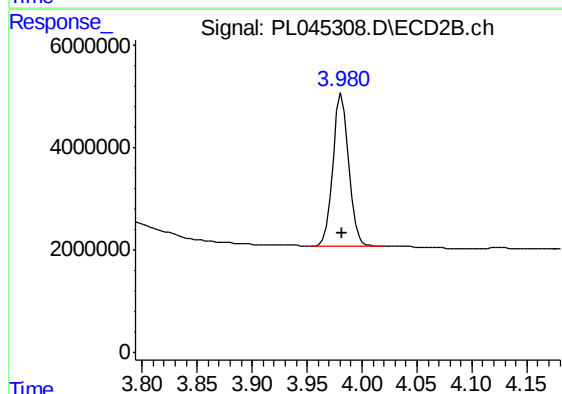


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 29971344
Conc: 14.00 ng/ml

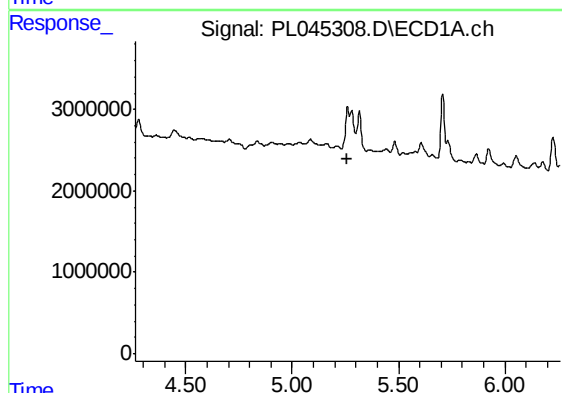


#10 gamma-Chlordane

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: -56265
Conc: N.D.

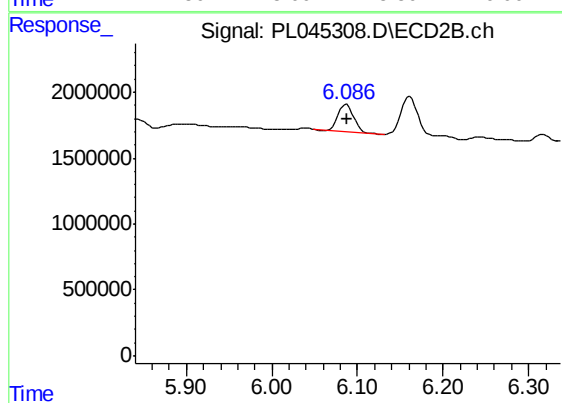

#10 gamma-Chlordane


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 2535680
Conc: 0.95 ng/ml

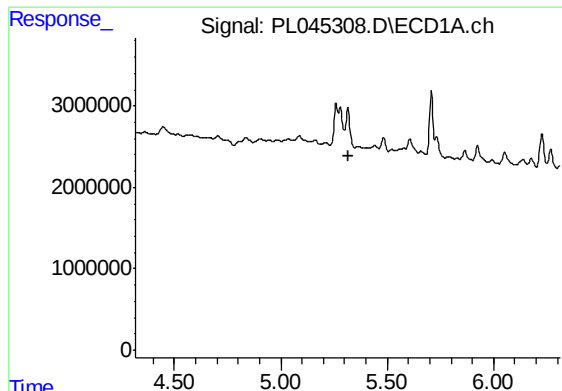

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B-7(3.5-4.5)

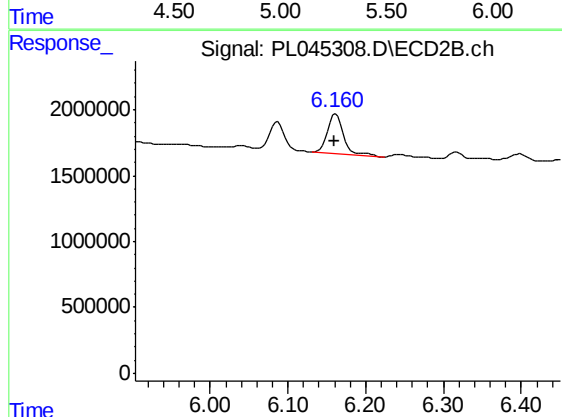


#11 alpha-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 4275460
Conc: 1.58 ng/ml

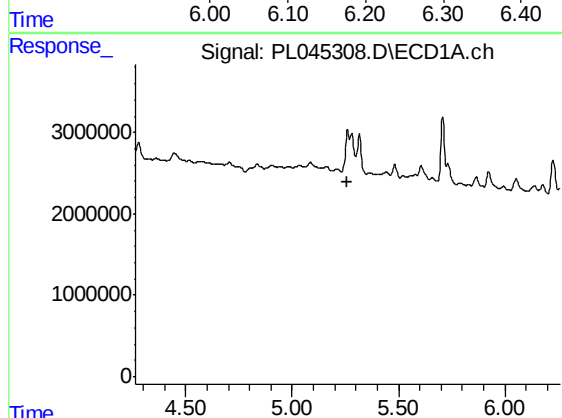


#25 Chlordane-3

R.T.: 5.261 min
Delta R.T.: -0.001 min
Response: -56265
Conc: N.D.

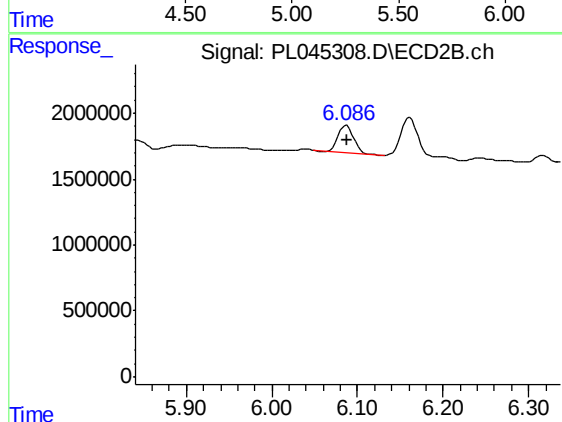

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: -0.001 min
Response: 2535680
Conc: 6.51 ng/ml

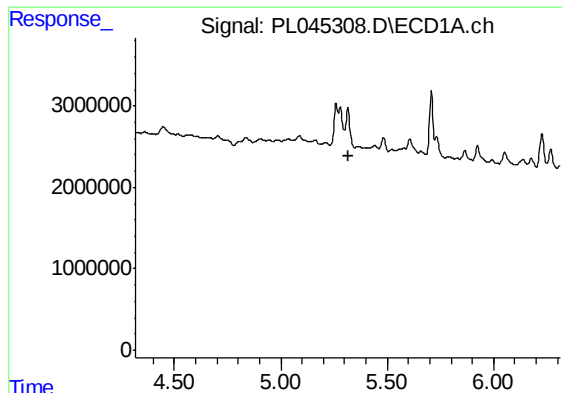

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B-7(3.5-4.5)

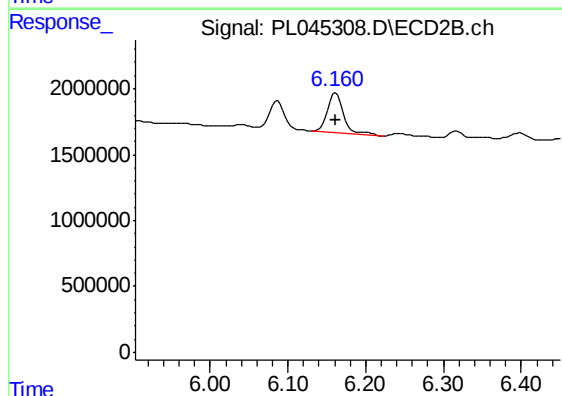


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 4275460
Conc: 9.14 ng/ml

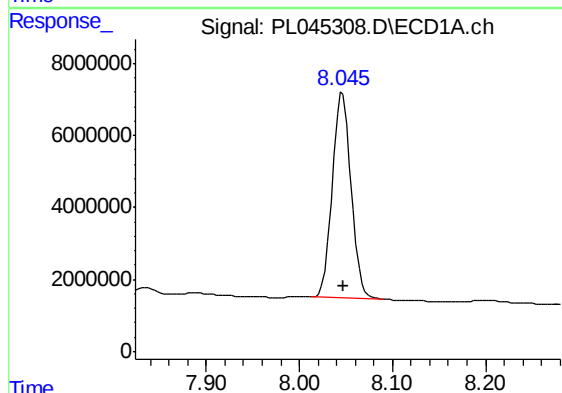

#28 Decachlorobiphenyl

R.T.: 8.046 min
Delta R.T.: 0.000 min
Response: 79651949
Conc: 9.52 ng/ml

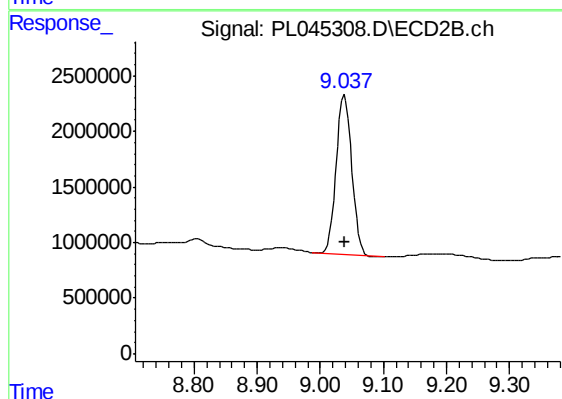

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 24474370
Conc: 10.71 ng/ml