

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030119\
 Data File : PL045310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2019 13:09
 Operator : AJ\SJ
 Sample : K1650-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-5(9-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 22:09:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	143.1E6	44066736	20.805	20.577
28)	SA Decachlor...	8.047	9.037	118.9E6	38360759	14.209	16.789
Target Compounds							
3)	MA gamma-BHC...	4.081	0.000	4900283	0	0.485	N.D. #
7)	B delta-BHC	0.000	5.016f	0	1447058	N.D.	0.673 #
10)	B gamma-Chl...	5.261	6.088	22059184	10894786	2.254	4.061 #
11)	B alpha-Chl...	5.317	6.161	14634664	13001363	1.509	4.819 #
23)	Chlordane-1	4.214	0.000	8489856	0	25.197	N.D. #
25)	Chlordane-3	5.261	6.088	22059184	10894786	19.232	27.962 #
26)	Chlordane-4	5.317	6.161	14634664	13001363	13.806	27.791 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030119\
Data File : PL045310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2019 13:09
Operator : AJ\SJ
Sample : K1650-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
B-5(9-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 22:09:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

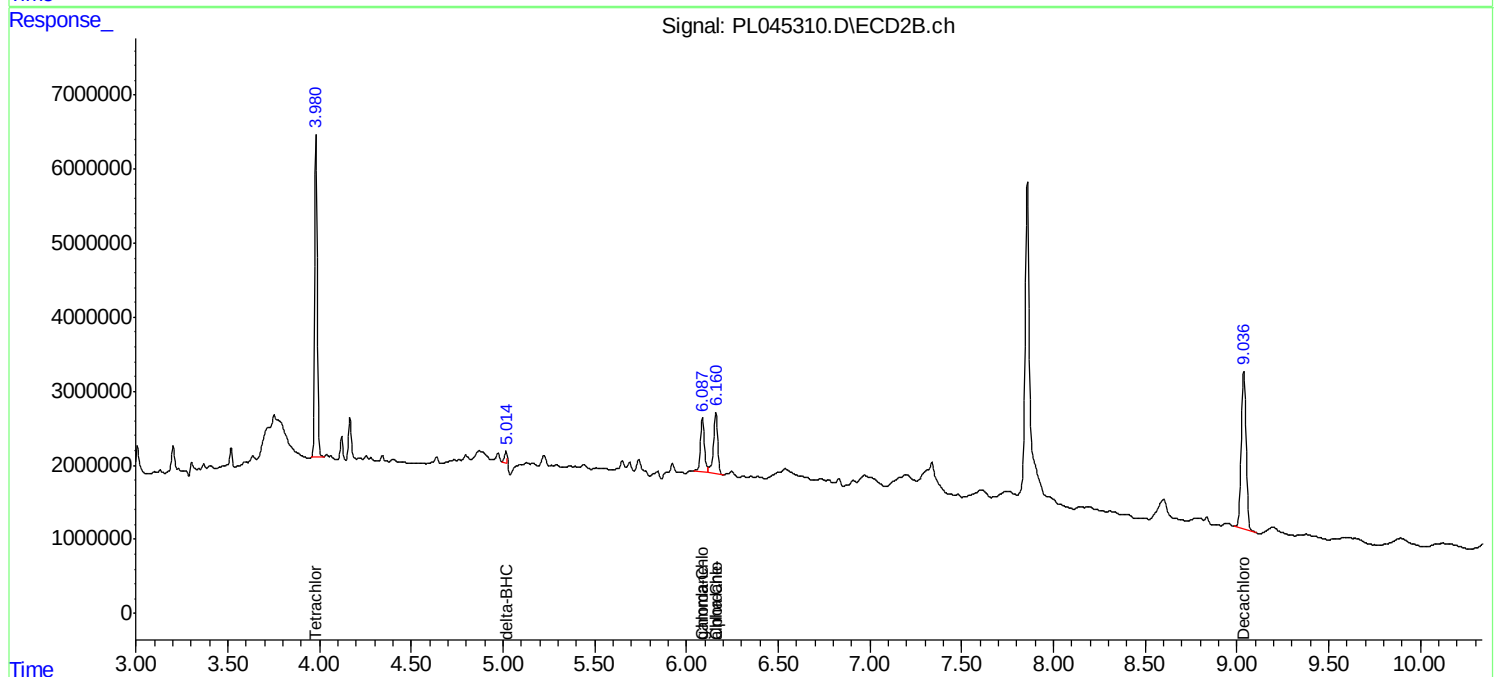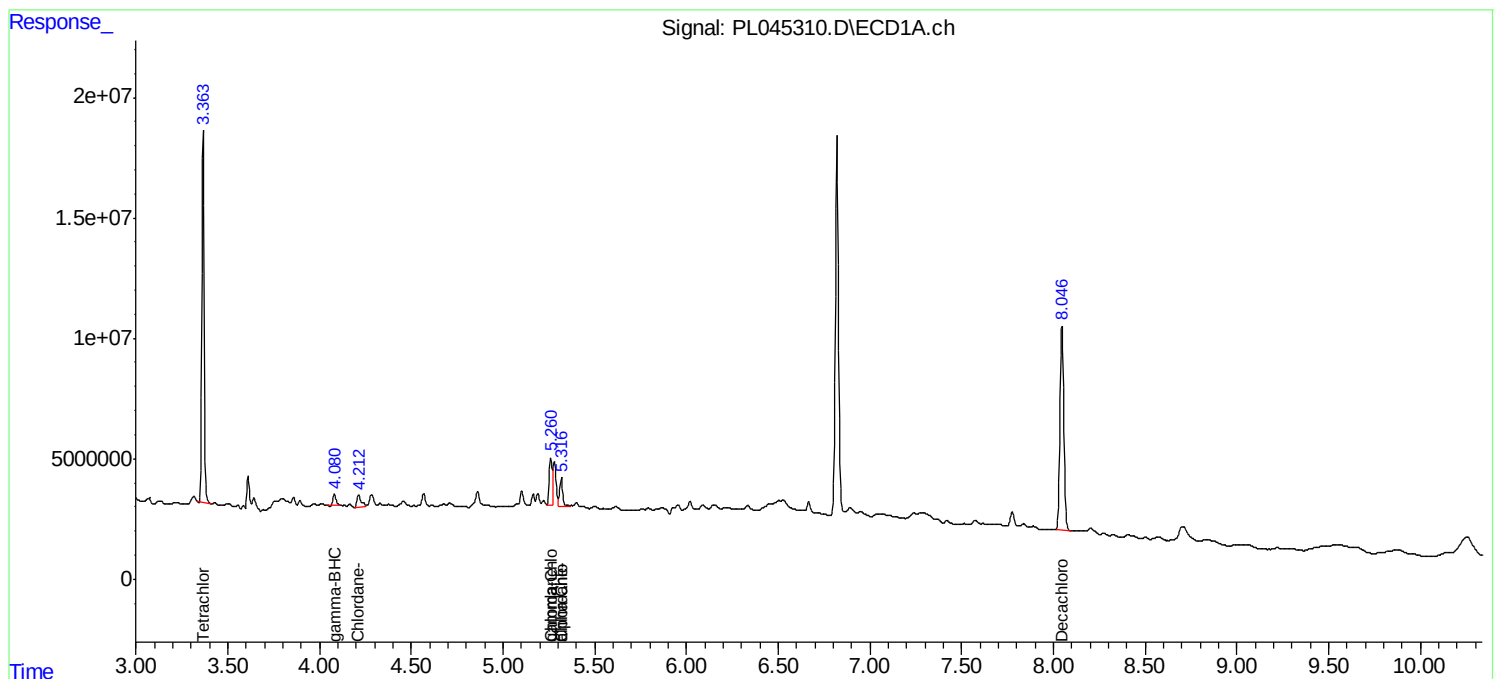


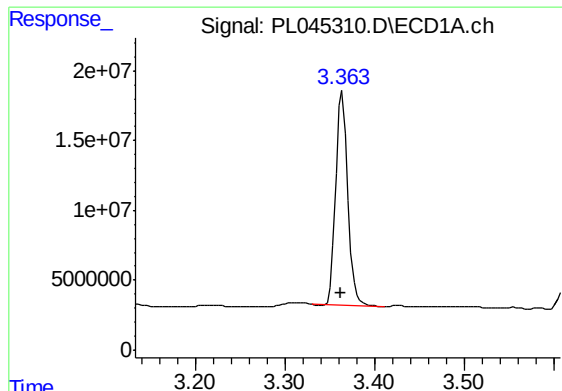

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.001 min
Response: 143122900
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-5(9-10)

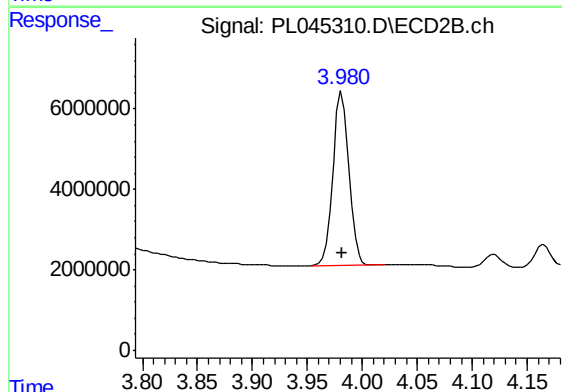


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 44066736
Conc: 20.58 ng/ml

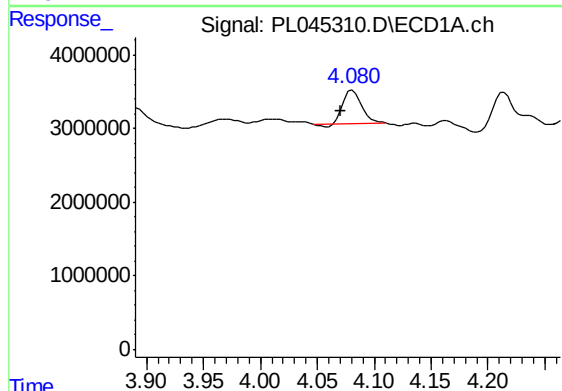


#3 gamma-BHC (Lindane)

R.T.: 4.081 min
Delta R.T.: 0.010 min
Response: 4900283
Conc: 0.48 ng/ml

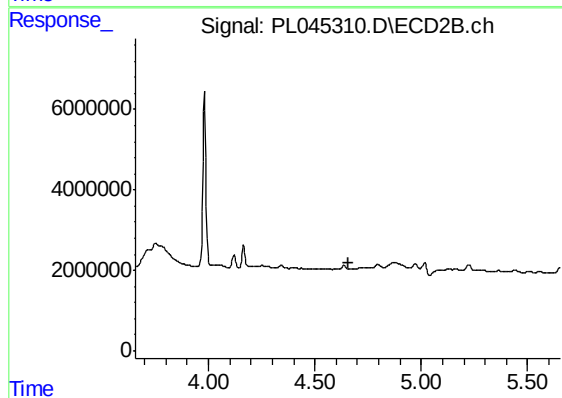

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

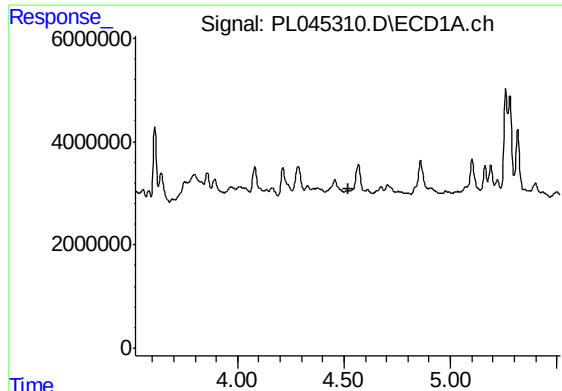

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B-5(9-10)

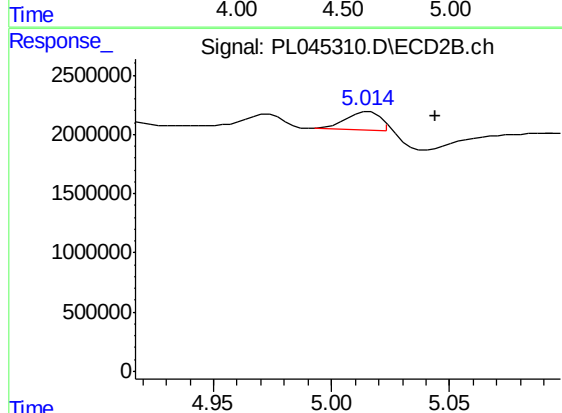


#7 delta-BHC

R.T.: 5.016 min
Delta R.T.: -0.028 min
Response: 1447058
Conc: 0.67 ng/ml

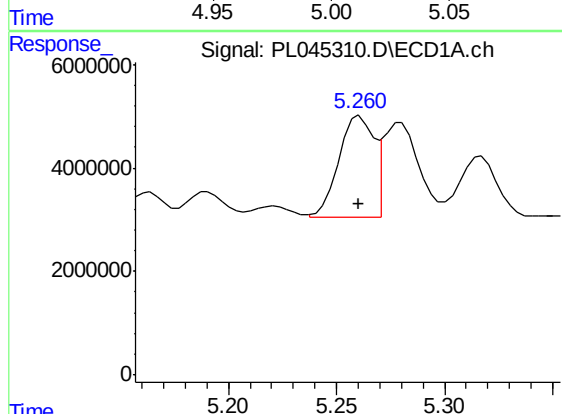


#10 gamma-Chlordane

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 22059184
Conc: 2.25 ng/ml

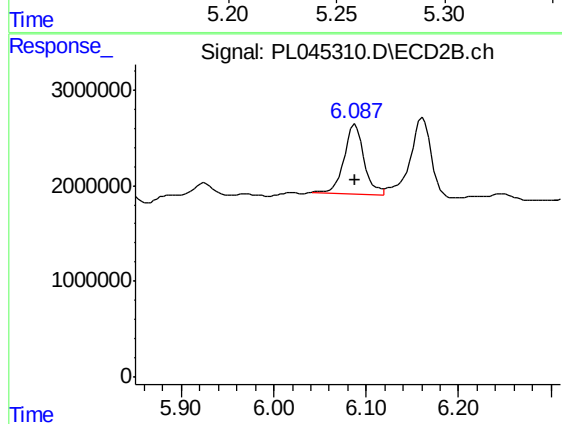

#10 gamma-Chlordane


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 10894786
Conc: 4.06 ng/ml

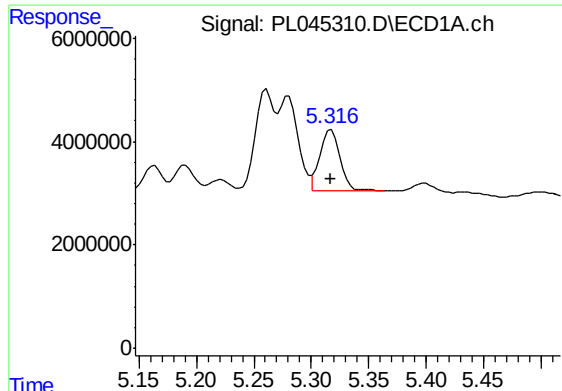

#11 alpha-Chlordane


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 14634664
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-5(9-10)

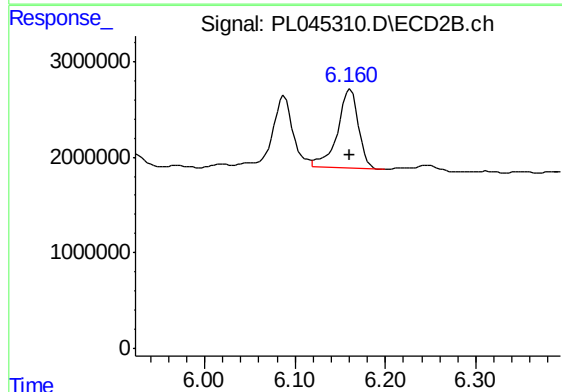


#11 alpha-Chlordane

R.T.: 6.161 min
Delta R.T.: 0.001 min
Response: 13001363
Conc: 4.82 ng/ml

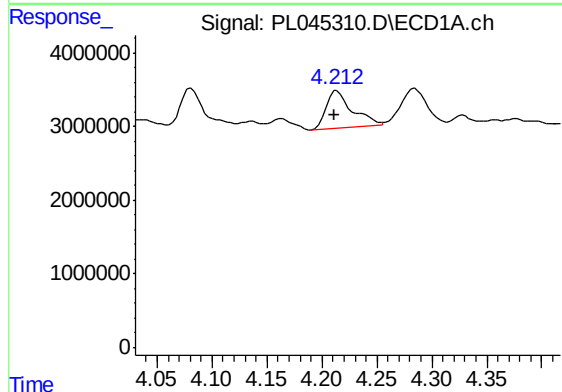


#23 Chlordane-1

R.T.: 4.214 min
Delta R.T.: 0.002 min
Response: 8489856
Conc: 25.20 ng/ml

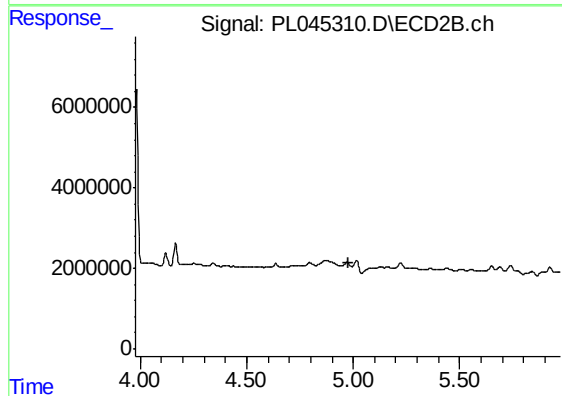

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

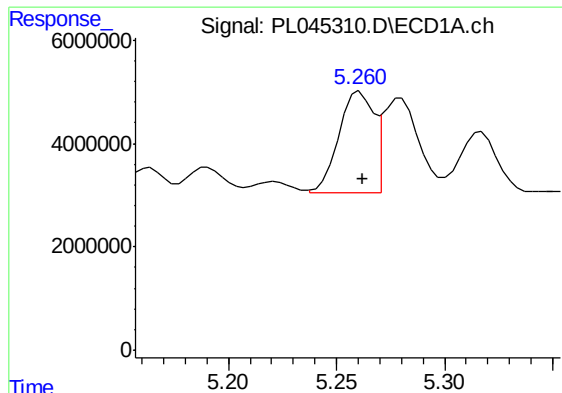

#25 Chlordane-3


R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 22059184
Conc: 19.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-5(9-10)

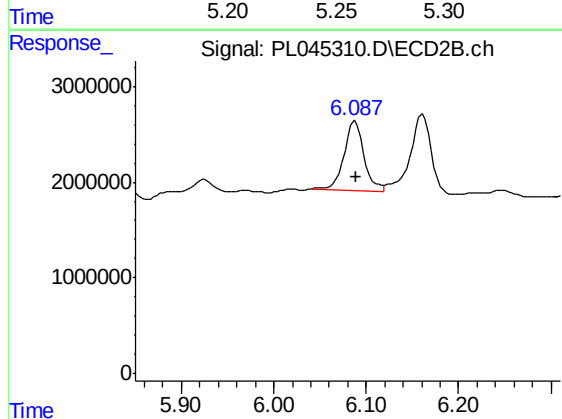


#25 Chlordane-3

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 10894786
Conc: 27.96 ng/ml

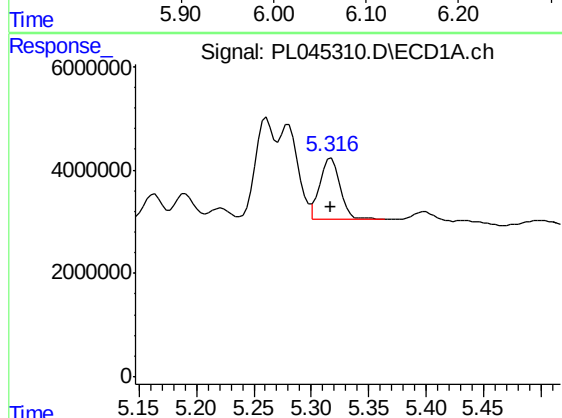


#26 Chlordane-4

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 14634664
Conc: 13.81 ng/ml

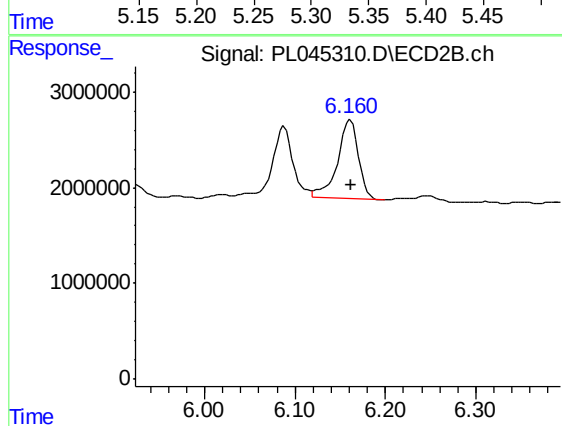

#26 Chlordane-4


R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 13001363
Conc: 27.79 ng/ml

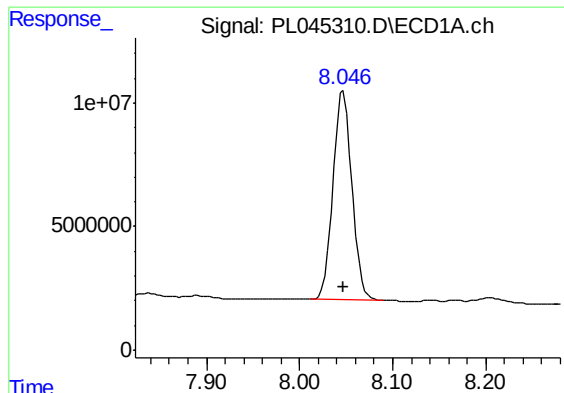

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 118893347
Conc: 14.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-5(9-10)

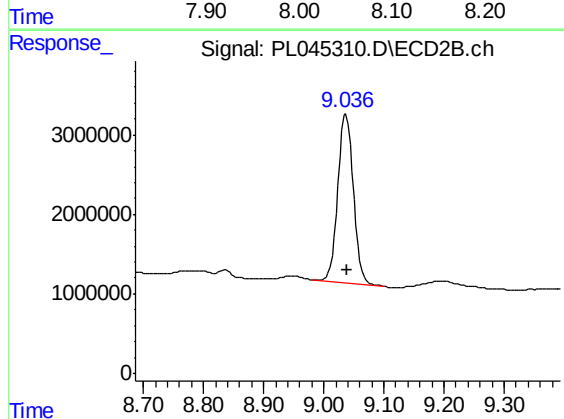

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 38360759
Conc: 16.79 ng/ml