

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030121\
 Data File : PL064996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2021 12:54
 Operator : AR\AJ
 Sample : M1506-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-022621

Manual Integrations
 APPROVED

Ankita
 3/2/2021 8:43:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 15:17:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.100	44017597	37771873	15.645	17.485
28)	SA Decachlor...	8.154	9.264	37128493	33620727	16.510	17.701
Target Compounds							
10)	B gamma-Chl...	5.353	6.248	9024287	18888399	2.574m	8.173 #
11)	B alpha-Chl...	5.410	6.319	18894737	39742561	5.455m	17.263m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030121\
Data File : PL064996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2021 12:54
Operator : AR\AJ
Sample : M1506-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OR-03-022621


Manual Integrations
APPROVED

Ankita
3/2/2021 8:43:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 15:17:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

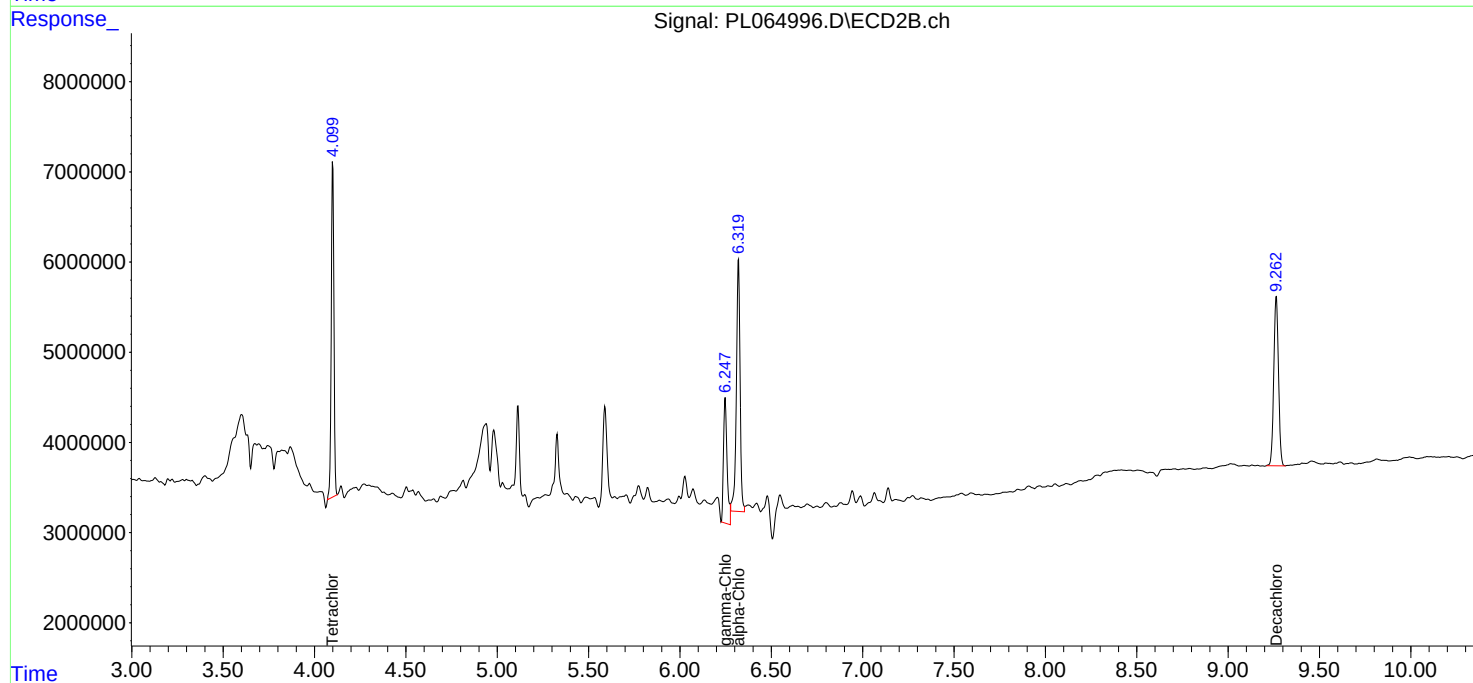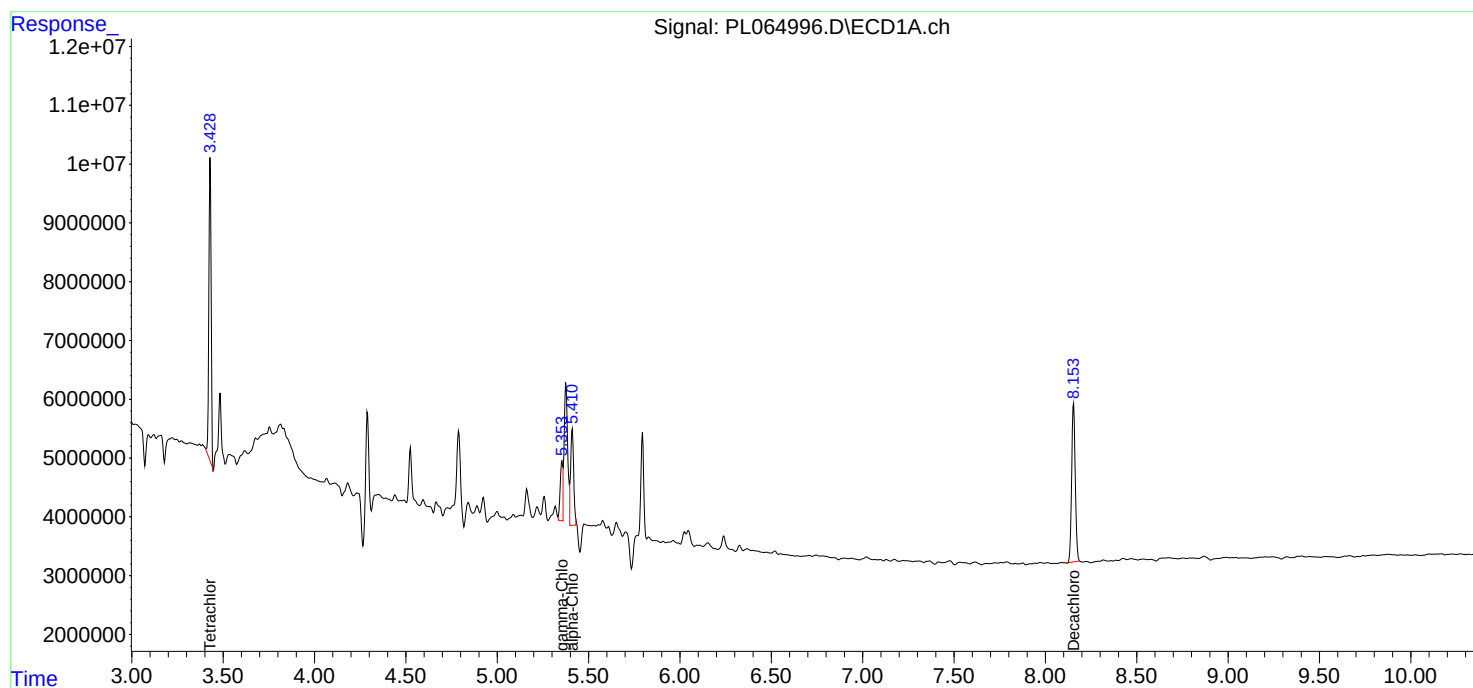

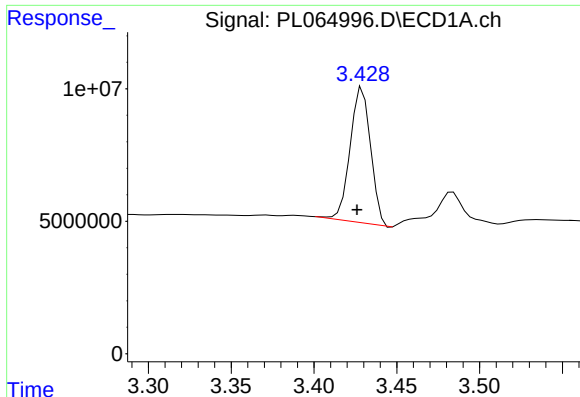


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: 0.003 min
Response: 44017597
Conc: 15.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-022621


Manual Integrations
APPROVED

Ankita
3/2/2021 8:43:34 AM

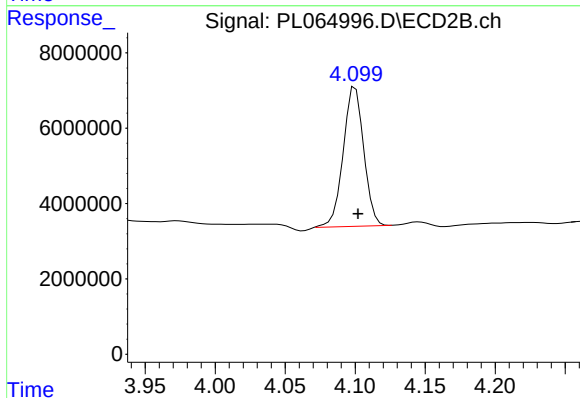


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.002 min
Response: 37771873
Conc: 17.49 ng/ml

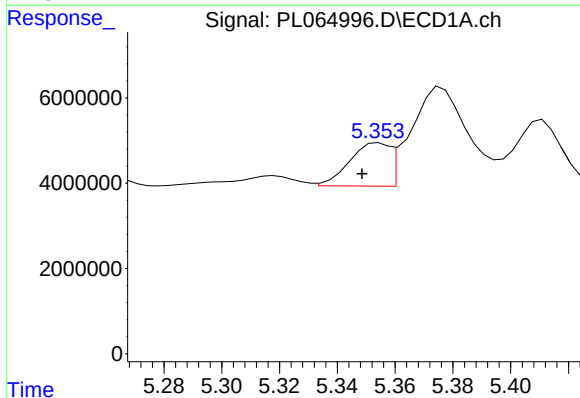


#10 gamma-Chlordane

R.T.: 5.353 min
Delta R.T.: 0.005 min
Response: 9024287
Conc: 2.57 ng/ml m

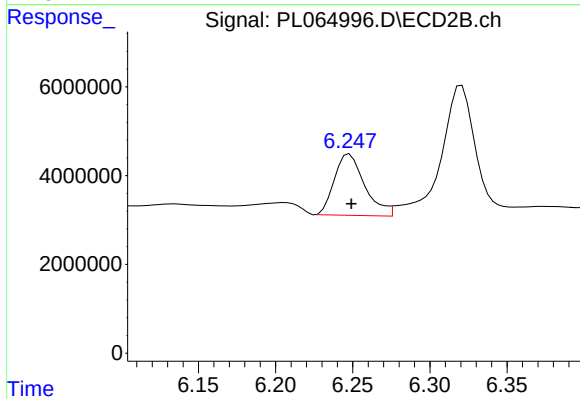

#10 gamma-Chlordane

R.T.: 6.248 min
Delta R.T.: -0.001 min
Response: 18888399
Conc: 8.17 ng/ml

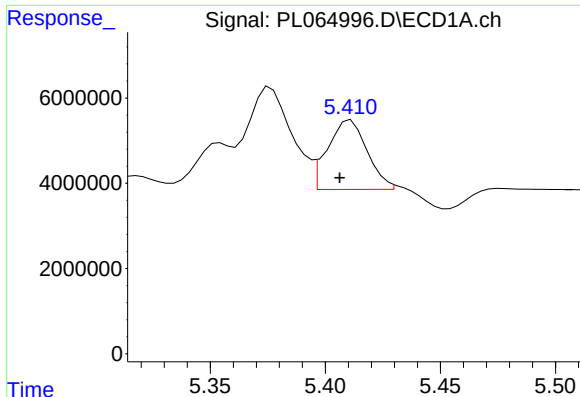


#11 alpha-Chlordane

R.T.: 5.410 min
Delta R.T.: 0.003 min
Response: 18894737
Conc: 5.46 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-022621


Manual Integrations
APPROVED

Ankita
3/2/2021 8:43:34 AM

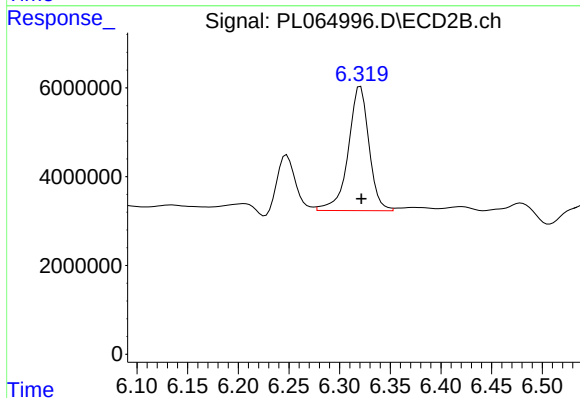


#11 alpha-Chlordane

R.T.: 6.319 min
Delta R.T.: -0.002 min
Response: 39742561
Conc: 17.26 ng/ml m

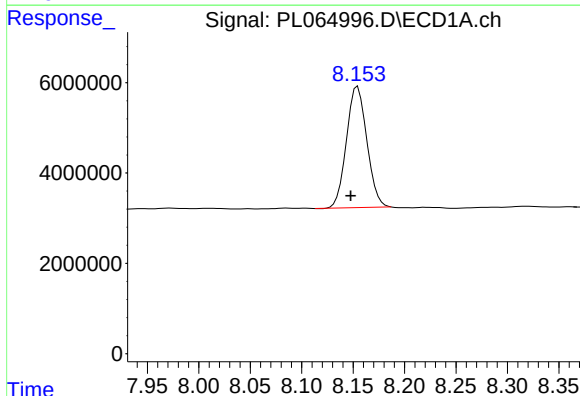

#28 Decachlorobiphenyl

R.T.: 8.154 min
Delta R.T.: 0.007 min
Response: 37128493
Conc: 16.51 ng/ml

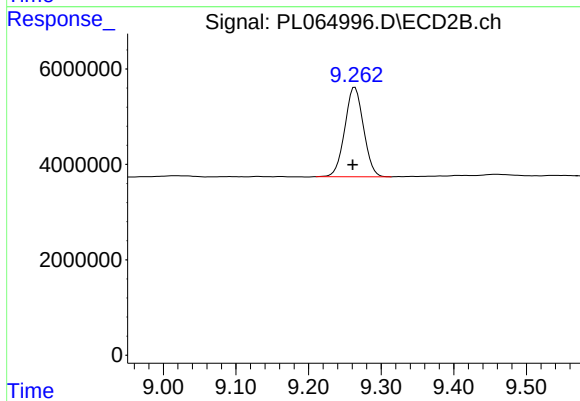

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: 0.003 min
Response: 33620727
Conc: 17.70 ng/ml