

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030122\
 Data File : PL073061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2022 09:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 13:06:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	5.487	6445799	30334387	20.114	20.903
28)	SA Decachlor...	10.436	11.330	10398168	32685538	22.215	20.719
Target Compounds							
2)	A alpha-BHC	5.330f	0.000	28012	0	0.066	N.D. #
5)	MB Aldrin	6.541f	0.000	13162	0	0.030	N.D. #
6)	B beta-BHC	6.146	6.679	164243	353384	0.737	0.392 #
7)	B delta-BHC	0.000	6.955	0	2148809	N.D.	1.135 #
9)	A Endosulfan I	7.507	8.334	22118	59449	0.050	0.037 #
11)	B alpha-Chl...	7.442	0.000	7140	0	0.015	N.D. #
13)	MA Dieldrin	7.761f	0.000	29644	0	0.066	N.D. #
20)	A Methoxychlor	9.086f	0.000	24986	0	0.100	N.D. #
21)	B Endrin ke...	9.323	0.000	9356	0	0.019	N.D. #
24)	Chlordane-2	6.665	0.000	6868	0	0.346	N.D. #
26)	Chlordane-4	7.442	0.000	7140	0	0.135	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030122\
Data File : PL073061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2022 09:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 13:06:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

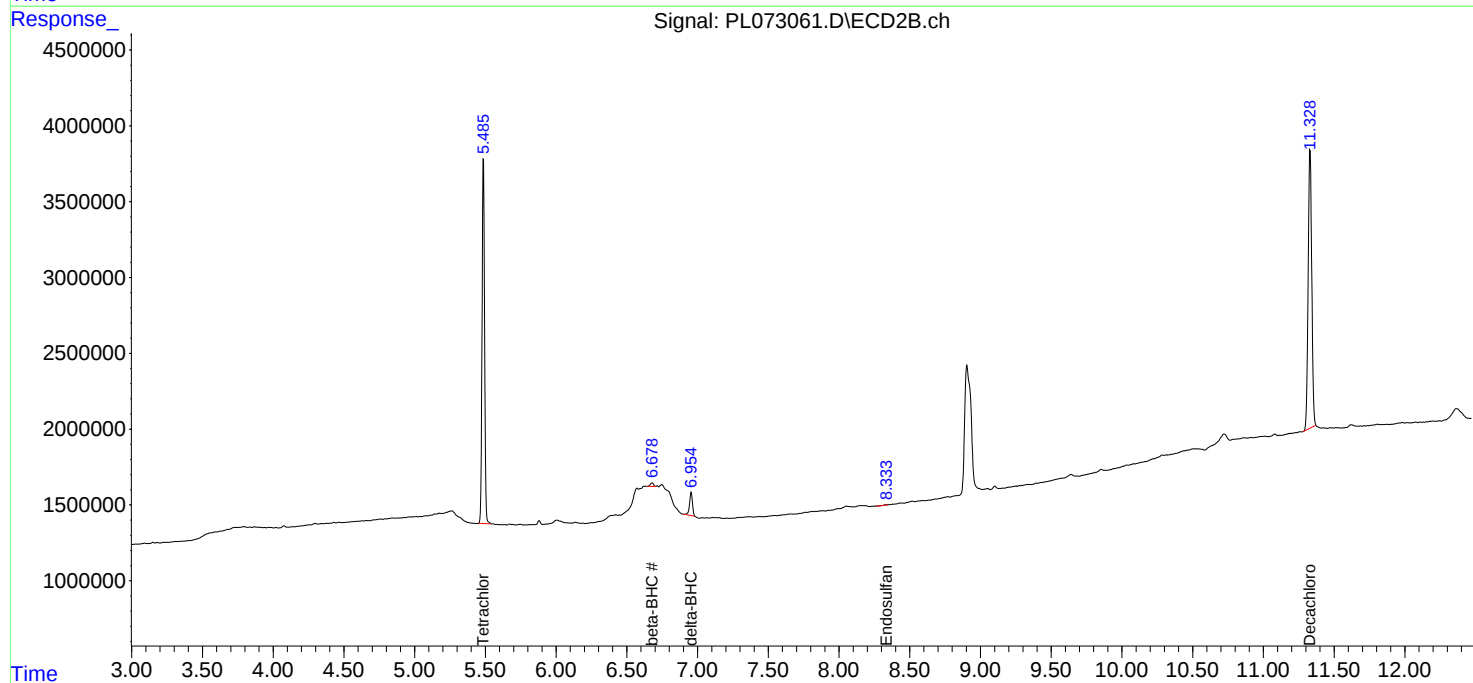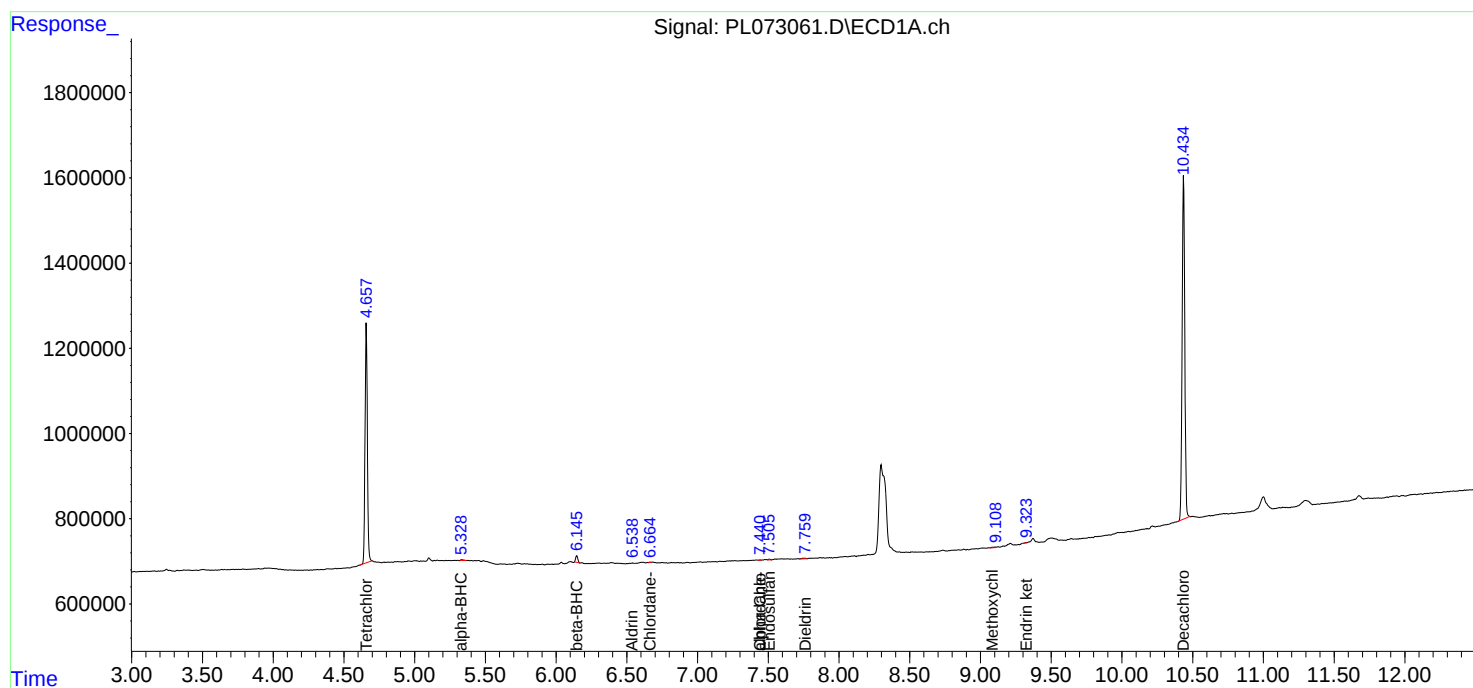


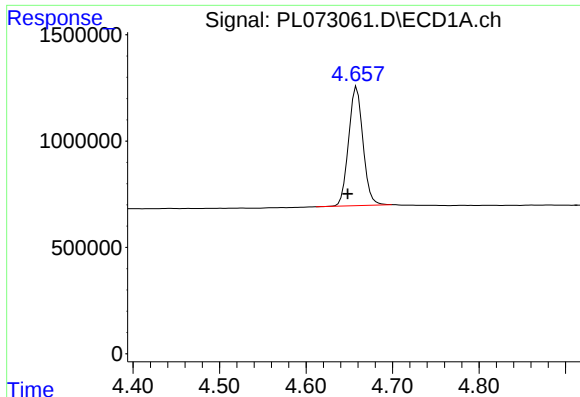

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.011 min
Response: 6445799
Conc: 20.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

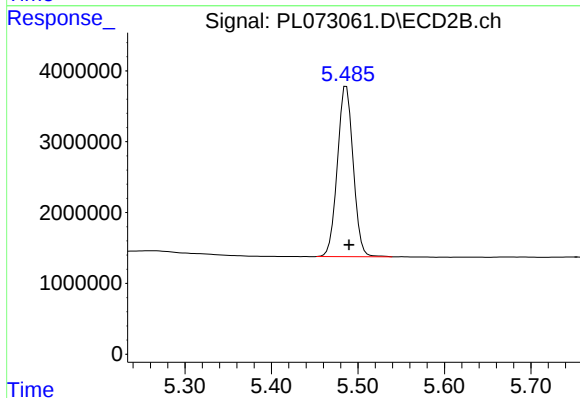


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.003 min
Response: 30334387
Conc: 20.90 ng/ml

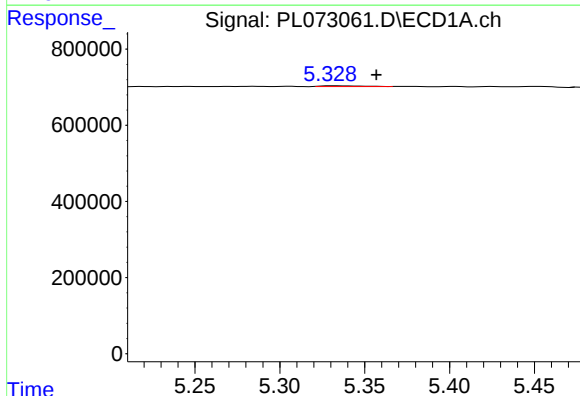


#2 alpha-BHC

R.T.: 5.330 min
Delta R.T.: -0.027 min
Response: 28012
Conc: 0.07 ng/ml

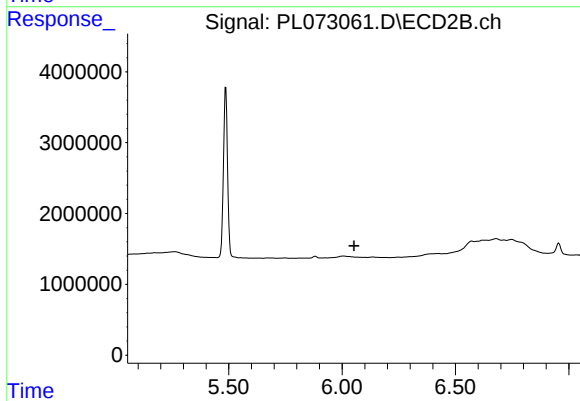

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

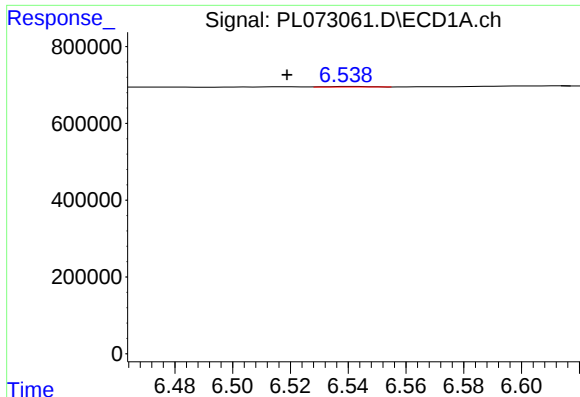

#5 Aldrin


R.T.: 6.541 min
Delta R.T.: 0.022 min
Response: 13162
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

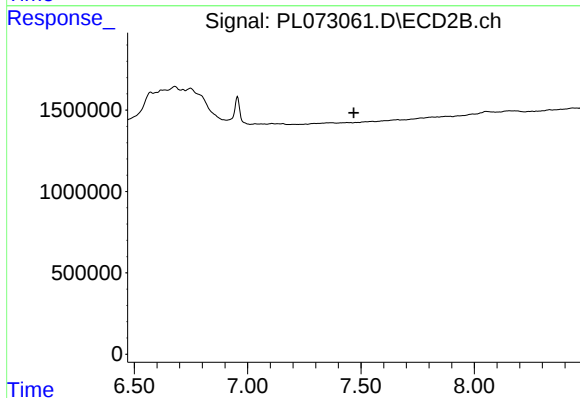


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.468 min
Response: 0
Conc: N.D.

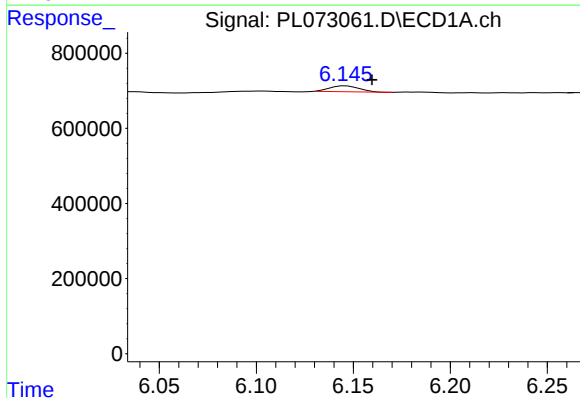


#6 beta-BHC

R.T.: 6.146 min
Delta R.T.: -0.014 min
Response: 164243
Conc: 0.74 ng/ml

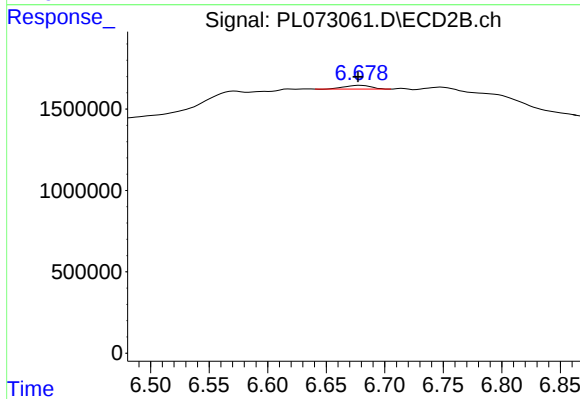

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.002 min
Response: 353384
Conc: 0.39 ng/ml

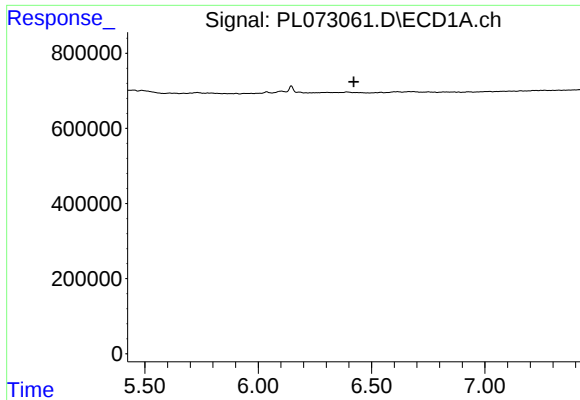

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

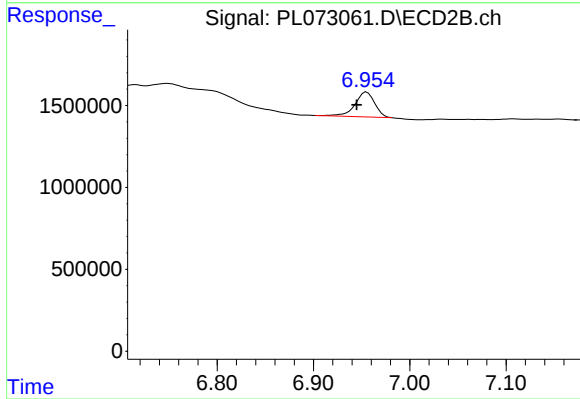


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.010 min
Response: 2148809
Conc: 1.14 ng/ml

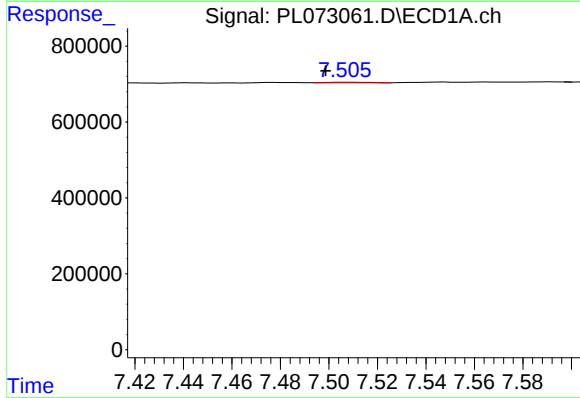


#9 Endosulfan I

R.T.: 7.507 min
Delta R.T.: 0.009 min
Response: 22118
Conc: 0.05 ng/ml

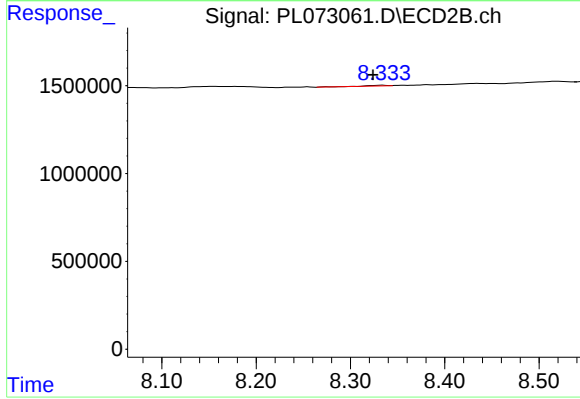

#9 Endosulfan I


R.T.: 8.334 min
Delta R.T.: 0.010 min
Response: 59449
Conc: 0.04 ng/ml

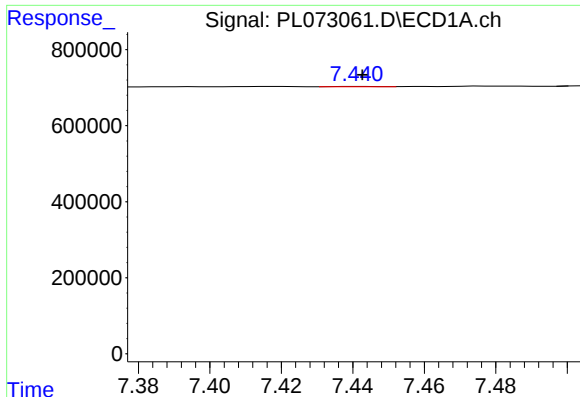

#11 alpha-Chlordane


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 7140
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

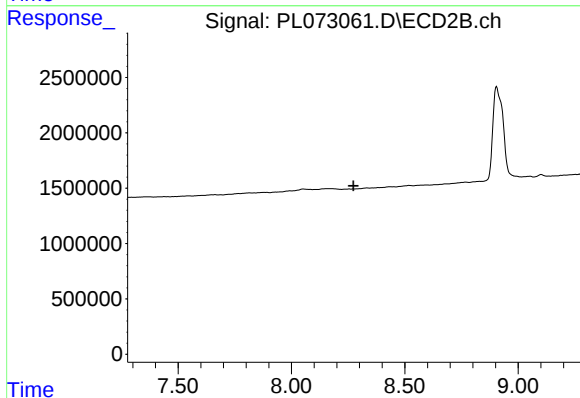


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.274 min
Response: 0
Conc: N.D.

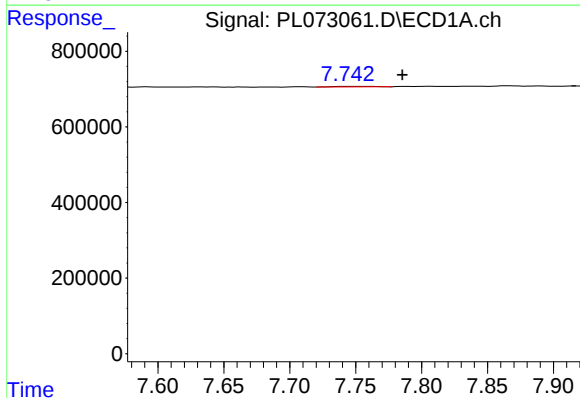


#13 Dieldrin

R.T.: 7.761 min
Delta R.T.: -0.025 min
Response: 29644
Conc: 0.07 ng/ml

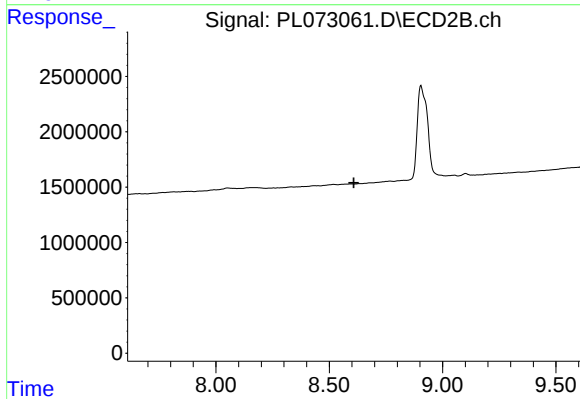

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.609 min
Response: 0
Conc: N.D.

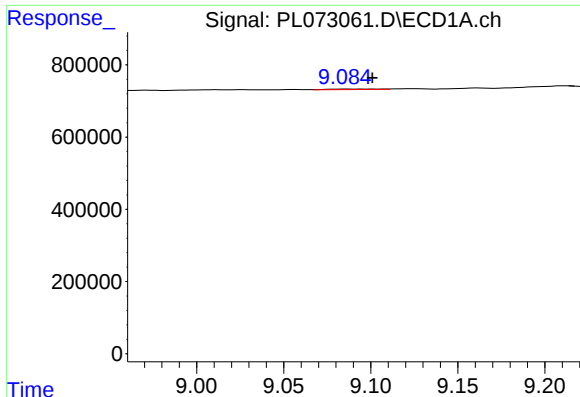

#20 Methoxychlor


R.T.: 9.086 min
Delta R.T.: -0.015 min
Response: 24986
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

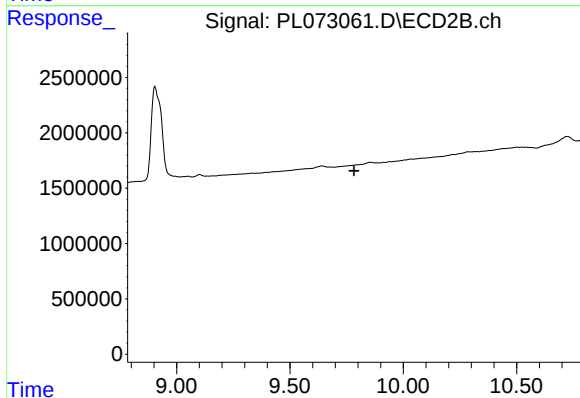


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.783 min
Response: 0
Conc: N.D.

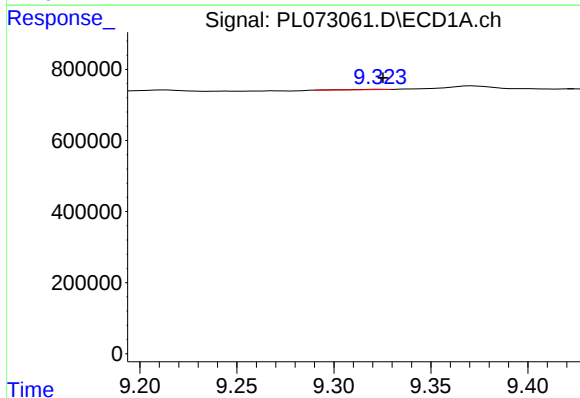


#21 Endrin ketone

R.T.: 9.323 min
Delta R.T.: -0.002 min
Response: 9356
Conc: 0.02 ng/ml

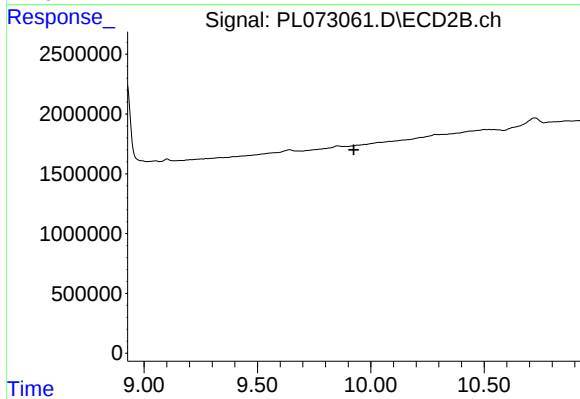

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.924 min
Response: 0
Conc: N.D.

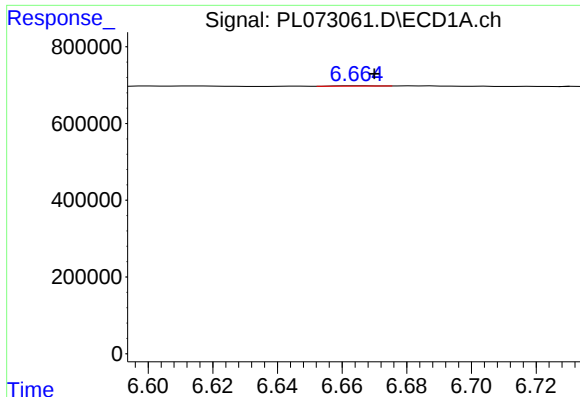

#24 Chlordane-2


R.T.: 6.665 min
Delta R.T.: -0.005 min
Response: 6868
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

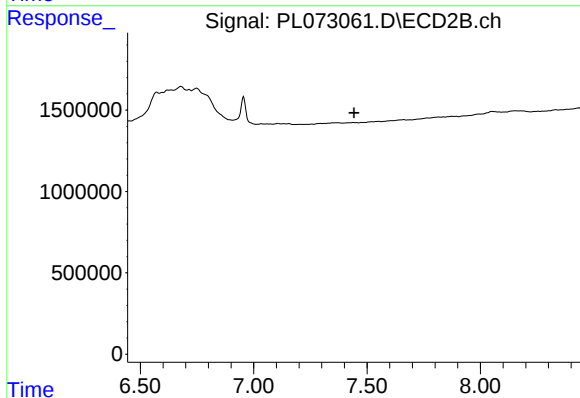


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.443 min
Response: 0
Conc: N.D.

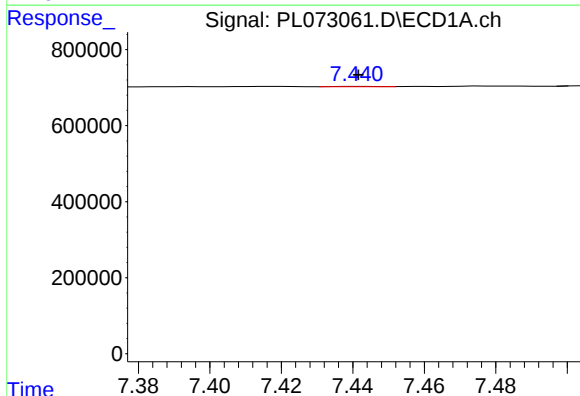


#26 Chlordane-4

R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 7140
Conc: 0.13 ng/ml

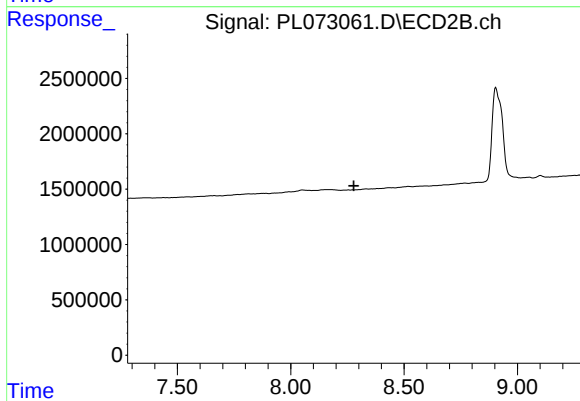

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.278 min
Response: 0
Conc: N.D.

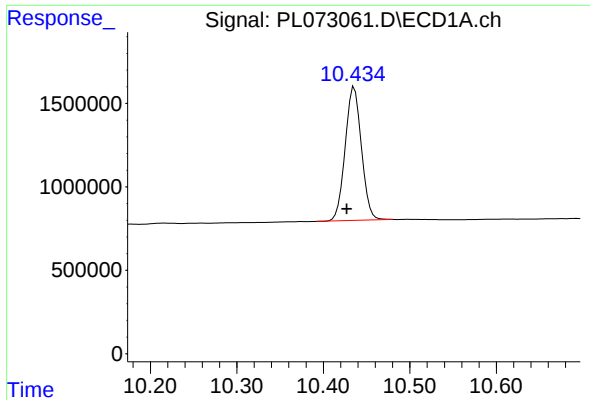

#28 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.009 min
Response: 10398168
Conc: 22.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

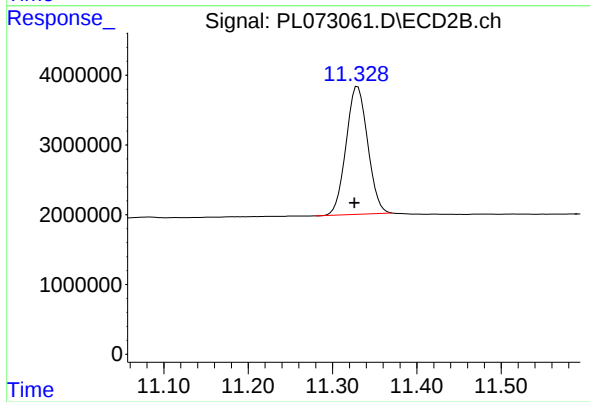

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: 0.004 min
Response: 32685538
Conc: 20.72 ng/ml