

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030122\
 Data File : PL073064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2022 10:32
 Operator : AR\AJ
 Sample : N1663-01RE 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-022422RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 13:06:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.656	5.487	772503	3233148	2.411	2.228
28)	SA Decachlor...	10.433	11.331	2041728	6389033	4.362	4.050
Target Compounds							
10)	B gamma-Chl...	7.379	8.193	348425	1864437	0.734	1.044 #
11)	B alpha-Chl...	7.449	8.279	478659	2873368	1.000	1.632 #
12)	B 4,4'-DDE	7.665	8.459	183889	595225	0.473	0.381



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030122\
Data File : PL073064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2022 10:32
Operator : AR\AJ
Sample : N1663-01RE 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-022422RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 13:06:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

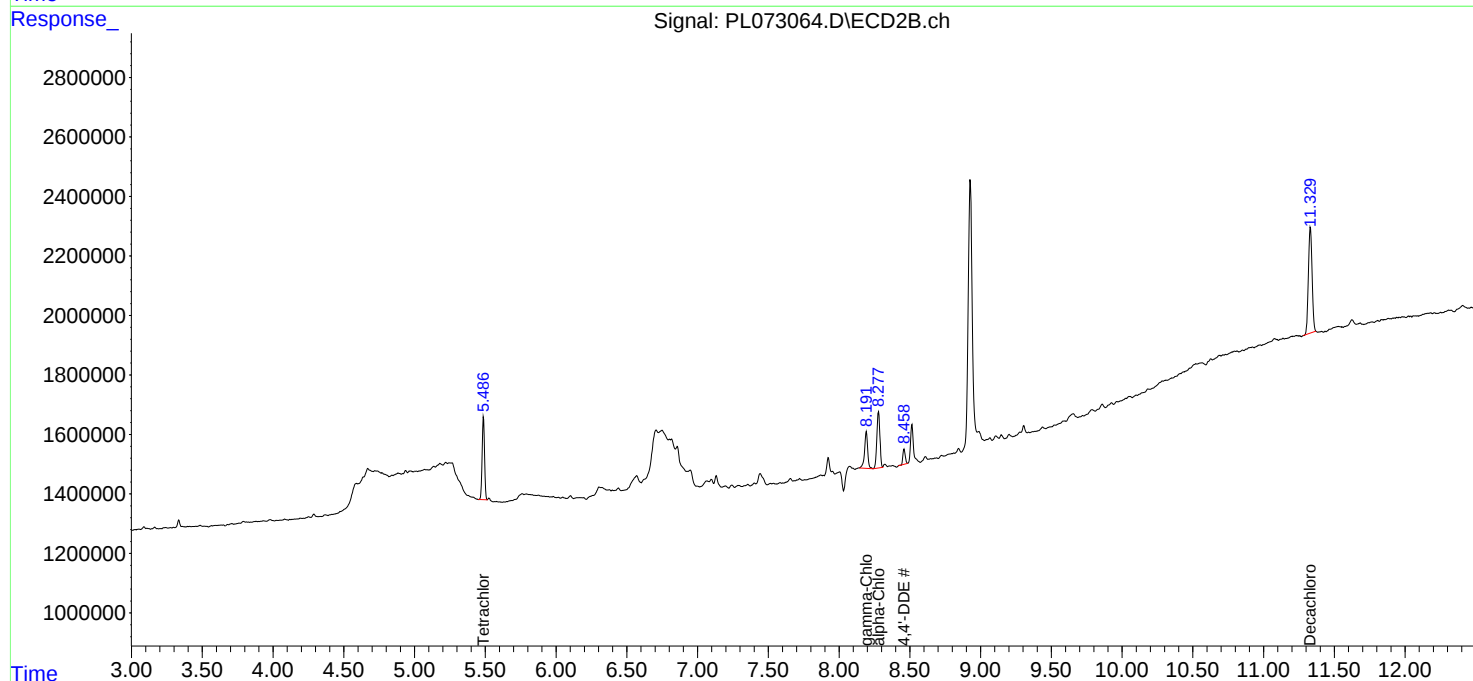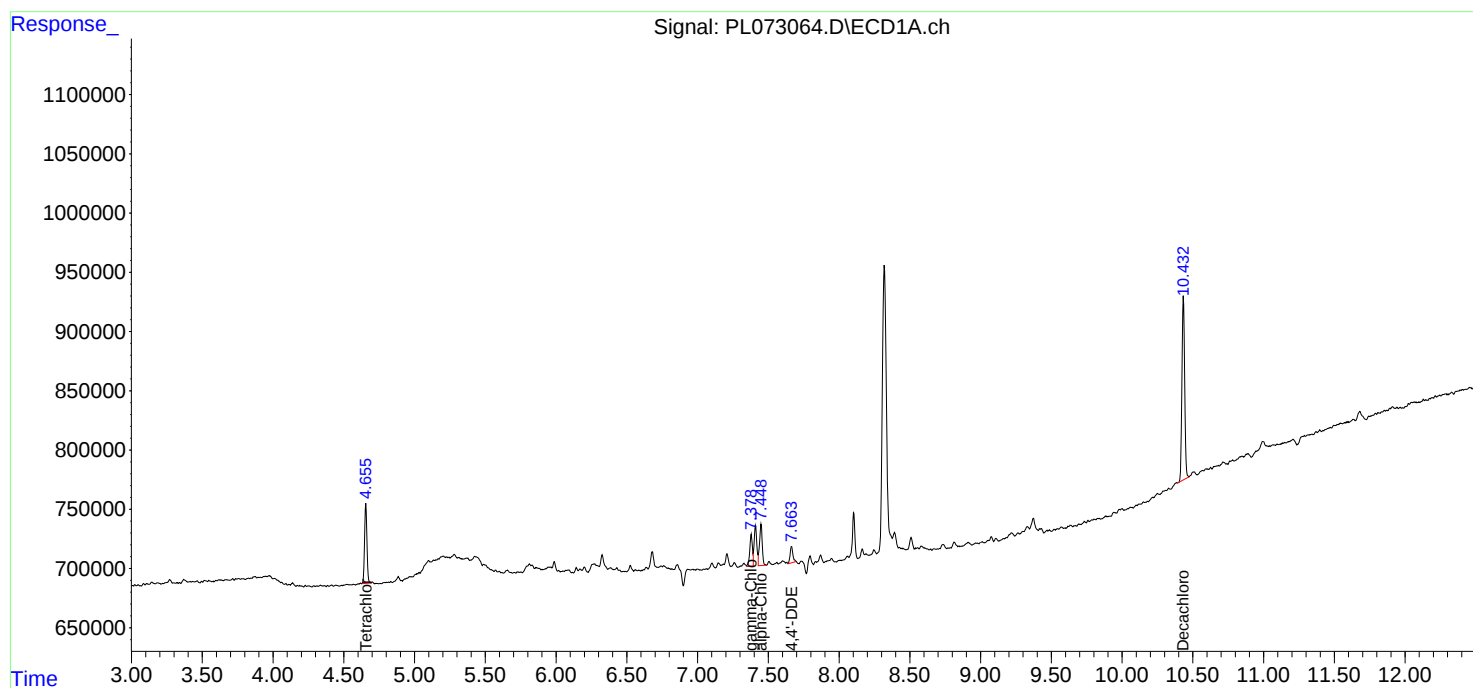


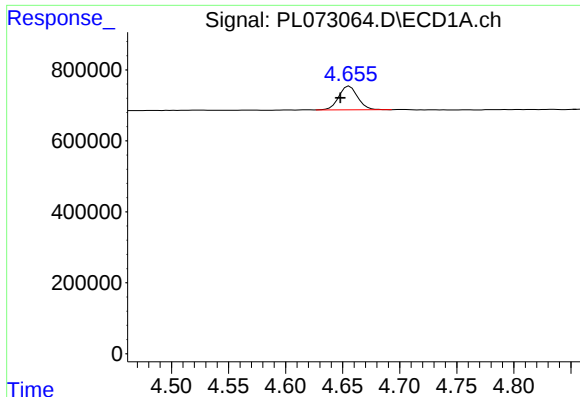

#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: 0.008 min
Response: 772503
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-022422RE

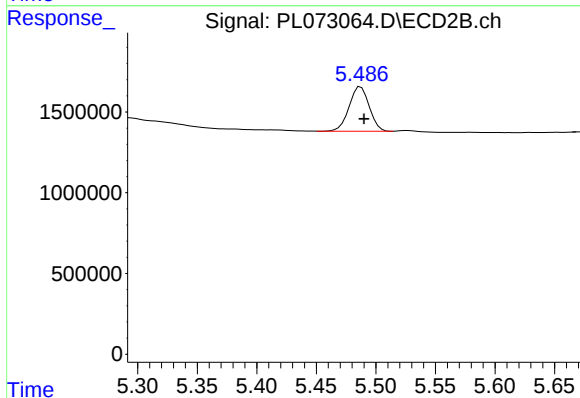


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.003 min
Response: 3233148
Conc: 2.23 ng/ml

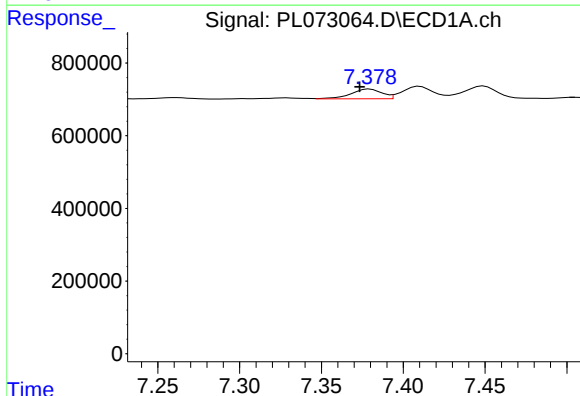


#10 gamma-Chlordane

R.T.: 7.379 min
Delta R.T.: 0.006 min
Response: 348425
Conc: 0.73 ng/ml

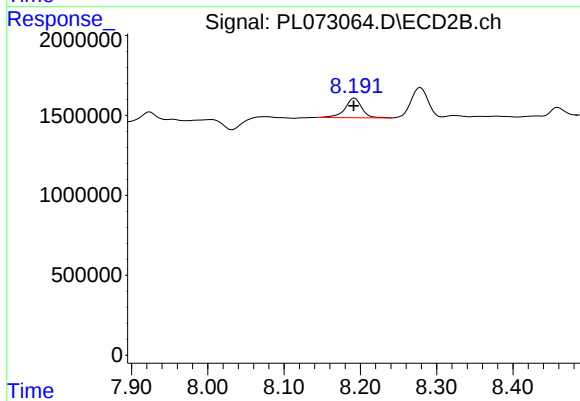

#10 gamma-Chlordane


R.T.: 8.193 min
Delta R.T.: 0.001 min
Response: 1864437
Conc: 1.04 ng/ml

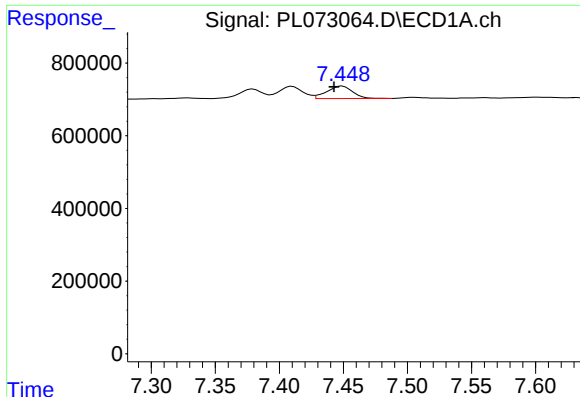

#11 alpha-Chlordane


R.T.: 7.449 min
Delta R.T.: 0.006 min
Response: 478659
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-022422RE

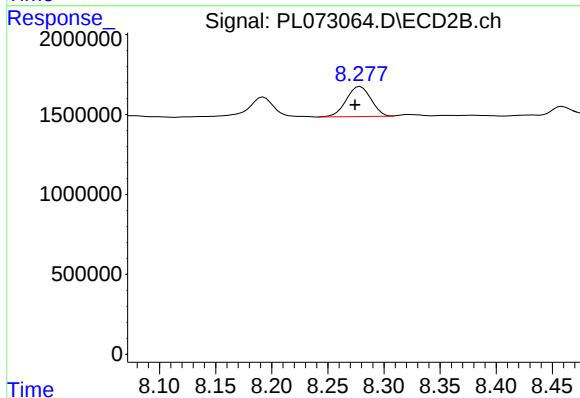


#11 alpha-Chlordane

R.T.: 8.279 min
Delta R.T.: 0.005 min
Response: 2873368
Conc: 1.63 ng/ml

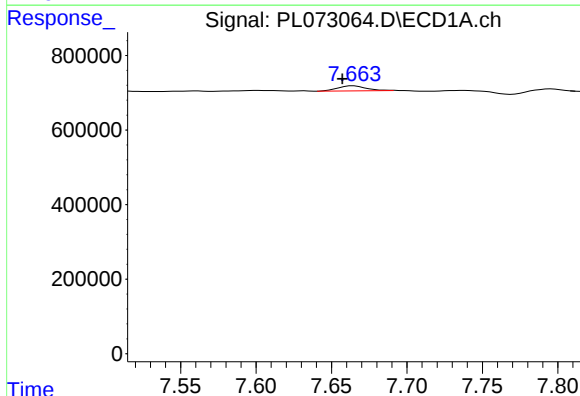


#12 4,4'-DDE

R.T.: 7.665 min
Delta R.T.: 0.007 min
Response: 183889
Conc: 0.47 ng/ml

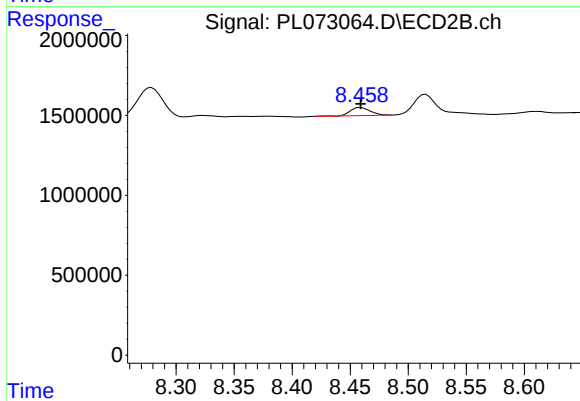

#12 4,4'-DDE


R.T.: 8.459 min
Delta R.T.: 0.000 min
Response: 595225
Conc: 0.38 ng/ml

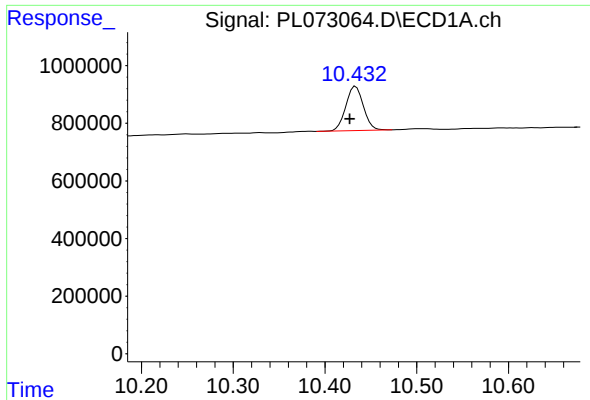

#28 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.006 min
Response: 2041728
Conc: 4.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-022422RE

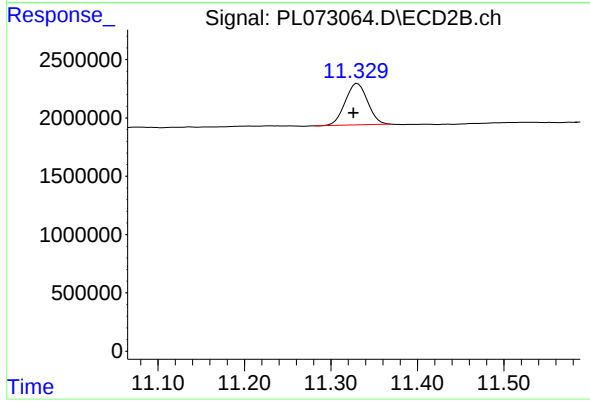

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.005 min
Response: 6389033
Conc: 4.05 ng/ml