

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 11:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 05:51:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.001	380.7E6	118.3E6	21.286	22.078
28)	SA Decachlor...	8.254	9.065	364.4E6	94267988	18.348	22.273
Target Compounds							
6)	B beta-BHC	0.000	4.887f	0	3816741	N.D.	1.144 #
8)	B Heptachlo...	0.000	5.874	0	1141670	N.D.	0.191 #
9)	A Endosulfan I	5.547	0.000	9594676	0	0.386	N.D. #
10)	B gamma-Chl...	0.000	6.113	0	140503	N.D.	0.023 #
23)	Chlordane-1	0.000	5.036f	0	3005205	N.D.	15.164 #
25)	Chlordane-3	0.000	6.113f	0	140503	N.D.	0.184 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 11:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 05:51:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

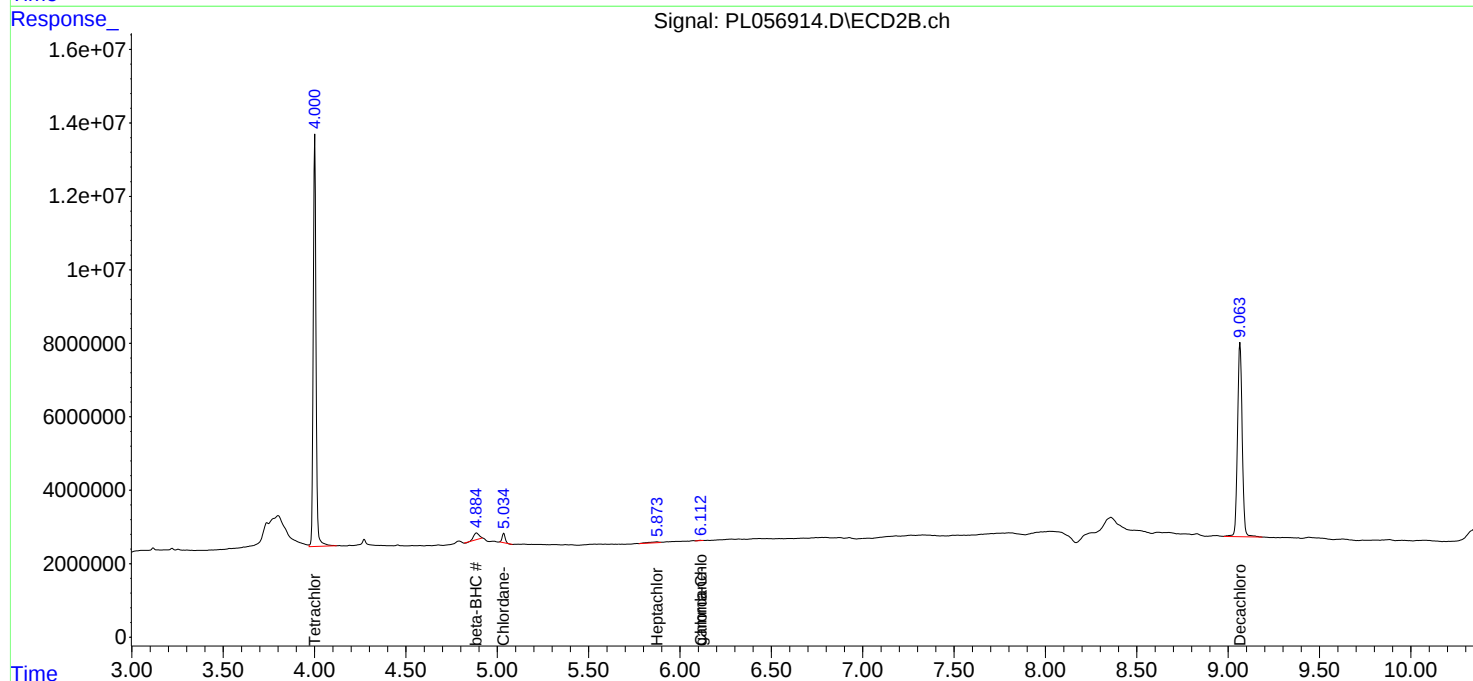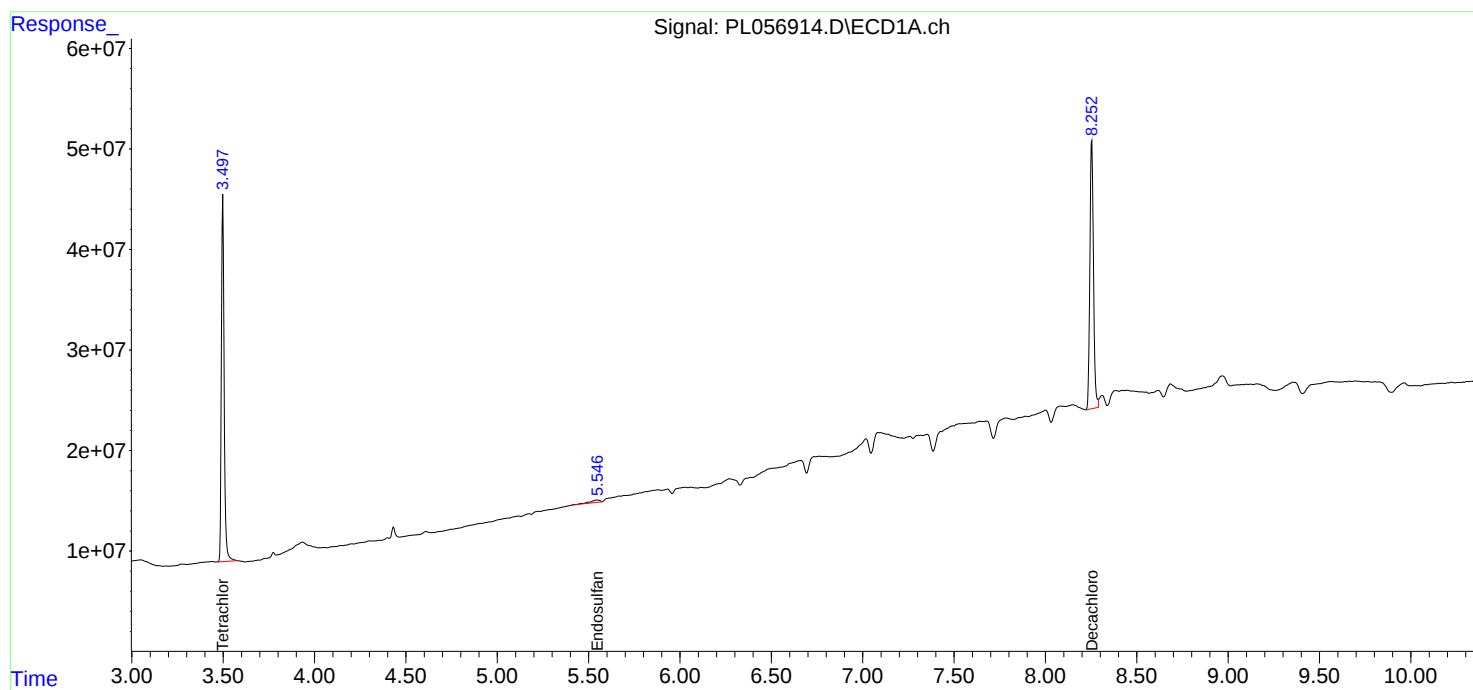


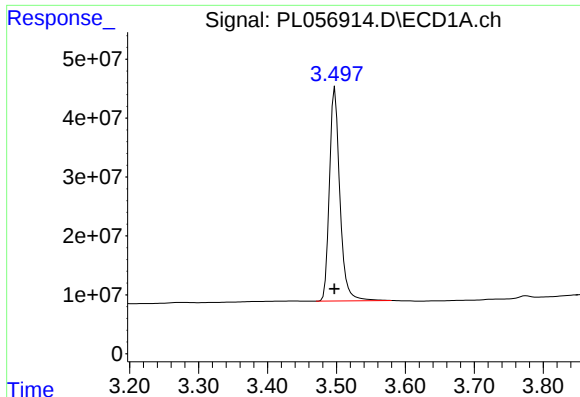

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 380657000
Conc: 21.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

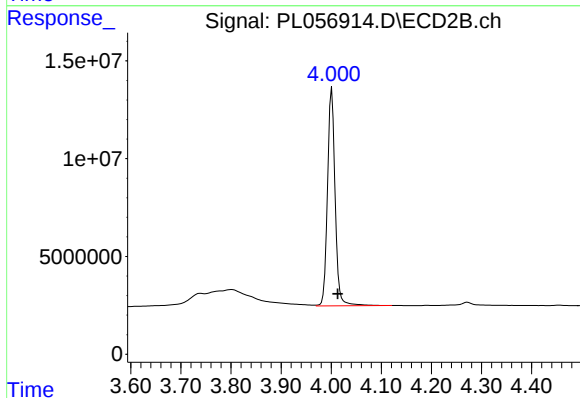


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.012 min
Response: 118316722
Conc: 22.08 ng/ml

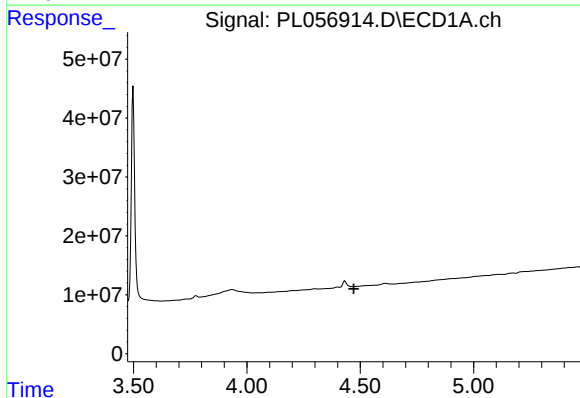


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.471 min
Response: 0
Conc: N.D.

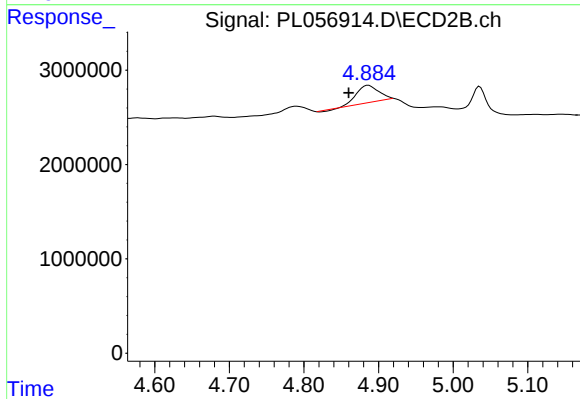

#6 beta-BHC


R.T.: 4.887 min
Delta R.T.: 0.027 min
Response: 3816741
Conc: 1.14 ng/ml

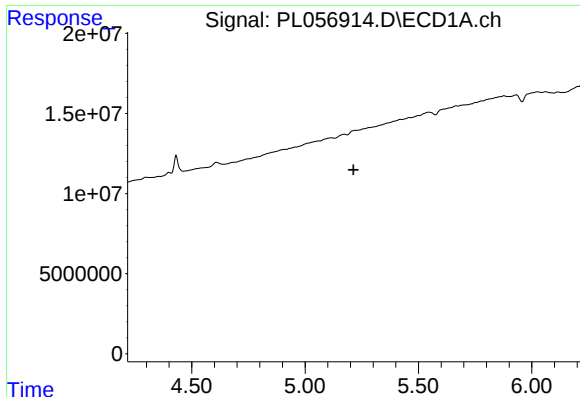

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

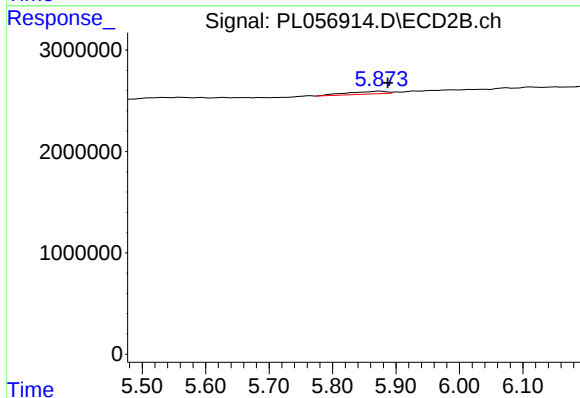


#8 Heptachlor epoxide

R.T.: 5.874 min
Delta R.T.: -0.013 min
Response: 1141670
Conc: 0.19 ng/ml

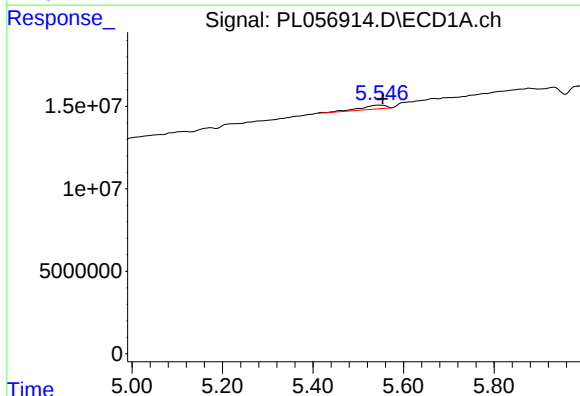


#9 Endosulfan I

R.T.: 5.547 min
Delta R.T.: -0.007 min
Response: 9594676
Conc: 0.39 ng/ml

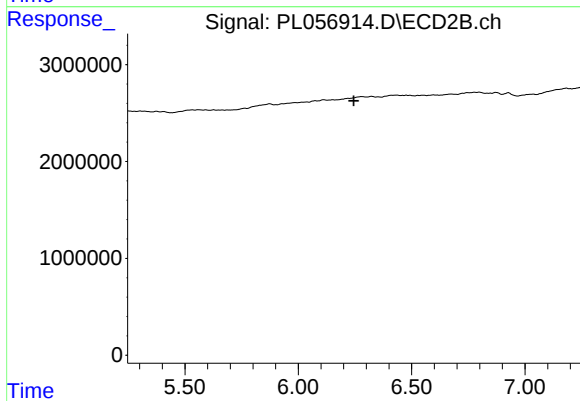

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.245 min
Response: 0
Conc: N.D.

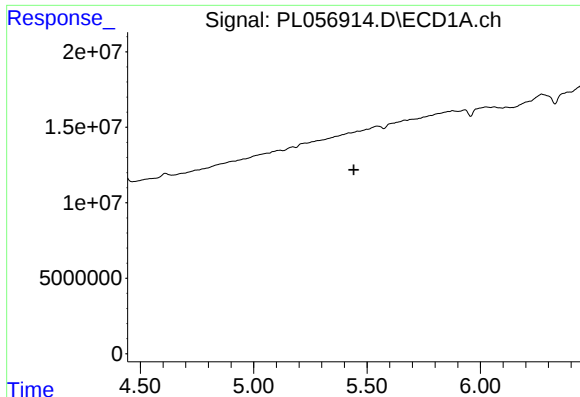

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

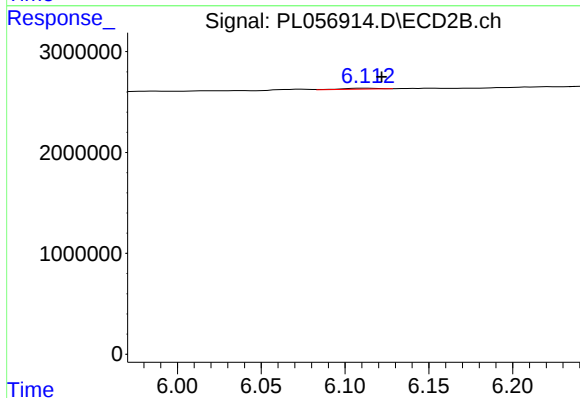


#10 gamma-Chlordane

R.T.: 6.113 min
Delta R.T.: -0.009 min
Response: 140503
Conc: 0.02 ng/ml

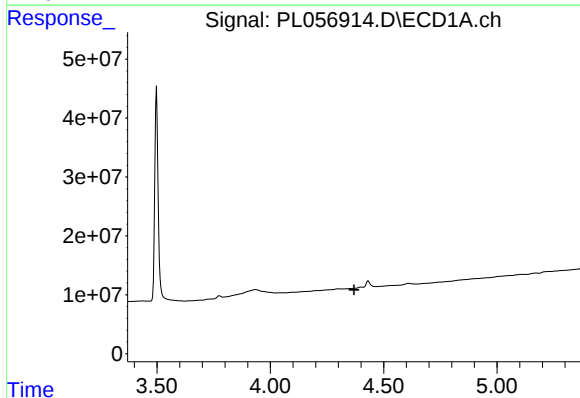


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.369 min
Response: 0
Conc: N.D.

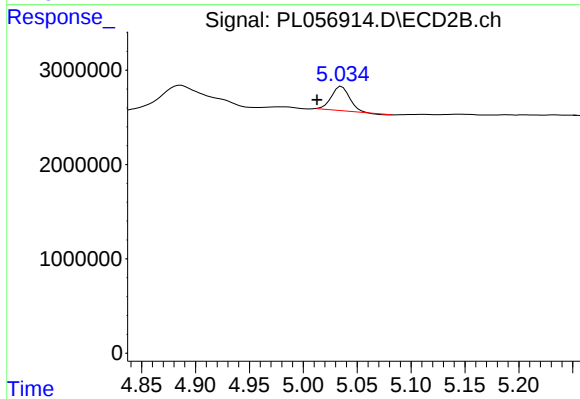

#23 Chlordane-1


R.T.: 5.036 min
Delta R.T.: 0.023 min
Response: 3005205
Conc: 15.16 ng/ml

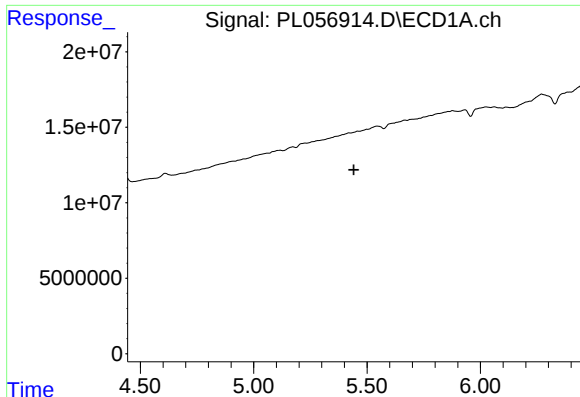

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

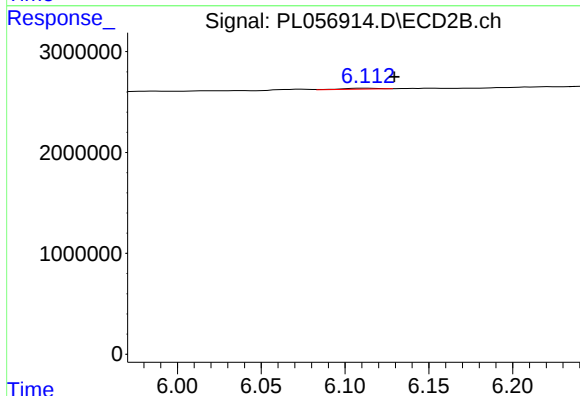


#25 Chlordane-3

R.T.: 6.113 min
Delta R.T.: -0.017 min
Response: 140503
Conc: 0.18 ng/ml

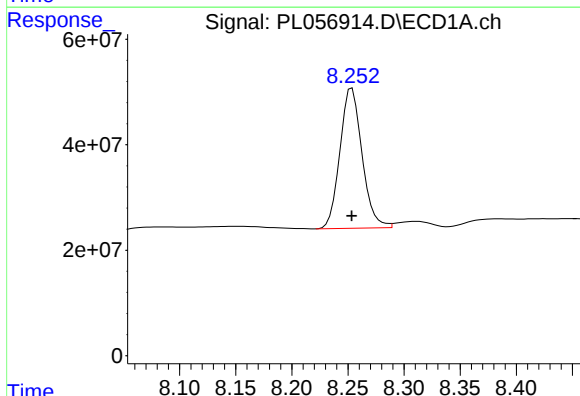

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 364442012
Conc: 18.35 ng/ml

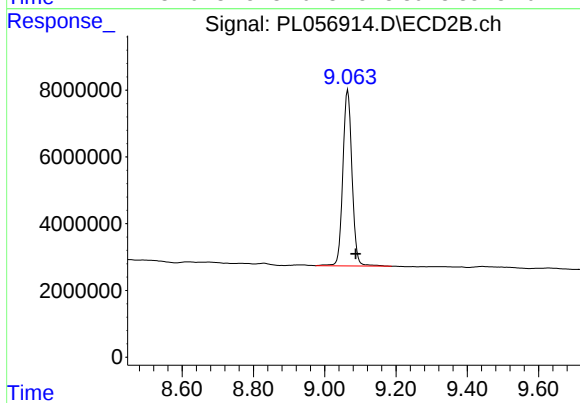

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: -0.022 min
Response: 94267988
Conc: 22.27 ng/ml