

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 12:32
 Operator : AJ\MA
 Sample : PB127187BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 05:52:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.001	363.3E6	116.7E6	20.316	21.781
28)	SA Decachlor...	8.259	9.069	424.4E6	97511752	21.367	23.040
Target Compounds							
3)	MA gamma-BHC...	0.000	4.676	0	353379	N.D.	0.046 #
4)	MA Heptachlor	4.526	0.000	16850100	0	0.599	N.D. #
8)	B Heptachlo...	5.222	0.000	1667612	0	0.063	N.D. #
9)	A Endosulfan I	5.554	0.000	12134850	0	0.488	N.D. #
15)	B Endosulfa...	6.305f	6.926	12619574	2271732	0.586	0.426 #
16)	A 4,4'-DDD	6.187	0.000	10017031	0	0.509	N.D. #
18)	B Endrin al...	6.505	0.000	39357372	0	1.989	N.D. #
23)	Chlordane-1	0.000	5.037f	0	3100059	N.D.	15.643 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 12:32
Operator : AJ\MA
Sample : PB127187BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 05:52:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

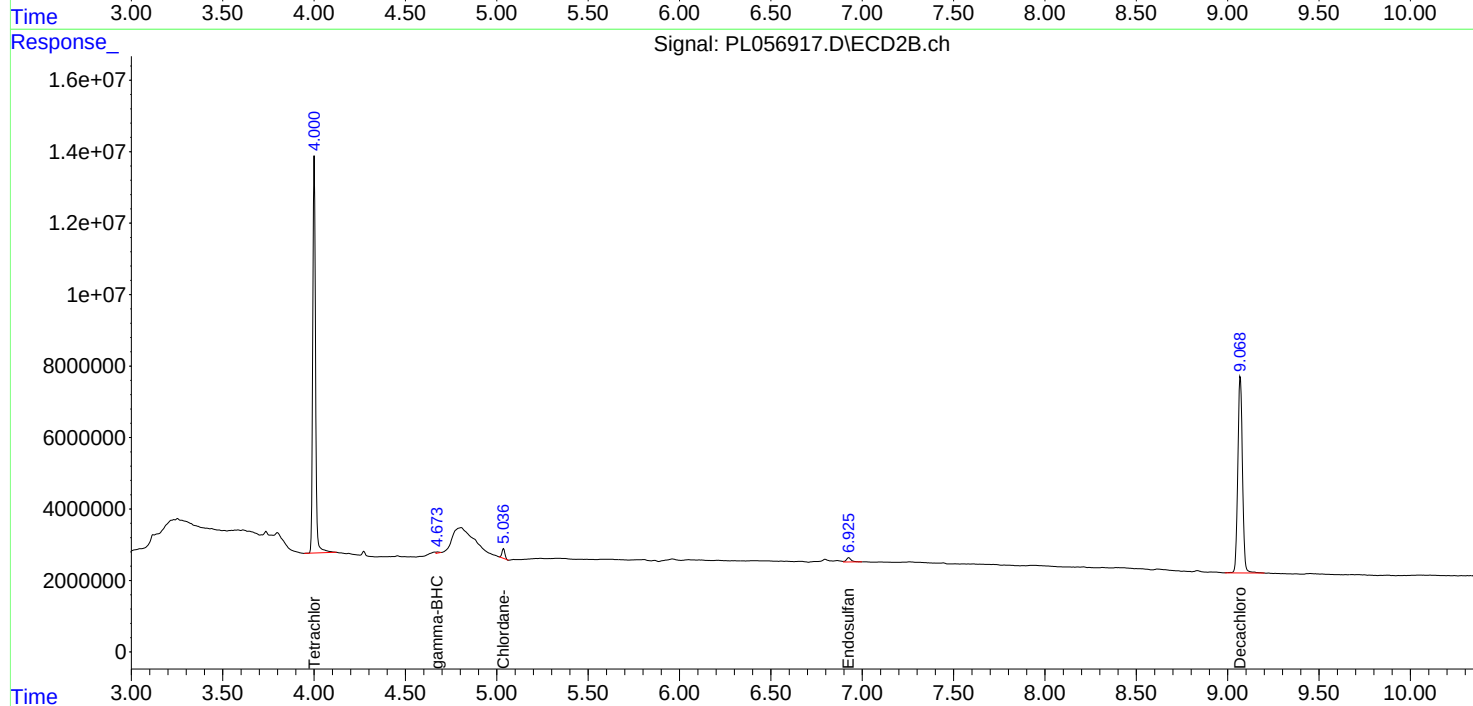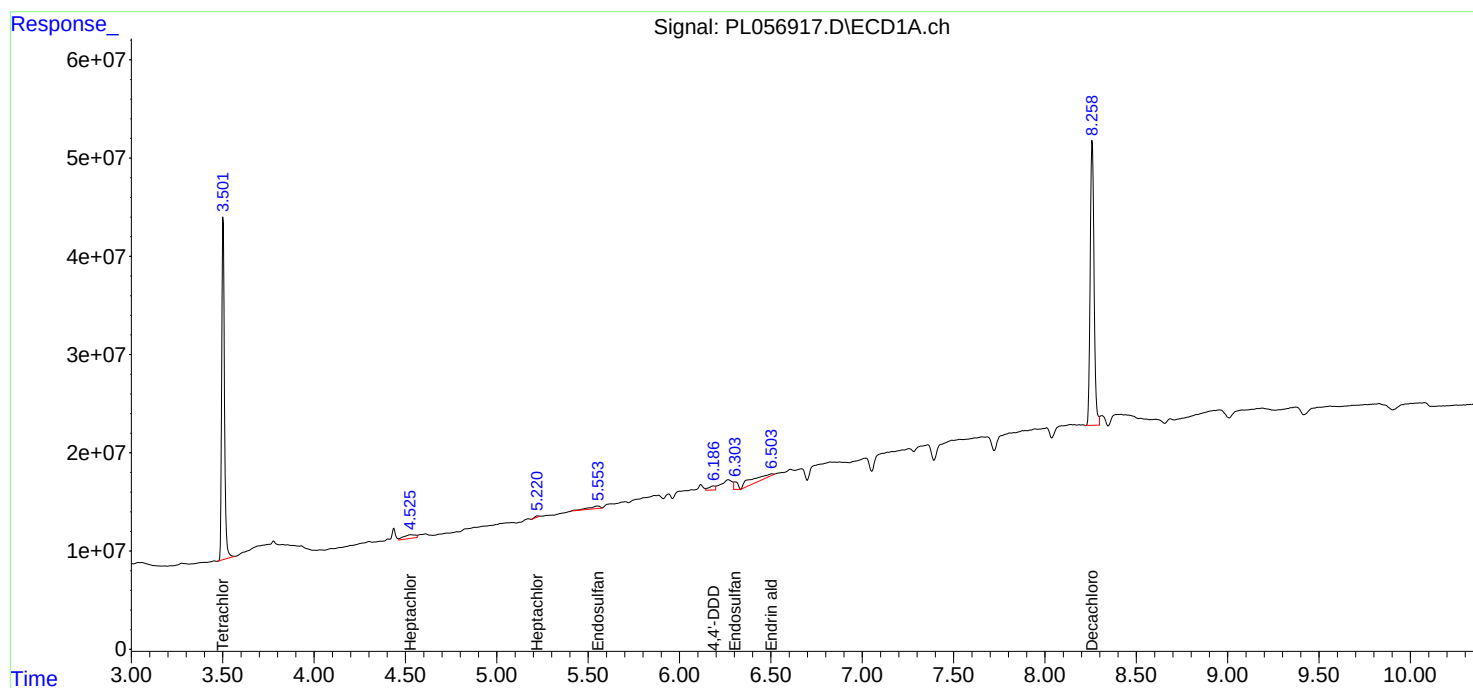


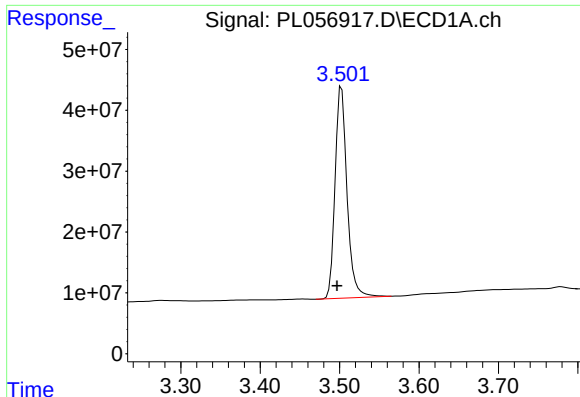

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.005 min
Response: 363314996
Conc: 20.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

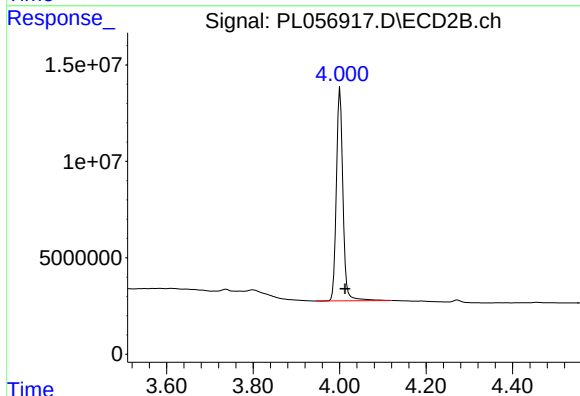


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.012 min
Response: 116724227
Conc: 21.78 ng/ml

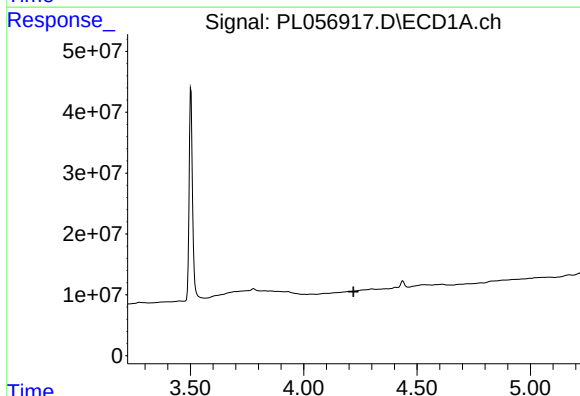


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.220 min
Response: 0
Conc: N.D.

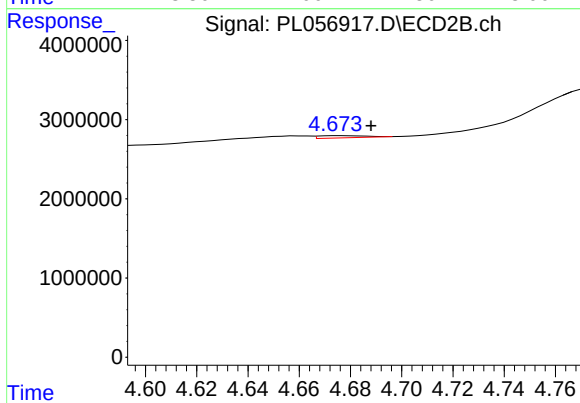

#3 gamma-BHC (Lindane)


R.T.: 4.676 min
Delta R.T.: -0.012 min
Response: 353379
Conc: 0.05 ng/ml

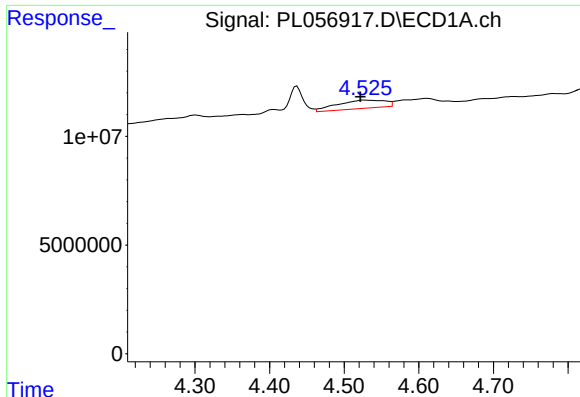

#4 Heptachlor


R.T.: 4.526 min
Delta R.T.: 0.005 min
Response: 16850100
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

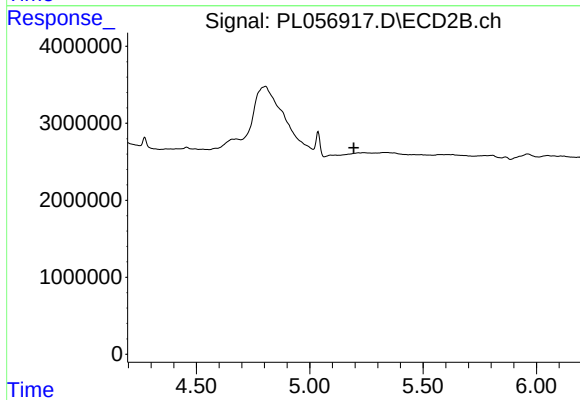


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.195 min
Response: 0
Conc: N.D.

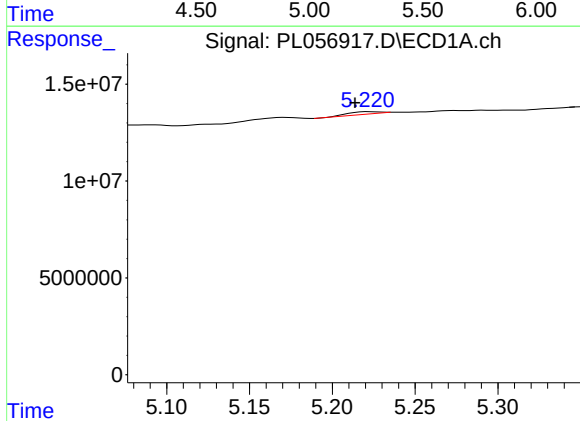


#8 Heptachlor epoxide

R.T.: 5.222 min
Delta R.T.: 0.008 min
Response: 1667612
Conc: 0.06 ng/ml

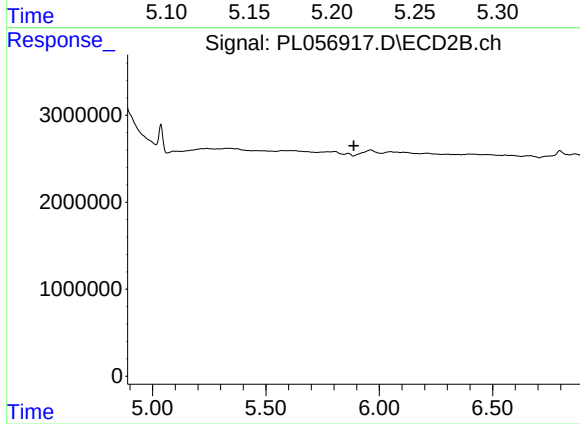

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.887 min
Response: 0
Conc: N.D.

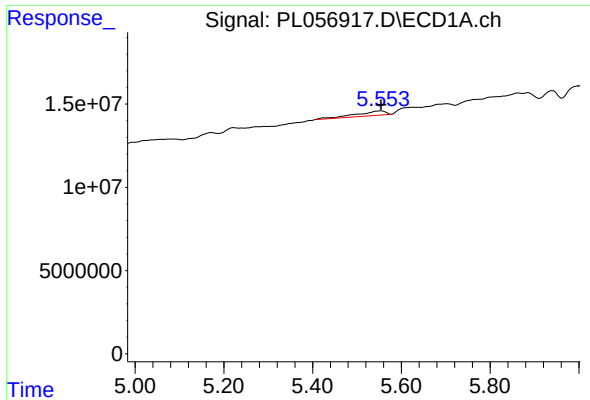

#9 Endosulfan I


R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 12134850
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

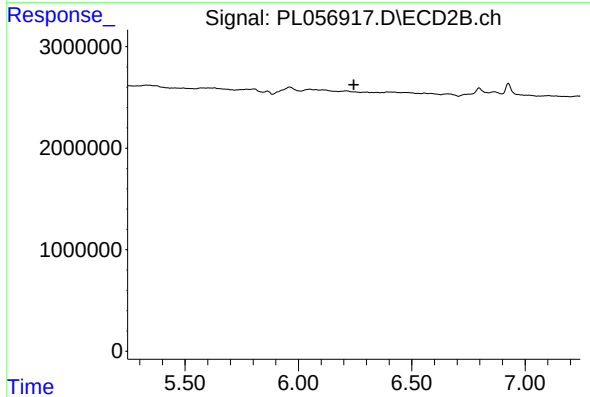


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

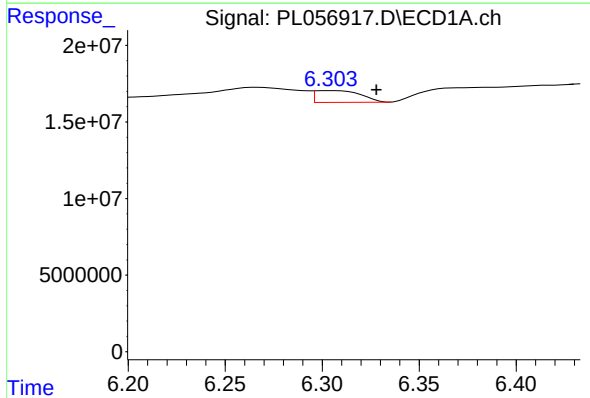


#15 Endosulfan II

R.T.: 6.305 min
Delta R.T.: -0.022 min
Response: 12619574
Conc: 0.59 ng/ml

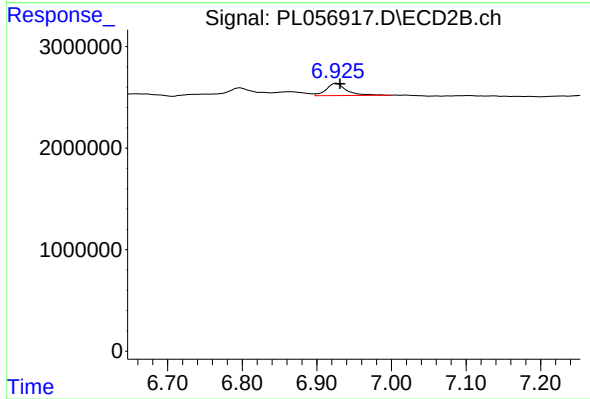

#15 Endosulfan II


R.T.: 6.926 min
Delta R.T.: -0.005 min
Response: 2271732
Conc: 0.43 ng/ml

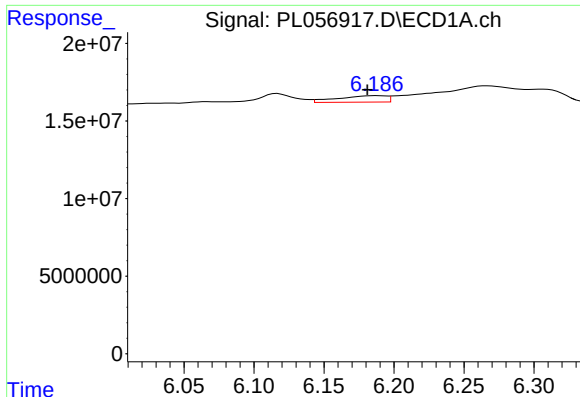

#16 4,4'-DDD


R.T.: 6.187 min
Delta R.T.: 0.006 min
Response: 10017031
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

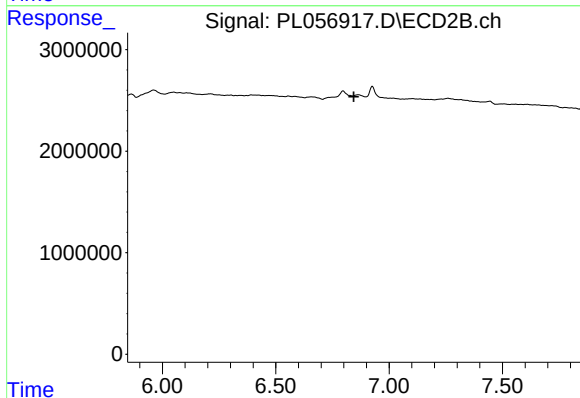


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.845 min
Response: 0
Conc: N.D.

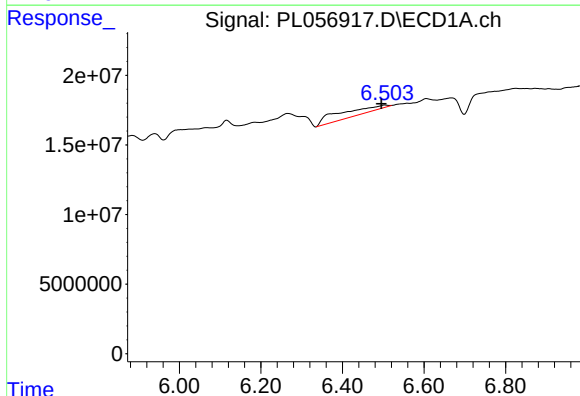


#18 Endrin aldehyde

R.T.: 6.505 min
Delta R.T.: 0.009 min
Response: 39357372
Conc: 1.99 ng/ml

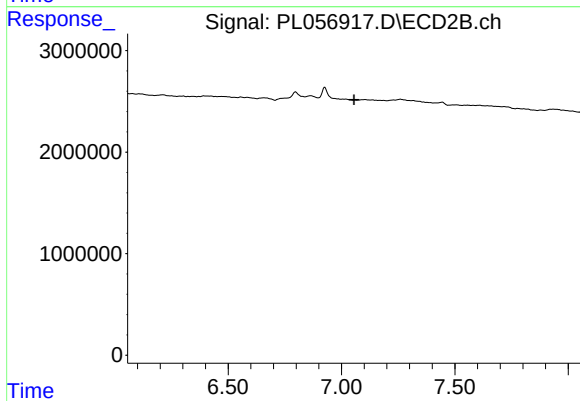

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.056 min
Response: 0
Conc: N.D.

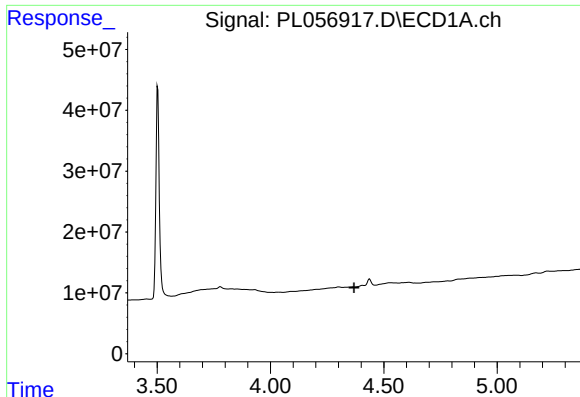

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

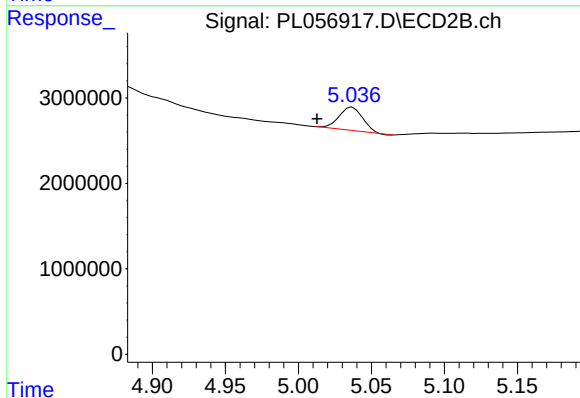


#23 Chlordane-1

R.T.: 5.037 min
Delta R.T.: 0.024 min
Response: 3100059
Conc: 15.64 ng/ml

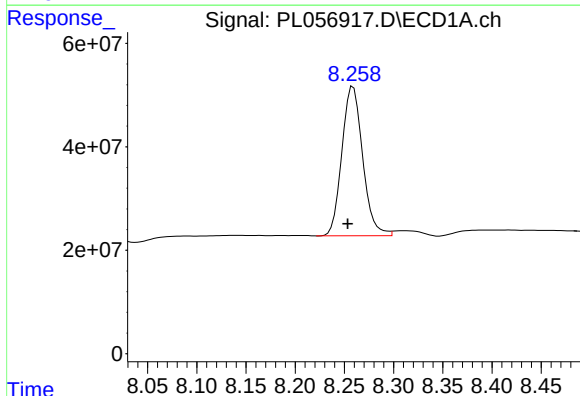

#28 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.006 min
Response: 424418390
Conc: 21.37 ng/ml

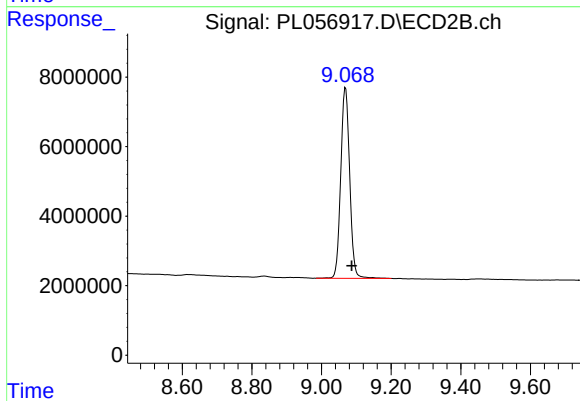

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: -0.018 min
Response: 97511752
Conc: 23.04 ng/ml