

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 19:49
 Operator : AJ\MA
 Sample : L1723-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 05:59:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.003	222.2E6	78703826	12.424	14.686
28)	SA Decachlor...	8.253	9.068	175.4E6	44659475	8.828	10.552
Target Compounds							
2)	A alpha-BHC	0.000	4.414	0	857672	N.D.	0.104 #
6)	B beta-BHC	0.000	4.886f	0	4233161	N.D.	1.269 #
23)	Chlordane-1	0.000	5.036f	0	2059035	N.D.	10.390 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 19:49
Operator : AJ\MA
Sample : L1723-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 05:59:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

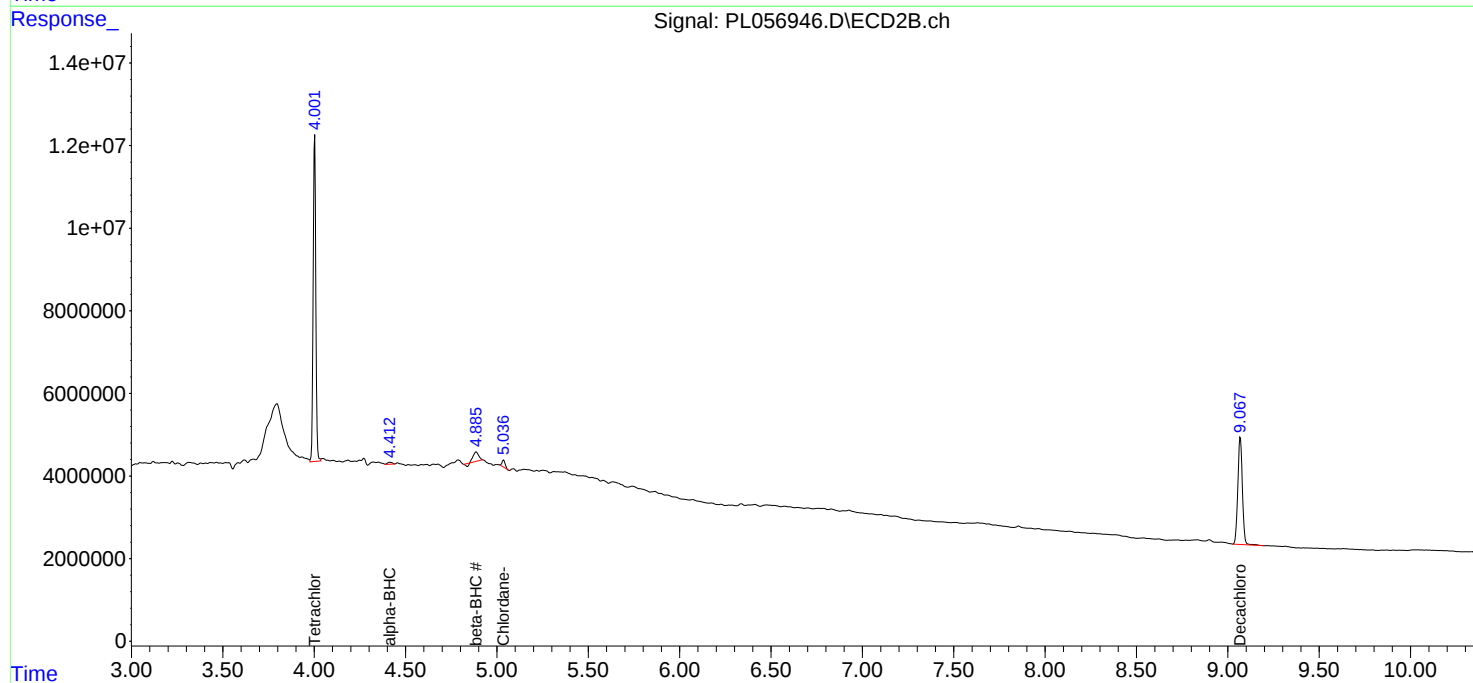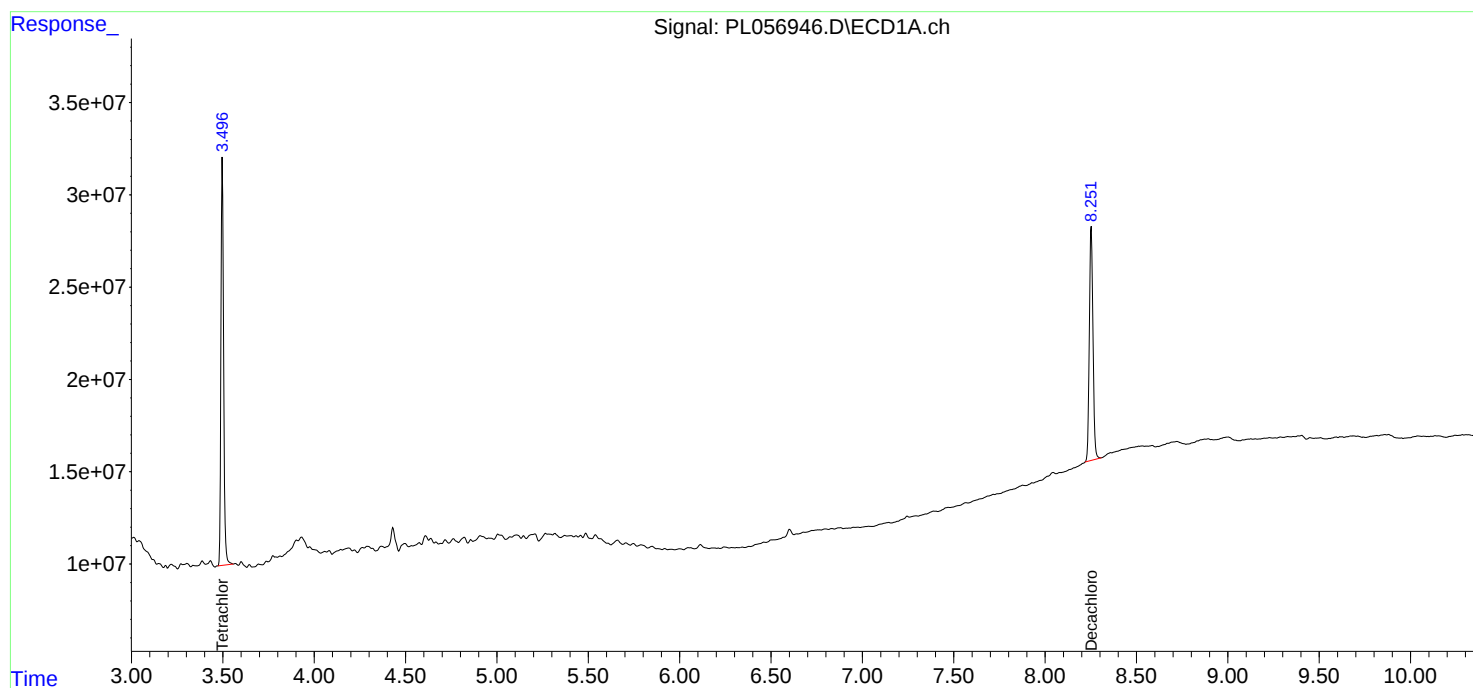


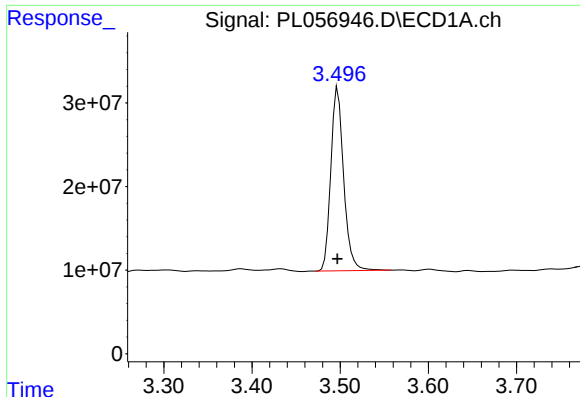

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 222174479
Conc: 12.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

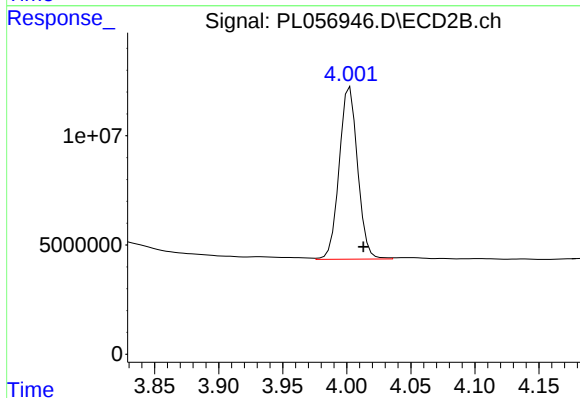


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.010 min
Response: 78703826
Conc: 14.69 ng/ml

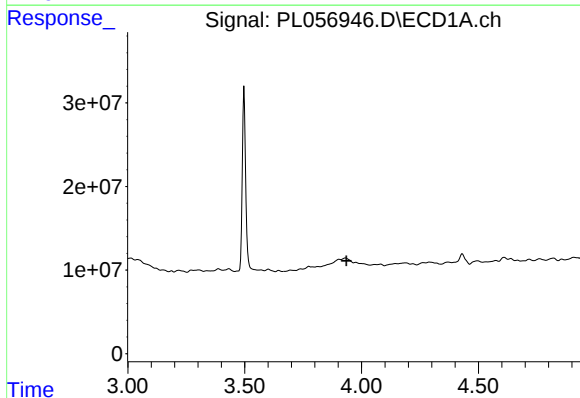


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

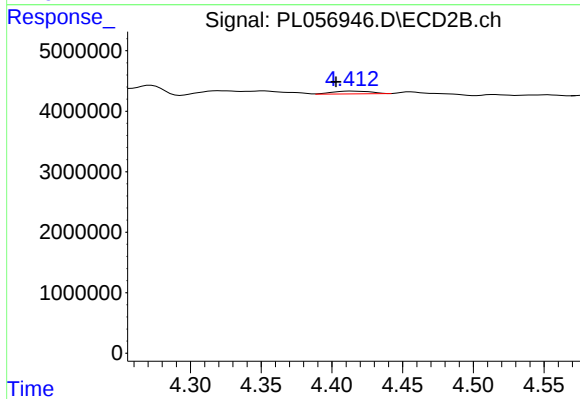

#2 alpha-BHC


R.T.: 4.414 min
Delta R.T.: 0.011 min
Response: 857672
Conc: 0.10 ng/ml

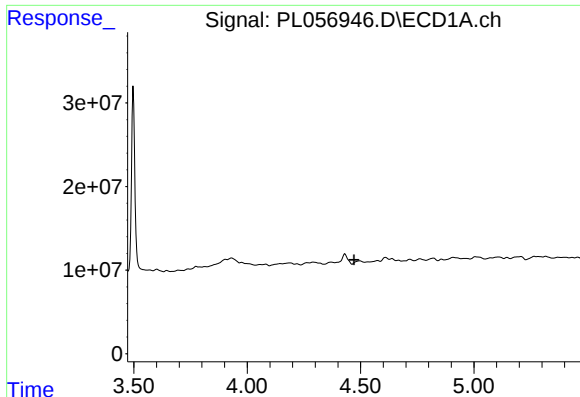

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

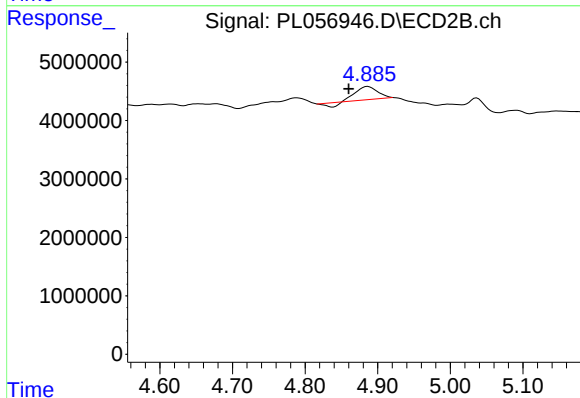


#6 beta-BHC

R.T.: 4.886 min
Delta R.T.: 0.026 min
Response: 4233161
Conc: 1.27 ng/ml

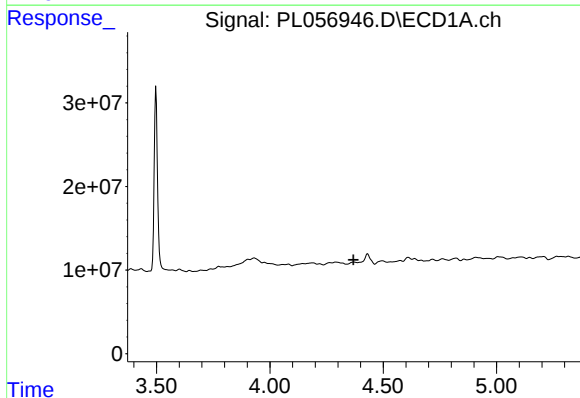


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.369 min
Response: 0
Conc: N.D.

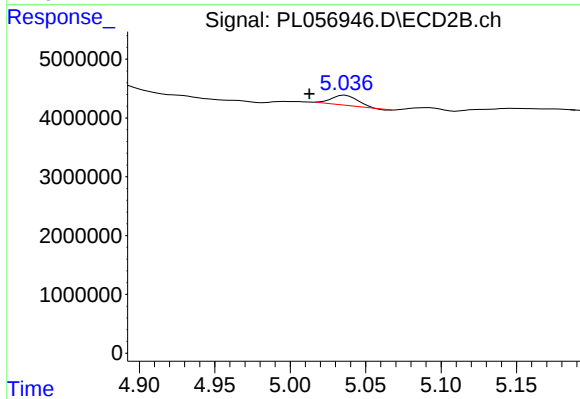

#23 Chlordane-1


R.T.: 5.036 min
Delta R.T.: 0.024 min
Response: 2059035
Conc: 10.39 ng/ml

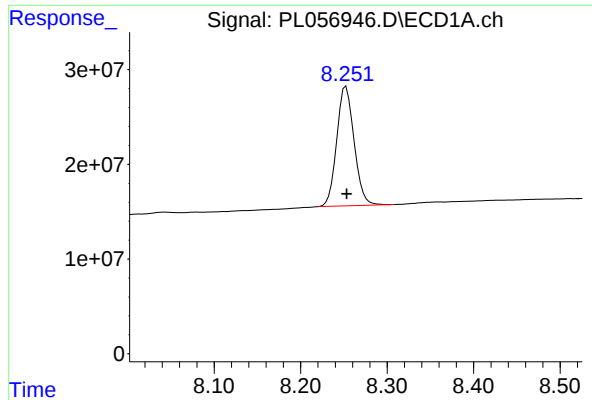

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 175353574
Conc: 8.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

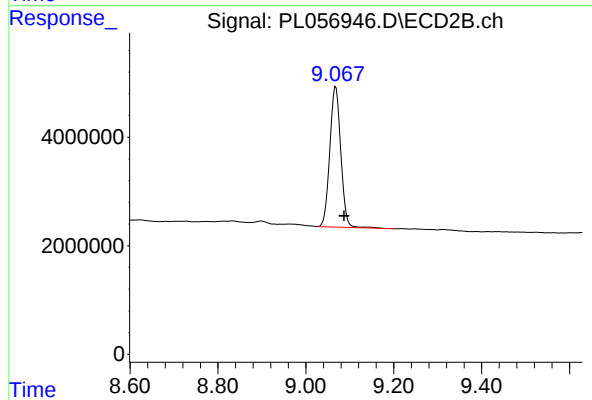

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.019 min
Response: 44659475
Conc: 10.55 ng/ml