

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 20:03
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 05:59:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.002	361.4E6	122.4E6	20.211	22.833
28)	SA Decachlor...	8.254	9.068	238.5E6	63984760	12.005	15.118 #
Target Compounds							
6)	B beta-BHC	0.000	4.883f	0	4568767	N.D.	1.370 #
23)	Chlordane-1	0.000	5.036f	0	3098868	N.D.	15.637 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 20:03
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 05:59:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

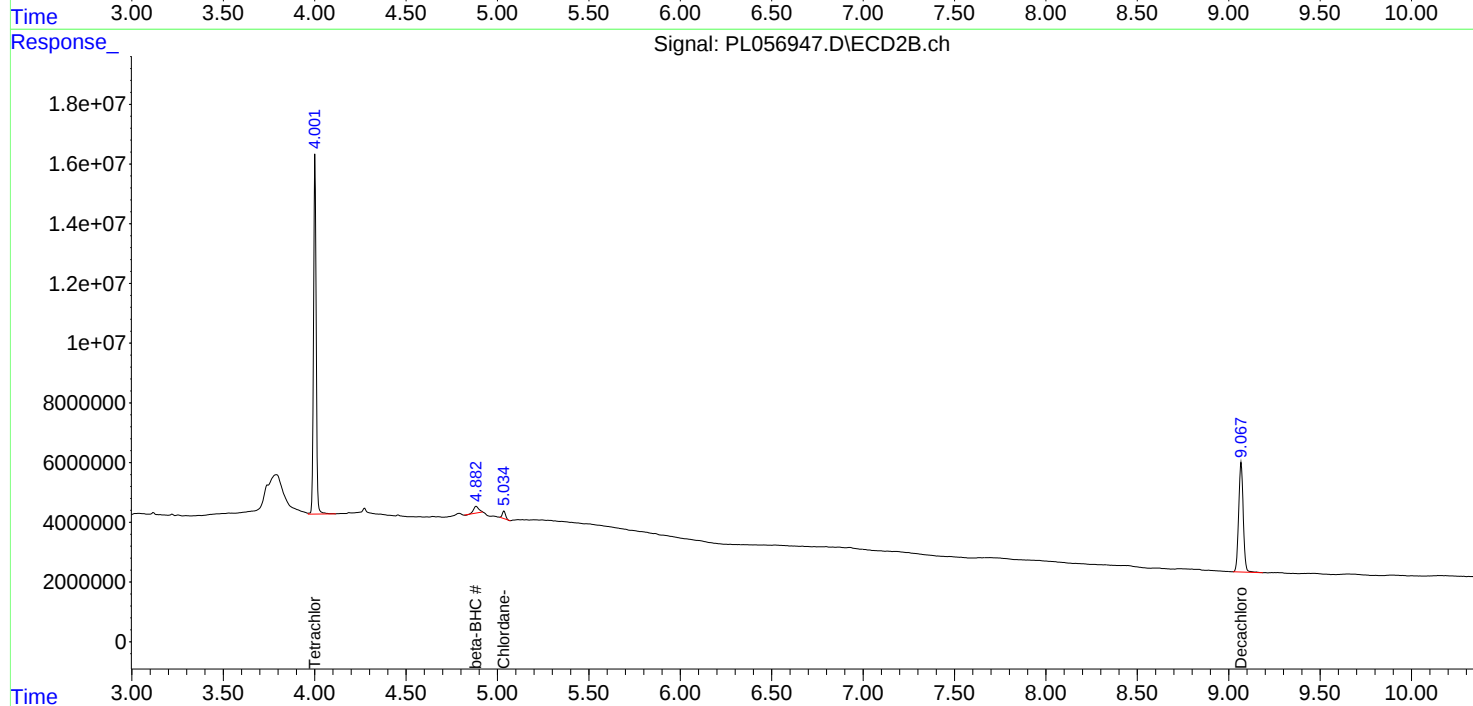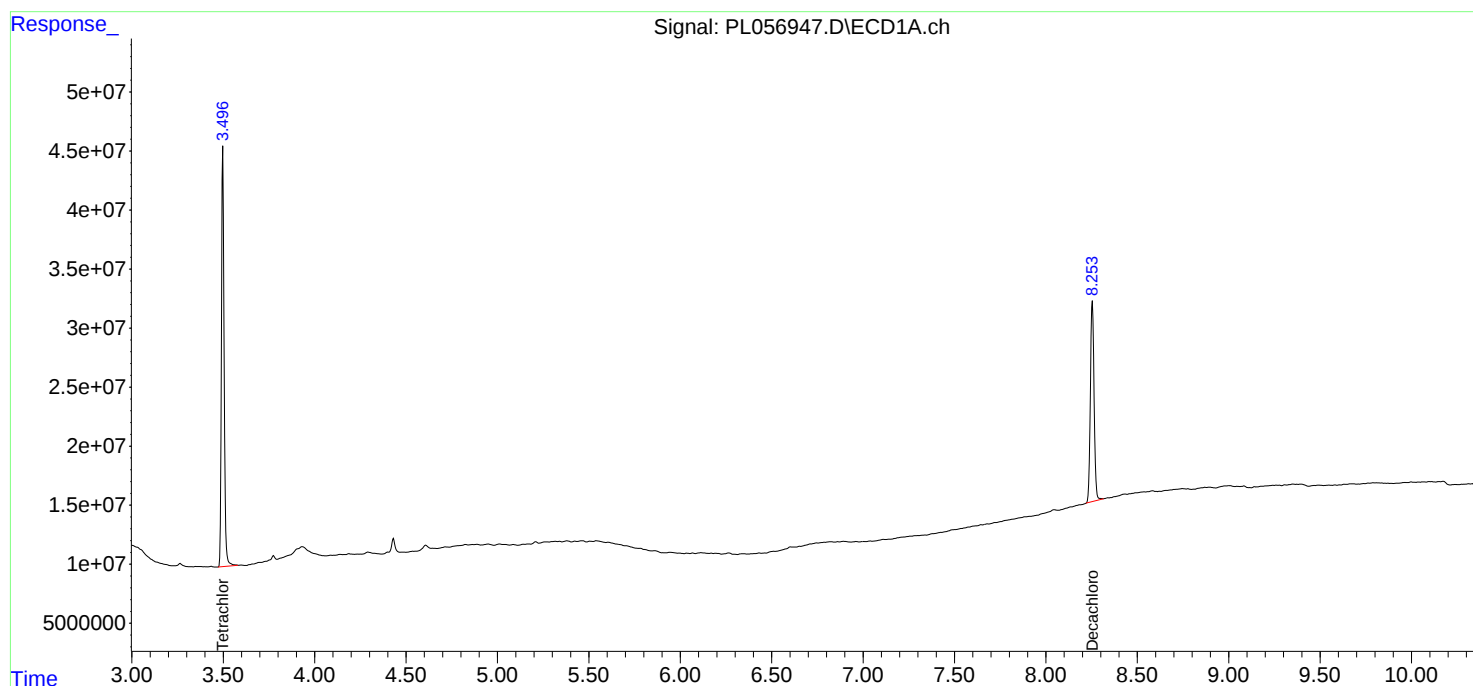


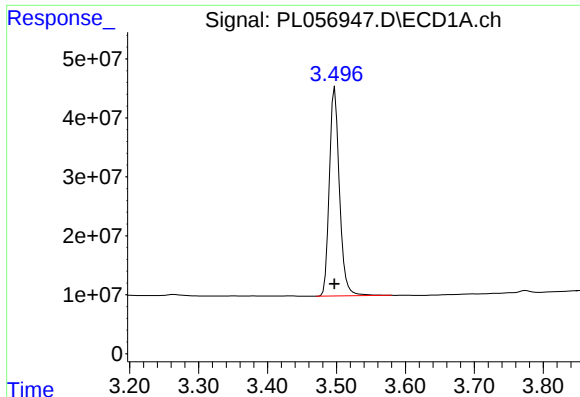

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 361442207
Conc: 20.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

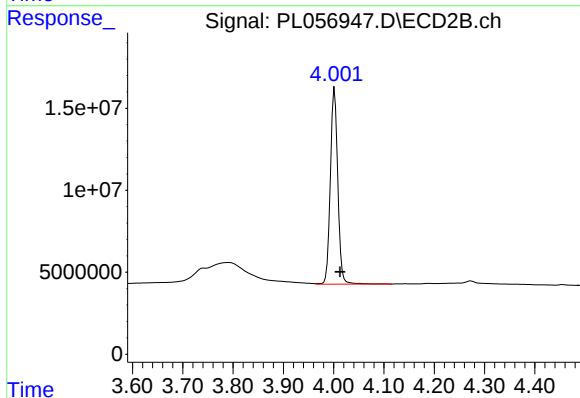


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.011 min
Response: 122359661
Conc: 22.83 ng/ml

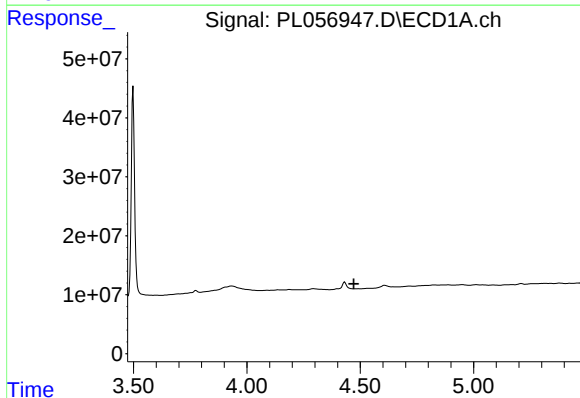


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.471 min
Response: 0
Conc: N.D.

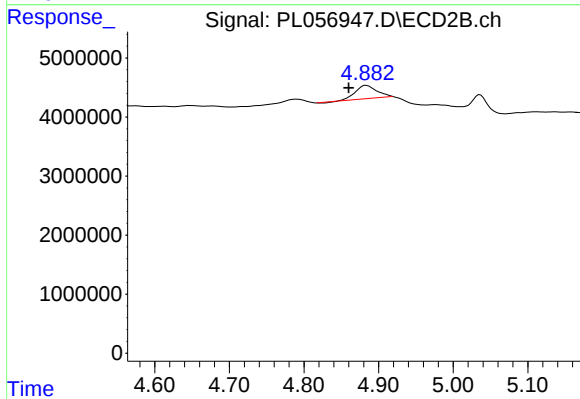

#6 beta-BHC


R.T.: 4.883 min
Delta R.T.: 0.023 min
Response: 4568767
Conc: 1.37 ng/ml

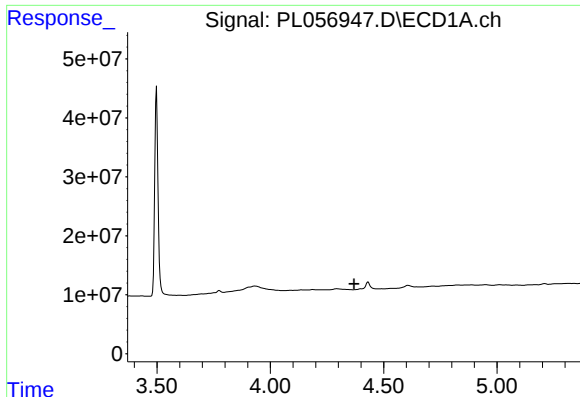

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

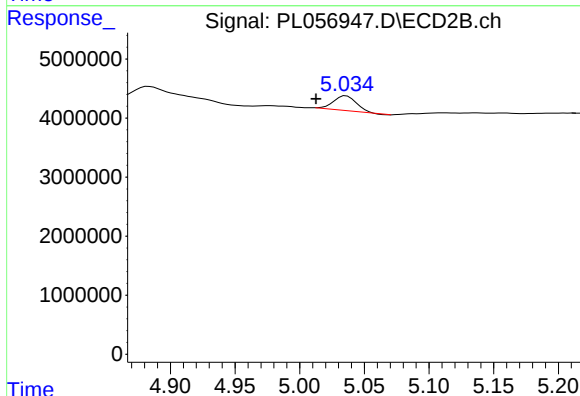


#23 Chlordane-1

R.T.: 5.036 min
Delta R.T.: 0.023 min
Response: 3098868
Conc: 15.64 ng/ml

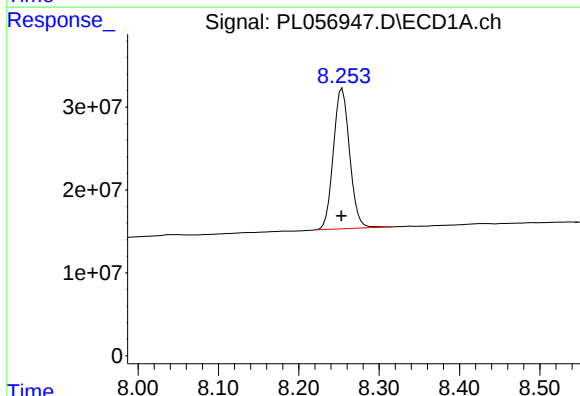

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 238461637
Conc: 12.01 ng/ml

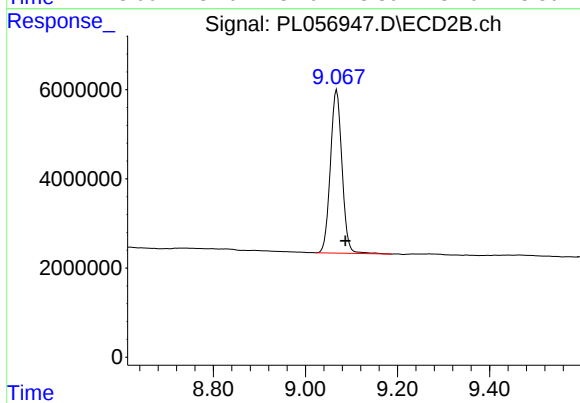

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.019 min
Response: 63984760
Conc: 15.12 ng/ml