

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 23:20
 Operator : AJ\MA
 Sample : L1743-18
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:03:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.003	213.6E6	72640891	11.942	13.555
28)	SA Decachlor...	8.254	9.069	174.7E6	45544664	8.793	10.761
Target Compounds							
2)	A alpha-BHC	0.000	4.429f	0	1020278	N.D.	0.124 #
4)	MA Heptachlor	0.000	5.205	0	1101338	N.D.	0.171 #
6)	B beta-BHC	0.000	4.888f	0	4448769	N.D.	1.334 #
10)	B gamma-Chl...	5.463f	6.106	14443747	1994132	0.529	0.333 #
11)	B alpha-Chl...	5.496	6.181	10212657	4236823	0.381	0.712 #
23)	Chlordane-1	4.371	5.037f	968133	2234898	1.390	11.277 #
25)	Chlordane-3	5.463f	6.106f	14443747	1994132	6.201	2.617 #
26)	Chlordane-4	5.496	6.181f	10212657	4236823	5.144	4.770


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 23:20
Operator : AJ\MA
Sample : L1743-18
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:03:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

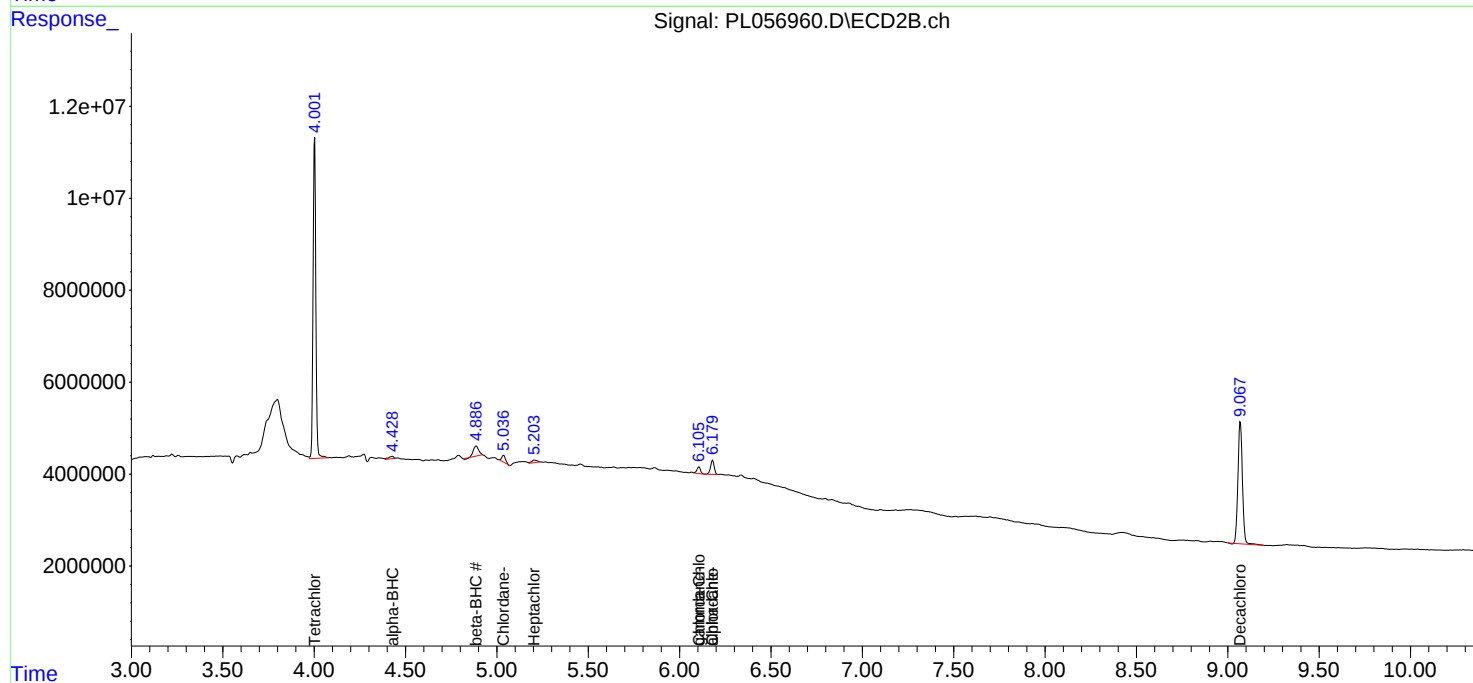


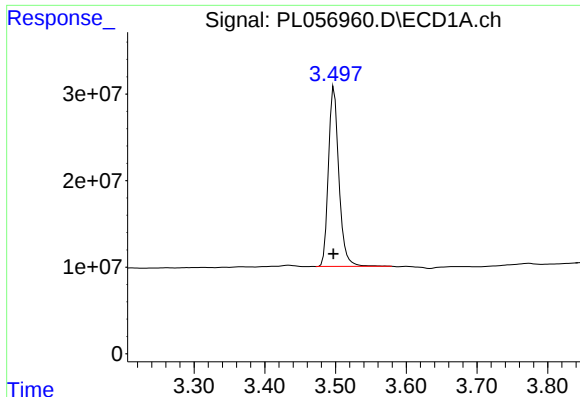

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.001 min
Response: 213569773
Conc: 11.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

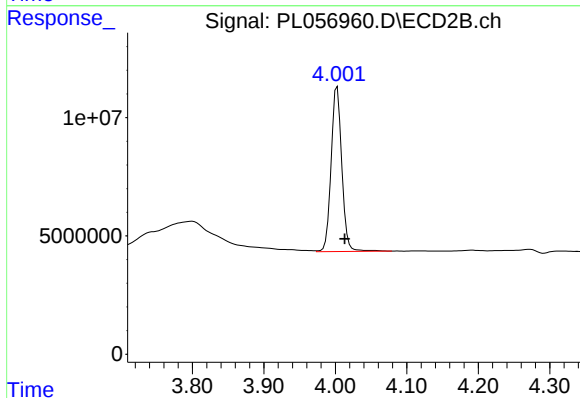


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.010 min
Response: 72640891
Conc: 13.56 ng/ml

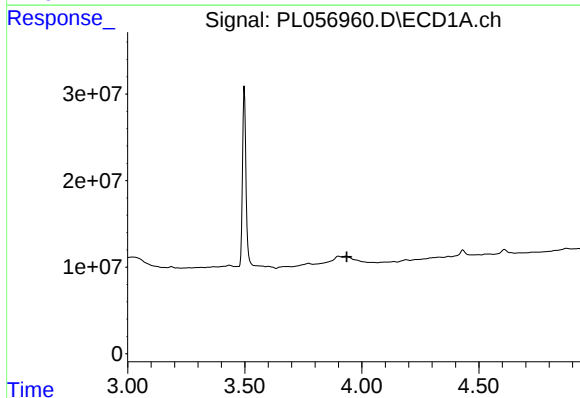


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

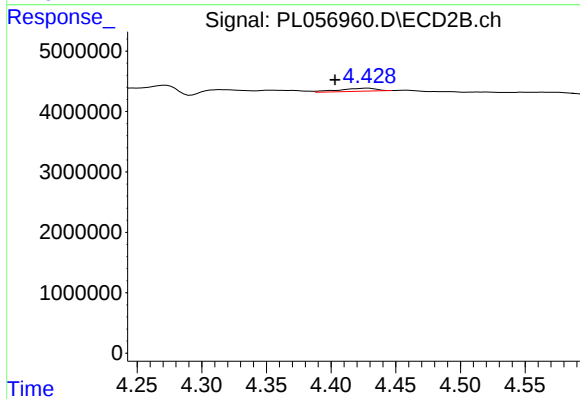

#2 alpha-BHC


R.T.: 4.429 min
Delta R.T.: 0.026 min
Response: 1020278
Conc: 0.12 ng/ml

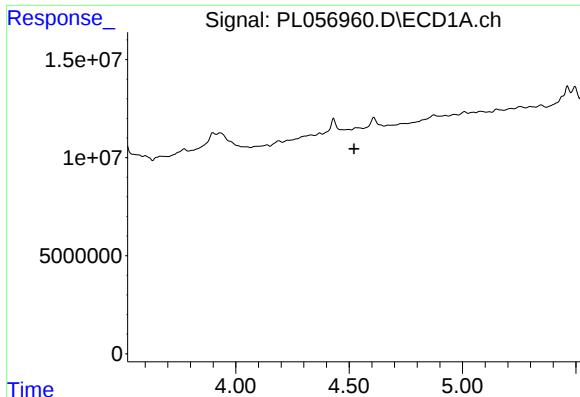

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.521 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

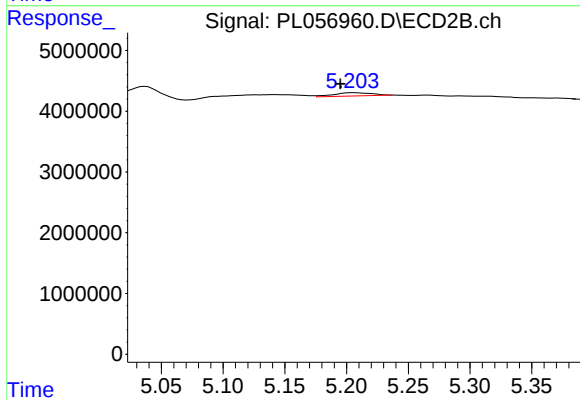


#4 Heptachlor

R.T.: 5.205 min
Delta R.T.: 0.010 min
Response: 1101338
Conc: 0.17 ng/ml

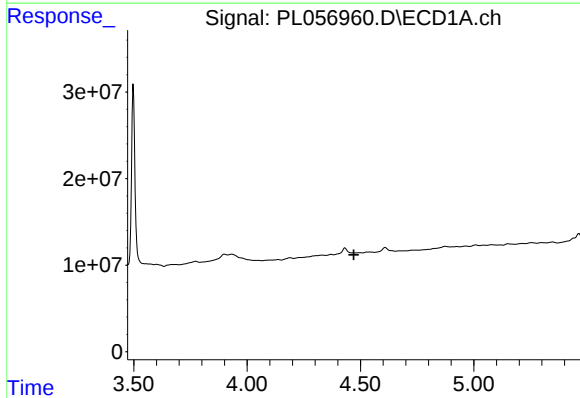


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.471 min
Response: 0
Conc: N.D.

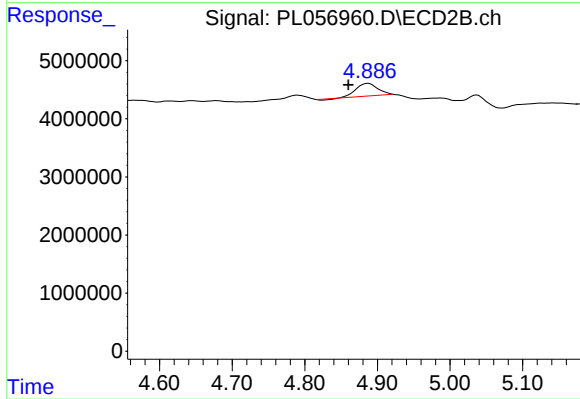

#6 beta-BHC


R.T.: 4.888 min
Delta R.T.: 0.028 min
Response: 4448769
Conc: 1.33 ng/ml

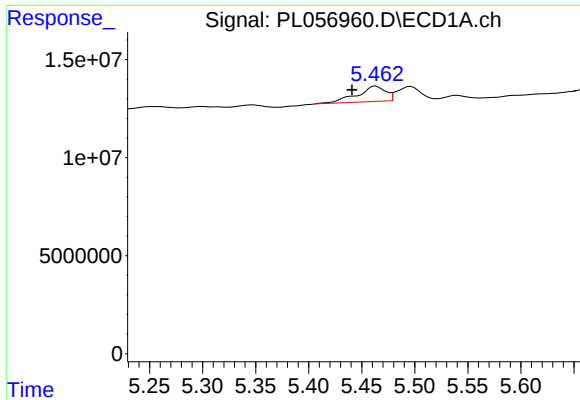

#10 gamma-Chlordane


R.T.: 5.463 min
Delta R.T.: 0.022 min
Response: 14443747
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

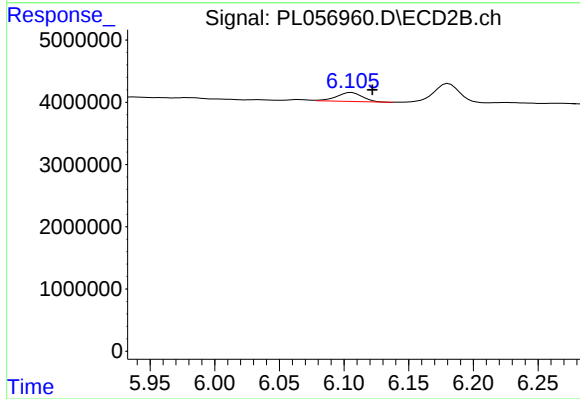


#10 gamma-Chlordane

R.T.: 6.106 min
Delta R.T.: -0.016 min
Response: 1994132
Conc: 0.33 ng/ml

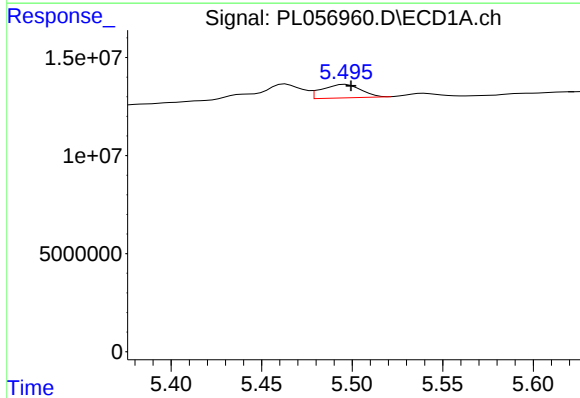


#11 alpha-Chlordane

R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 10212657
Conc: 0.38 ng/ml

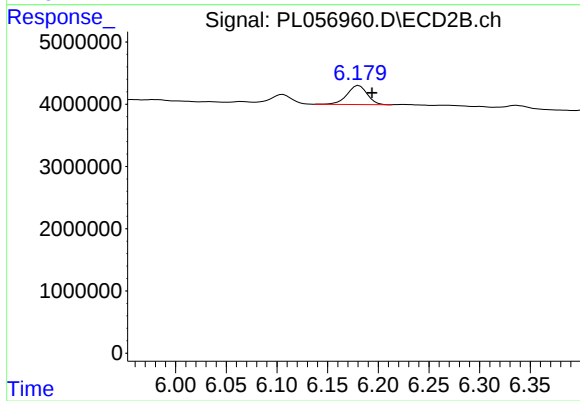

#11 alpha-Chlordane


R.T.: 6.181 min
Delta R.T.: -0.013 min
Response: 4236823
Conc: 0.71 ng/ml

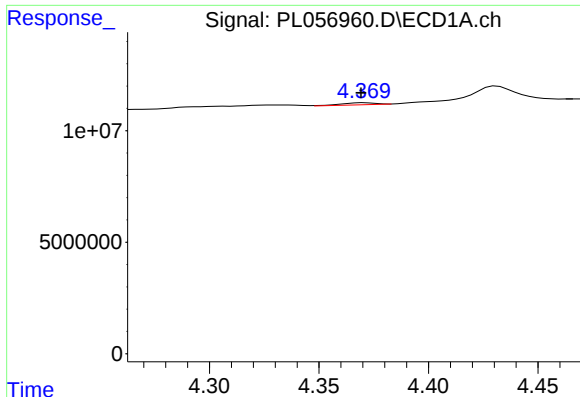

#23 Chlordane-1


R.T.: 4.371 min
Delta R.T.: 0.002 min
Response: 968133
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

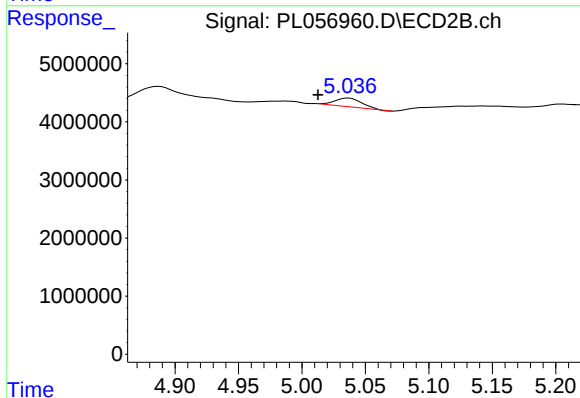


#23 Chlordane-1

R.T.: 5.037 min
Delta R.T.: 0.024 min
Response: 2234898
Conc: 11.28 ng/ml

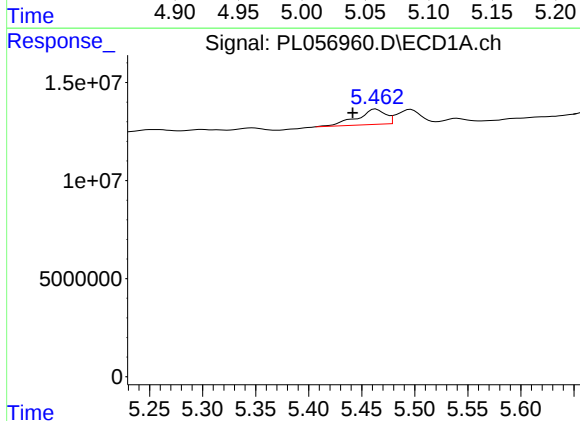


#25 Chlordane-3

R.T.: 5.463 min
Delta R.T.: 0.022 min
Response: 14443747
Conc: 6.20 ng/ml

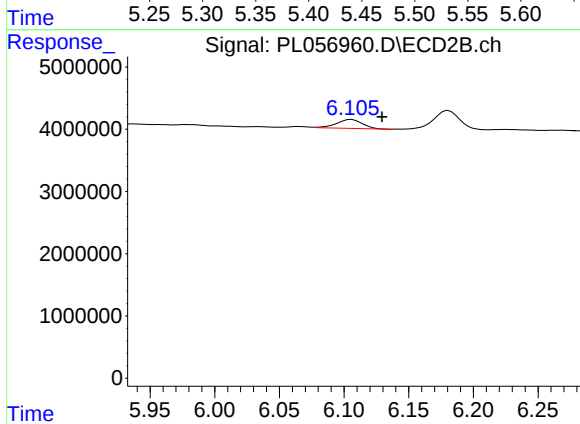

#25 Chlordane-3


R.T.: 6.106 min
Delta R.T.: -0.024 min
Response: 1994132
Conc: 2.62 ng/ml

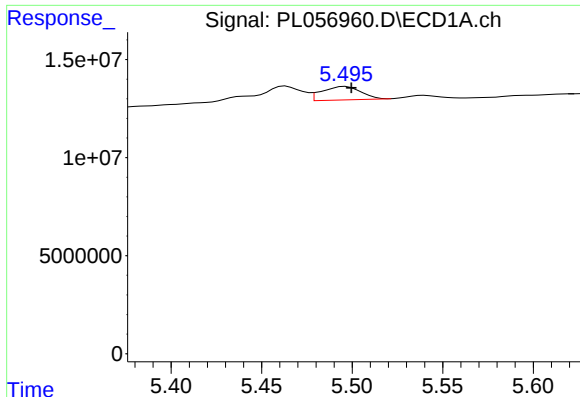

#26 Chlordane-4


R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 10212657
Conc: 5.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

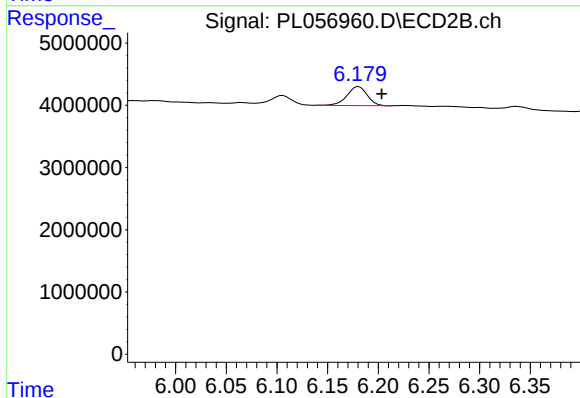


#26 Chlordane-4

R.T.: 6.181 min
Delta R.T.: -0.022 min
Response: 4236823
Conc: 4.77 ng/ml

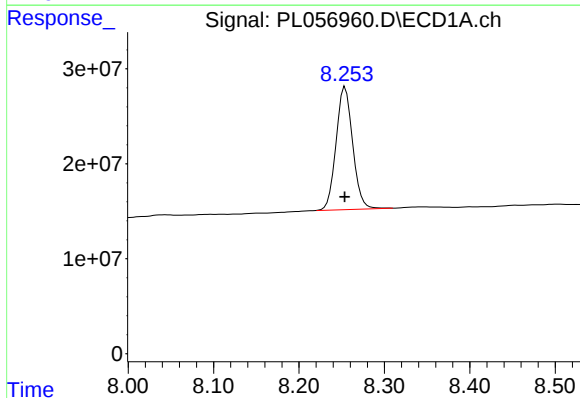

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 174663126
Conc: 8.79 ng/ml

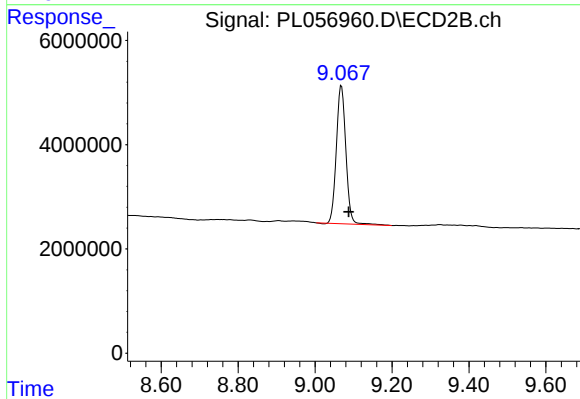

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: -0.018 min
Response: 45544664
Conc: 10.76 ng/ml