

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
 Data File : PL056927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2020 15:06
 Operator : AJ\MA
 Sample : L1744-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 05:54:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 27 13:35:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.001	373.1E6	125.3E6	20.862	23.375
28)	SA Decachlor...	8.253	9.066	389.4E6	90896741	19.603	21.477
Target Compounds							
12)	B 4,4'-DDE	5.663	6.337	16257674	4124097	0.632	0.708



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030220\
Data File : PL056927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2020 15:06
Operator : AJ\MA
Sample : L1744-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 05:54:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022720.M
Quant Title : GC Extractables
QLast Update : Thu Feb 27 13:35:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

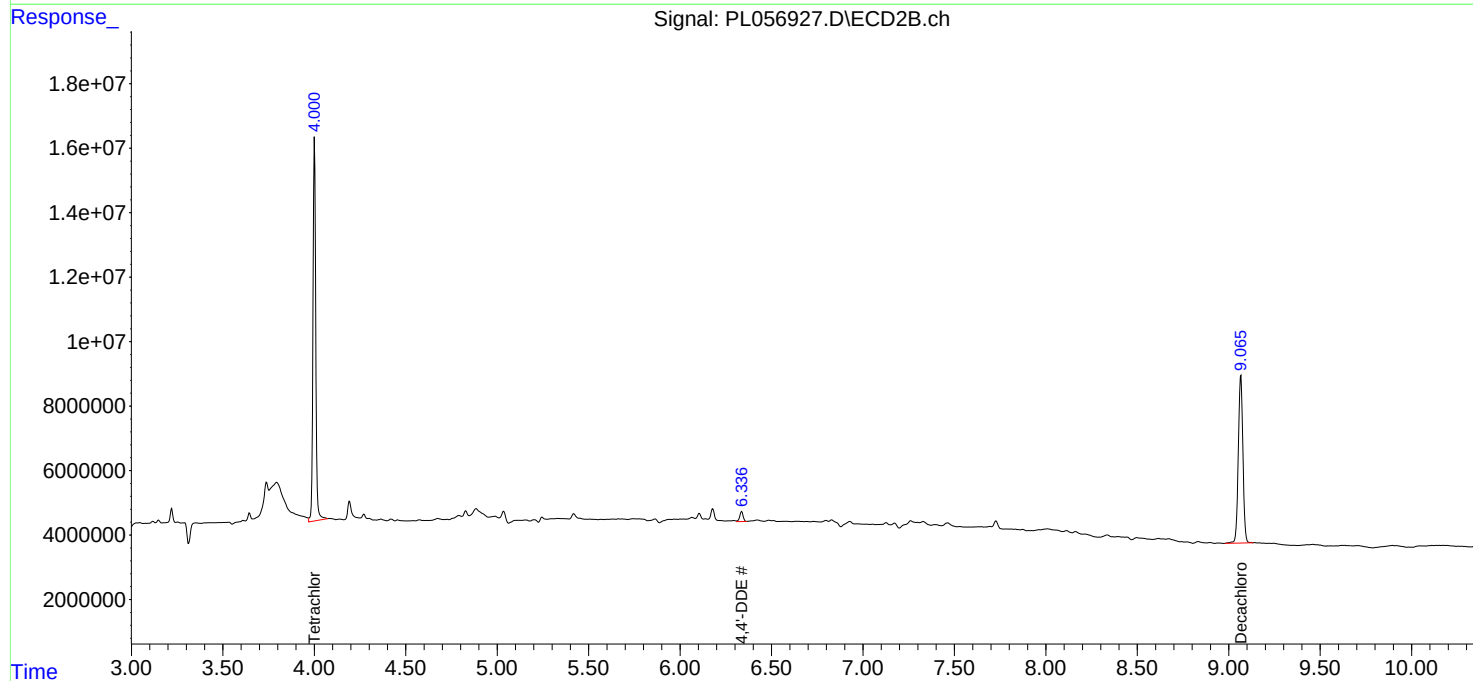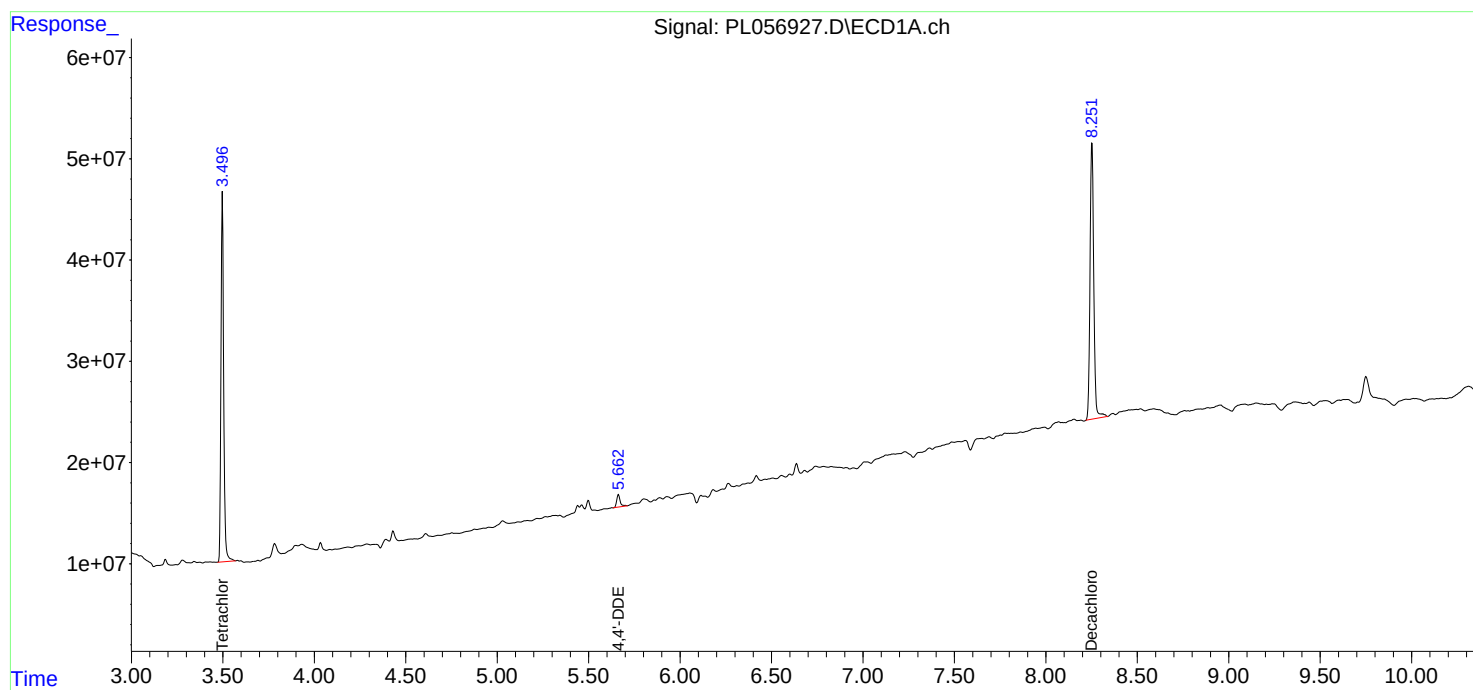


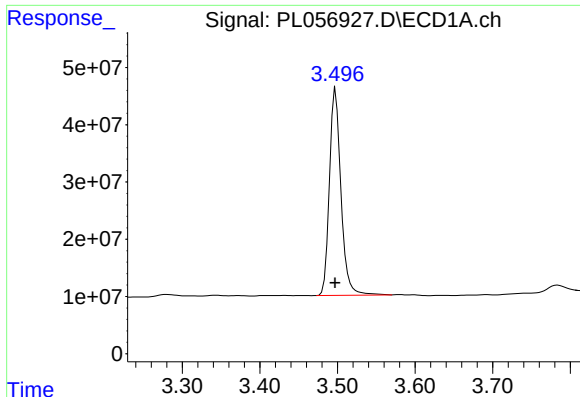

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 373078521
Conc: 20.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

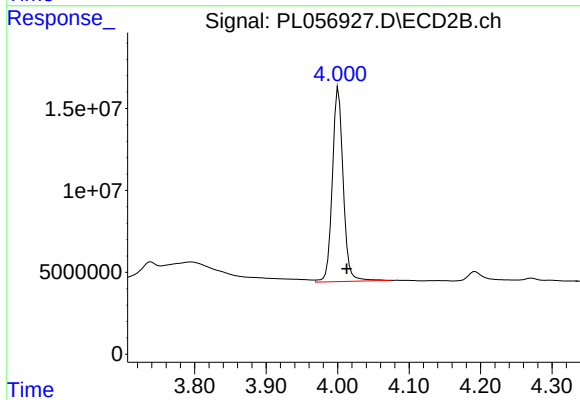


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.012 min
Response: 125264805
Conc: 23.37 ng/ml

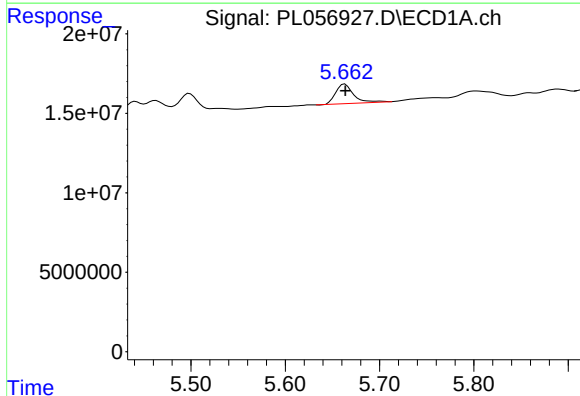


#12 4,4'-DDE

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 16257674
Conc: 0.63 ng/ml

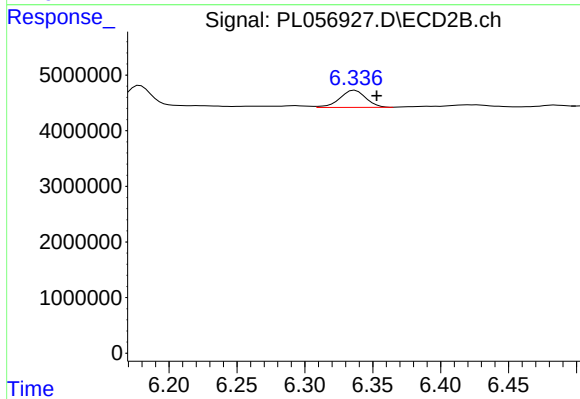

#12 4,4'-DDE


R.T.: 6.337 min
Delta R.T.: -0.016 min
Response: 4124097
Conc: 0.71 ng/ml

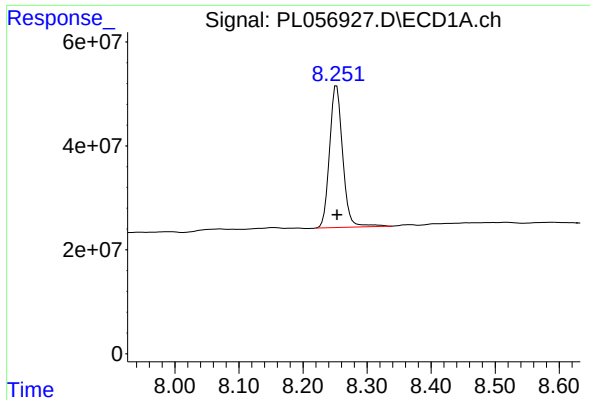

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 389375533
Conc: 19.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

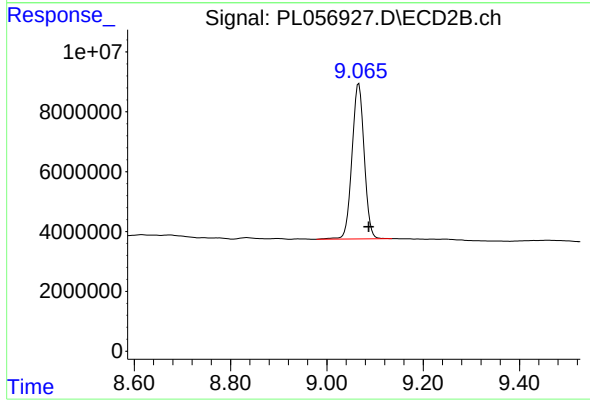

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: -0.021 min
Response: 90896741
Conc: 21.48 ng/ml