

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030221\
 Data File : PL065014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2021 14:21
 Operator : AR\AJ
 Sample : M1525-0110X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 15:46:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.099	6687673	5192508	2.377	2.404
28)	SA Decachlor...	8.146	9.256	5349443	4789500	2.379	2.522
Target Compounds							
5)	MB Aldrin	4.678	0.000	2897748	0	0.778	N.D. #
9)	A Endosulfan I	5.470	0.000	3953272	0	1.233	N.D. #
10)	B gamma-Chl...	5.369f	6.244	20673475	5186588	5.896	2.244 #
11)	B alpha-Chl...	5.404	6.316	11558238	13773474	3.337	5.983 #
12)	B 4,4'-DDE	5.571	0.000	4082129	0	1.304	N.D. #
23)	Chlordane-1	4.284	0.000	6750831	0	59.386	N.D. #
25)	Chlordane-3	5.369f	6.244	20673475	5186588	62.911	16.963 #
26)	Chlordane-4	5.404	6.316	11558238	13773474	42.008	37.178



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030221\
Data File : PL065014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2021 14:21
Operator : AR\AJ
Sample : M1525-0110X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 15:46:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

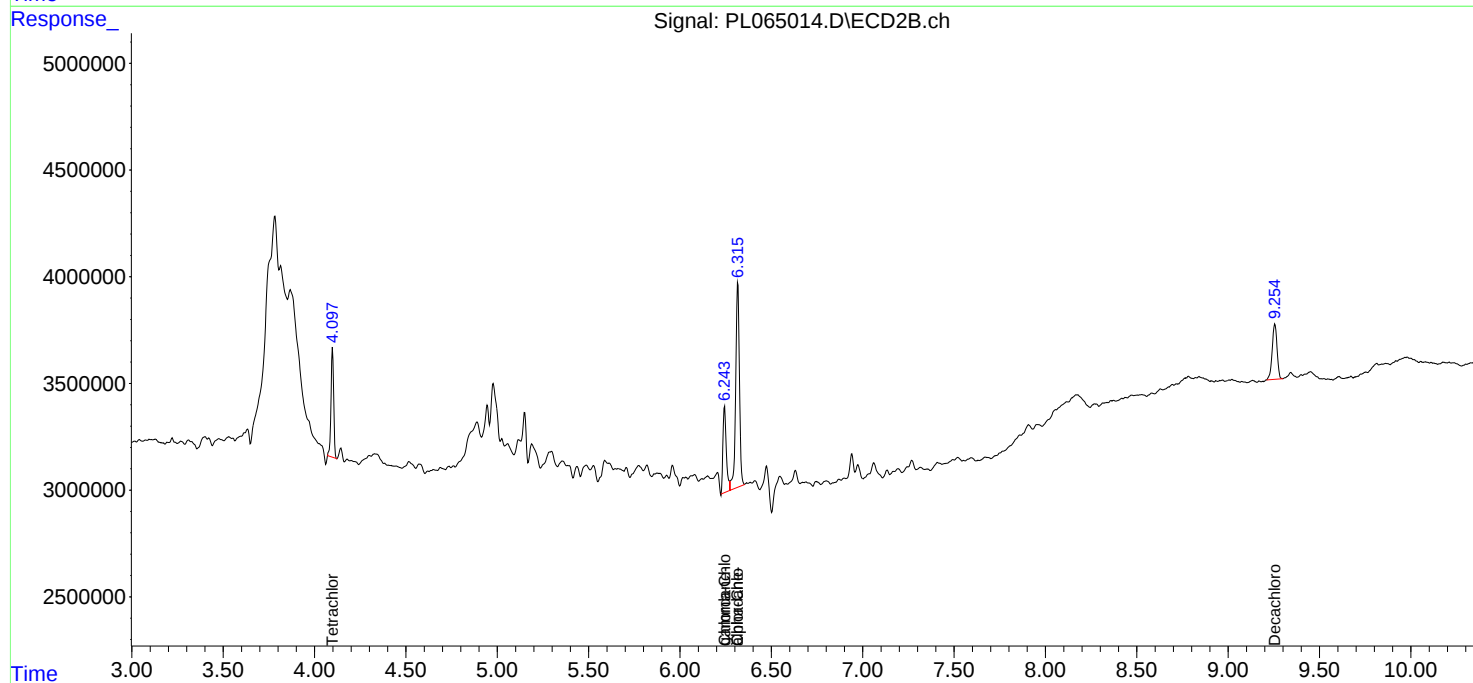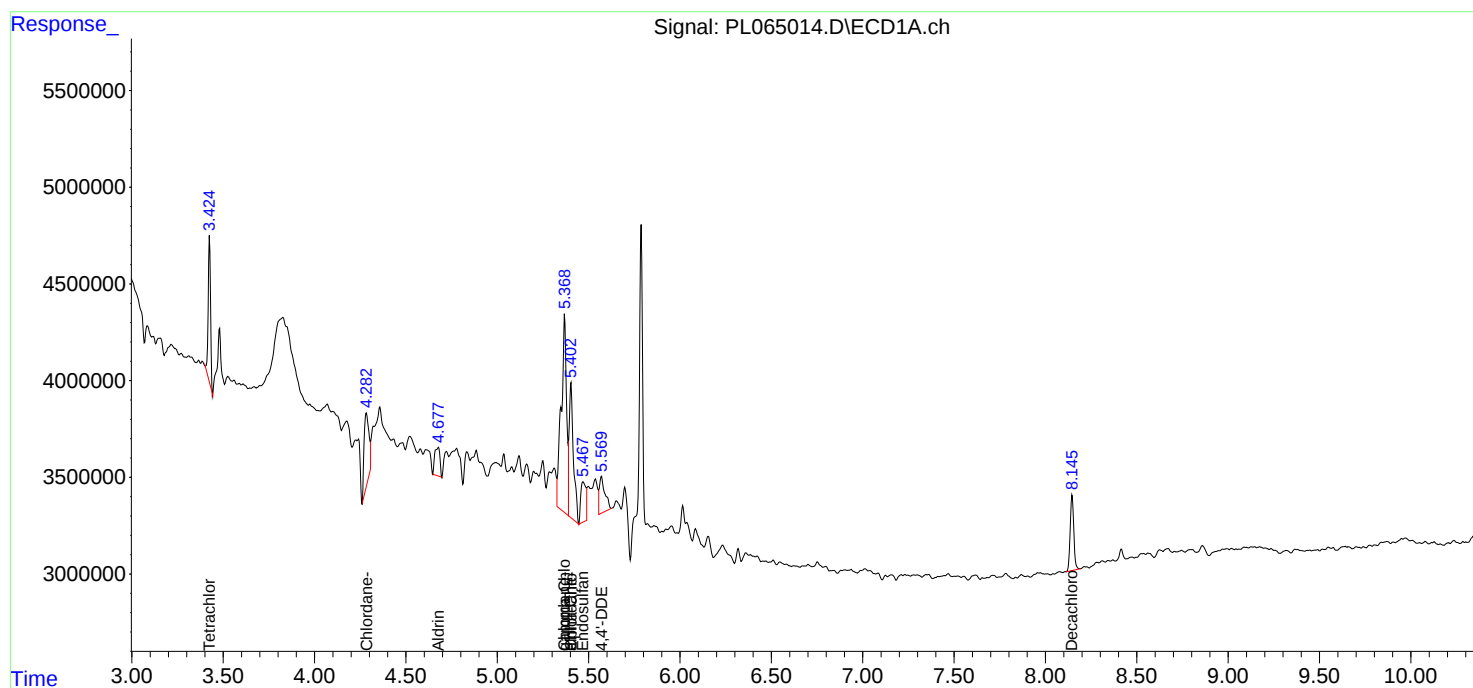


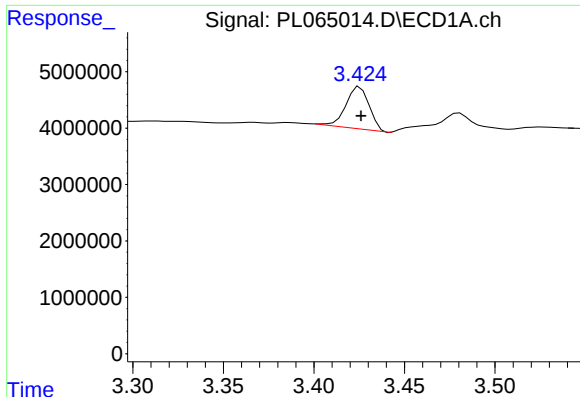

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 6687673
Conc: 2.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

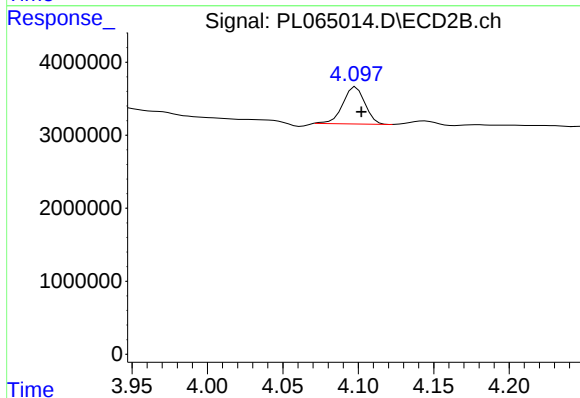


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.004 min
Response: 5192508
Conc: 2.40 ng/ml

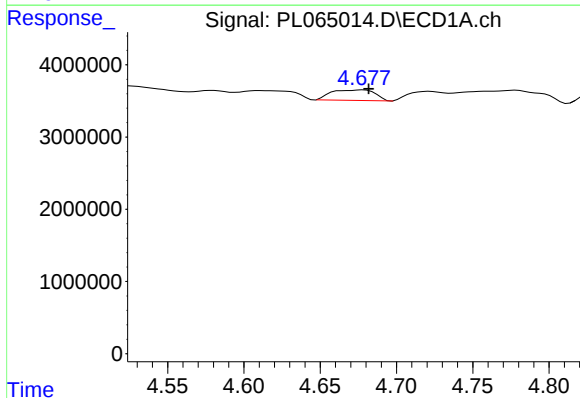


#5 Aldrin

R.T.: 4.678 min
Delta R.T.: -0.003 min
Response: 2897748
Conc: 0.78 ng/ml

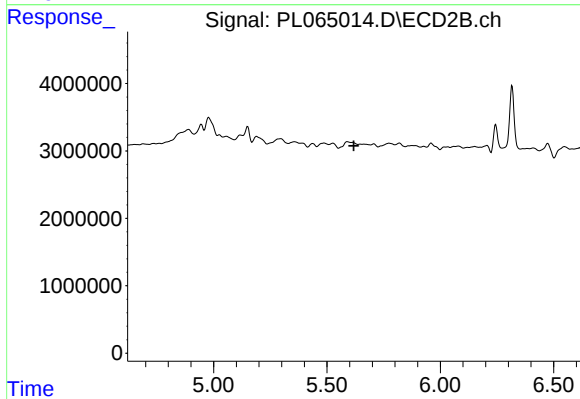

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

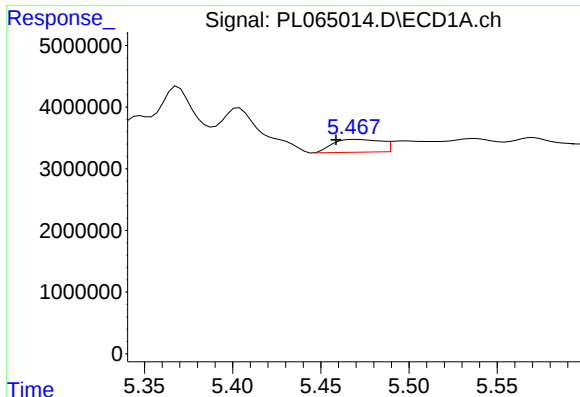

#9 Endosulfan I


R.T.: 5.470 min
Delta R.T.: 0.011 min
Response: 3953272
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

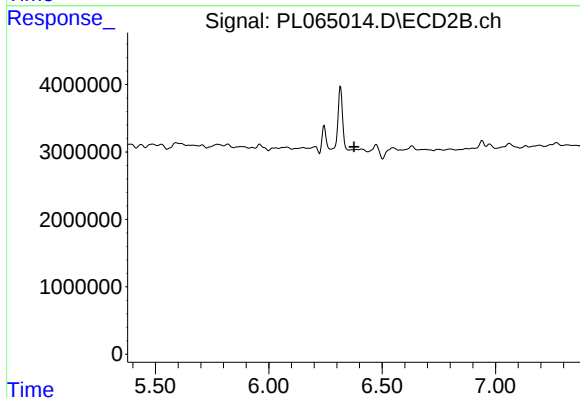


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

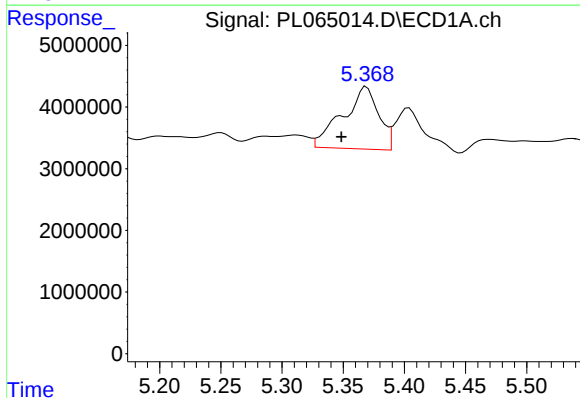


#10 gamma-Chlordane

R.T.: 5.369 min
Delta R.T.: 0.020 min
Response: 20673475
Conc: 5.90 ng/ml

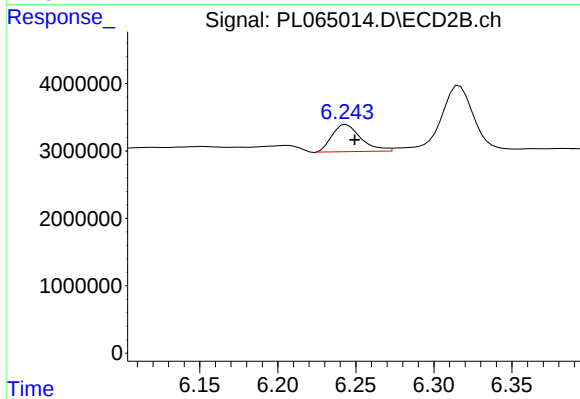

#10 gamma-Chlordane


R.T.: 6.244 min
Delta R.T.: -0.005 min
Response: 5186588
Conc: 2.24 ng/ml

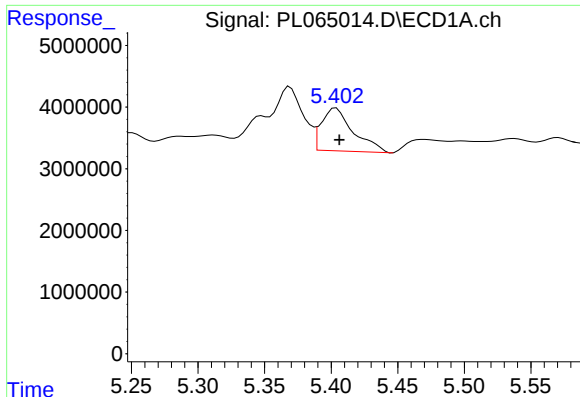

#11 alpha-Chlordane


R.T.: 5.404 min
Delta R.T.: -0.002 min
Response: 11558238
Conc: 3.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

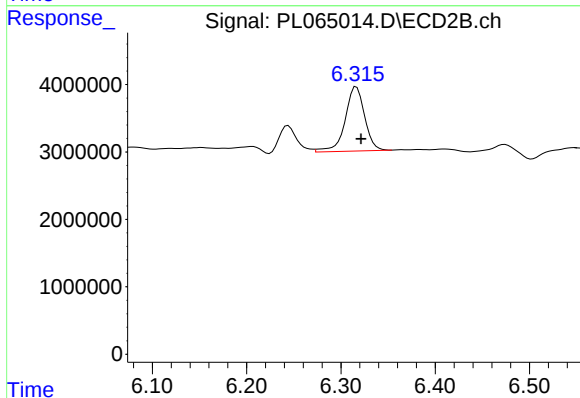


#11 alpha-Chlordane

R.T.: 6.316 min
Delta R.T.: -0.005 min
Response: 13773474
Conc: 5.98 ng/ml

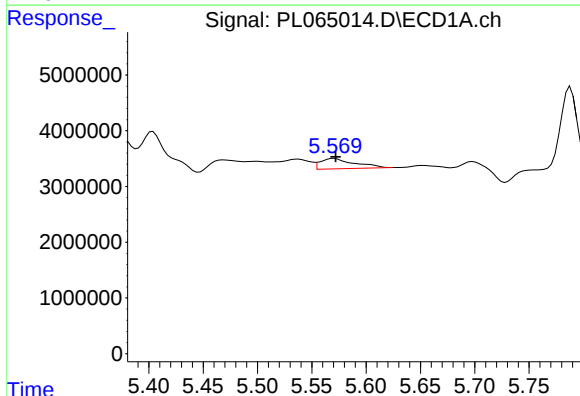


#12 4,4'-DDE

R.T.: 5.571 min
Delta R.T.: -0.001 min
Response: 4082129
Conc: 1.30 ng/ml

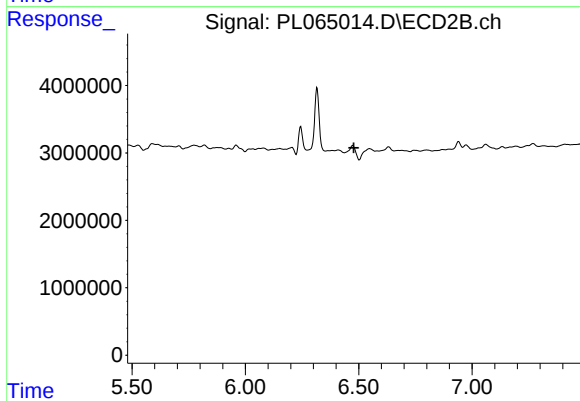

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.478 min
Response: 0
Conc: N.D.

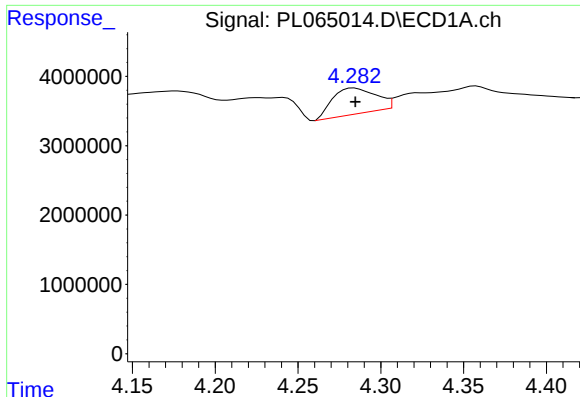

#23 Chlordane-1


R.T.: 4.284 min
Delta R.T.: 0.000 min
Response: 6750831
Conc: 59.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

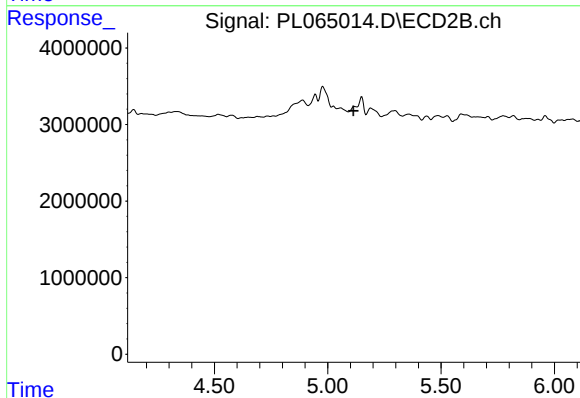


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

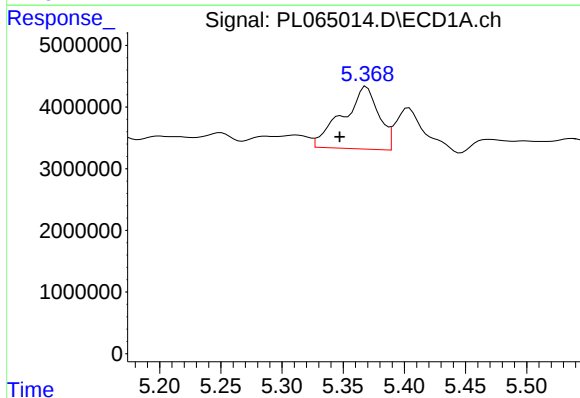


#25 Chlordane-3

R.T.: 5.369 min
Delta R.T.: 0.022 min
Response: 20673475
Conc: 62.91 ng/ml

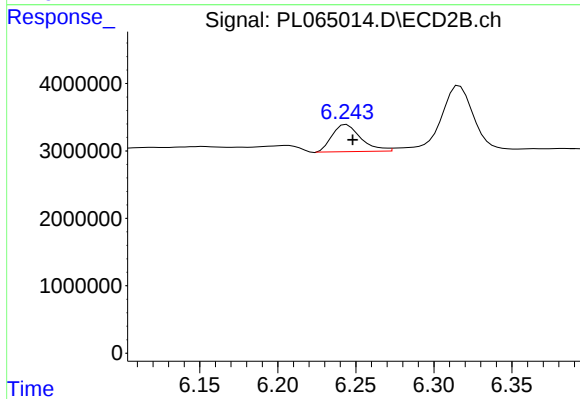

#25 Chlordane-3


R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 5186588
Conc: 16.96 ng/ml

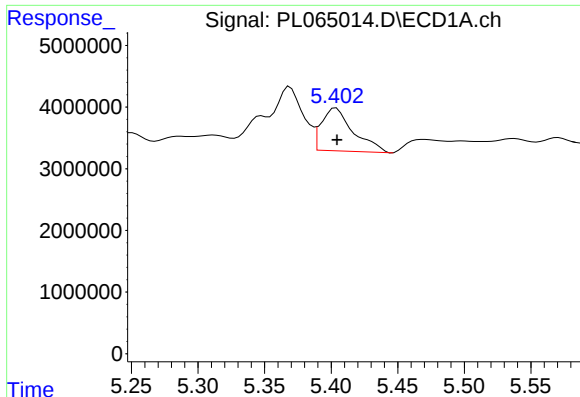

#26 Chlordane-4


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 11558238
Conc: 42.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

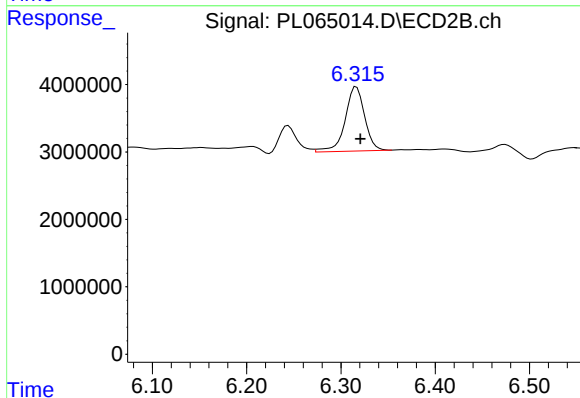


#26 Chlordane-4

R.T.: 6.316 min
Delta R.T.: -0.004 min
Response: 13773474
Conc: 37.18 ng/ml

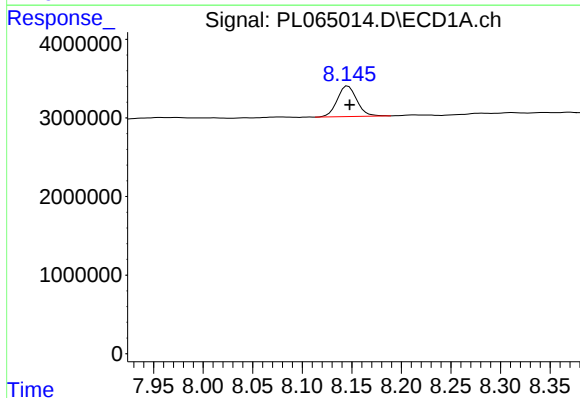

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 5349443
Conc: 2.38 ng/ml

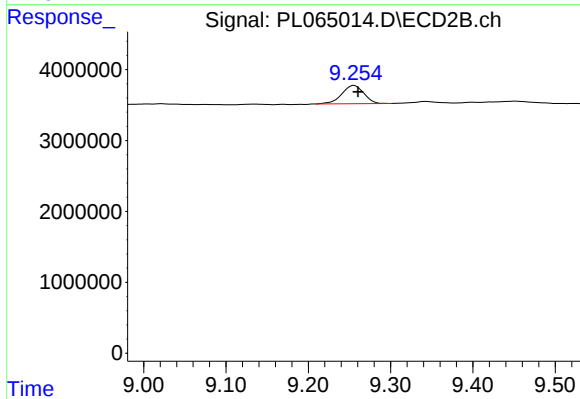

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 4789500
Conc: 2.52 ng/ml