

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030221\
 Data File : PL065007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2021 12:39
 Operator : AR\AJ
 Sample : M1526-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 STOCK-PILE

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:17:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 15:44:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	4.099	53608952	46837044	19.054	21.682
28)	SA Decachlor...	8.153	9.259	54197974	44174843	24.101	23.258
Target Compounds							
10)	B gamma-Chl...	5.353	6.249	2025994	1070168	0.578m	0.463m
11)	B alpha-Chl...	5.410	6.319	1717807	2042937	0.496m	0.887m#
17)	MA 4,4'-DDT	6.327	7.267	2082066	12184211	0.923m	7.991m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030221\
Data File : PL065007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2021 12:39
Operator : AR\AJ
Sample : M1526-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 15:44:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

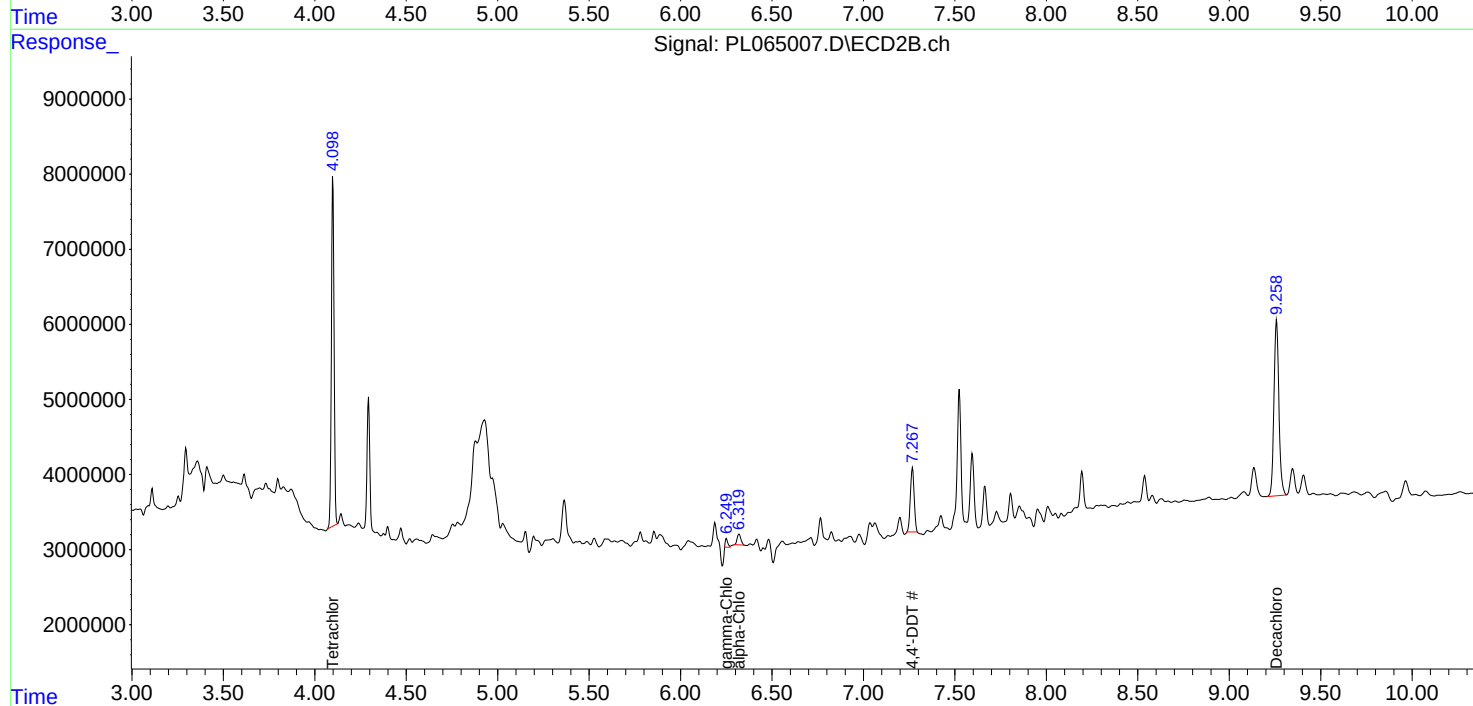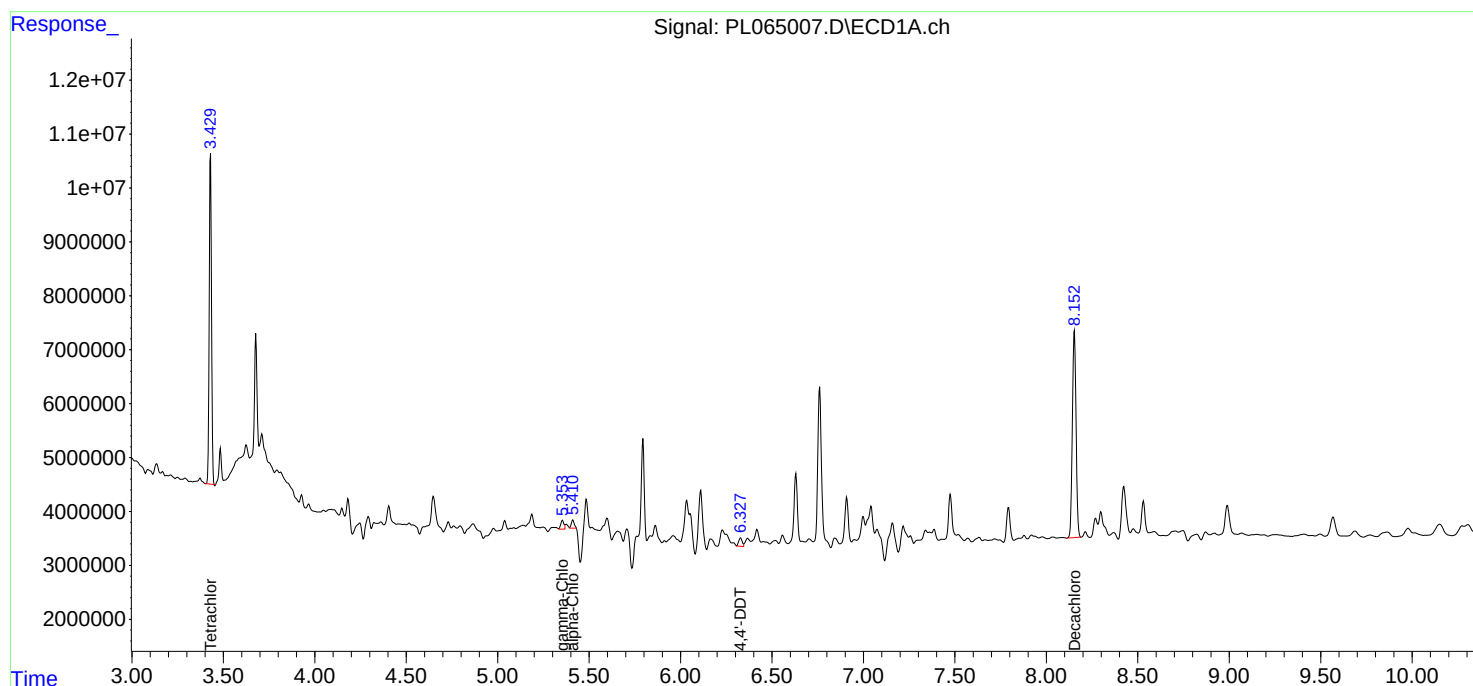

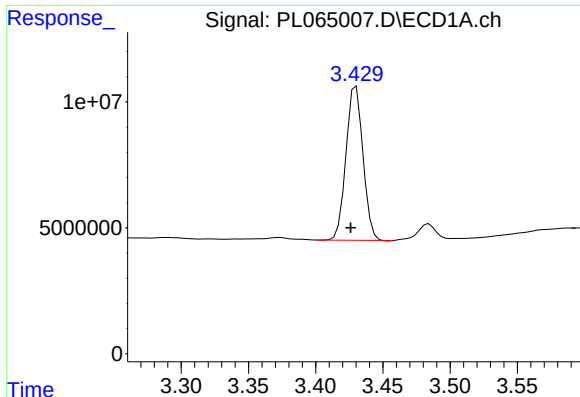


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: 0.004 min
Response: 53608952
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:12 AM

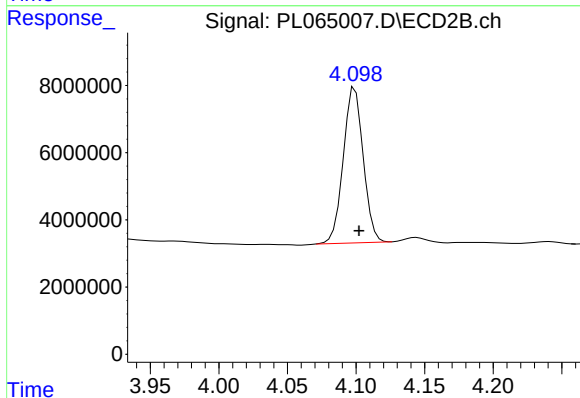


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.003 min
Response: 46837044
Conc: 21.68 ng/ml

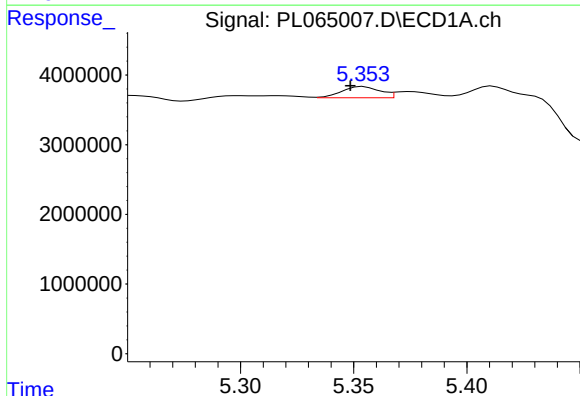


#10 gamma-Chlordane

R.T.: 5.353 min
Delta R.T.: 0.004 min
Response: 2025994
Conc: 0.58 ng/ml m

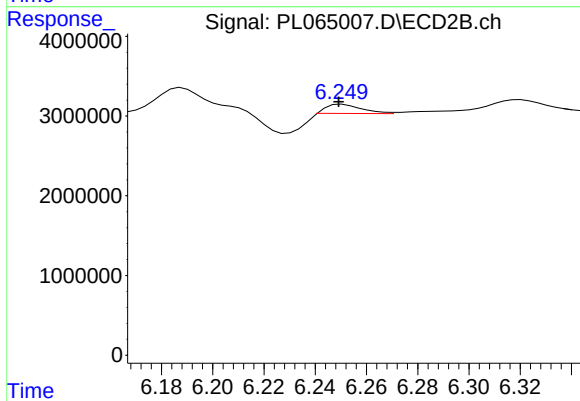

#10 gamma-Chlordane

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 1070168
Conc: 0.46 ng/ml m

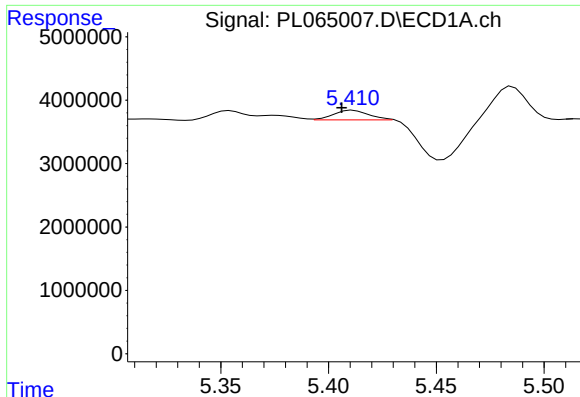


#11 alpha-Chlordane

R.T.: 5.410 min
Delta R.T.: 0.004 min
Response: 1717807
Conc: 0.50 ng/ml m

Instrument :
ECD_L
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:12 AM

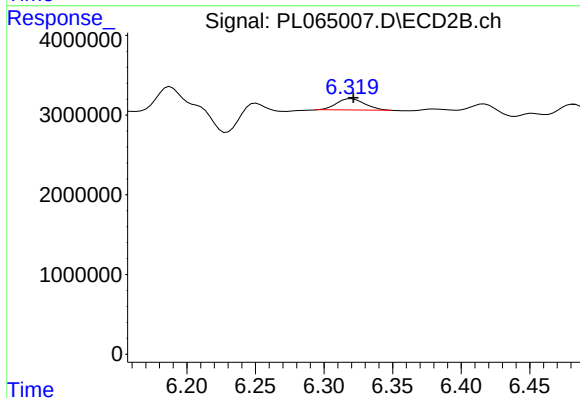


#11 alpha-Chlordane

R.T.: 6.319 min
Delta R.T.: -0.003 min
Response: 2042937
Conc: 0.89 ng/ml m

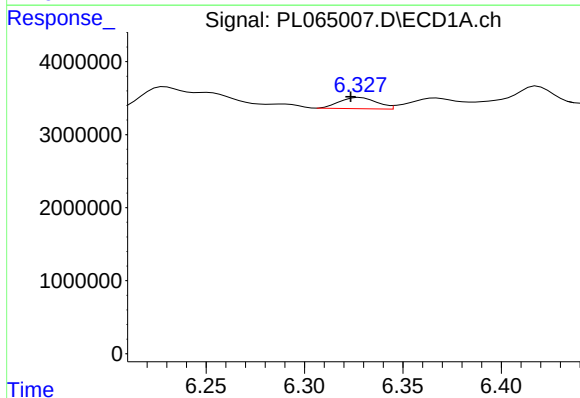


#17 4,4'-DDT

R.T.: 6.327 min
Delta R.T.: 0.003 min
Response: 2082066
Conc: 0.92 ng/ml m

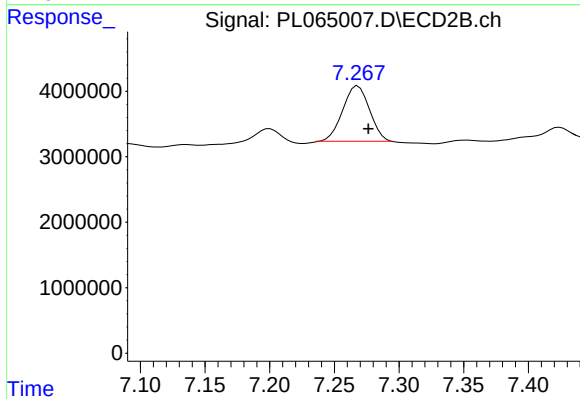

#17 4,4'-DDT

R.T.: 7.267 min
Delta R.T.: -0.009 min
Response: 12184211
Conc: 7.99 ng/ml m

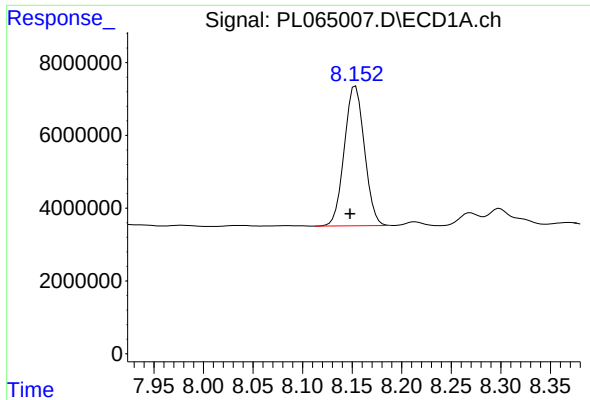


#28 Decachlorobiphenyl

R.T.: 8.153 min
Delta R.T.: 0.006 min
Response: 54197974
Conc: 24.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCK-PILE

Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:12 AM

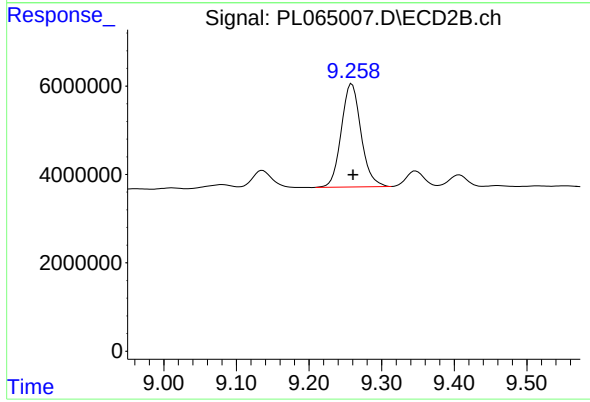

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 44174843
Conc: 23.26 ng/ml