

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 17:39
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 23:30:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 02 23:28:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	2.665	224.0E6	259.4E6	101.787	102.480
28)	SA Decachlor...	8.764	7.793	146.0E6	187.7E6	95.228	95.881
Target Compounds							
23)	Chlordane-1	4.481	3.657	98474653	83663421	1013.110	1009.611
24)	Chlordane-2	5.008	4.232	97190865	99105479	963.612	975.702
25)	Chlordane-3	5.714	4.861	378.6E6	285.2E6	1033.653	1046.578
26)	Chlordane-4	5.795	4.922	446.6E6	291.8E6	1019.591	1040.789
27)	Chlordane-5	6.636	5.589	72747138	71512735	998.625	1010.616



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 17:39
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 23:30:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 02 23:28:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

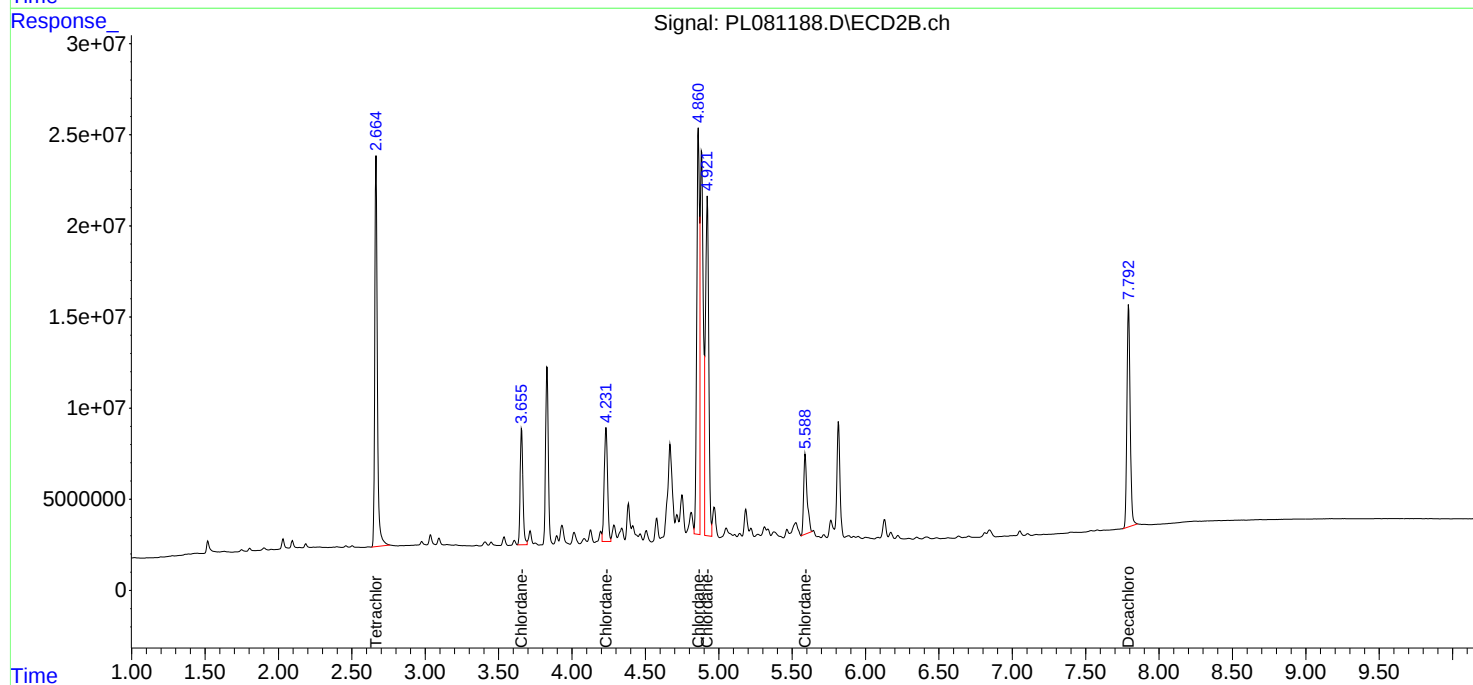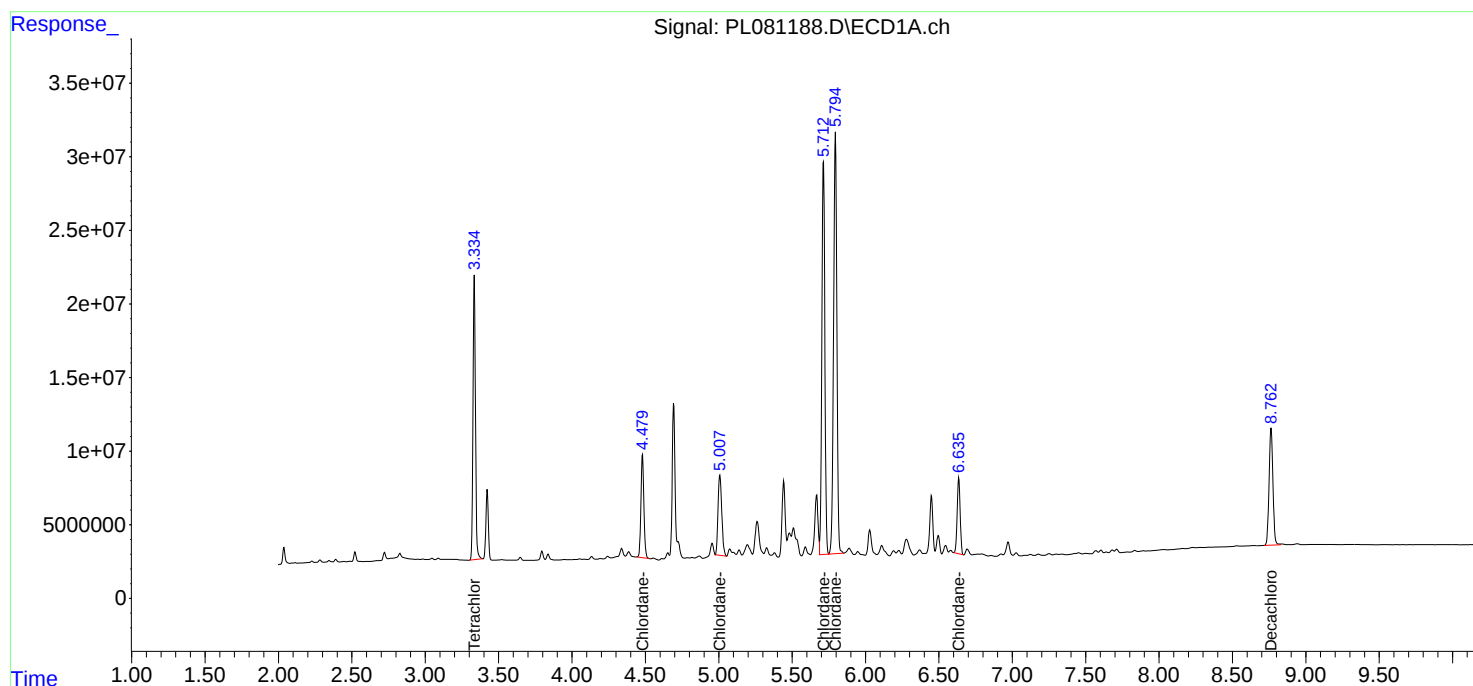


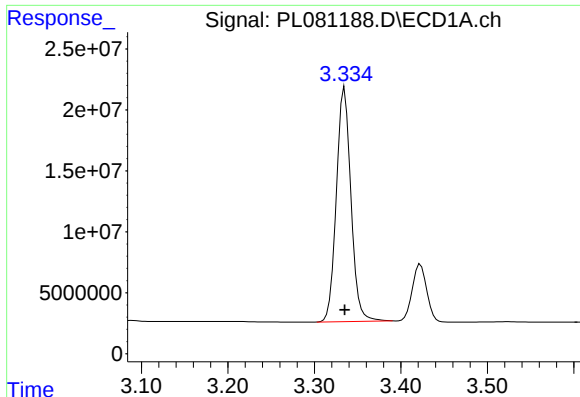

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 224048895
Conc: 101.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

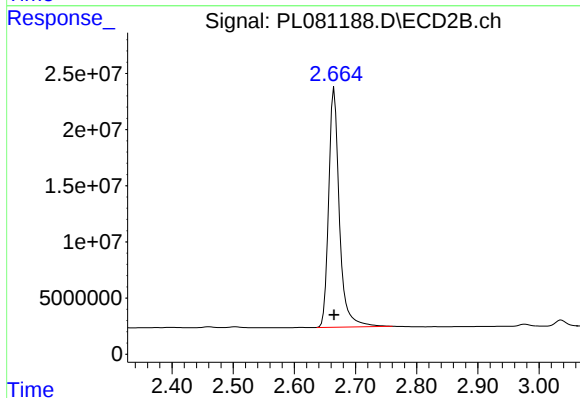


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 259360621
Conc: 102.48 ng/ml

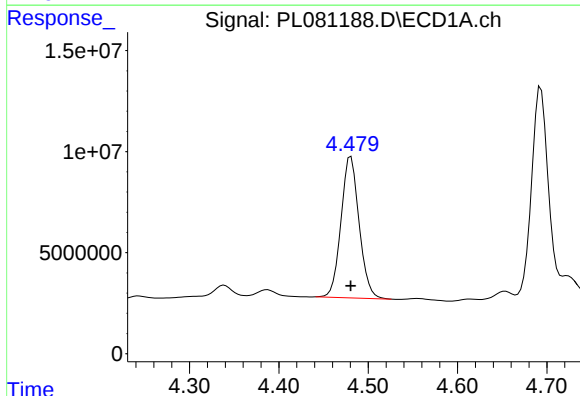


#23 Chlordane-1

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 98474653
Conc: 1013.11 ng/ml

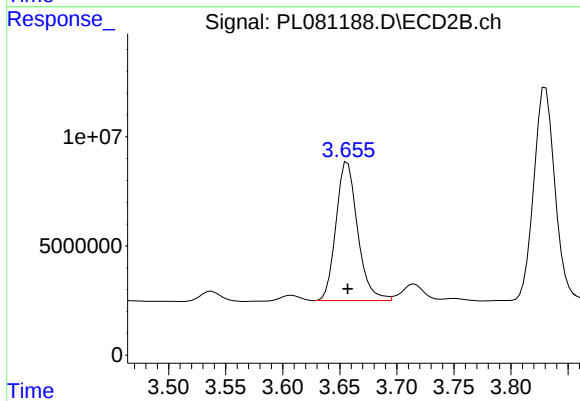

#23 Chlordane-1


R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 83663421
Conc: 1009.61 ng/ml

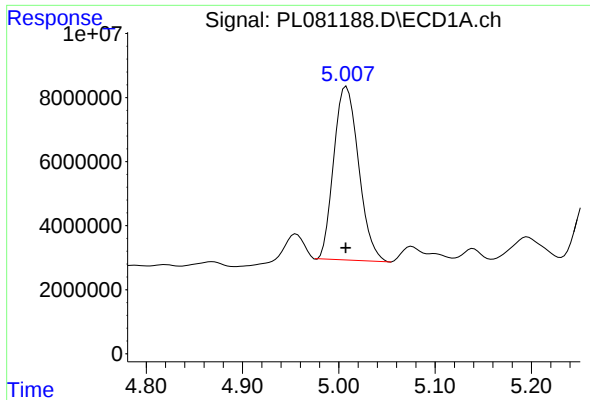

#24 Chlordane-2


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 97190865
Conc: 963.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

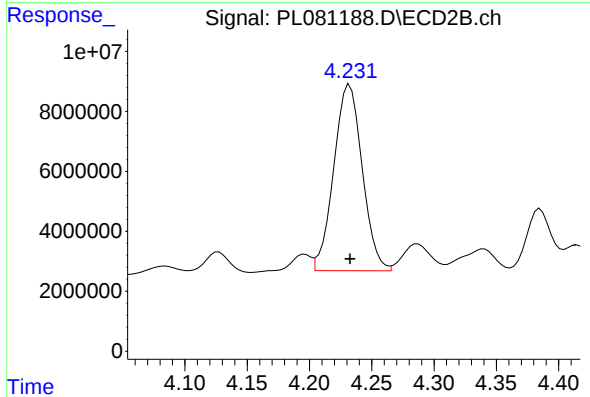


#24 Chlordane-2

R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 99105479
Conc: 975.70 ng/ml

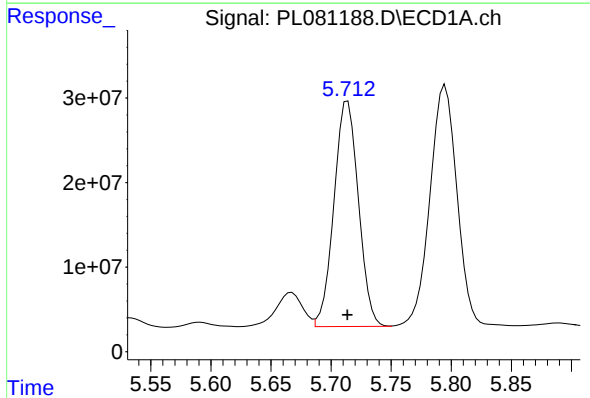


#25 Chlordane-3

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 378612322
Conc: 1033.65 ng/ml

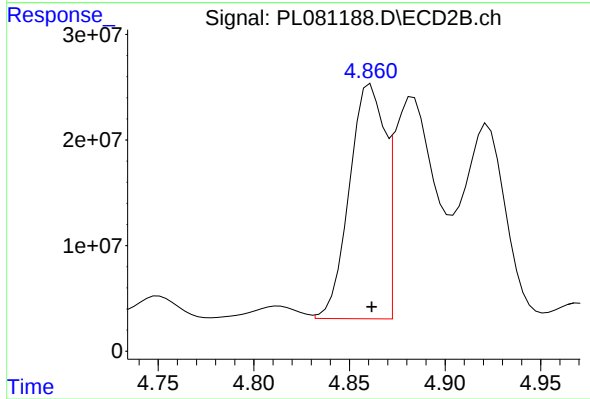

#25 Chlordane-3


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 285232619
Conc: 1046.58 ng/ml

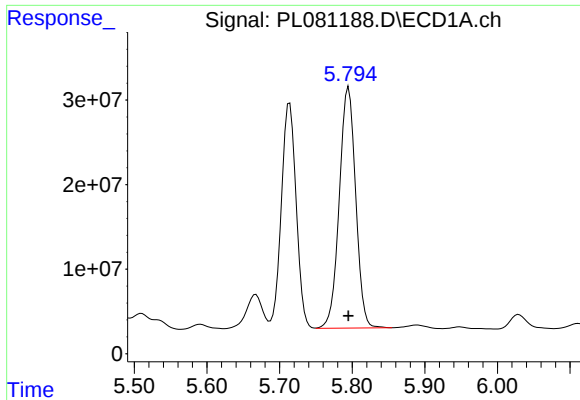

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 446631314
Conc: 1019.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

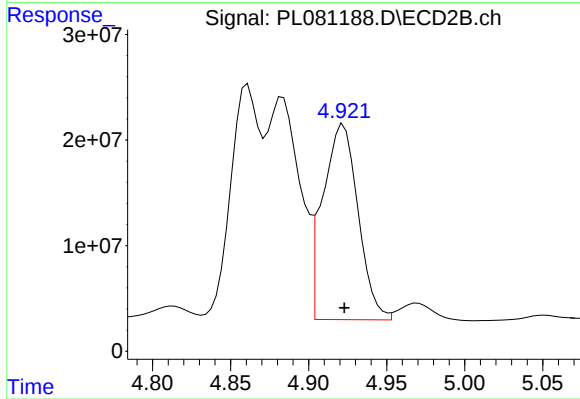


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 291767103
Conc: 1040.79 ng/ml

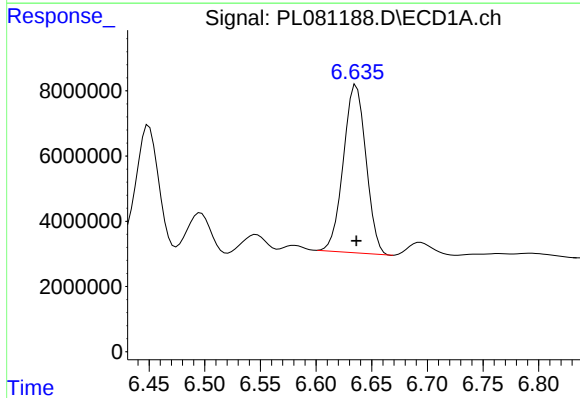


#27 Chlordane-5

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 72747138
Conc: 998.62 ng/ml

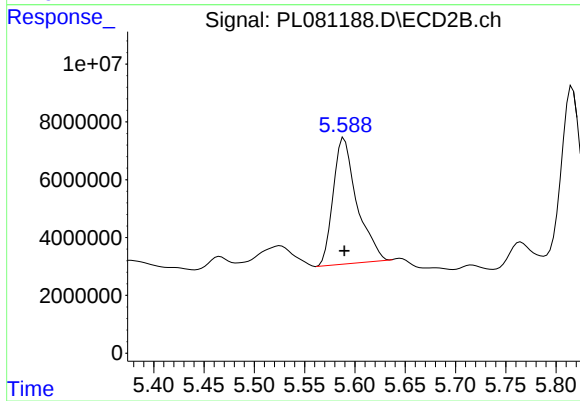

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 71512735
Conc: 1010.62 ng/ml

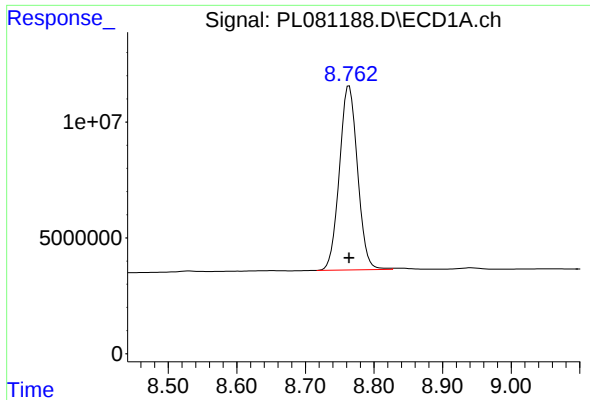

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 146025608
Conc: 95.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

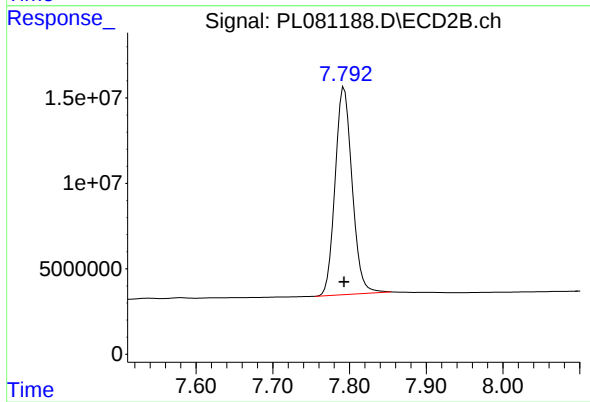

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 187671357
Conc: 95.88 ng/ml