

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 16:16
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 01:53:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.336	2.667	50338569	46270372	23.299	22.863
28) SA Decachlor...	8.765	7.794	35337323	44243408	23.179	23.097
Target Compounds						
9) A Endosulfan I	5.840	4.980	24933523	25238811	11.802	11.150
10) B gamma-Chl...	5.714	4.861	28772260	27477119	12.609	11.225
12) B 4,4'-DDE	5.970	5.115	44318843	42208112	22.651	21.503
13) MA Dieldrin	6.115	5.245	48286248	50202369	23.070	22.269
19) B Endosulfa...	6.929	6.220	38424036	40142072	21.400	20.885
20) A Methoxychlor	7.277	6.501	96312076	104.3E6	111.813	112.338
21) B Endrin ke...	7.408	6.726	41874167	49010077	23.084	22.763



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 16:16
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 01:53:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

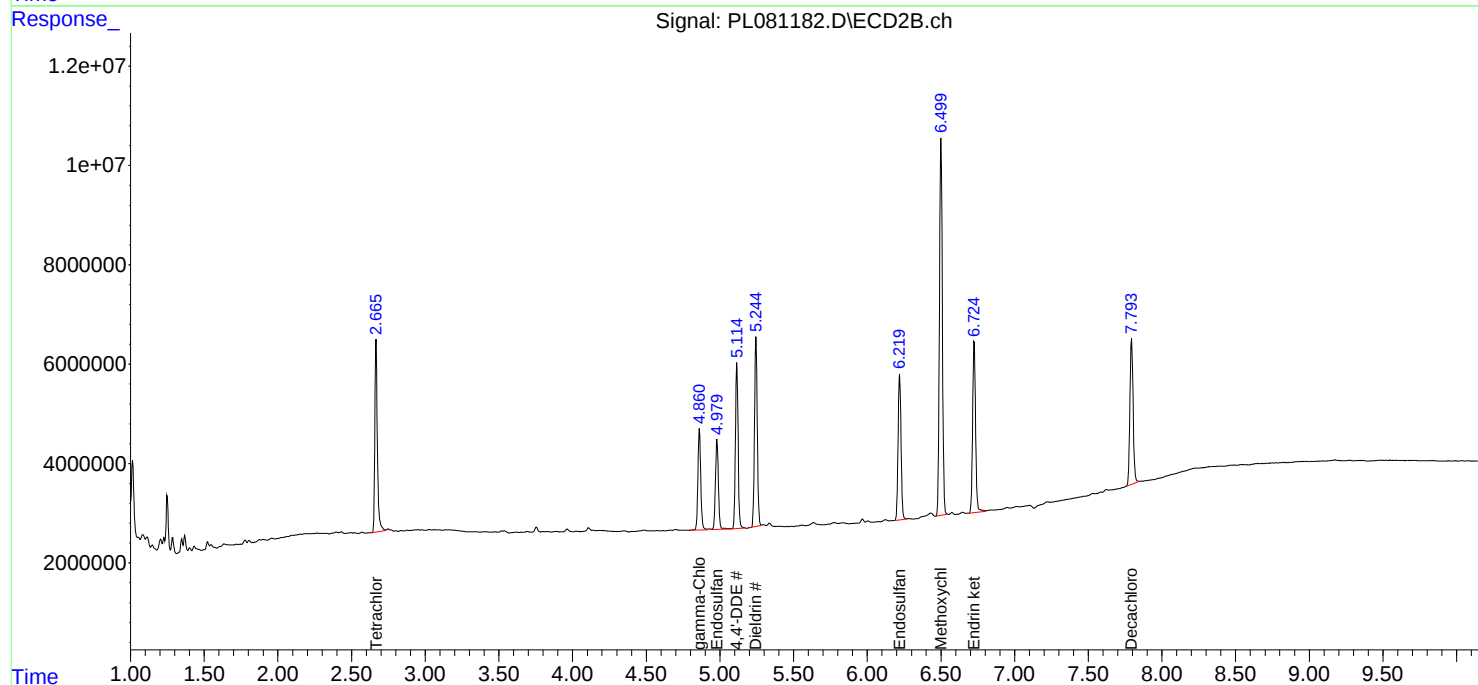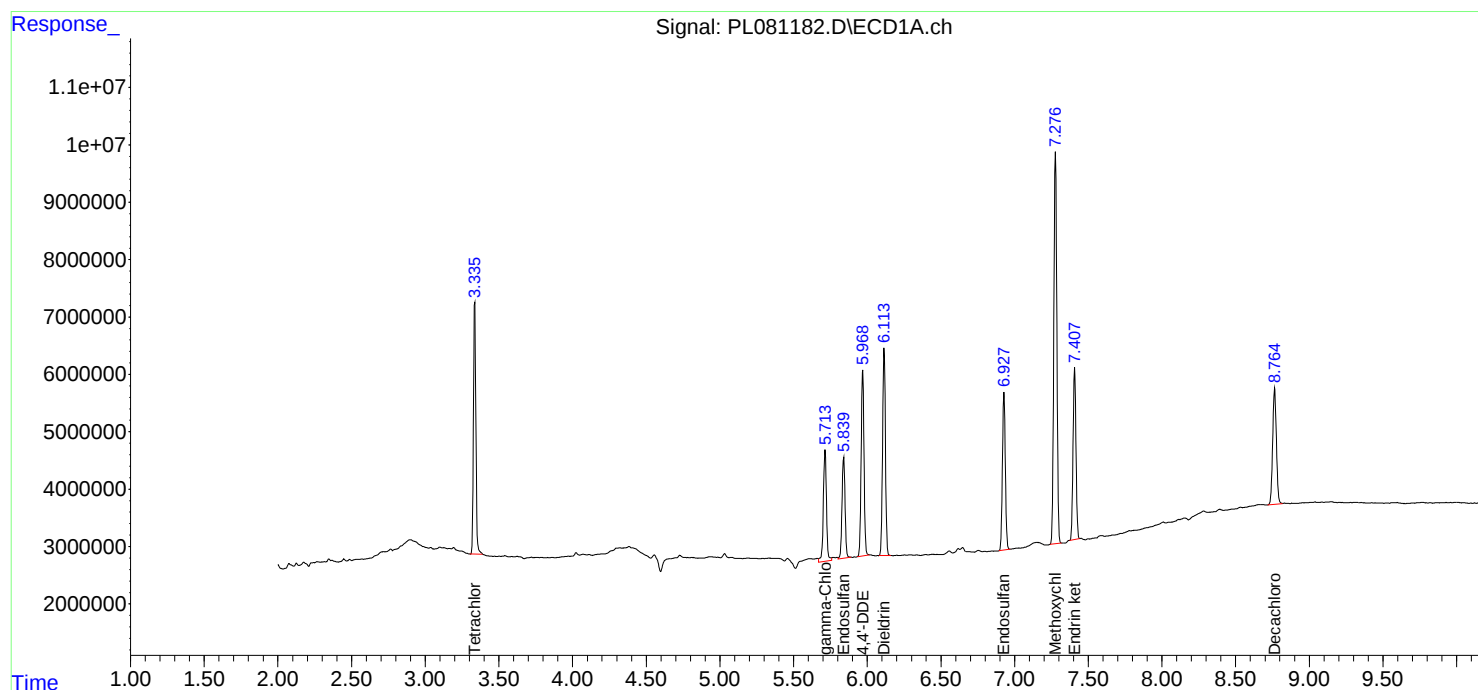


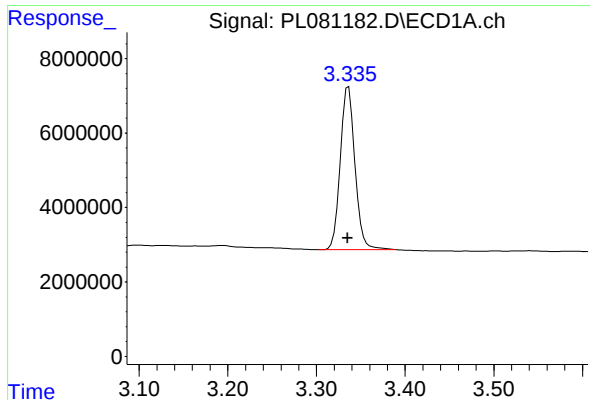

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.001 min
Response: 50338569
Conc: 23.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

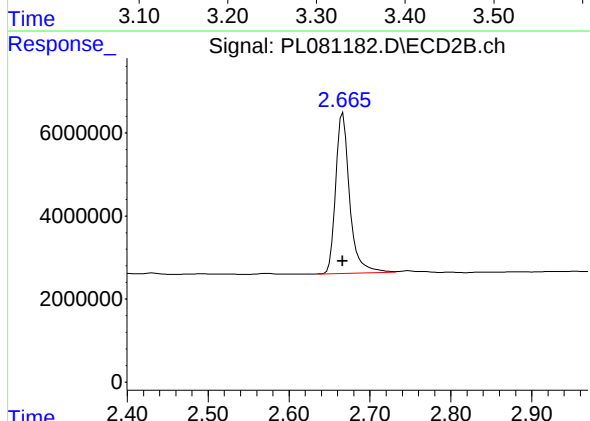


#1 Tetrachloro-m-xylene

R.T.: 2.667 min
Delta R.T.: 0.000 min
Response: 46270372
Conc: 22.86 ng/ml

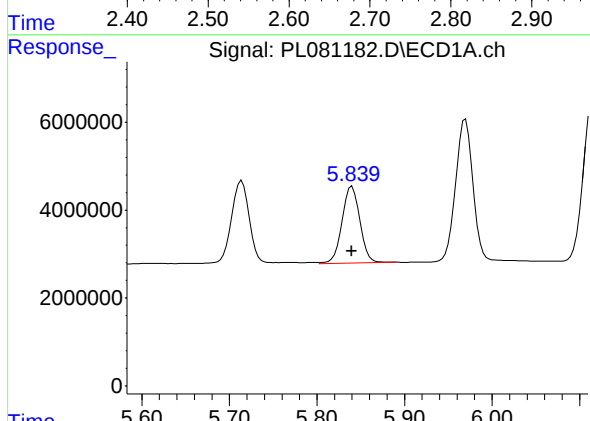


#9 Endosulfan I

R.T.: 5.840 min
Delta R.T.: 0.000 min
Response: 24933523
Conc: 11.80 ng/ml

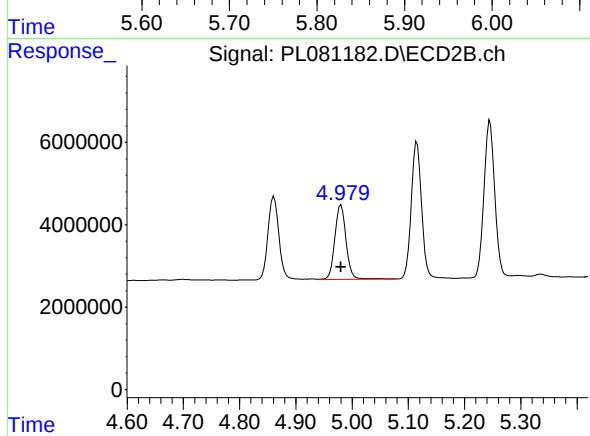

#9 Endosulfan I


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 25238811
Conc: 11.15 ng/ml

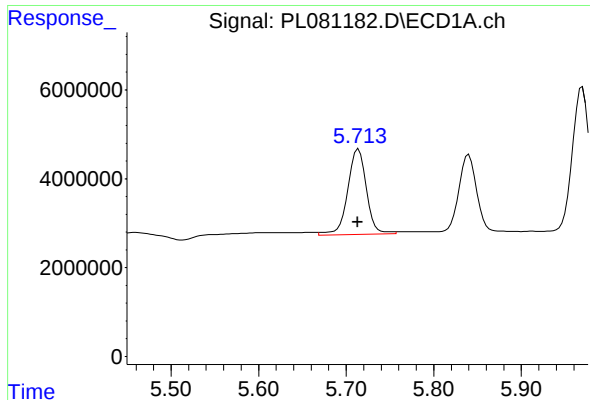

#10 gamma-Chlordane


R.T.: 5.714 min
Delta R.T.: 0.001 min
Response: 28772260
Conc: 12.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

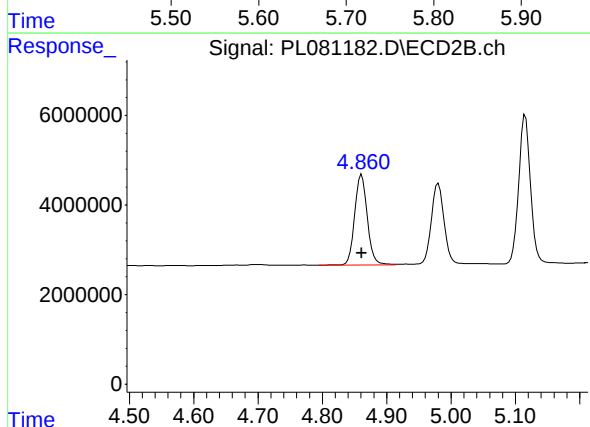


#10 gamma-Chlordane

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 27477119
Conc: 11.23 ng/ml

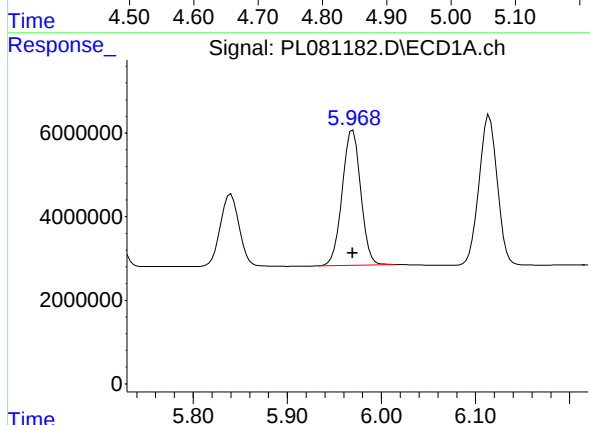


#12 4,4'-DDE

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 44318843
Conc: 22.65 ng/ml

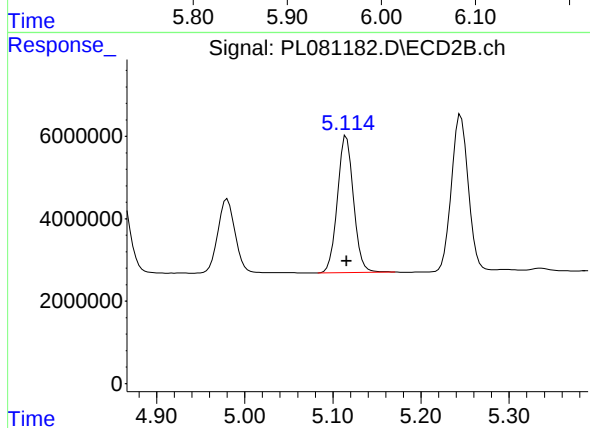

#12 4,4'-DDE


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 42208112
Conc: 21.50 ng/ml

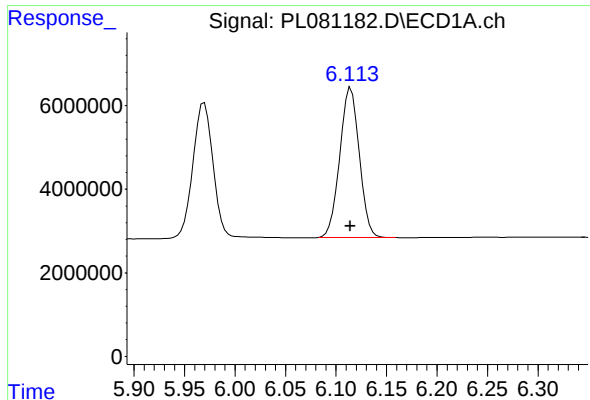

#13 Dieldrin


R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 48286248
Conc: 23.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

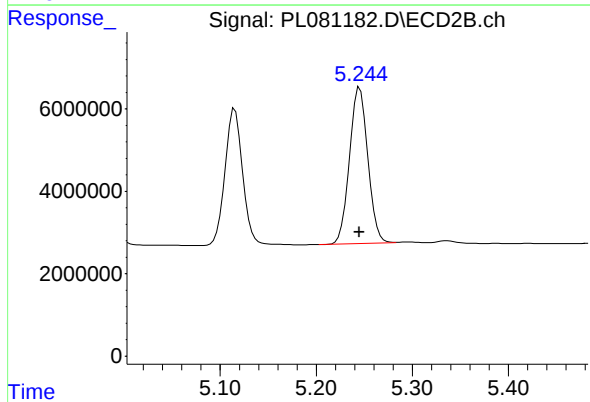


#13 Dieldrin

R.T.: 5.245 min
Delta R.T.: 0.000 min
Response: 50202369
Conc: 22.27 ng/ml

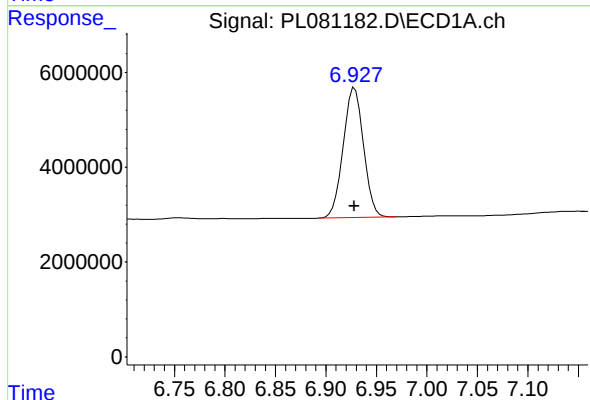


#19 Endosulfan Sulfate

R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 38424036
Conc: 21.40 ng/ml

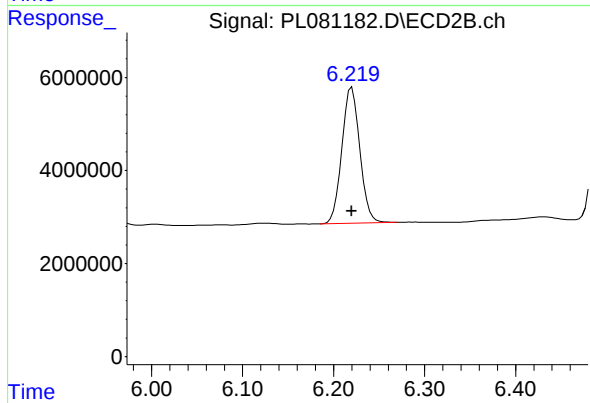

#19 Endosulfan Sulfate


R.T.: 6.220 min
Delta R.T.: 0.000 min
Response: 40142072
Conc: 20.88 ng/ml

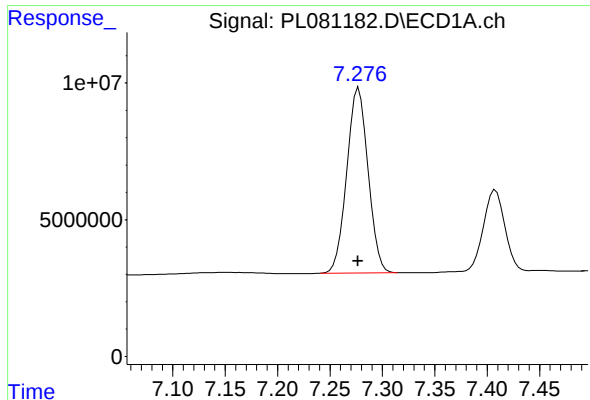

#20 Methoxychlor


R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 96312076
Conc: 111.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

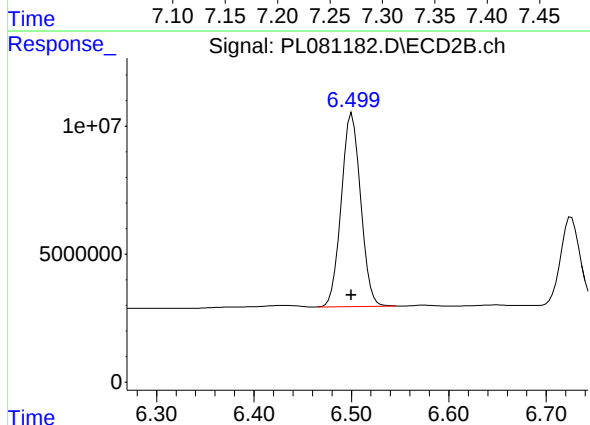


#20 Methoxychlor

R.T.: 6.501 min
Delta R.T.: 0.000 min
Response: 104260174
Conc: 112.34 ng/ml

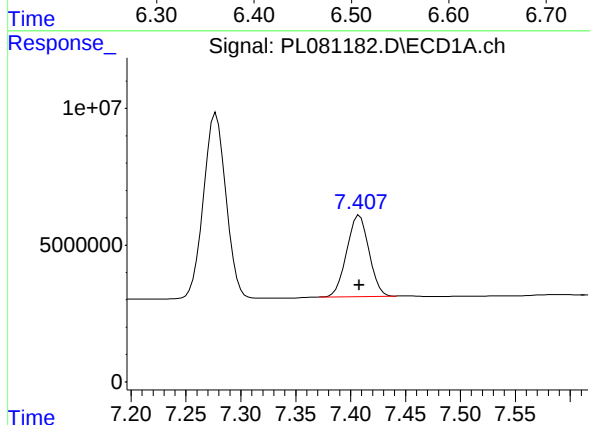


#21 Endrin ketone

R.T.: 7.408 min
Delta R.T.: 0.000 min
Response: 41874167
Conc: 23.08 ng/ml

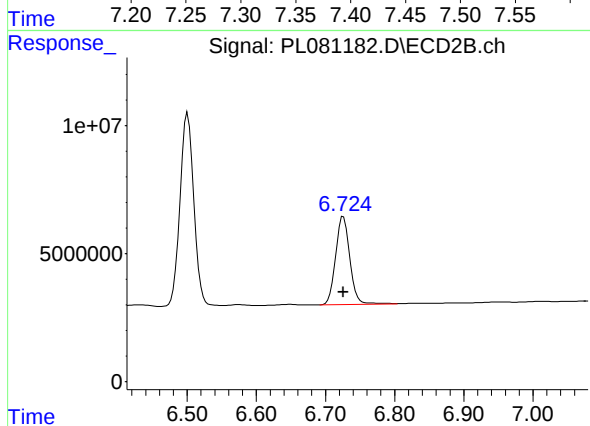

#21 Endrin ketone


R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 49010077
Conc: 22.76 ng/ml

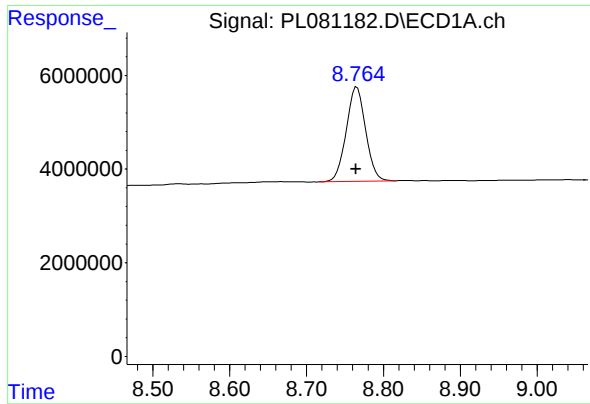

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.001 min
Response: 35337323
Conc: 23.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

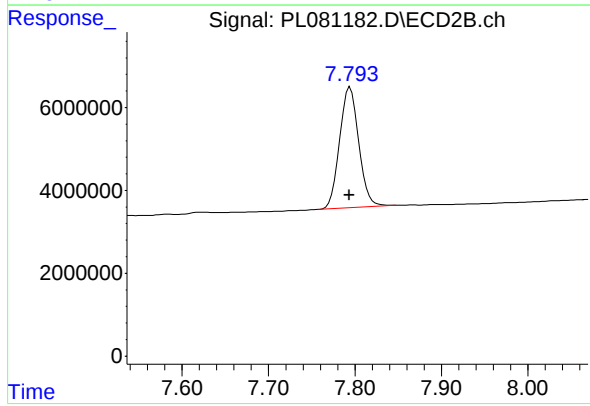

#28 Decachlorobiphenyl

R.T.: 7.794 min
Delta R.T.: 0.000 min
Response: 44243408
Conc: 23.10 ng/ml