

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 17:39
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 23:43:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 02 23:43:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	2.665	224.0E6	259.4E6	100.886	101.225
28) SA Decachlor...	8.764	7.793	146.0E6	187.7E6	97.556	97.897
Target Compounds						
23) Chlordane-1	4.481	3.657	98474653	83663421	1006.512	1004.782
24) Chlordane-2	5.008	4.232	97190865	99105479	981.469	987.702
25) Chlordane-3	5.714	4.861	378.6E6	285.2E6	1016.548	1022.759
26) Chlordane-4	5.795	4.922	446.6E6	291.8E6	1009.701	1019.987
27) Chlordane-5	6.636	5.589	72747138	71512735	999.312	1005.280



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 17:39
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 23:43:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 02 23:43:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

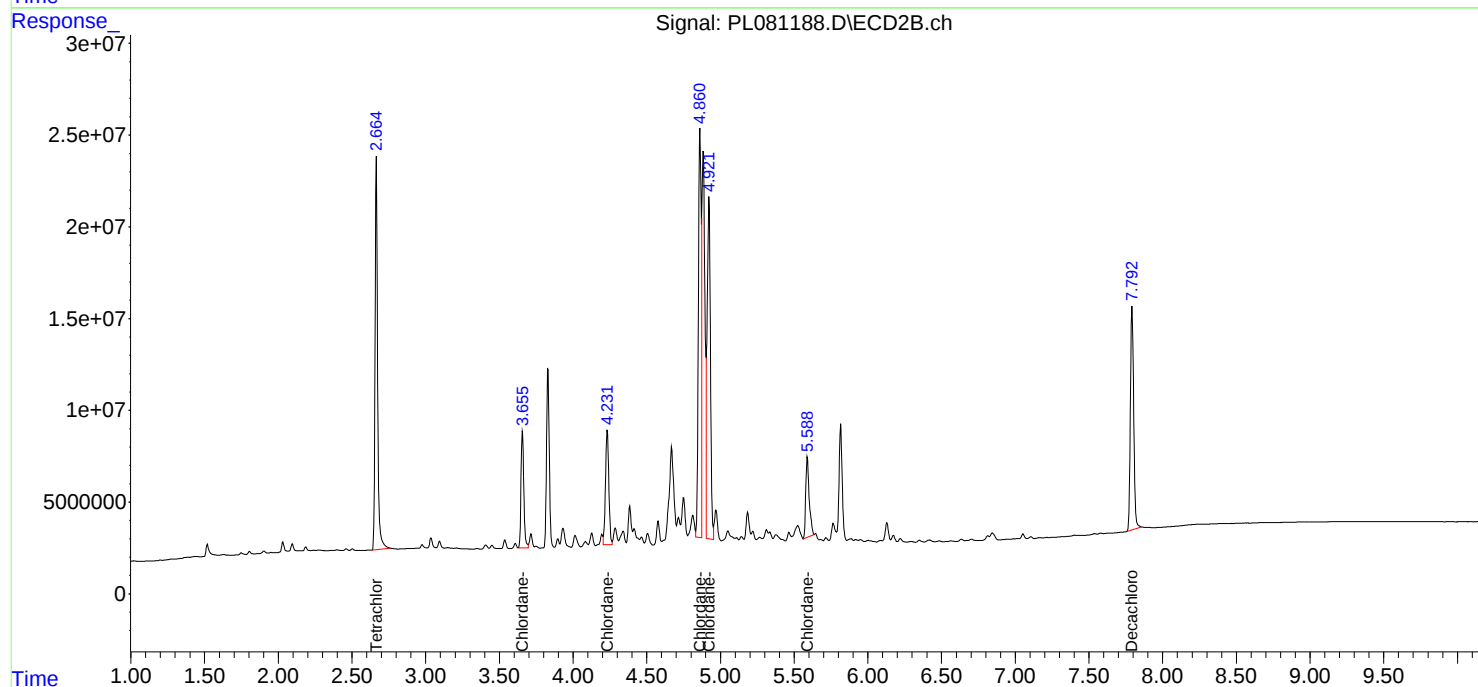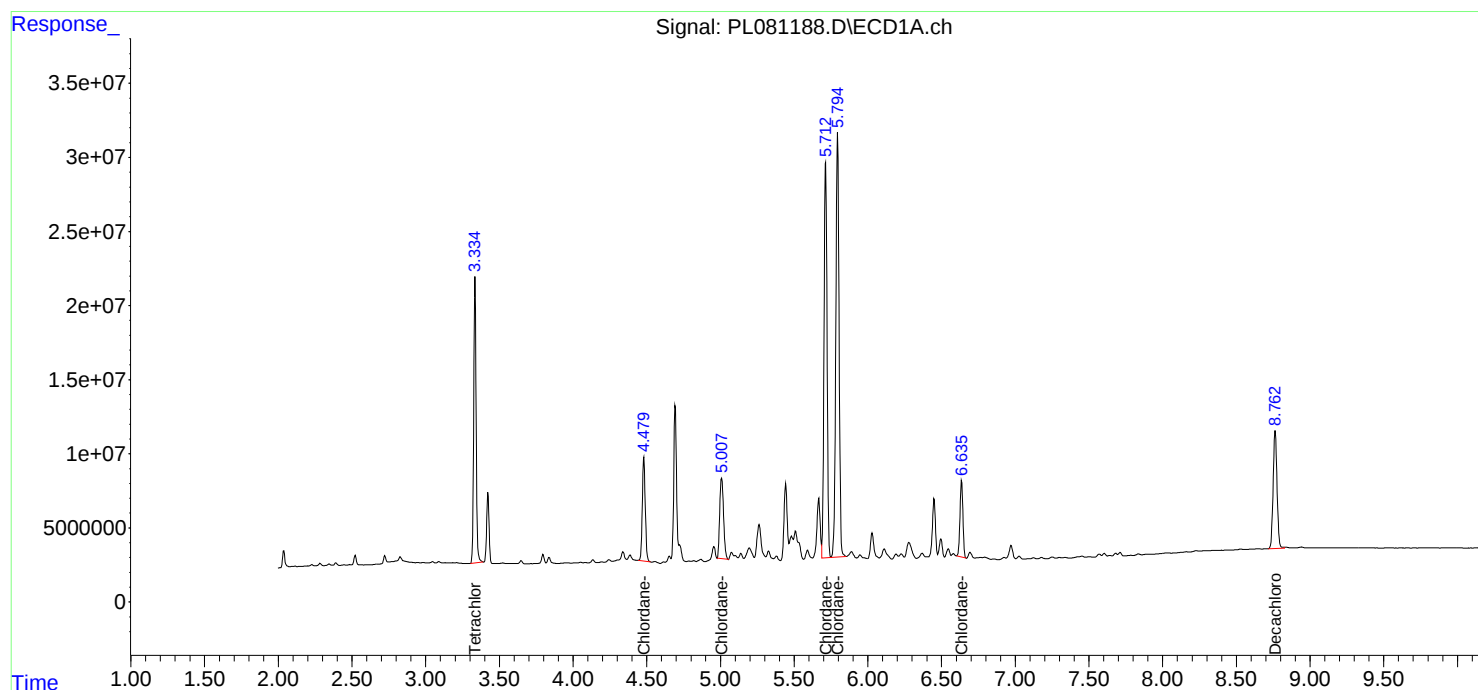


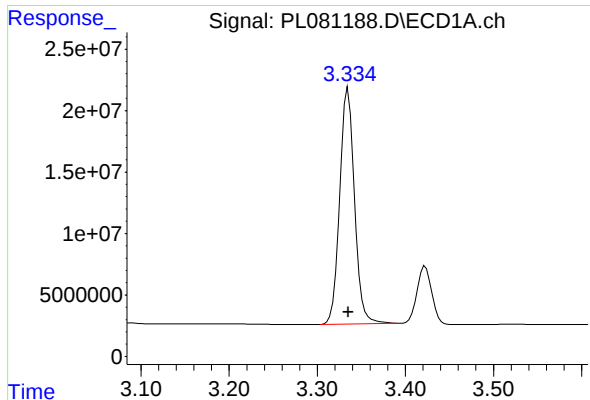

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 224048895
Conc: 100.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

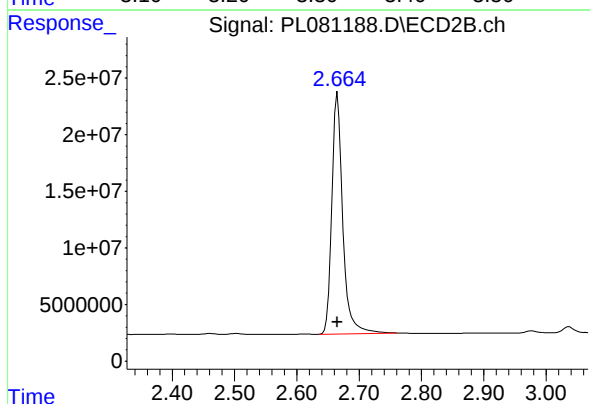


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 259360621
Conc: 101.22 ng/ml

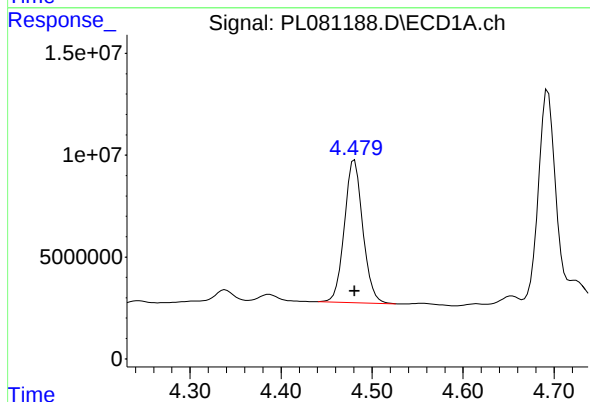


#23 Chlordane-1

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 98474653
Conc: 1006.51 ng/ml

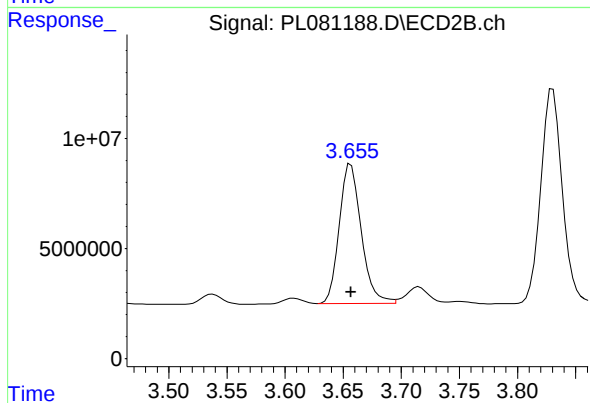

#23 Chlordane-1


R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 83663421
Conc: 1004.78 ng/ml

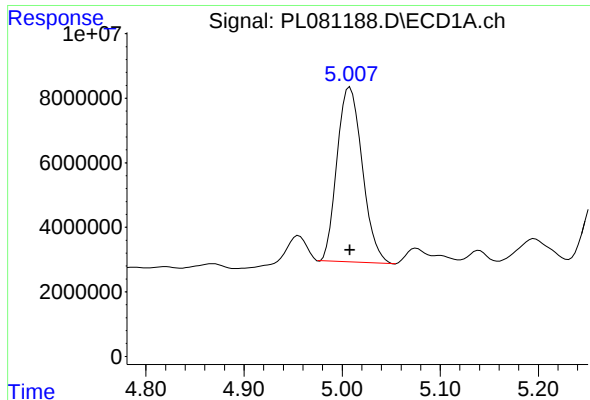

#24 Chlordane-2


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 97190865
Conc: 981.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

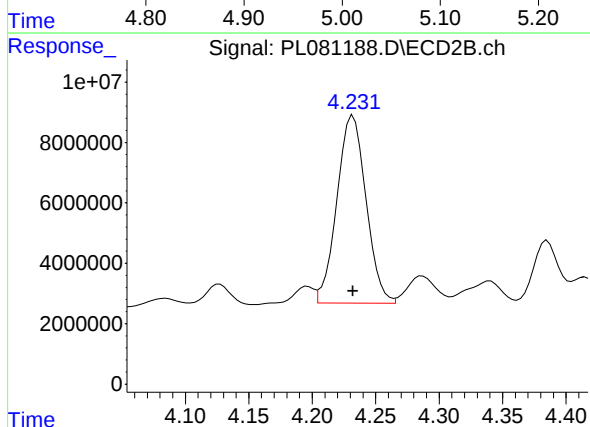


#24 Chlordane-2

R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 99105479
Conc: 987.70 ng/ml

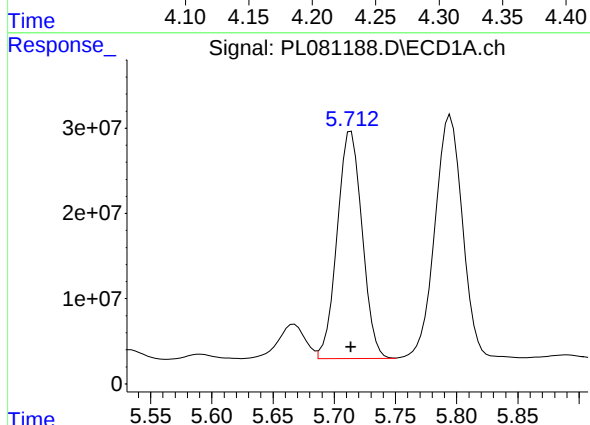


#25 Chlordane-3

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 378612322
Conc: 1016.55 ng/ml

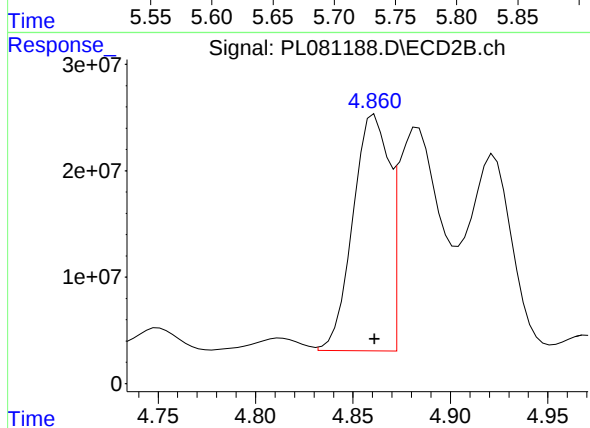

#25 Chlordane-3


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 285232619
Conc: 1022.76 ng/ml

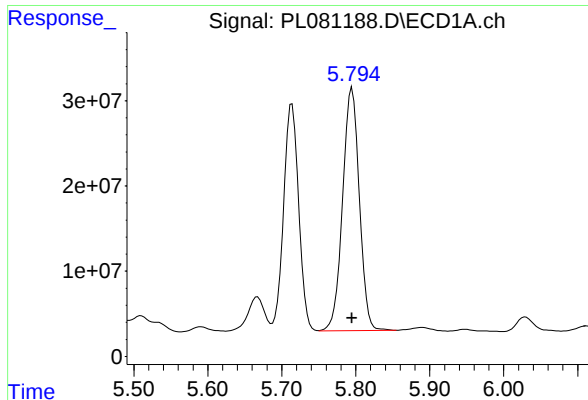

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 446631314
Conc: 1009.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

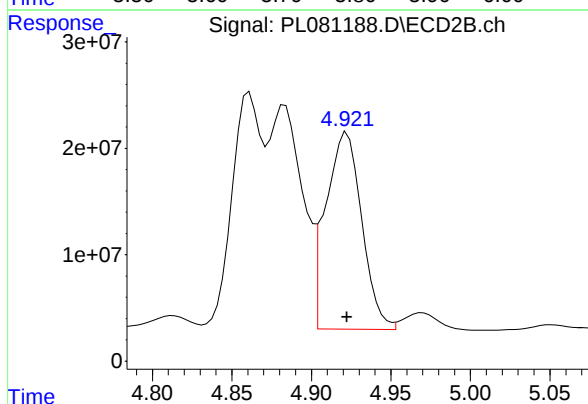


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 291767103
Conc: 1019.99 ng/ml

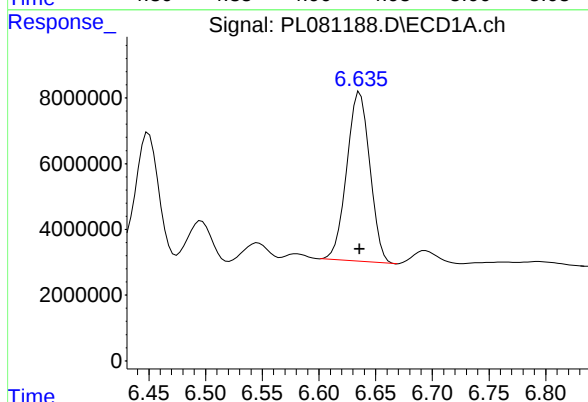


#27 Chlordane-5

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 72747138
Conc: 999.31 ng/ml

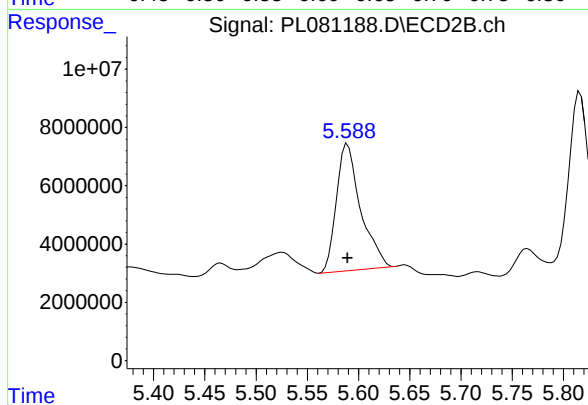

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 71512735
Conc: 1005.28 ng/ml

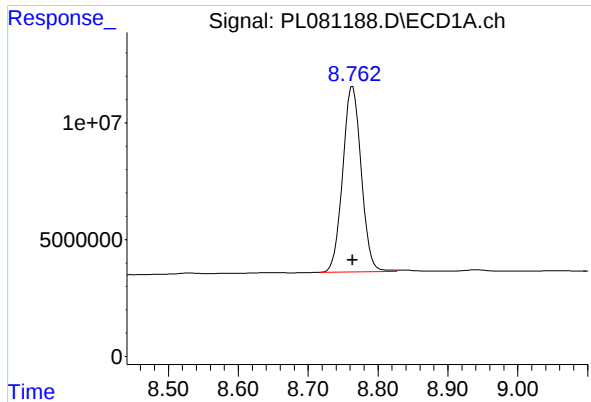

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 146025608
Conc: 97.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

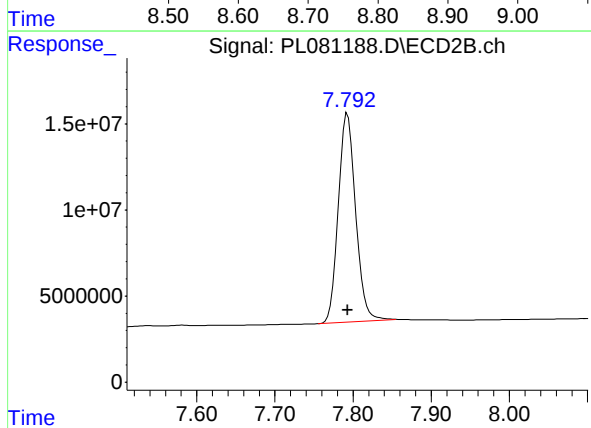

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 187671357
Conc: 97.90 ng/ml