

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 17:53
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 23:49:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 02 23:48:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	2.665	166.4E6	192.9E6	74.944	75.184
28) SA Decachlor...	8.763	7.793	111.2E6	143.5E6	74.522	74.887
Target Compounds						
23) Chlordane-1	4.481	3.657	73427101	62356589	750.334	749.260
24) Chlordane-2	5.008	4.232	73812702	74880180	746.919	747.508
25) Chlordane-3	5.714	4.861	279.9E6	210.3E6	751.009	752.756
26) Chlordane-4	5.794	4.922	331.8E6	215.2E6	750.084	751.538
27) Chlordane-5	6.636	5.589	54633143	53858094	750.322	754.720



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 17:53
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 23:49:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 02 23:48:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

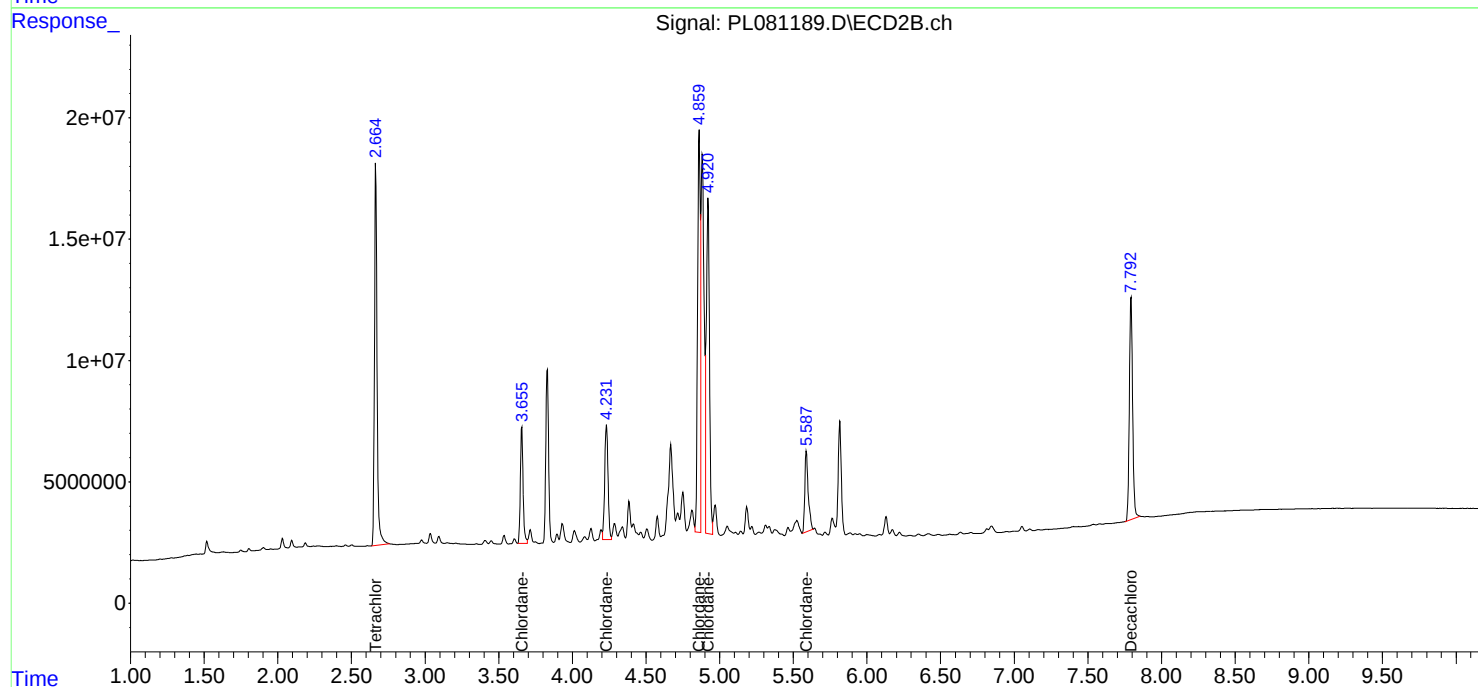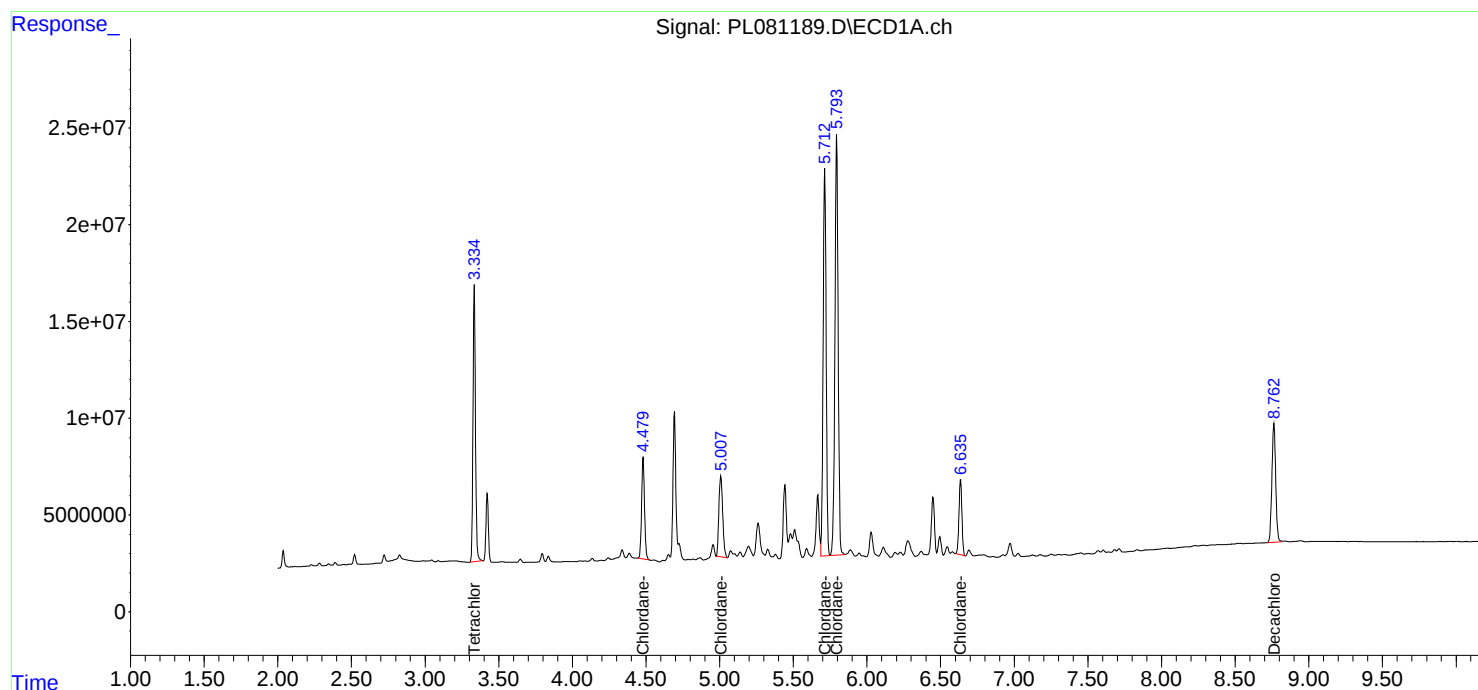


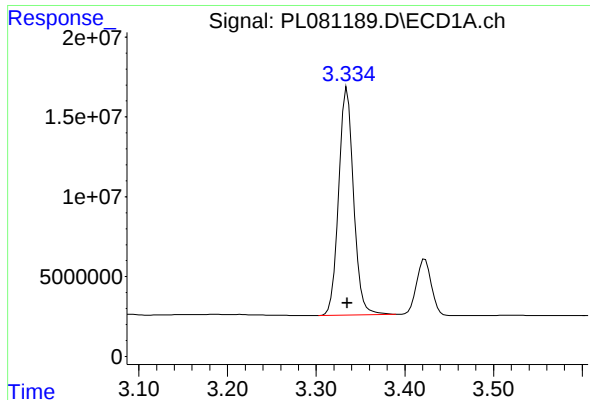

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 166375792
Conc: 74.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

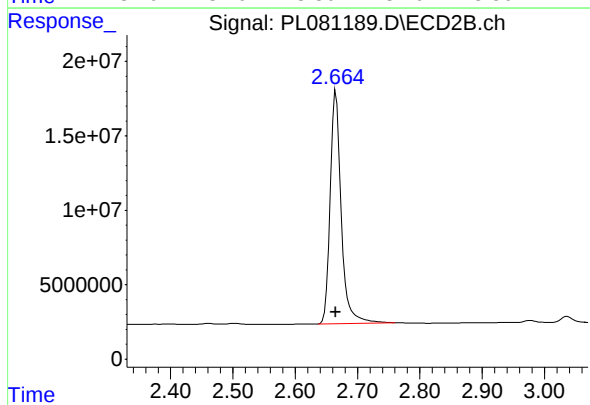


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 192874346
Conc: 75.18 ng/ml

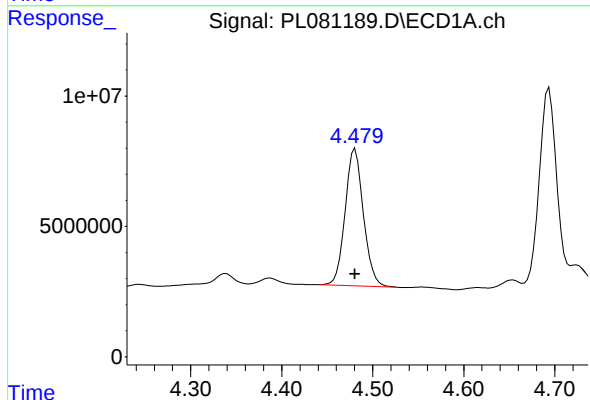


#23 Chlordane-1

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 73427101
Conc: 750.33 ng/ml

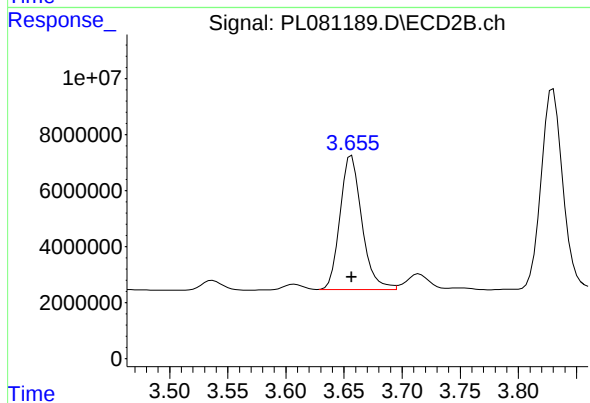

#23 Chlordane-1


R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 62356589
Conc: 749.26 ng/ml

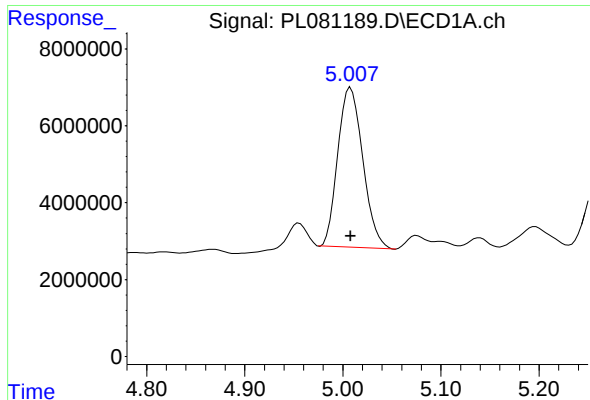

#24 Chlordane-2


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 73812702
Conc: 746.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

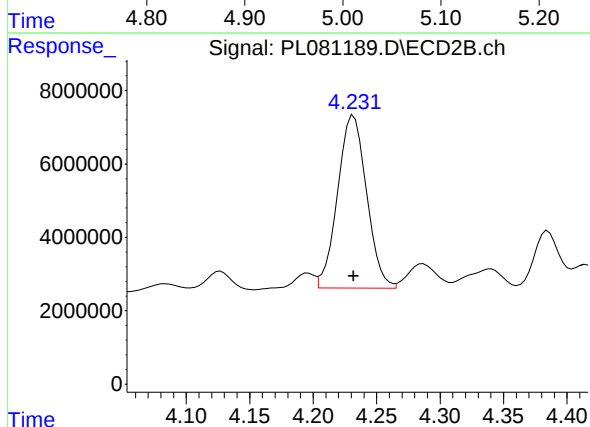


#24 Chlordane-2

R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 74880180
Conc: 747.51 ng/ml

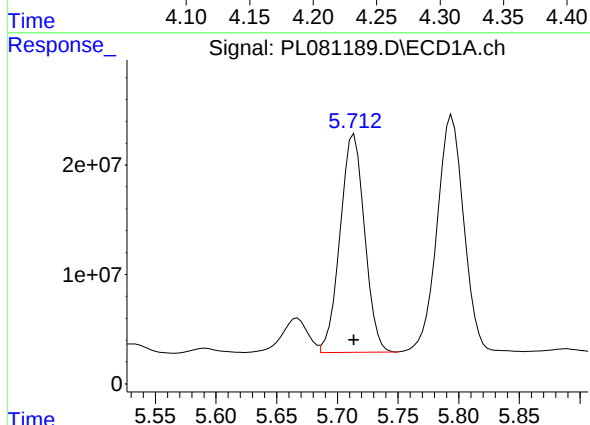


#25 Chlordane-3

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 279901039
Conc: 751.01 ng/ml

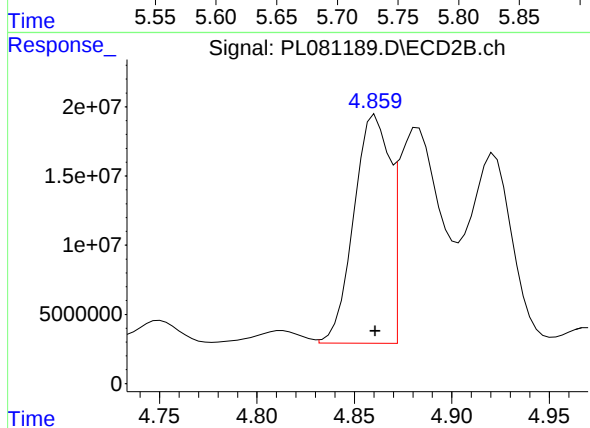

#25 Chlordane-3


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 210319001
Conc: 752.76 ng/ml

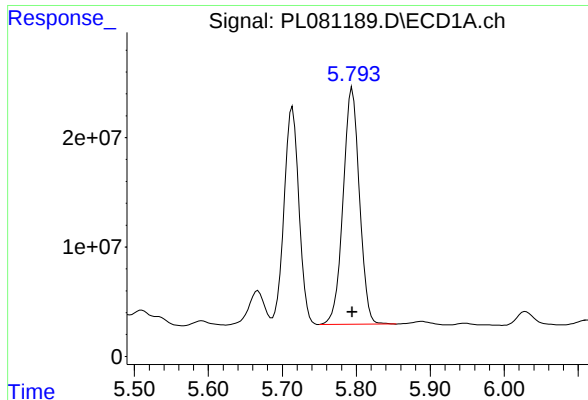

#26 Chlordane-4


R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 331810687
Conc: 750.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

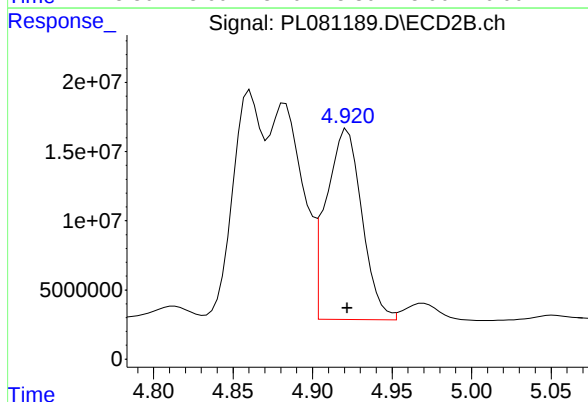


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 215198063
Conc: 751.54 ng/ml

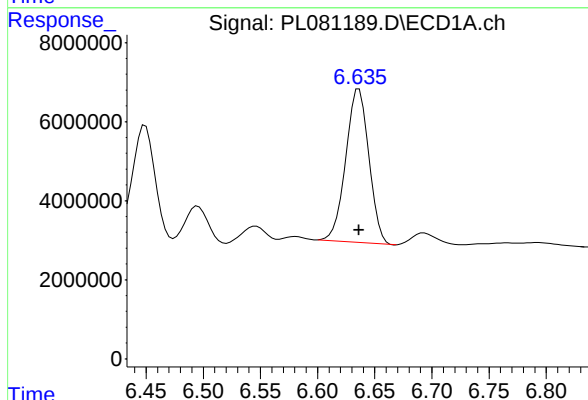


#27 Chlordane-5

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 54633143
Conc: 750.32 ng/ml

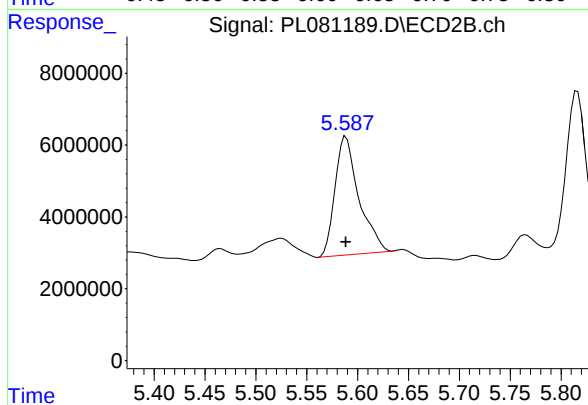

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 53858094
Conc: 754.72 ng/ml

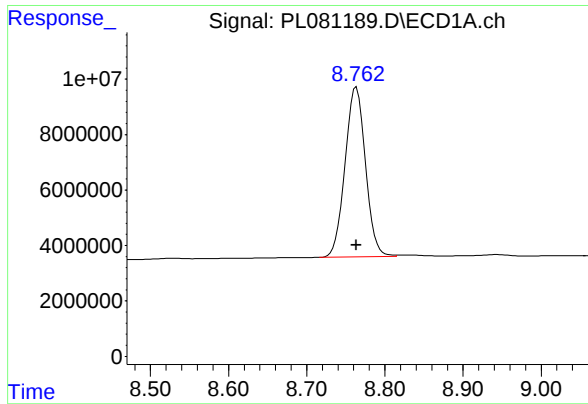

#28 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: 0.000 min
Response: 111193369
Conc: 74.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

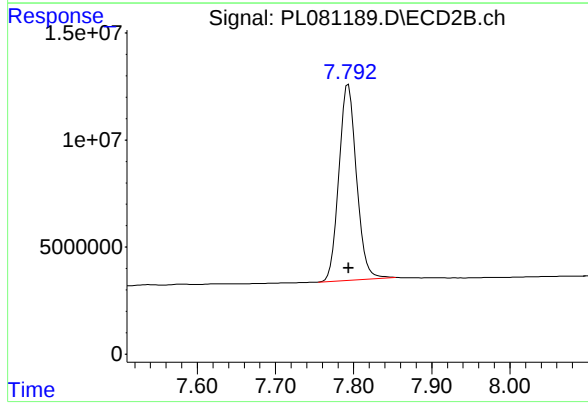

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 143453099
Conc: 74.89 ng/ml