

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 18:07
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 23:31:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 02 23:28:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	2.665	110.1E6	126.5E6	50.000	50.000
28) SA Decachlor...	8.763	7.793	76671691	97866418	50.000	50.000
Target Compounds						
23) Chlordane-1	4.481	3.657	48600170	41433511	500.000	500.000
24) Chlordane-2	5.007	4.233	50430522	50786732	500.000	500.000
25) Chlordane-3	5.713	4.862	183.1E6	136.3E6	500.000	500.000
26) Chlordane-4	5.795	4.923	219.0E6	140.2E6	500.000	500.000
27) Chlordane-5	6.636	5.589	36423660	35380774	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 18:07
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 23:31:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 02 23:28:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

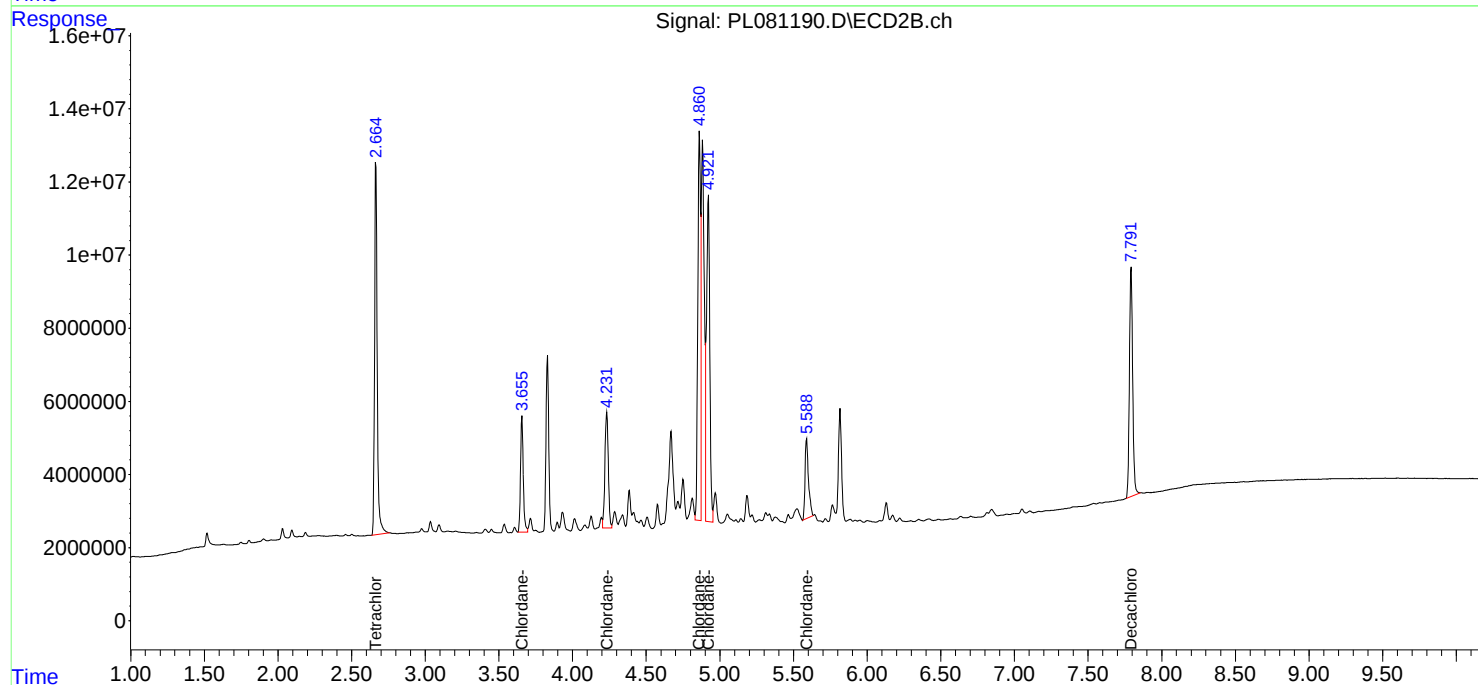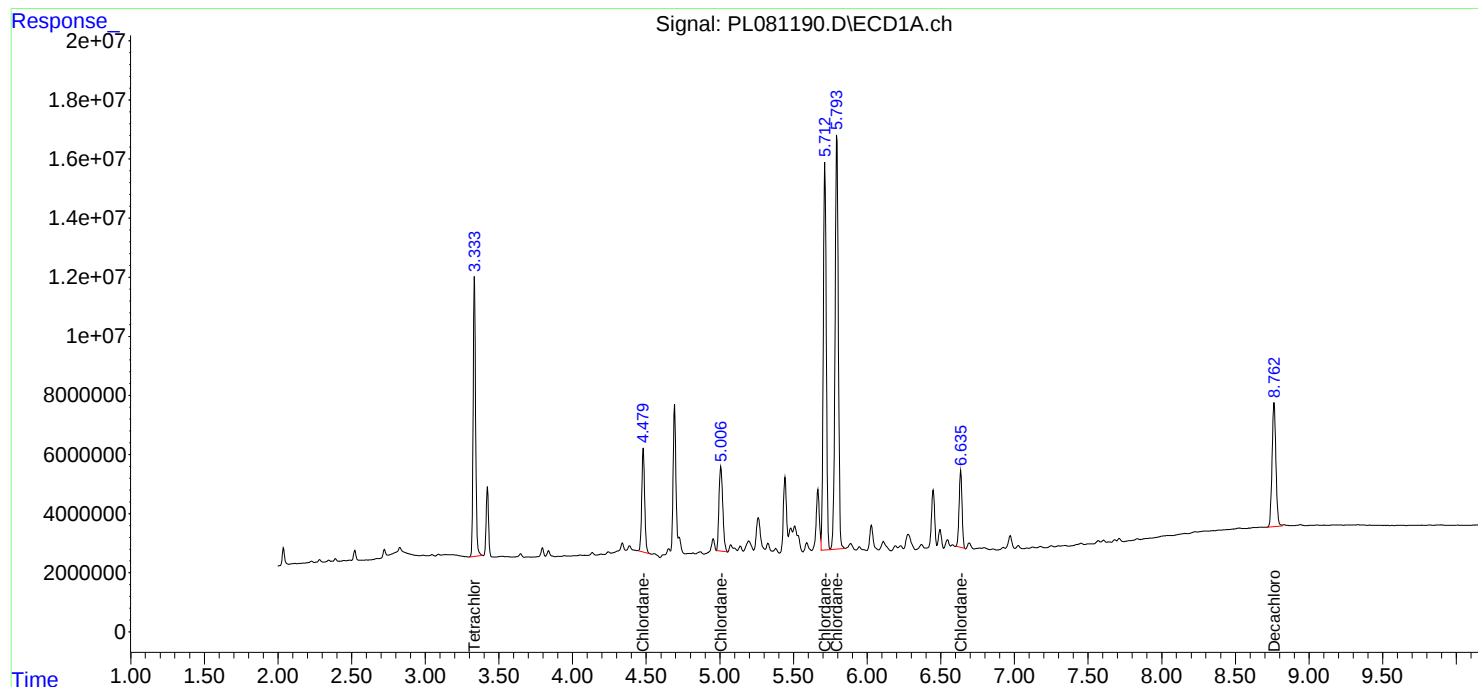


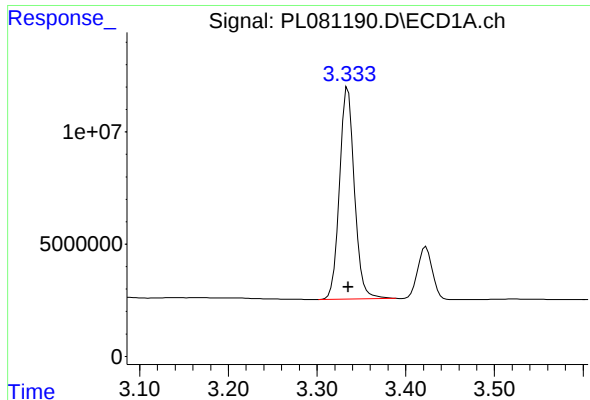

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 110057581
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

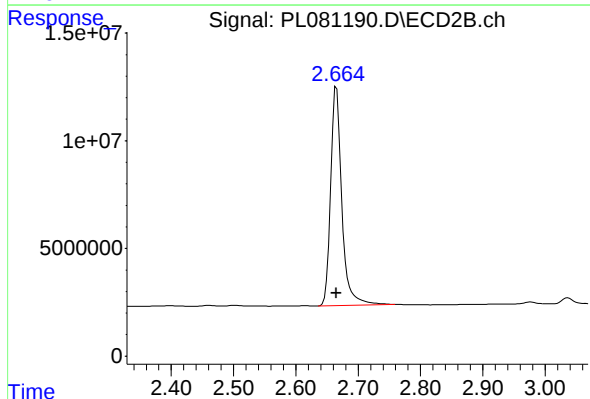


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 126542384
Conc: 50.00 ng/ml

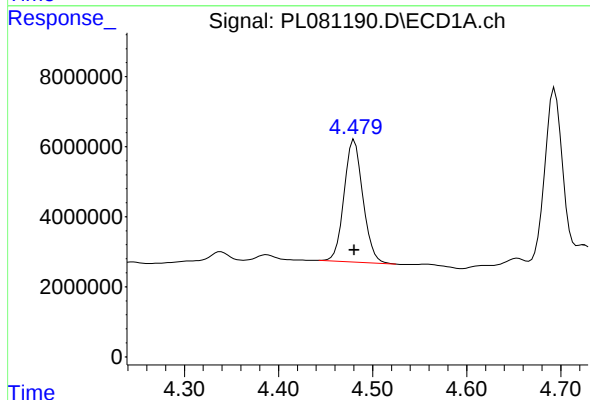


#23 Chlordane-1

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 48600170
Conc: 500.00 ng/ml

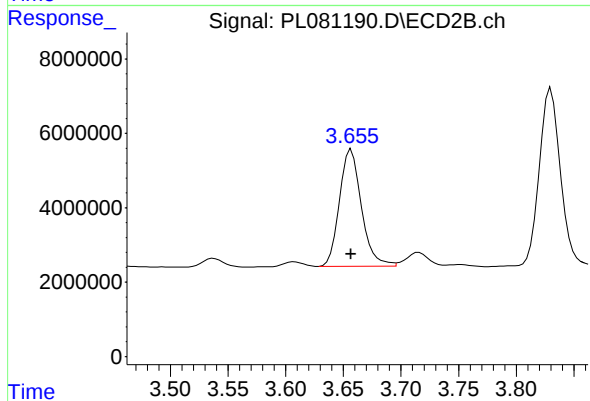

#23 Chlordane-1


R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 41433511
Conc: 500.00 ng/ml

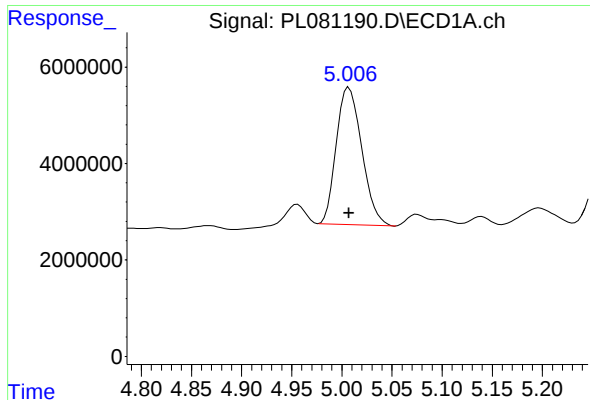

#24 Chlordane-2


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 50430522
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

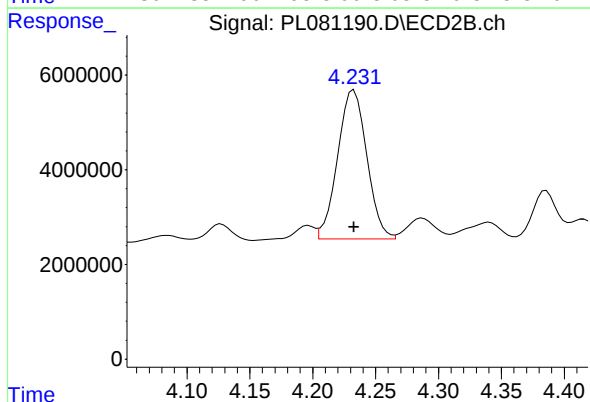


#24 Chlordane-2

R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 50786732
Conc: 500.00 ng/ml

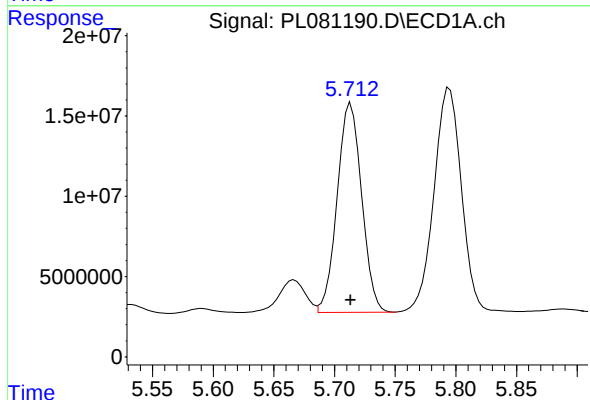


#25 Chlordane-3

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 183142926
Conc: 500.00 ng/ml

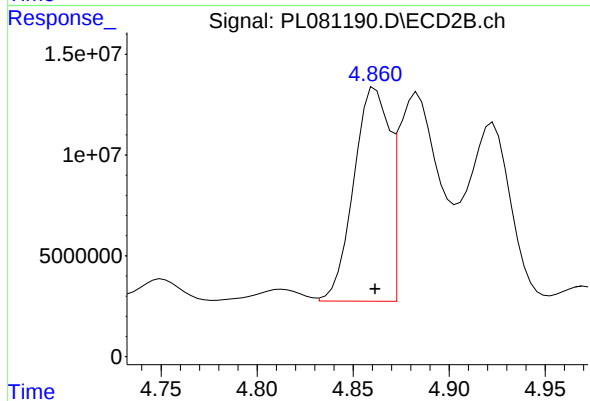

#25 Chlordane-3


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 136269136
Conc: 500.00 ng/ml

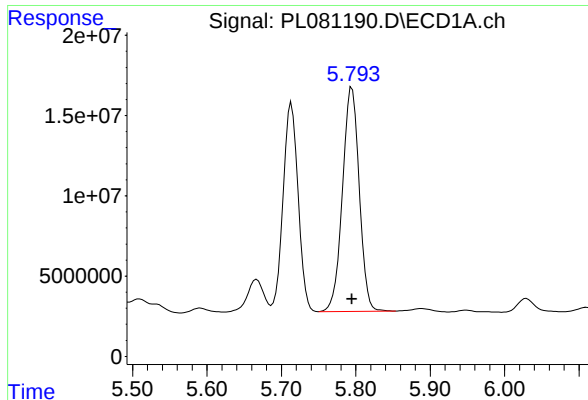

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 219024690
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

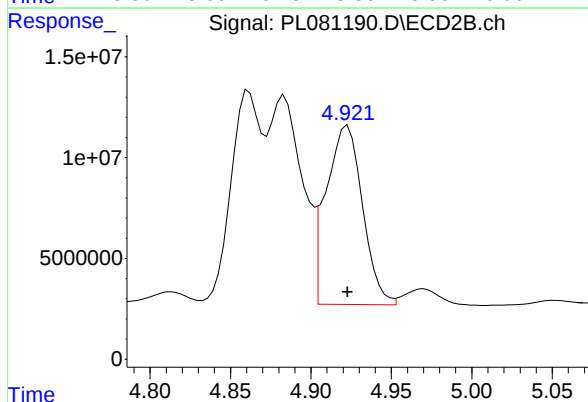


#26 Chlordane-4

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 140166294
Conc: 500.00 ng/ml

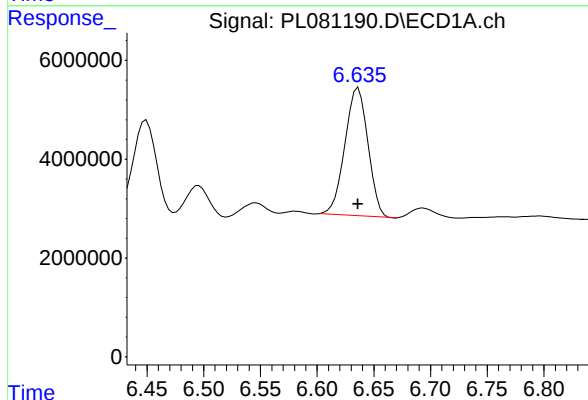


#27 Chlordane-5

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 36423660
Conc: 500.00 ng/ml

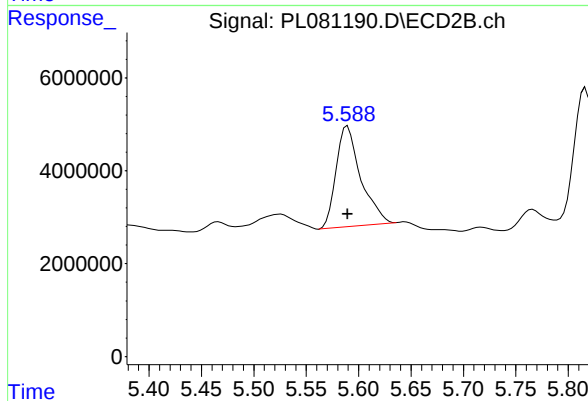

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 35380774
Conc: 500.00 ng/ml

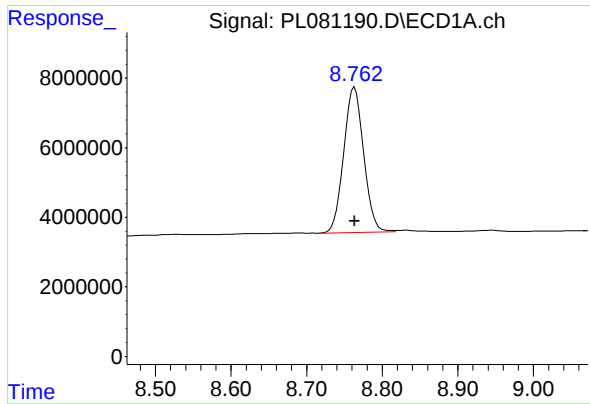

#28 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: 0.000 min
Response: 76671691
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

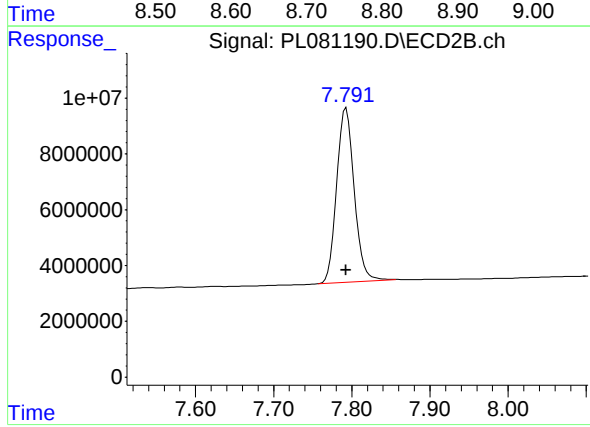

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 97866418
Conc: 50.00 ng/ml