

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 18:35
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 01:42:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:12:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	2.665	10888953	11821623	4.958	4.735
28)	SA Decachlor...	8.764	7.793	8434057	10465892	5.454	5.325
Target Compounds							
23)	Chlordane-1	4.480	3.657	4528843	4117034	47.305	49.929
24)	Chlordane-2	5.007	4.232	5153803	5472547	51.497	53.459
25)	Chlordane-3	5.713	4.861	17969594	12802277	49.127	47.370
26)	Chlordane-4	5.795	4.923	22185856	13836683	50.476	49.269
27)	Chlordane-5	6.635	5.589	4220025	3156846	55.996	45.695



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 18:35
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 01:42:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:12:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

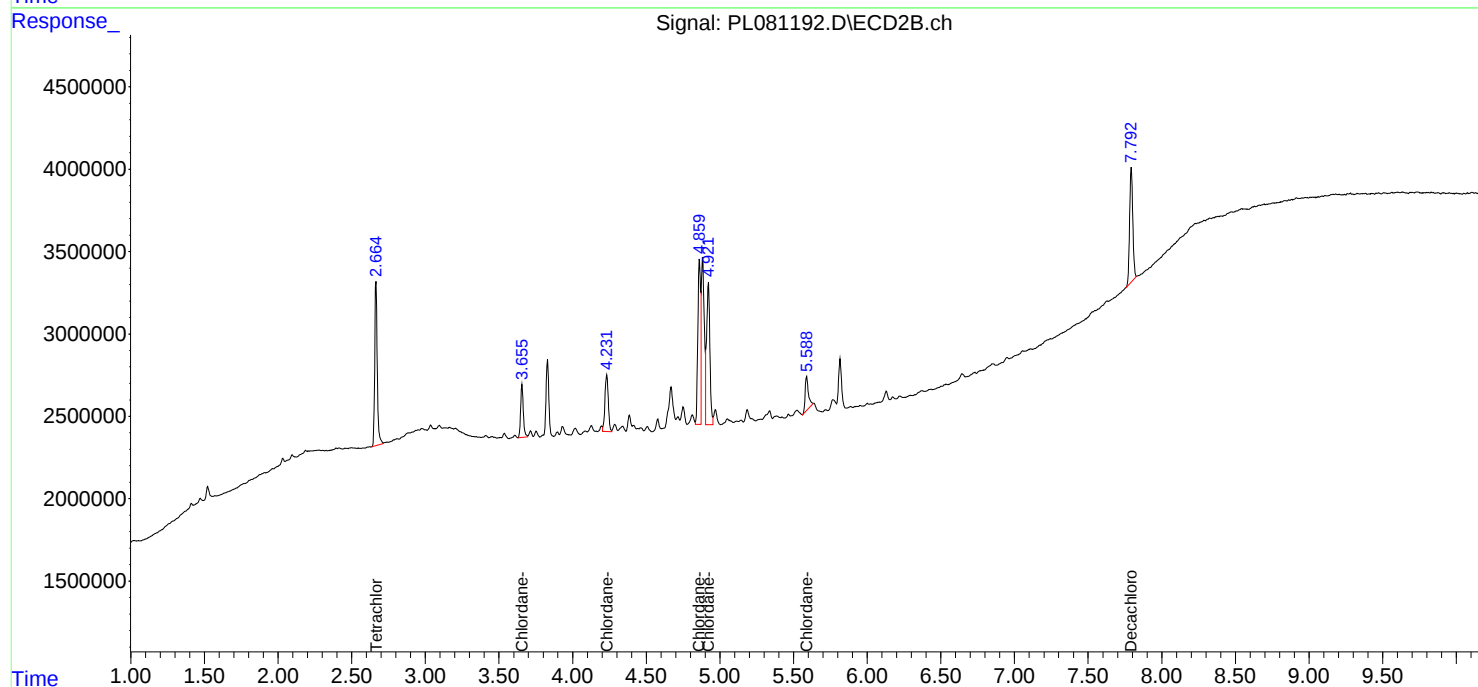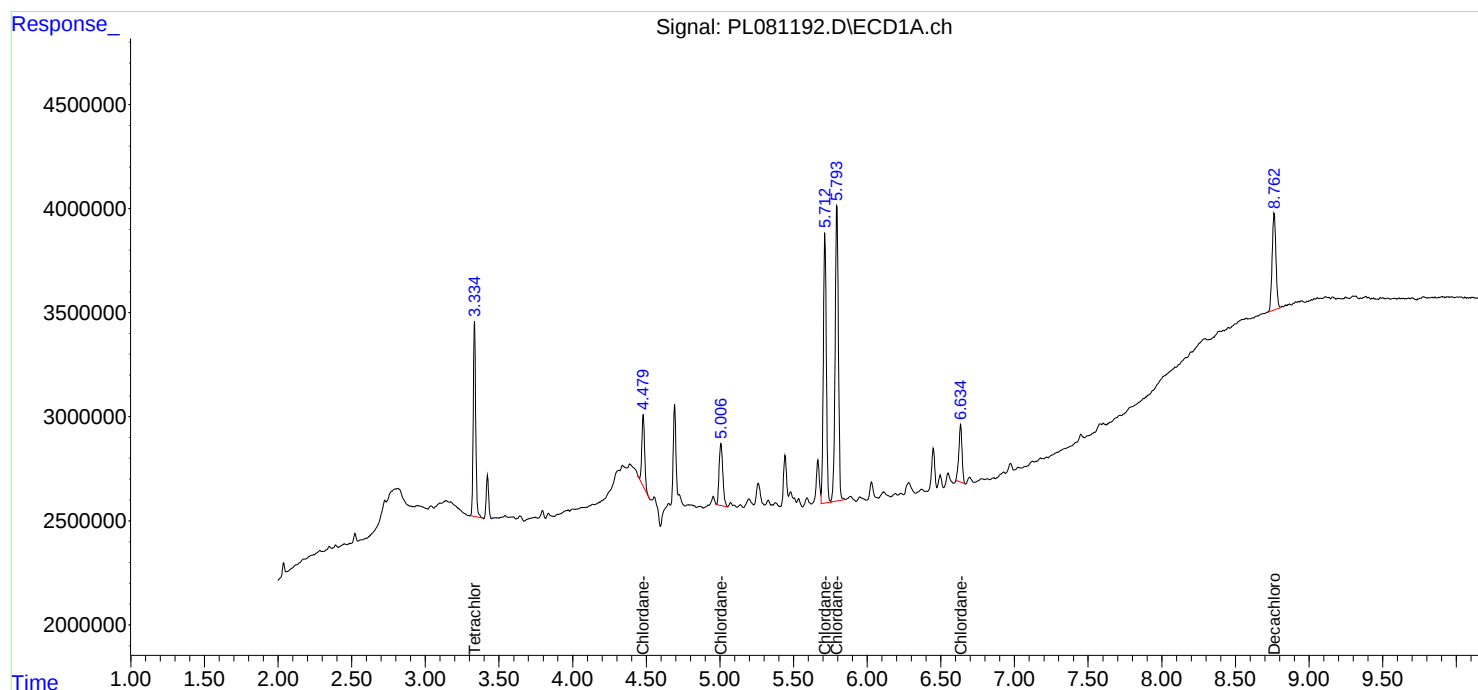


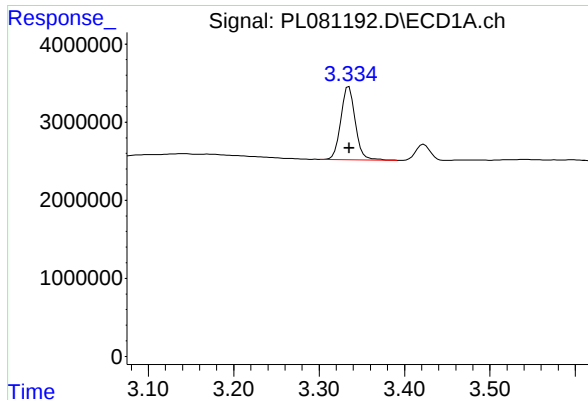

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 10888953
Conc: 4.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

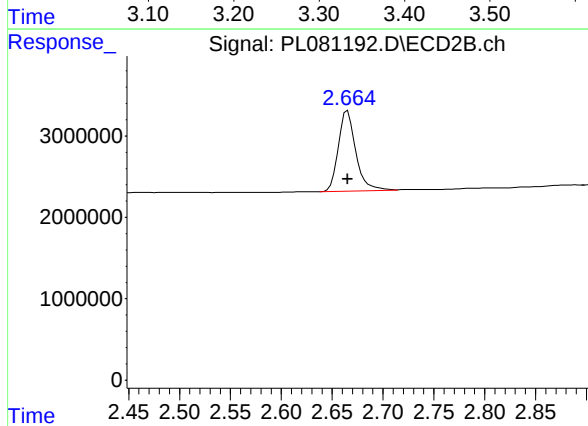


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 11821623
Conc: 4.73 ng/ml

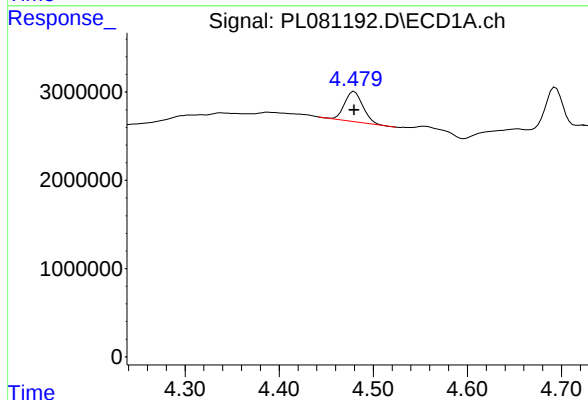


#23 Chlordane-1

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 4528843
Conc: 47.31 ng/ml

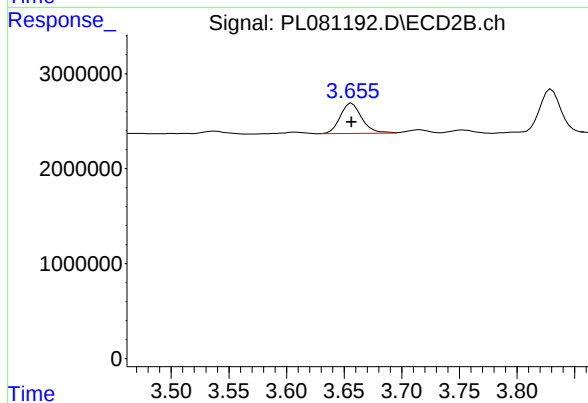

#23 Chlordane-1


R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 4117034
Conc: 49.93 ng/ml

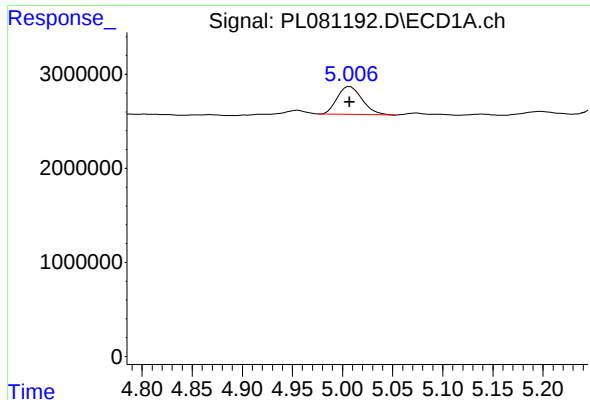

#24 Chlordane-2


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 5153803
Conc: 51.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

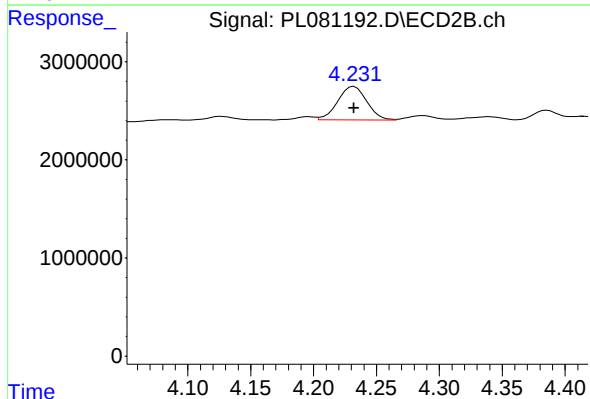


#24 Chlordane-2

R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 5472547
Conc: 53.46 ng/ml

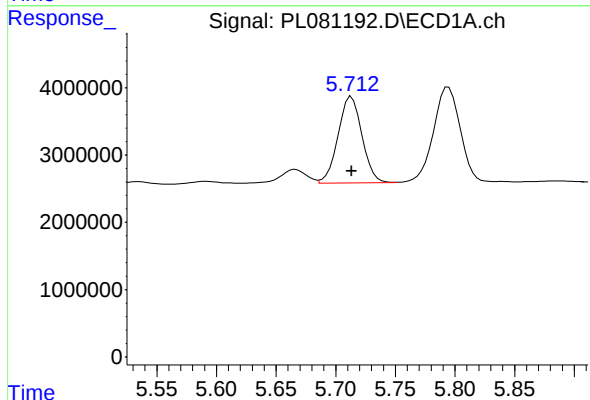


#25 Chlordane-3

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 17969594
Conc: 49.13 ng/ml

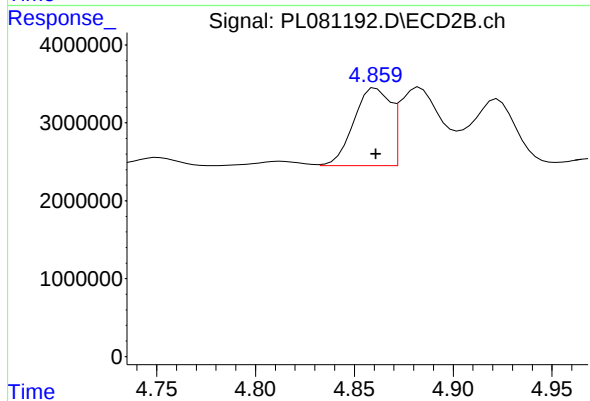

#25 Chlordane-3


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 12802277
Conc: 47.37 ng/ml

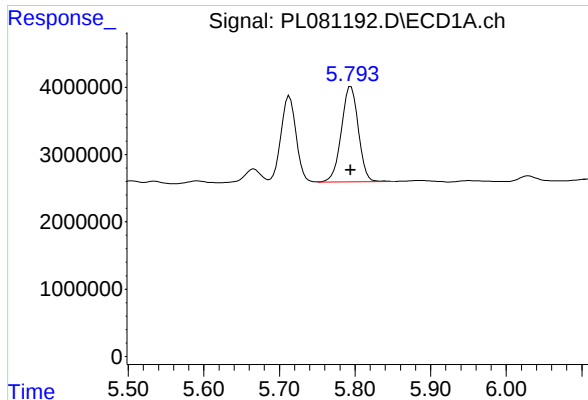

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 22185856
Conc: 50.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

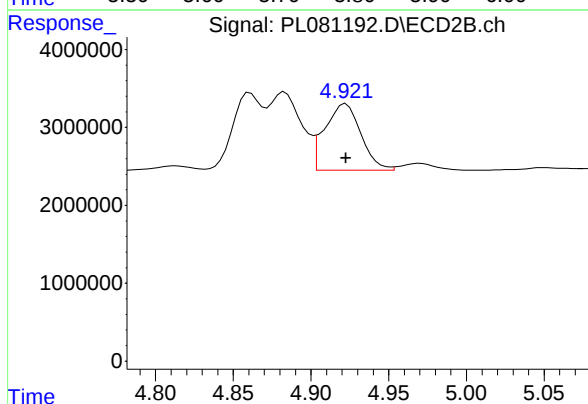


#26 Chlordane-4

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 13836683
Conc: 49.27 ng/ml

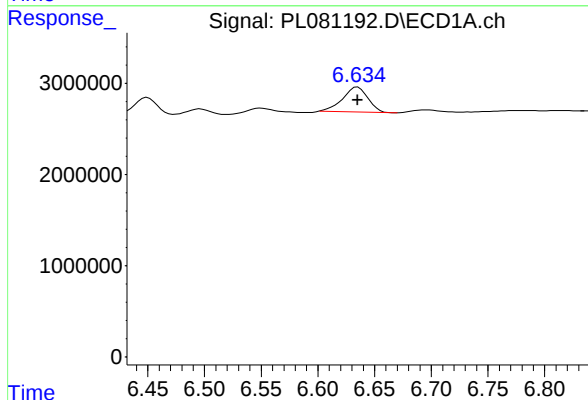


#27 Chlordane-5

R.T.: 6.635 min
Delta R.T.: 0.000 min
Response: 4220025
Conc: 56.00 ng/ml

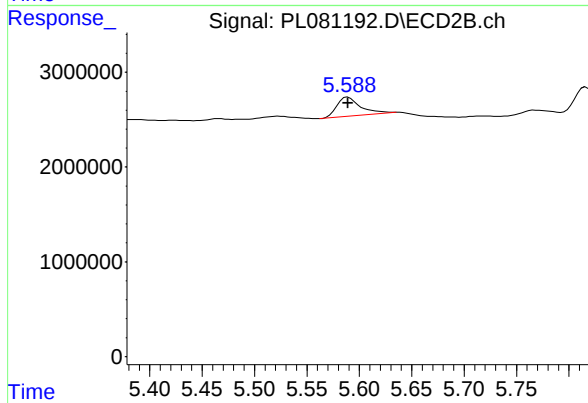

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 3156846
Conc: 45.70 ng/ml

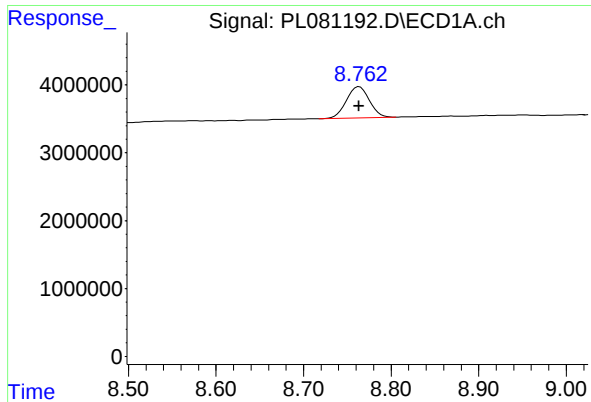

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 8434057
Conc: 5.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

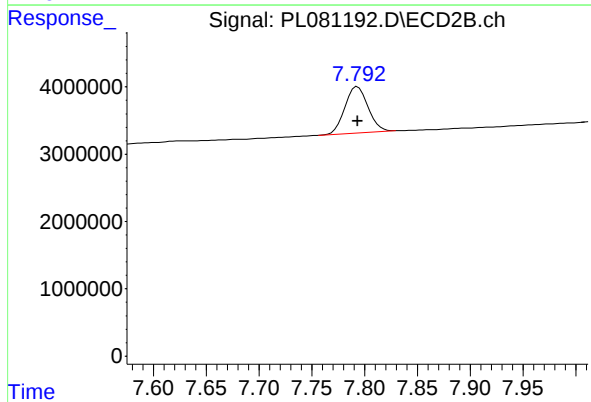

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 10465892
Conc: 5.33 ng/ml