

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
 Data File : PL081199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 20:26
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL030223

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 01:46:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:46:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	2.665	107.9E6	125.5E6	49.127	50.276
28)	SA Decachlor...	8.764	7.793	75352147	96361170	48.731	49.031
Target Compounds							
23)	Chlordane-1	4.480	3.656	54101891	45532668	565.113	552.197
24)	Chlordane-2	5.007	4.232	56169339	56366632	561.245	550.621
25)	Chlordane-3	5.713	4.861	205.9E6	152.2E6	562.867	563.006
26)	Chlordane-4	5.795	4.922	246.3E6	158.5E6	560.320	564.519
27)	Chlordane-5	6.636	5.589	40971847	39611736	543.663	573.382



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030223\
Data File : PL081199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 20:26
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL030223

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 01:46:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:46:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

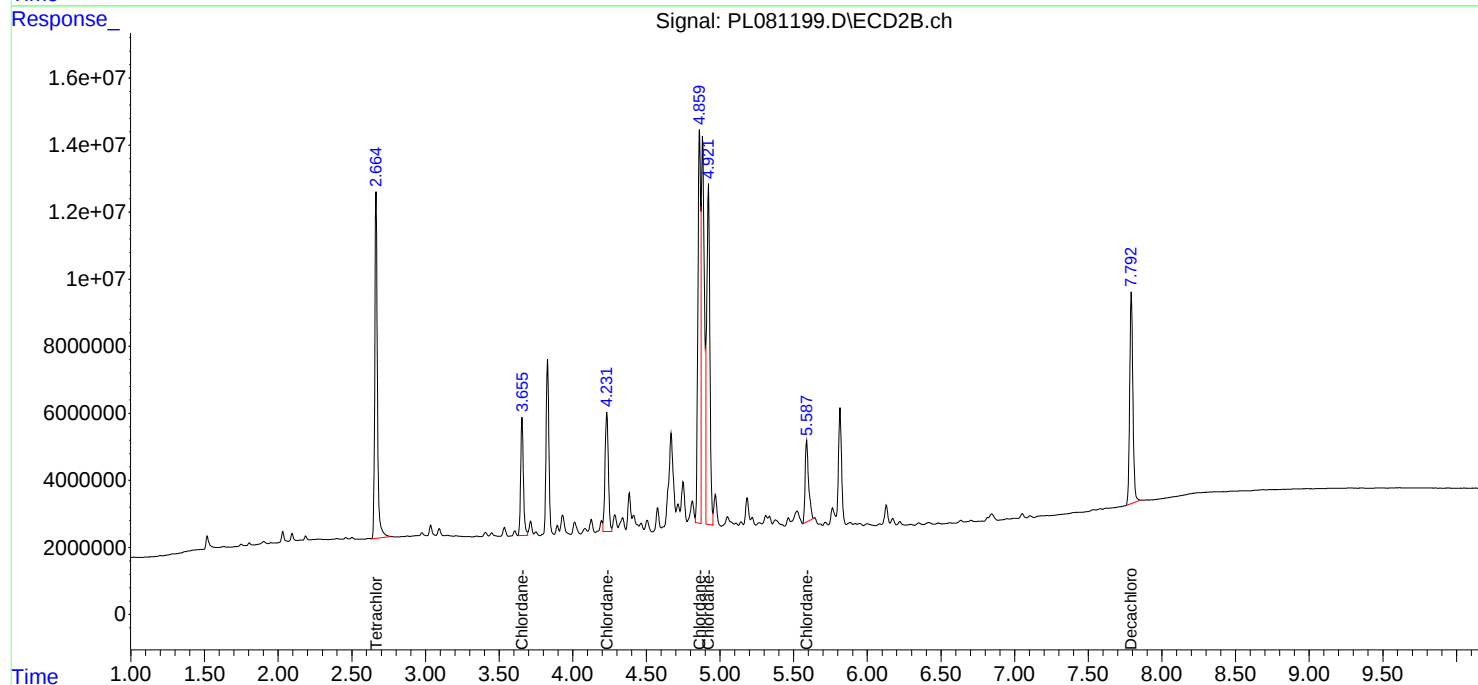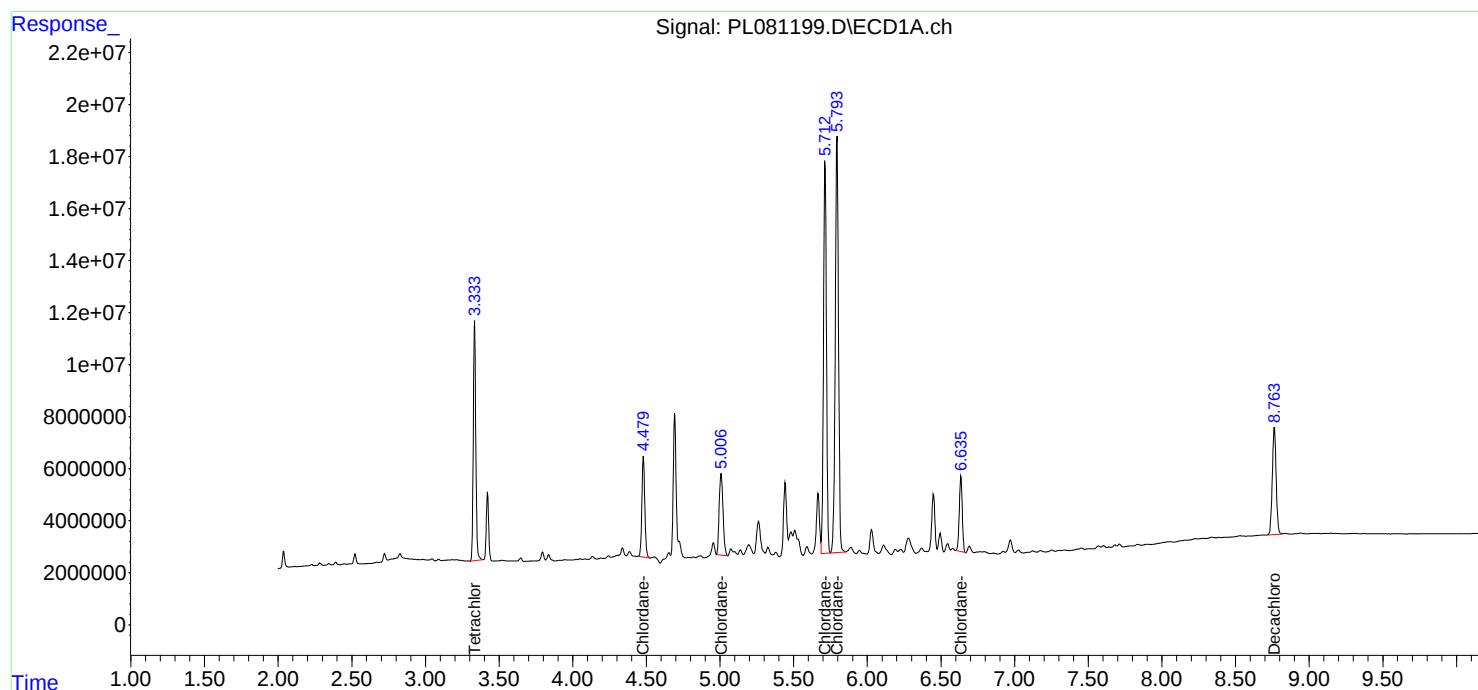


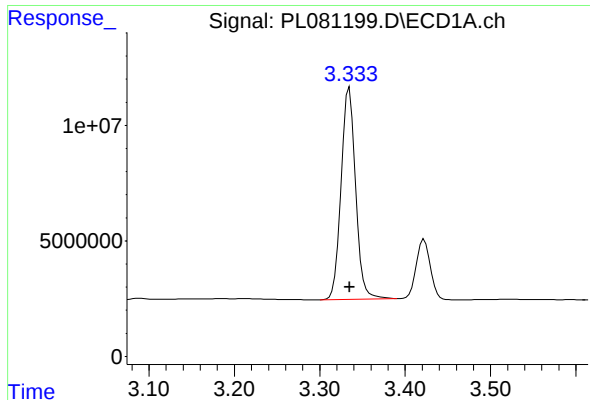

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.000 min
Response: 107901324
Conc: 49.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030223

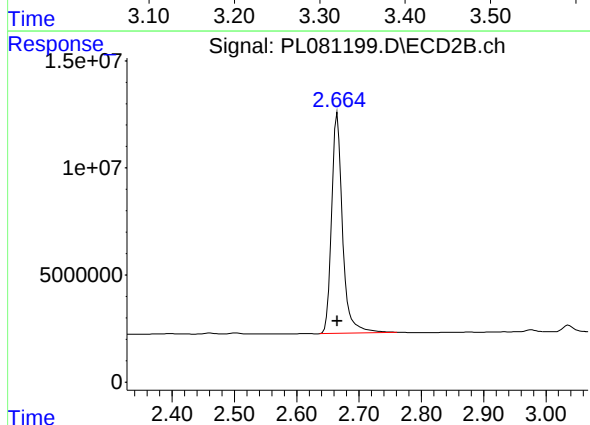


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.000 min
Response: 125531811
Conc: 50.28 ng/ml

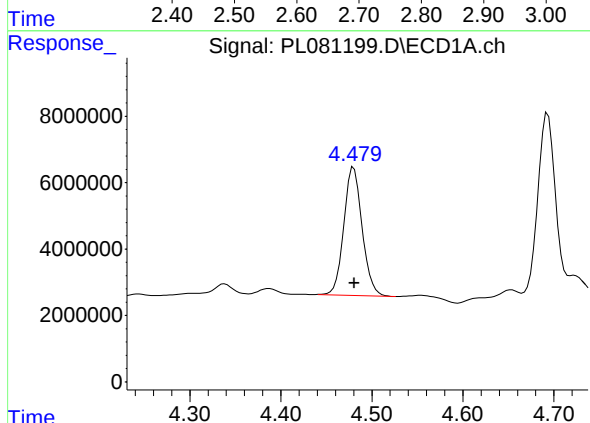


#23 Chlordane-1

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 54101891
Conc: 565.11 ng/ml

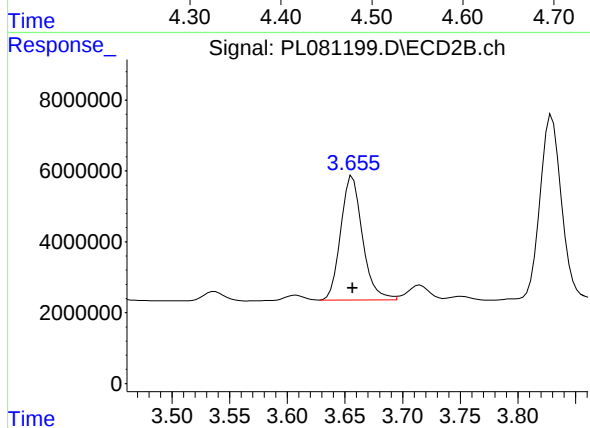

#23 Chlordane-1


R.T.: 3.656 min
Delta R.T.: 0.000 min
Response: 45532668
Conc: 552.20 ng/ml

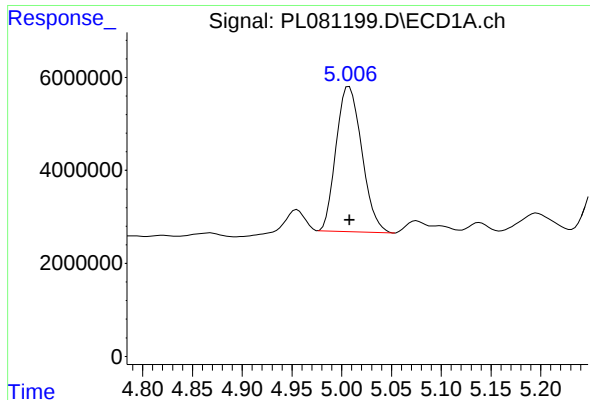

#24 Chlordane-2


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 56169339
Conc: 561.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030223

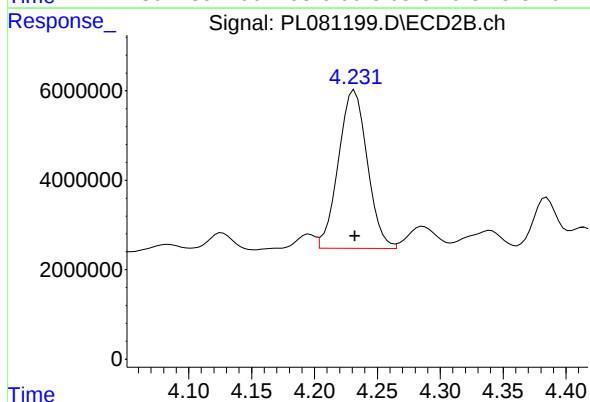


#24 Chlordane-2

R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 56366632
Conc: 550.62 ng/ml

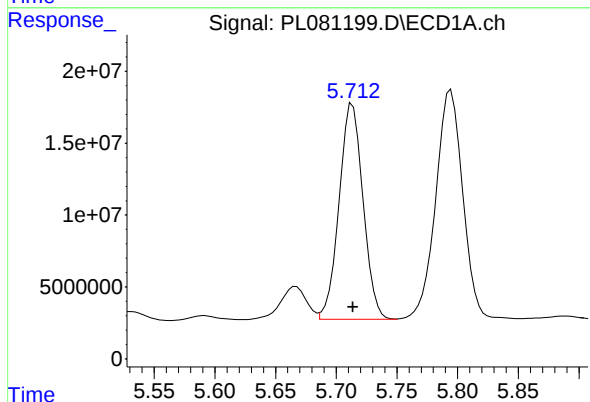


#25 Chlordane-3

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 205883937
Conc: 562.87 ng/ml

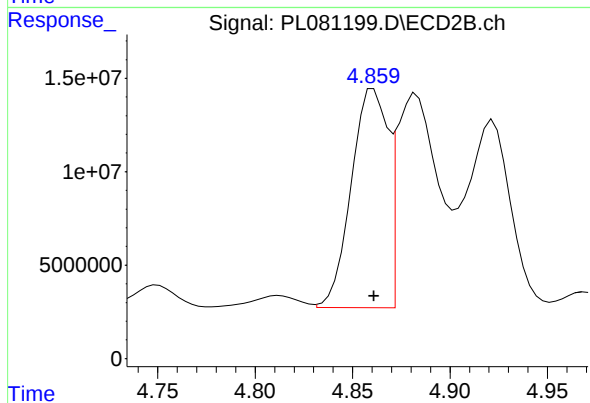

#25 Chlordane-3


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 152158512
Conc: 563.01 ng/ml

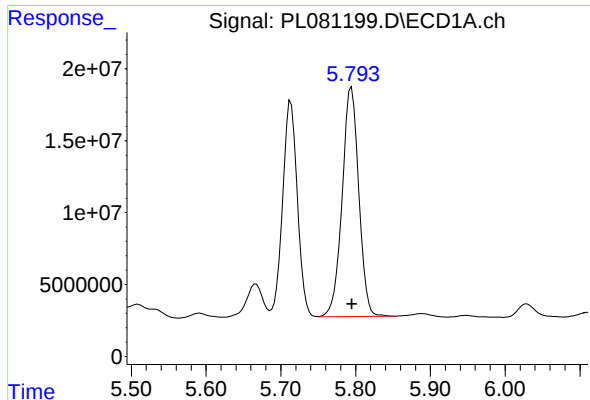

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 246279329
Conc: 560.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030223

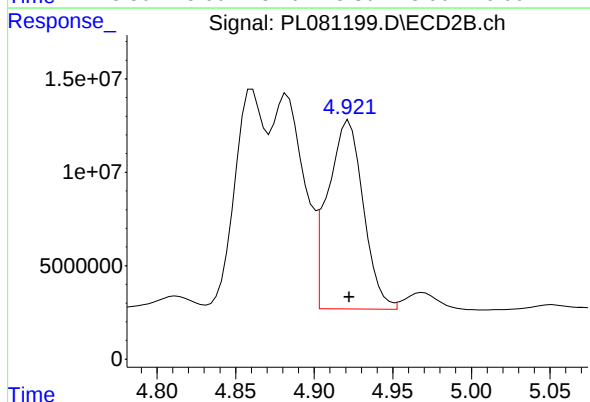


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 158539028
Conc: 564.52 ng/ml

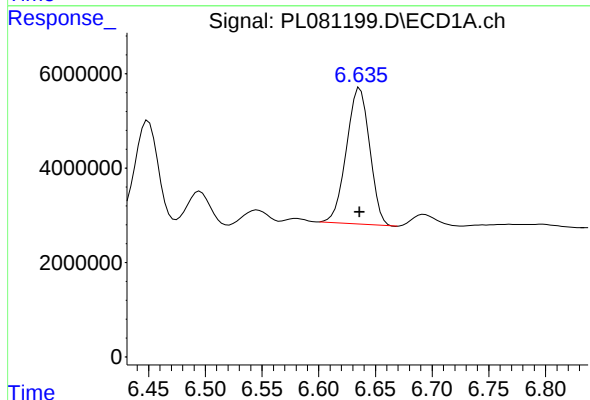


#27 Chlordane-5

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 40971847
Conc: 543.66 ng/ml

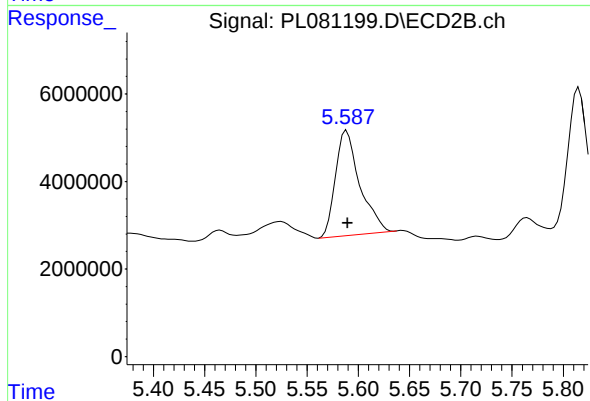

#27 Chlordane-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 39611736
Conc: 573.38 ng/ml

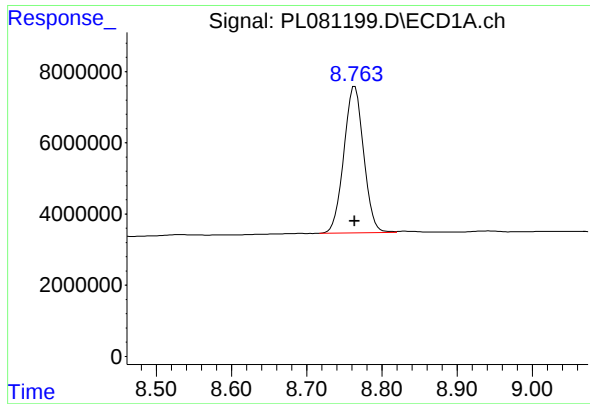

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 75352147
Conc: 48.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030223

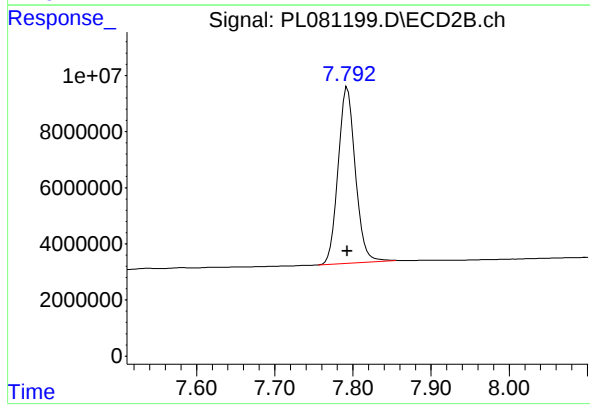

#28 Decachlorobiphenyl

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 96361170
Conc: 49.03 ng/ml