

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030320\  
 Data File : PL056964.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Mar 2020 20:08  
 Operator : AJ\MA  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 99 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 04 04:34:24 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030320.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Mar 04 03:55:01 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds


| Target Compounds |              |       |        |         |          |              |
|------------------|--------------|-------|--------|---------|----------|--------------|
| 4) MA            | Heptachlor   | 0.000 | 5.139  | 0       | 18626899 | N.D. 5.985 # |
| 15) B            | Endosulfa... | 0.000 | 6.872  | 0       | 1841303  | N.D. 0.656 # |
| 16) A            | 4,4'-DDD     | 0.000 | 6.732f | 0       | 4093920  | N.D. 1.681 # |
| 23)              | Chlordane-1  | 4.333 | 0.000  | 2829598 | 0        | 9.309 N.D. # |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030320\  
Data File : PL056964.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Mar 2020 20:08  
Operator : AJ\MA  
Sample : HEXANE  
Misc :  
ALS Vial : 99 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 04 04:34:24 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030320.M  
Quant Title : GC Extractables  
QLast Update : Wed Mar 04 03:55:01 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

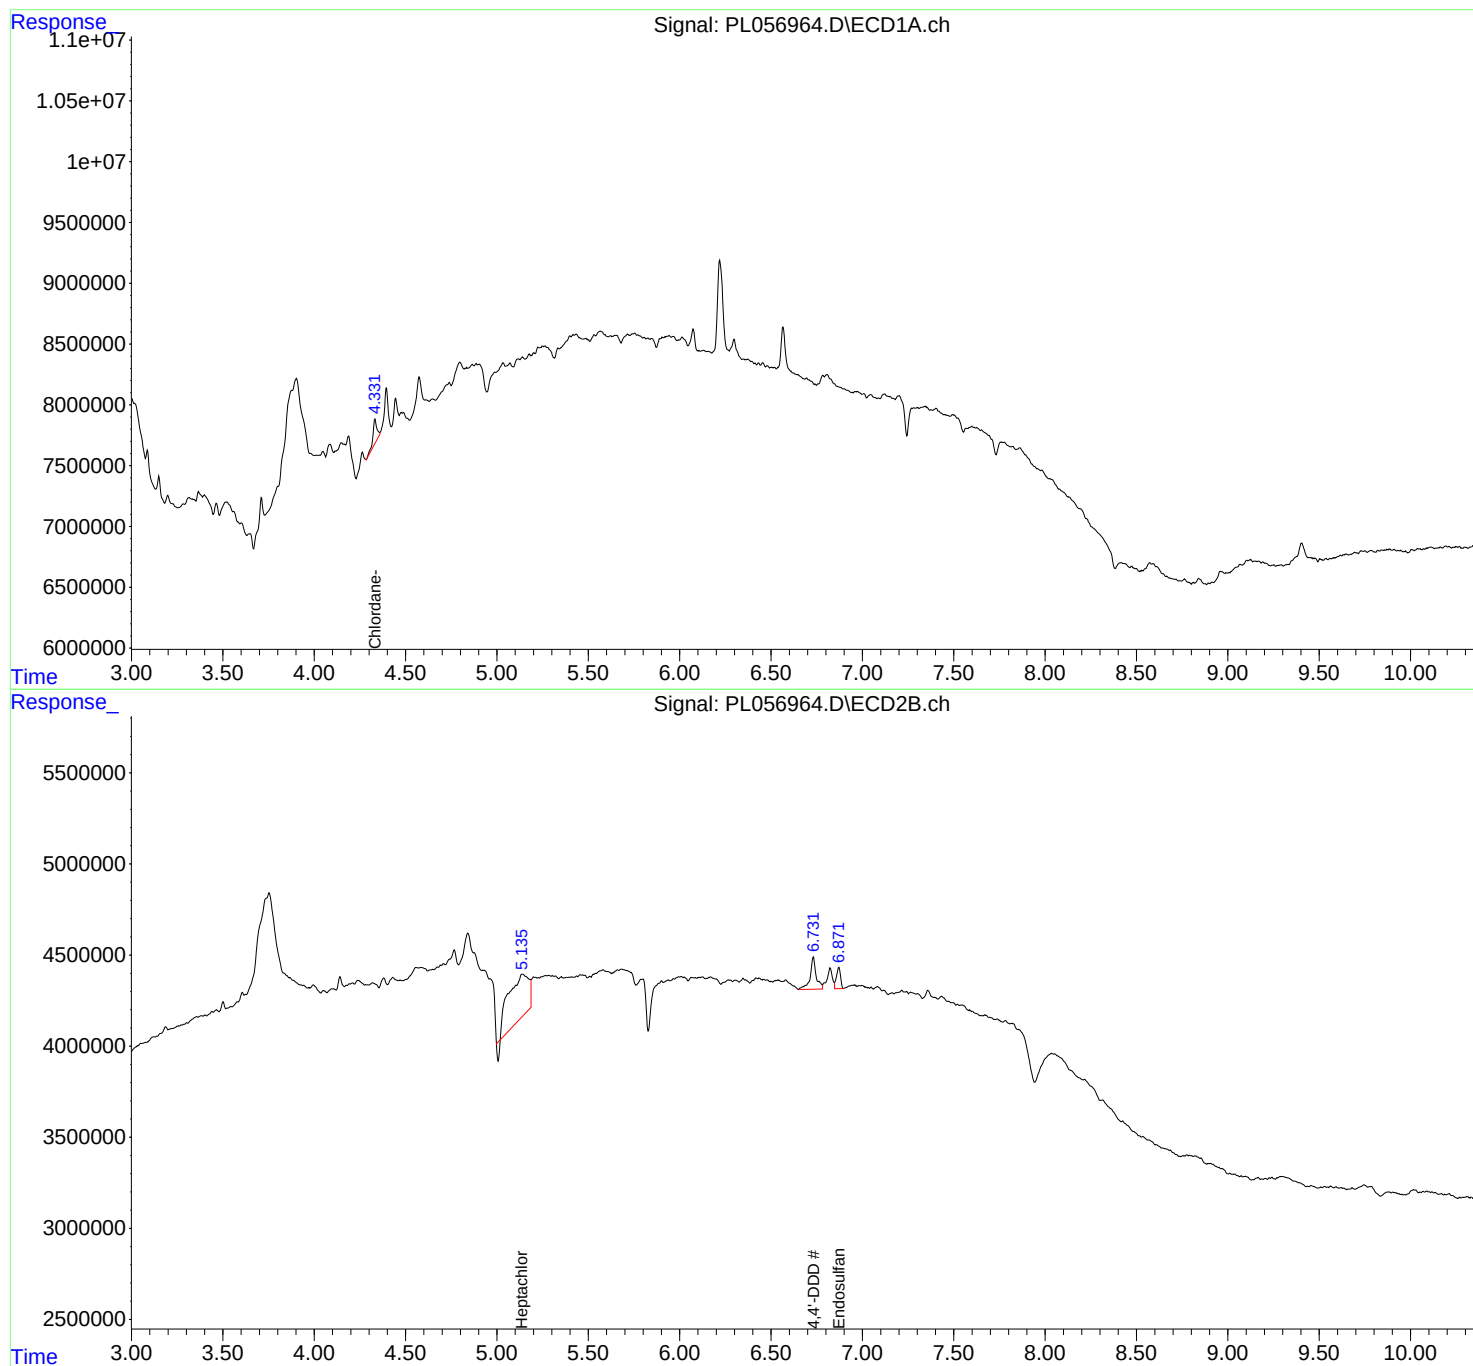

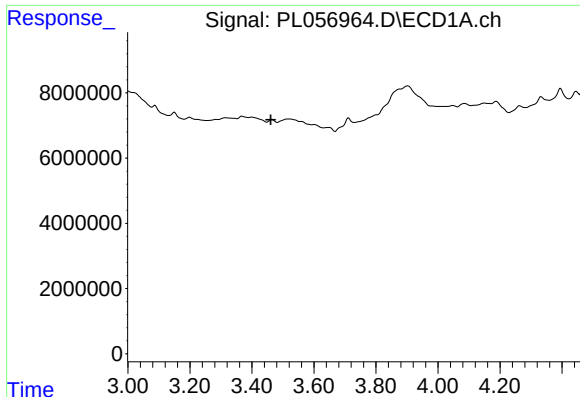


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.461 min  
Response: 0  
Conc: N.D.

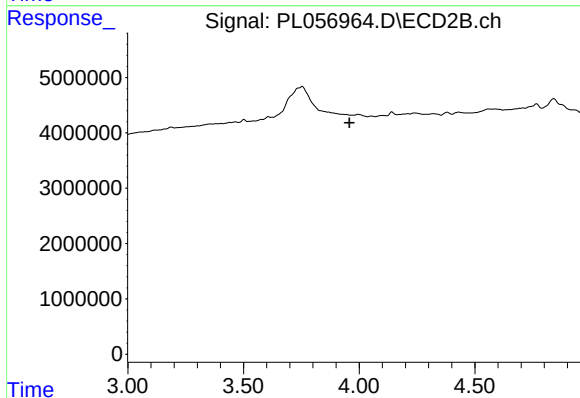


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.958 min  
Response: 0  
Conc: N.D.

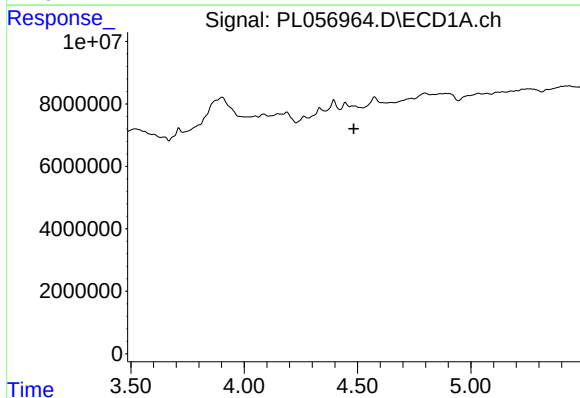


#4 Heptachlor

R.T.: 0.000 min  
Exp R.T. : 4.483 min  
Response: 0  
Conc: N.D.

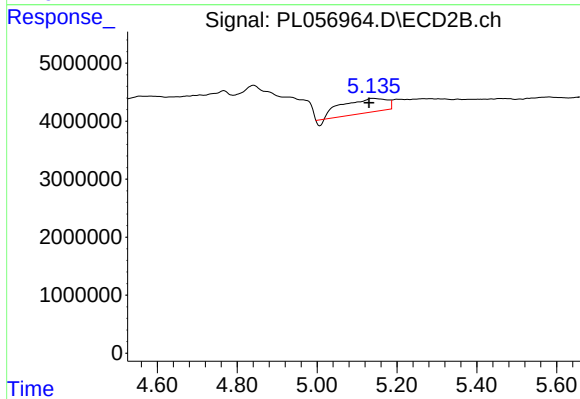


#4 Heptachlor

R.T.: 5.139 min  
Delta R.T.: 0.009 min  
Response: 18626899  
Conc: 5.98 ng/ml

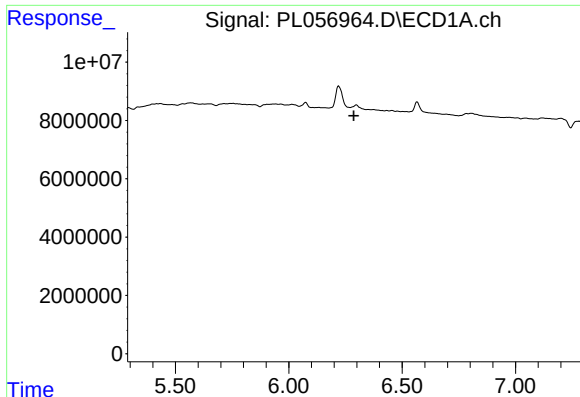


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 6.287 min  
Response: 0  
Conc: N.D.

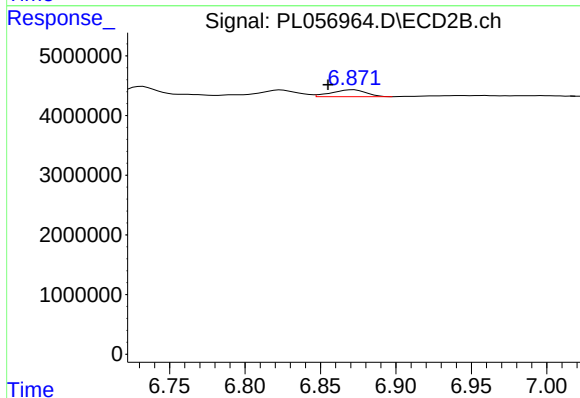


#15 Endosulfan II

R.T.: 6.872 min  
Delta R.T.: 0.017 min  
Response: 1841303  
Conc: 0.66 ng/ml

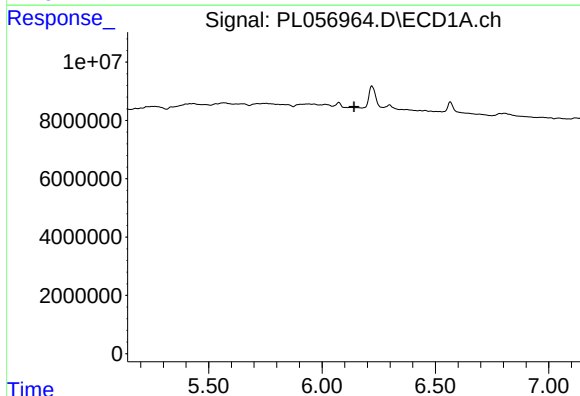


#16 4,4'-DDD

R.T.: 0.000 min  
Exp R.T. : 6.141 min  
Response: 0  
Conc: N.D.

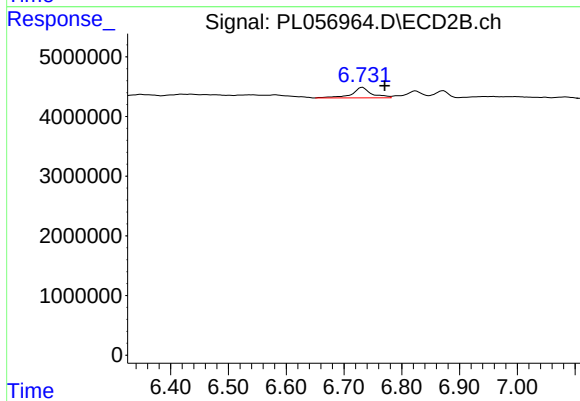


#16 4,4'-DDD

R.T.: 6.732 min  
Delta R.T.: -0.039 min  
Response: 4093920  
Conc: 1.68 ng/ml

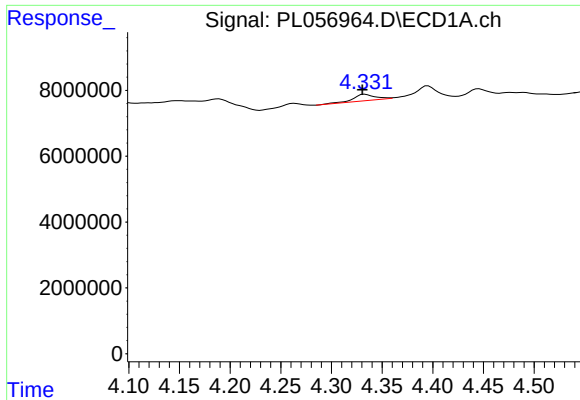


#23 Chlordane-1

R.T.: 4.333 min  
Delta R.T.: 0.002 min  
Response: 2829598  
Conc: 9.31 ng/ml

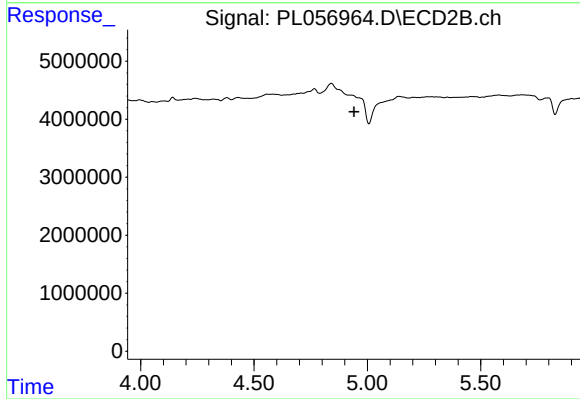


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T. : 4.942 min  
Response: 0  
Conc: N.D.

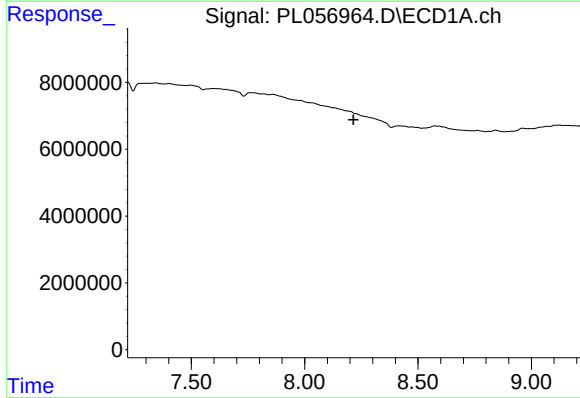

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.216 min  
Response: 0  
Conc: N.D.

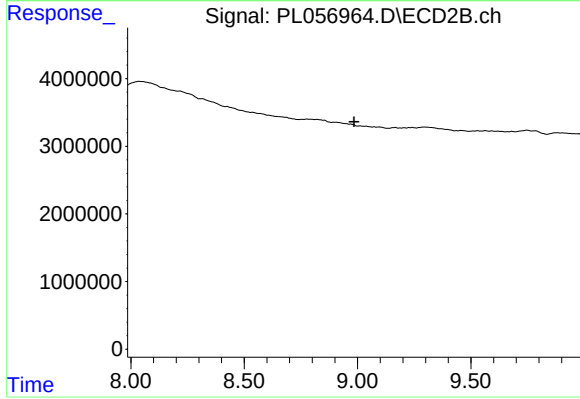

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.984 min  
Response: 0  
Conc: N.D.