

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL056967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2020 20:51
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 04:34:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	192.3E6	48001243	22.565	22.499
28)	SA Decachlor...	8.215	8.983	219.7E6	48735458	22.727	22.937
Target Compounds							
4)	MA Heptachlor	0.000	5.141	0	25756279	N.D.	8.275 #
9)	A Endosulfan I	5.513	6.171	117.4E6	30331195	10.356	10.858
10)	B gamma-Chl...	5.402	6.050	125.7E6	30942369	10.121	10.336
12)	B 4,4'-DDE	5.623	6.281	248.1E6	59535348	21.171	20.978
13)	MA Dieldrin	5.756	6.427	260.3E6	62896467	21.293	21.370
16)	A 4,4'-DDD	0.000	6.731f	0	2871045	N.D.	1.179 #
19)	B Endosulfa...	6.669	7.200	202.9E6	51952763	20.316	20.716
20)	A Methoxychlor	6.926	7.527	562.9E6	139.2E6	112.893	111.383
21)	B Endrin ke...	7.160	7.668	232.9E6	57664756	20.628	21.042
25)	Chlordane-3	5.402	6.050	125.7E6	30942369	116.541	81.645 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL056967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2020 20:51
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 04:34:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

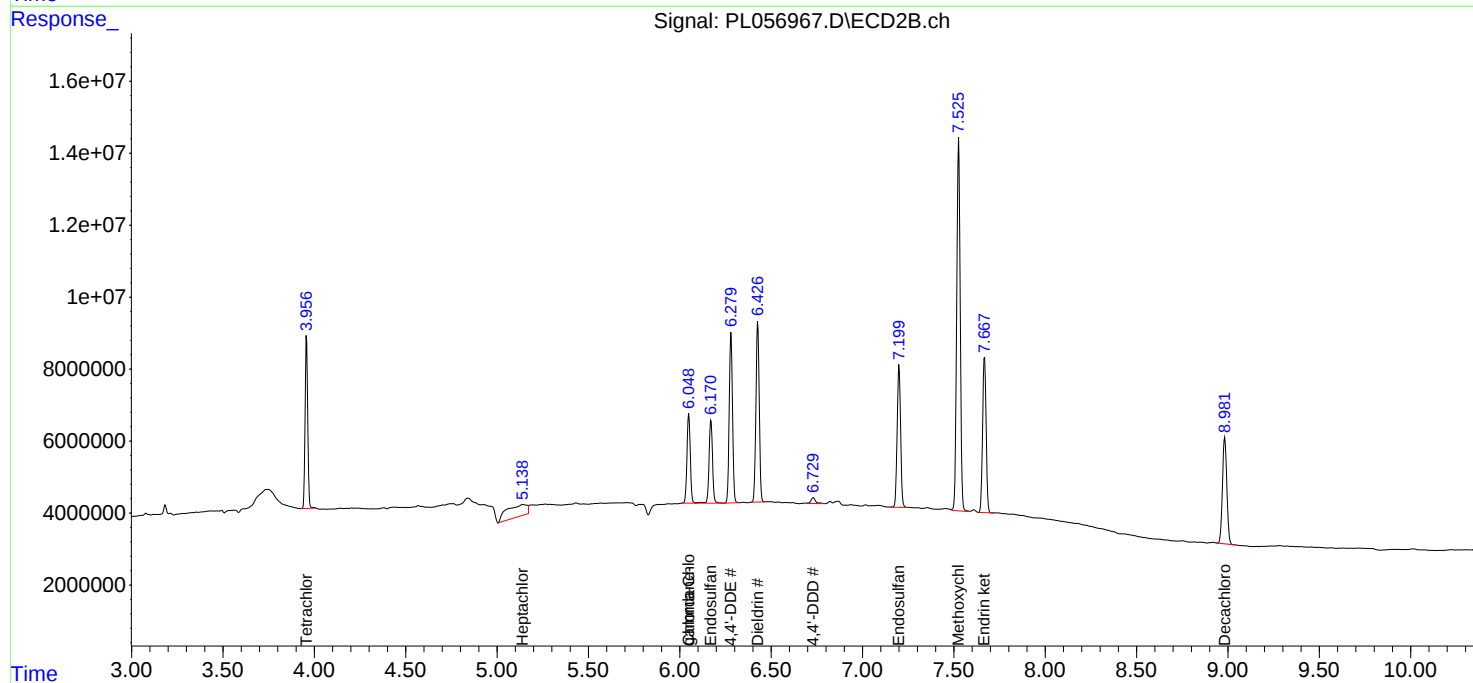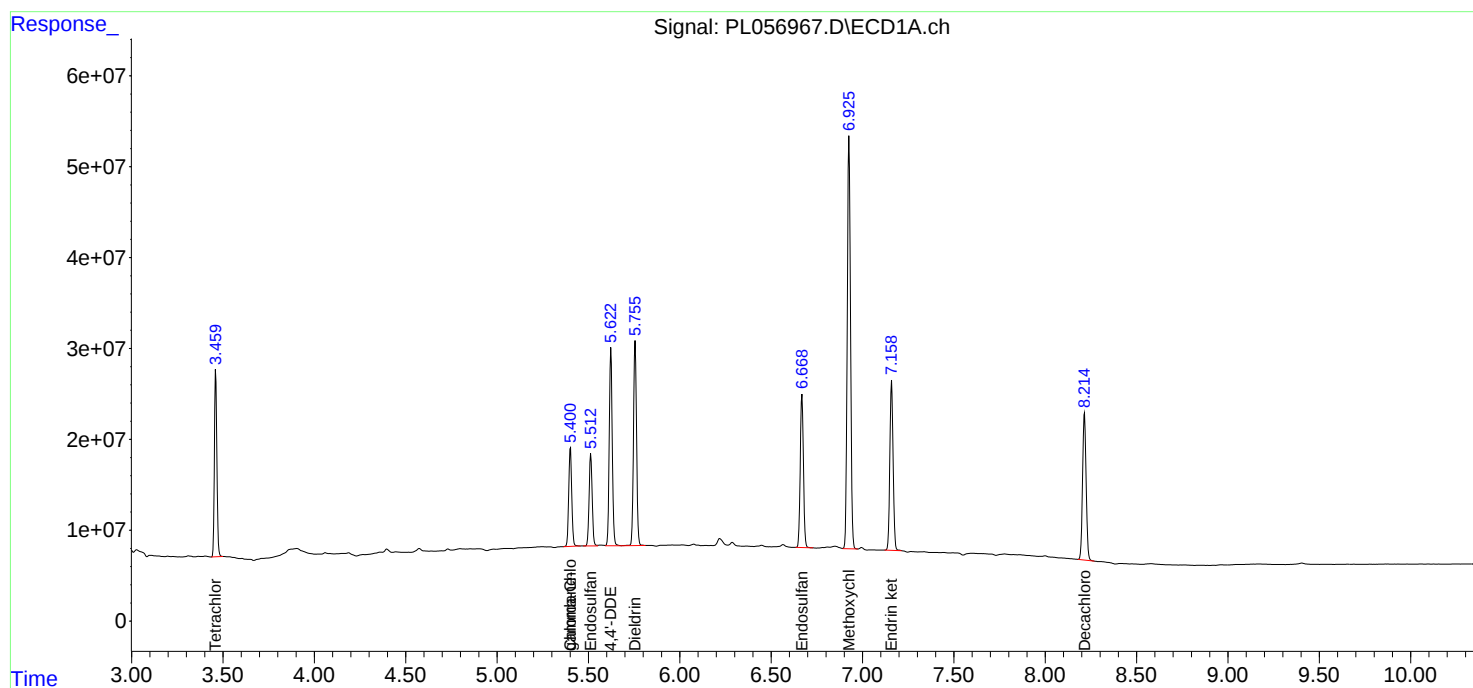

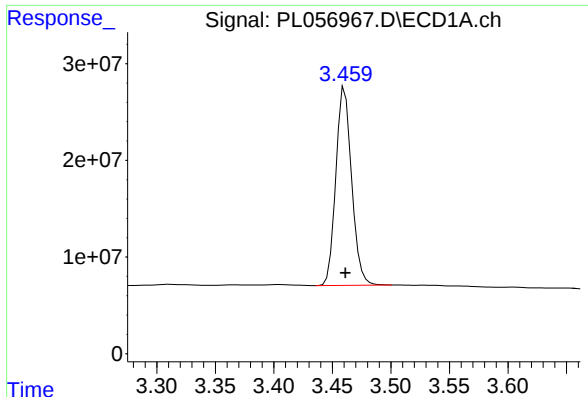


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 192308935
Conc: 22.57 ng/ml

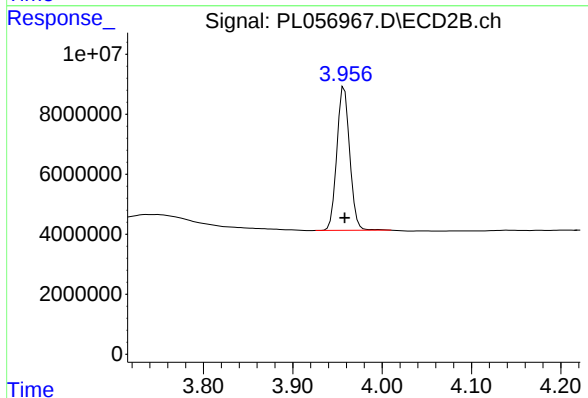


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 48001243
Conc: 22.50 ng/ml

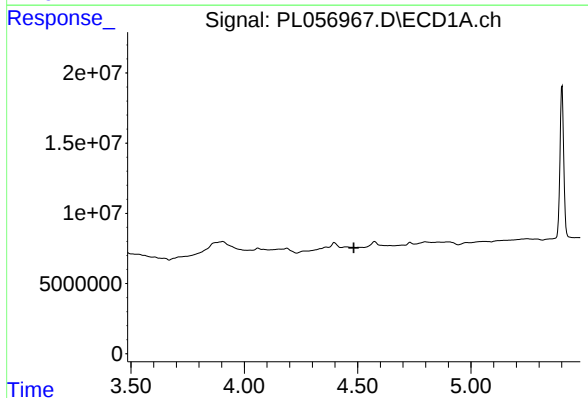


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

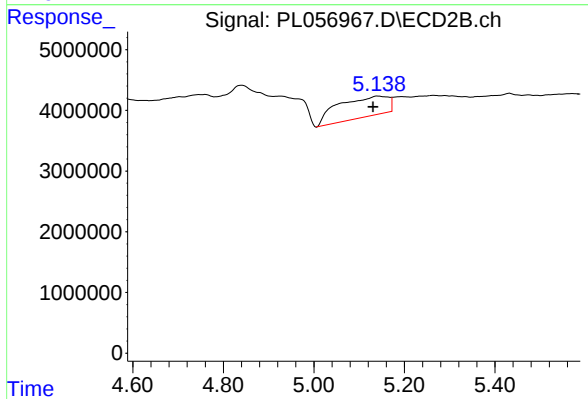


#4 Heptachlor

R.T.: 5.141 min
Delta R.T.: 0.011 min
Response: 25756279
Conc: 8.28 ng/ml

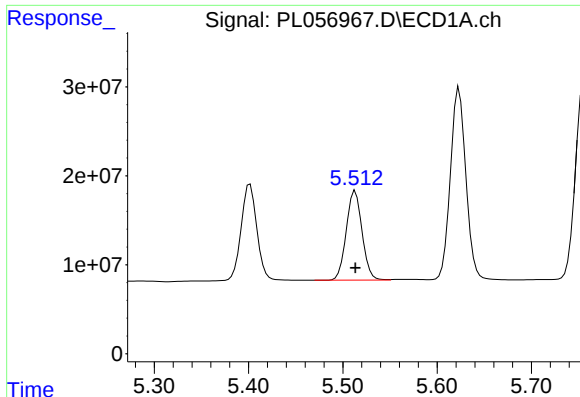


#9 Endosulfan I

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 117394540
Conc: 10.36 ng/ml

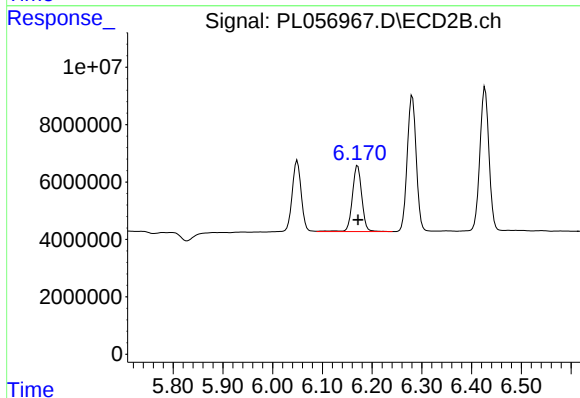


#9 Endosulfan I

R.T.: 6.171 min
Delta R.T.: -0.001 min
Response: 30331195
Conc: 10.86 ng/ml

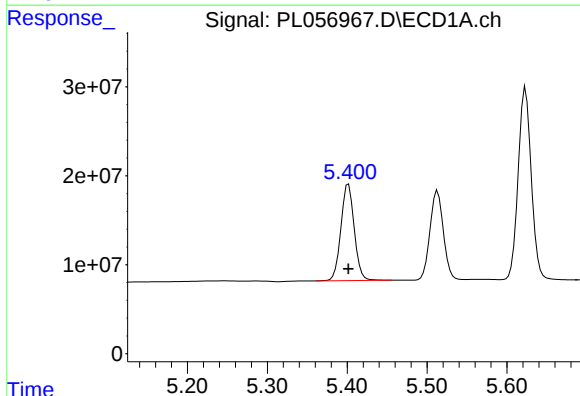


#10 gamma-Chlordane

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 125704299
Conc: 10.12 ng/ml

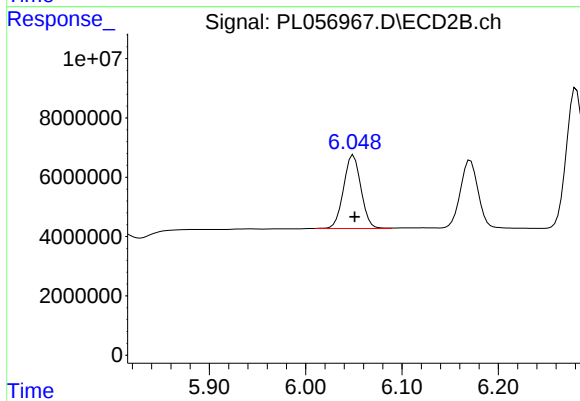


#10 gamma-Chlordane

R.T.: 6.050 min
Delta R.T.: -0.001 min
Response: 30942369
Conc: 10.34 ng/ml

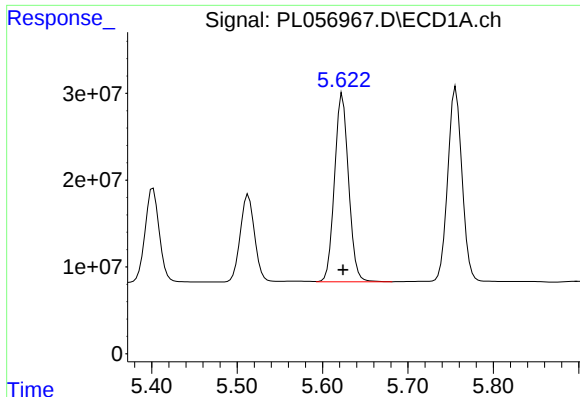


#12 4,4'-DDE

R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 248080221
Conc: 21.17 ng/ml

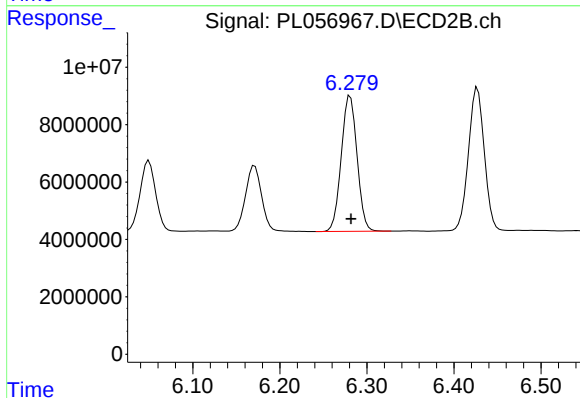


#12 4,4'-DDE

R.T.: 6.281 min
Delta R.T.: 0.000 min
Response: 59535348
Conc: 20.98 ng/ml

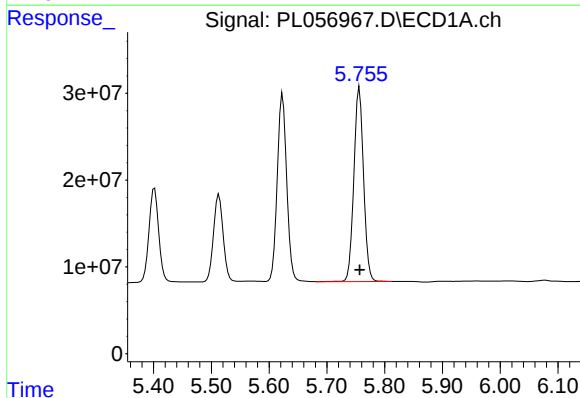


#13 Dieldrin

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 260338059
Conc: 21.29 ng/ml

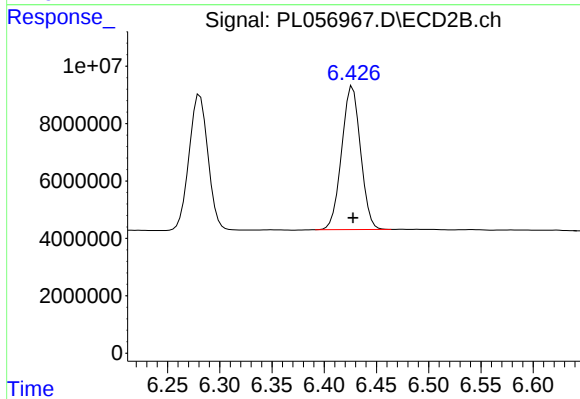


#13 Dieldrin

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 62896467
Conc: 21.37 ng/ml

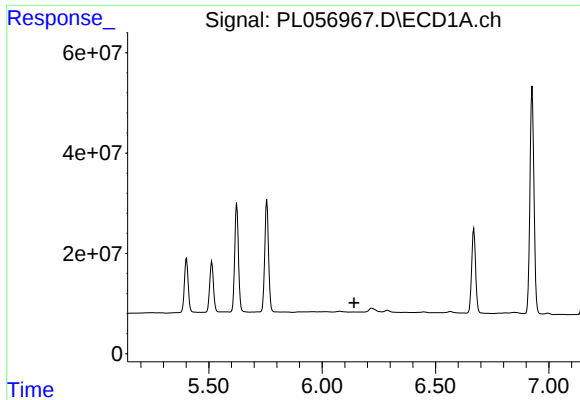


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

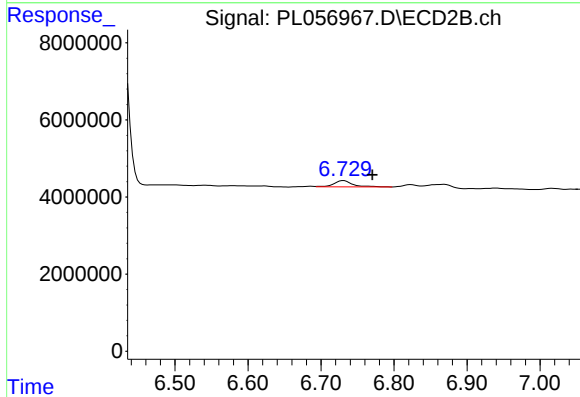


#16 4,4'-DDD

R.T.: 6.731 min
Delta R.T.: -0.040 min
Response: 2871045
Conc: 1.18 ng/ml

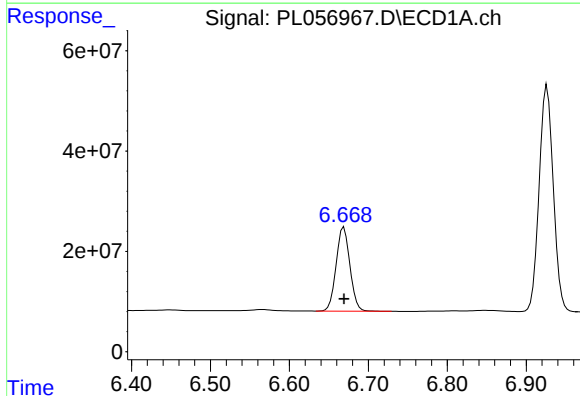


#19 Endosulfan Sulfate

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 202895468
Conc: 20.32 ng/ml

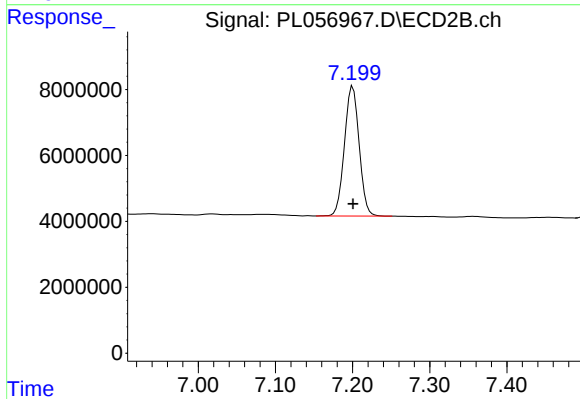


#19 Endosulfan Sulfate

R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 51952763
Conc: 20.72 ng/ml

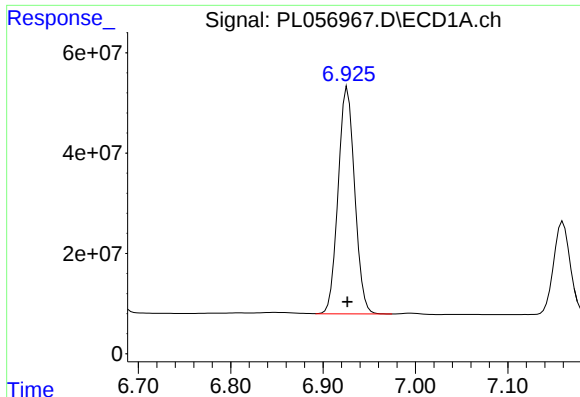


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 562902082
Conc: 112.89 ng/ml

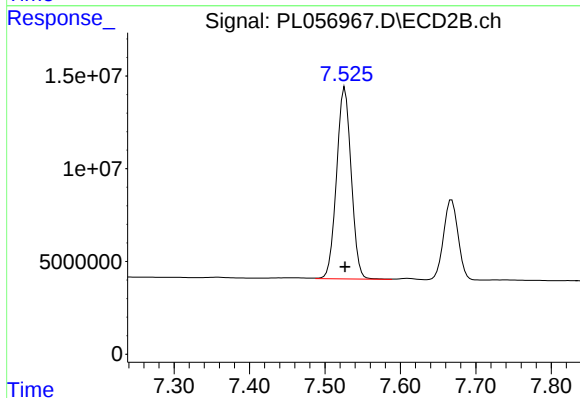


#20 Methoxychlor

R.T.: 7.527 min
Delta R.T.: 0.000 min
Response: 139152271
Conc: 111.38 ng/ml

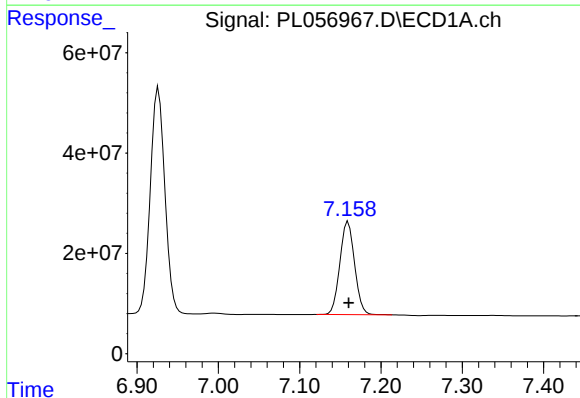


#21 Endrin ketone

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 232946210
Conc: 20.63 ng/ml

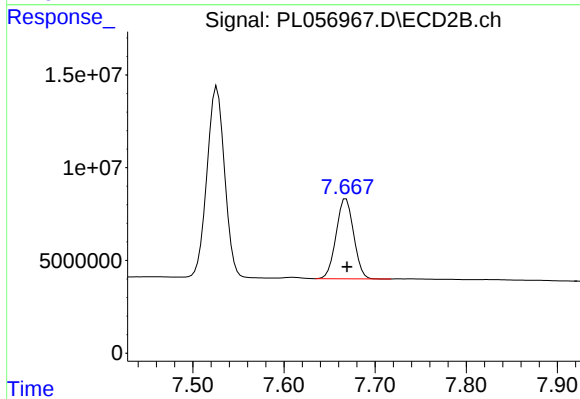


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: -0.001 min
Response: 57664756
Conc: 21.04 ng/ml

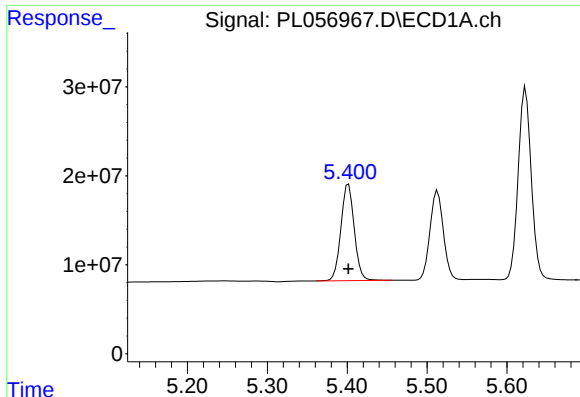


#25 Chlordane-3

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 125704299
Conc: 116.54 ng/ml

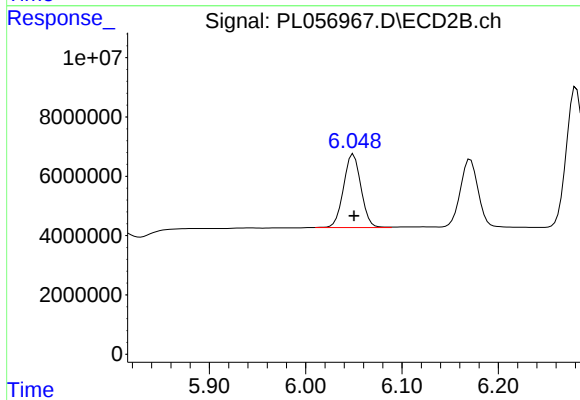


#25 Chlordane-3

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 30942369
Conc: 81.64 ng/ml

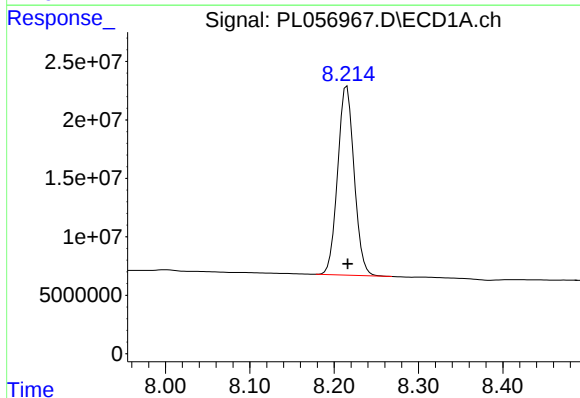

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.000 min
Response: 219656826
Conc: 22.73 ng/ml

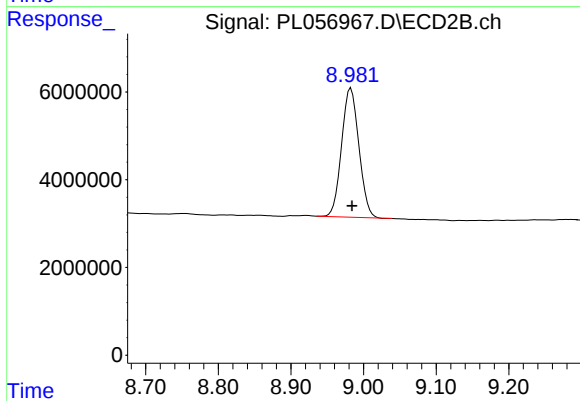

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: -0.002 min
Response: 48735458
Conc: 22.94 ng/ml