

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL056970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2020 21:33
 Operator : AJ\MA
 Sample : PSTDICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 02:57:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 02:56:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	425.2E6	104.4E6	50.000	50.000
28)	SA Decachlor...	8.216	8.984	470.6E6	102.7E6	50.000	50.000
Target Compounds							
2)	A alpha-BHC	3.898	4.345	744.0E6	158.0E6	50.000	50.000
3)	MA gamma-BHC...	4.182	4.627	684.3E6	153.1E6	50.000	50.000
4)	MA Heptachlor	4.483	5.131	680.8E6	151.7E6	50.000	50.000
5)	MB Aldrin	4.731	5.432	653.7E6	147.6E6	50.000	50.000
6)	B beta-BHC	4.434	4.800	260.6E6	67784038	50.000	50.000
7)	B delta-BHC	4.638	5.014	663.8E6	126.9E6	50.000	50.000
8)	B Heptachlo...	5.174	5.817	605.5E6	134.8E6	50.000	50.000
9)	A Endosulfan I	5.513	6.172	570.3E6	135.0E6	50.000	50.000
10)	B gamma-Chl...	5.402	6.051	620.5E6	146.5E6	50.000	50.000
11)	B alpha-Chl...	5.460	6.123	613.7E6	146.7E6	50.000	50.000
12)	B 4,4'-DDE	5.624	6.282	591.7E6	139.7E6	50.000	50.000
13)	MA Dieldrin	5.757	6.428	612.8E6	144.7E6	50.000	50.000
14)	MA Endrin	6.014	6.645	547.0E6	125.8E6	50.000	50.000
15)	B Endosulfa...	6.287	6.855	533.3E6	132.2E6	50.000	50.000
16)	A 4,4'-DDD	6.141	6.771	489.3E6	119.2E6	50.000	50.000
17)	MA 4,4'-DDT	6.381	7.068	499.1E6	122.3E6	50.000	50.000
18)	B Endrin al...	6.456	6.979	441.8E6	112.6E6	50.000	50.000
19)	B Endosulfa...	6.669	7.201	499.1E6	122.8E6	50.000	50.000
20)	A Methoxychlor	6.926	7.527	249.3E6	62099548	50.000	50.000
21)	B Endrin ke...	7.160	7.669	564.3E6	134.5E6	50.000	50.000
22)	Mirex	7.348	8.119	396.4E6	93031121	50.000	50.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL056970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2020 21:33
Operator : AJ\MA
Sample : PSTDICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 02:57:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 02:56:27 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

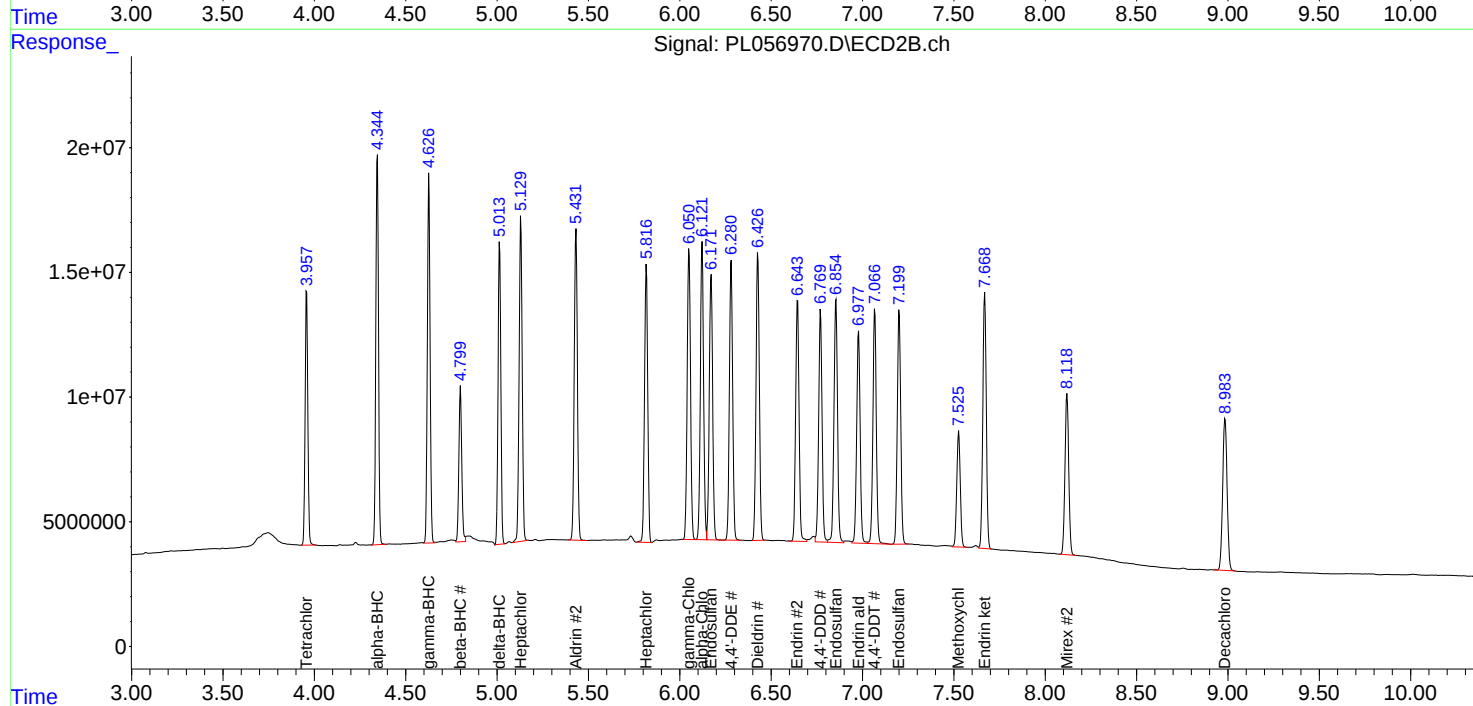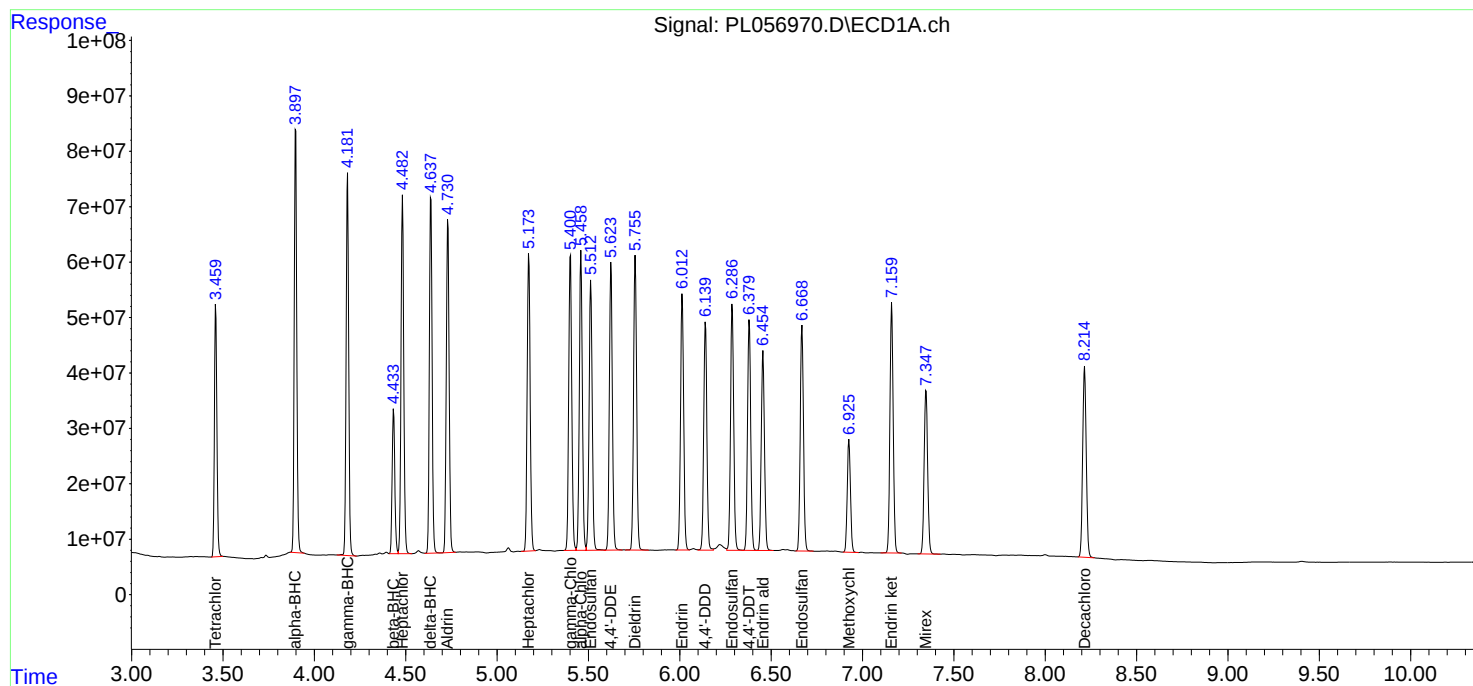

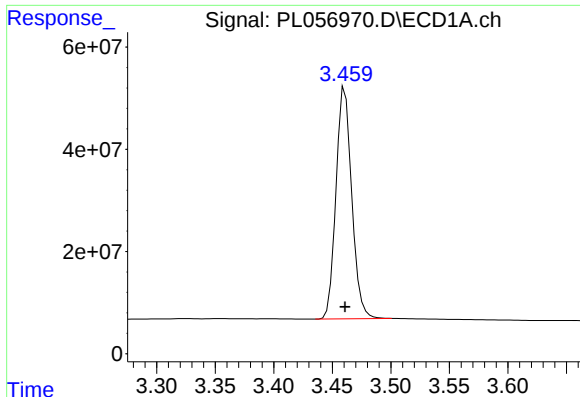


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 425238811
Conc: 50.00 ng/ml

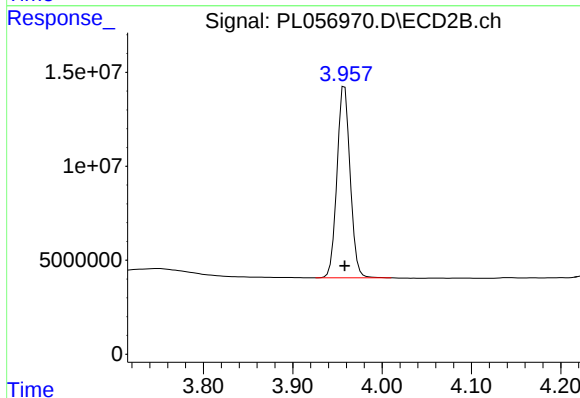


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 104391644
Conc: 50.00 ng/ml

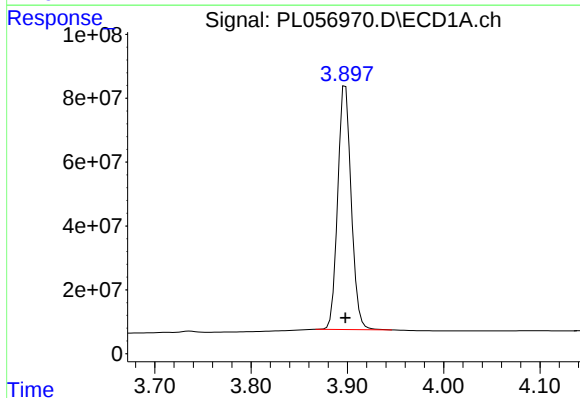


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 744045698
Conc: 50.00 ng/ml

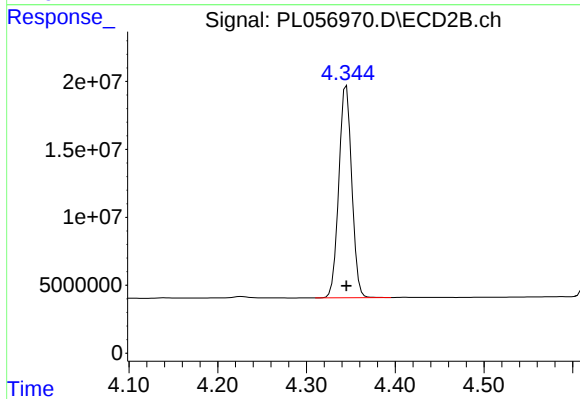


#2 alpha-BHC

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 157961740
Conc: 50.00 ng/ml

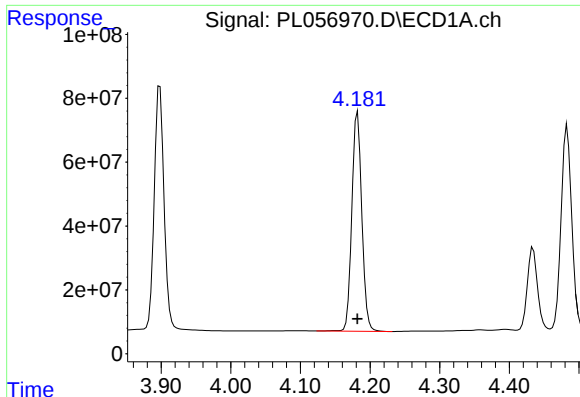


#3 gamma-BHC (Lindane)

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 684252002
Conc: 50.00 ng/ml

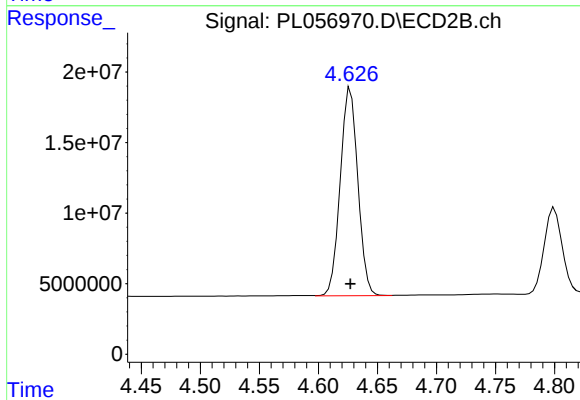


#3 gamma-BHC (Lindane)

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 153104752
Conc: 50.00 ng/ml

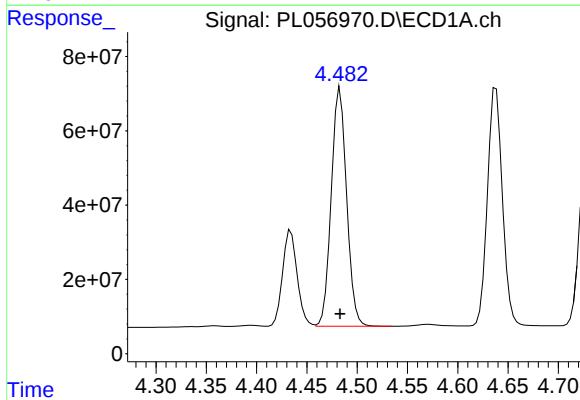


#4 Heptachlor

R.T.: 4.483 min
Delta R.T.: 0.000 min
Response: 680757073
Conc: 50.00 ng/ml

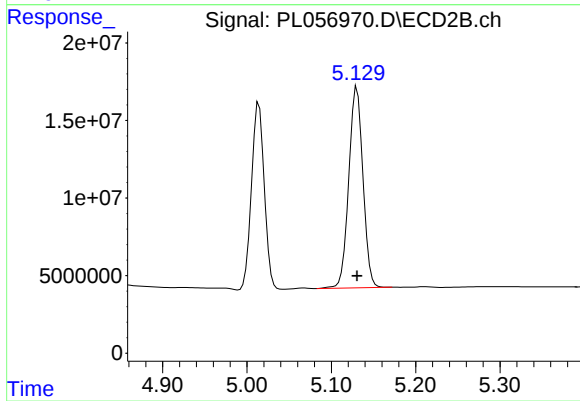


#4 Heptachlor

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 151682874
Conc: 50.00 ng/ml

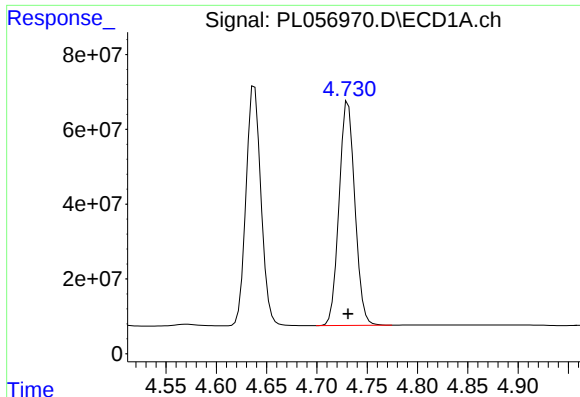


#5 Aldrin

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 653664262
Conc: 50.00 ng/ml

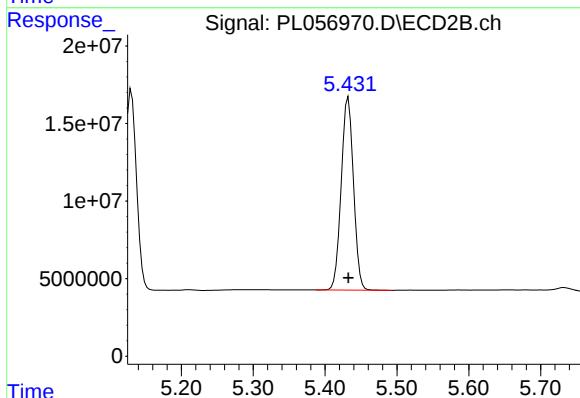


#5 Aldrin

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 147591813
Conc: 50.00 ng/ml

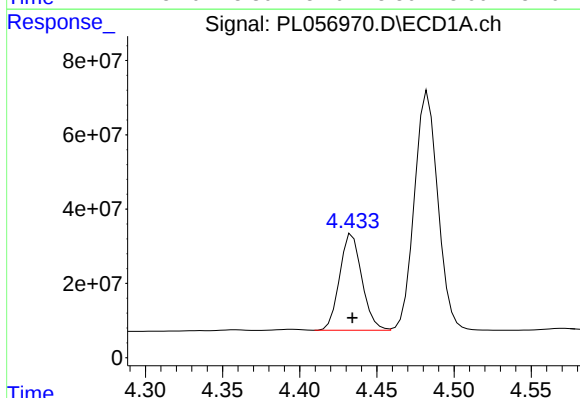


#6 beta-BHC

R.T.: 4.434 min
Delta R.T.: 0.000 min
Response: 260645774
Conc: 50.00 ng/ml

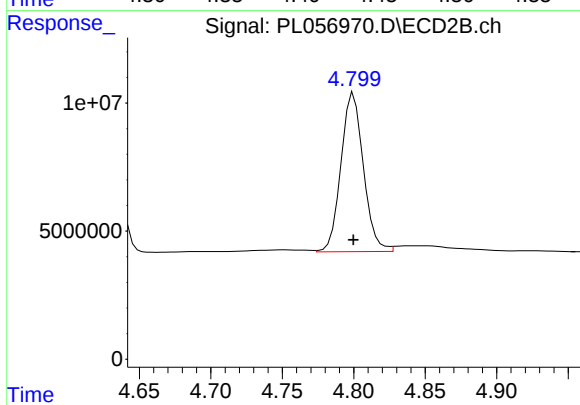


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 67784038
Conc: 50.00 ng/ml

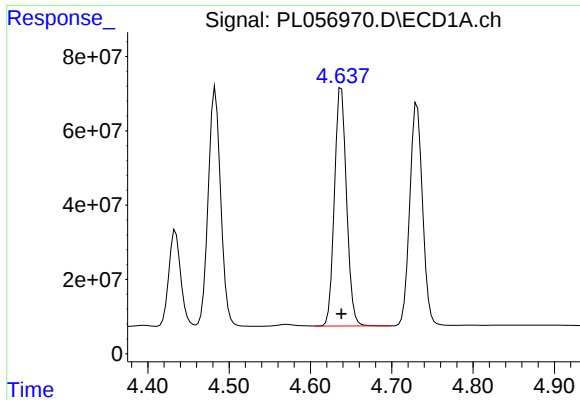


#7 delta-BHC

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 663821545
Conc: 50.00 ng/ml

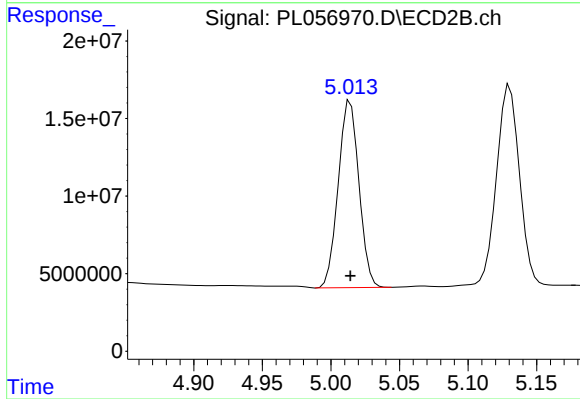


#7 delta-BHC

R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 126942247
Conc: 50.00 ng/ml

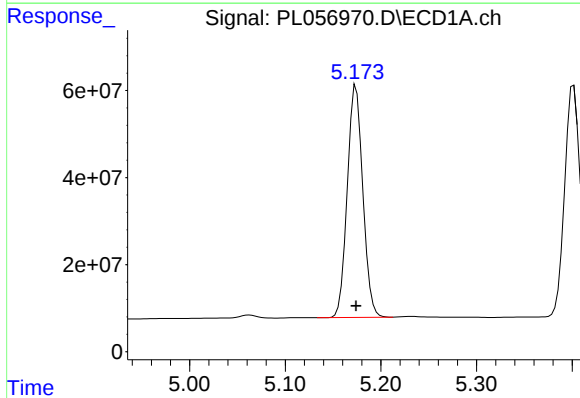


#8 Heptachlor epoxide

R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 605531431
Conc: 50.00 ng/ml

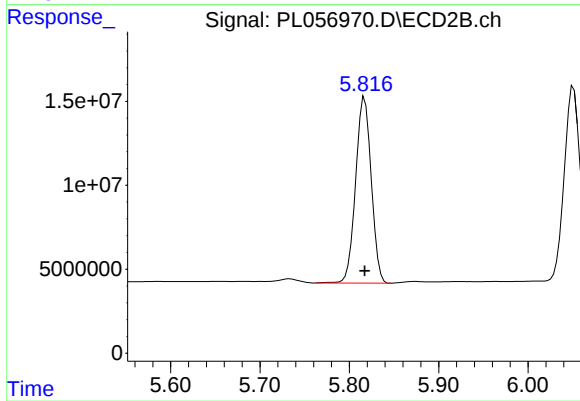


#8 Heptachlor epoxide

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 134753665
Conc: 50.00 ng/ml

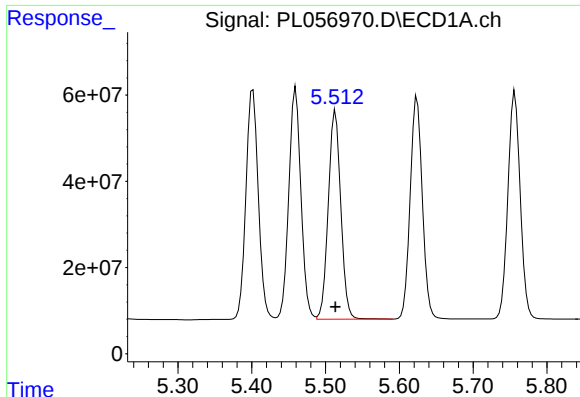


#9 Endosulfan I

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 570328291
Conc: 50.00 ng/ml

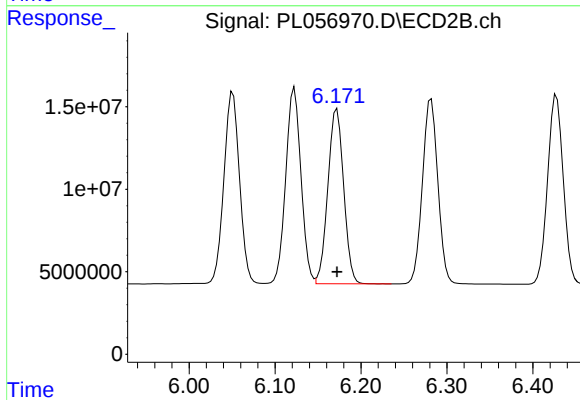


#9 Endosulfan I

R.T.: 6.172 min
Delta R.T.: 0.000 min
Response: 134989998
Conc: 50.00 ng/ml

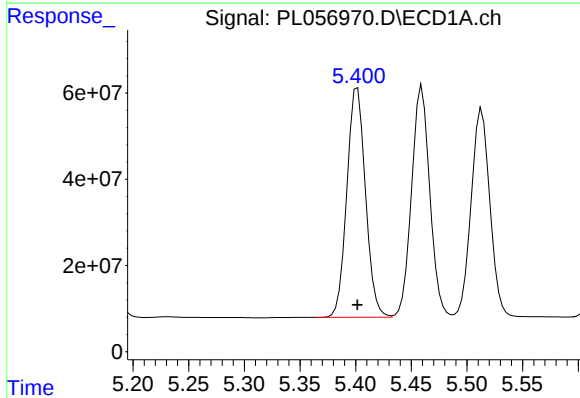


#10 gamma-Chlordane

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 620534432
Conc: 50.00 ng/ml

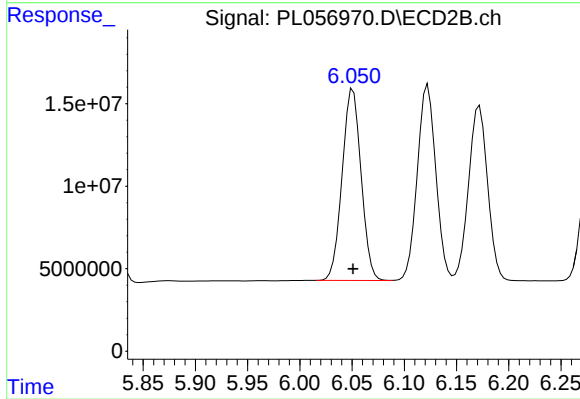


#10 gamma-Chlordane

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 146503471
Conc: 50.00 ng/ml

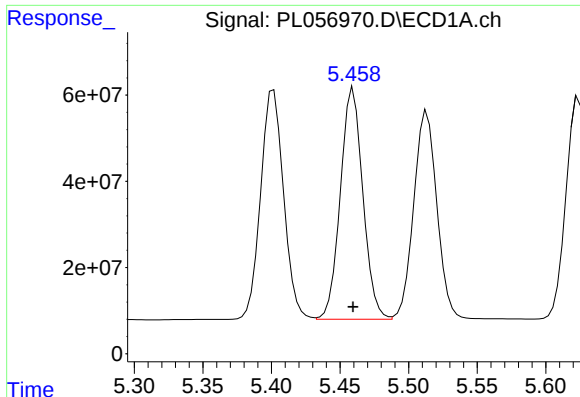


#11 alpha-Chlordane

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 613705834
Conc: 50.00 ng/ml

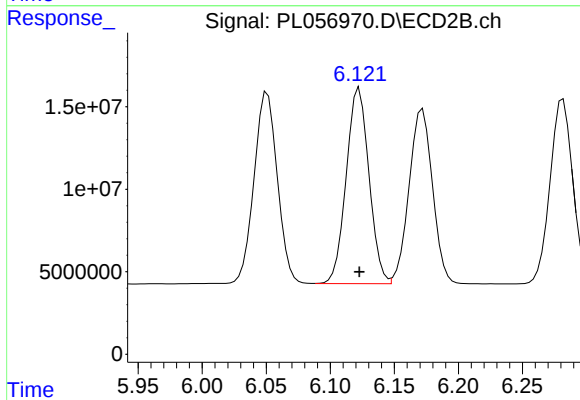


#11 alpha-Chlordane

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 146670591
Conc: 50.00 ng/ml

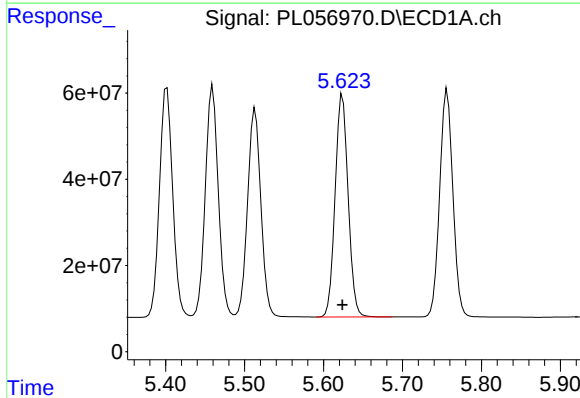


#12 4,4'-DDE

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 591682447
Conc: 50.00 ng/ml

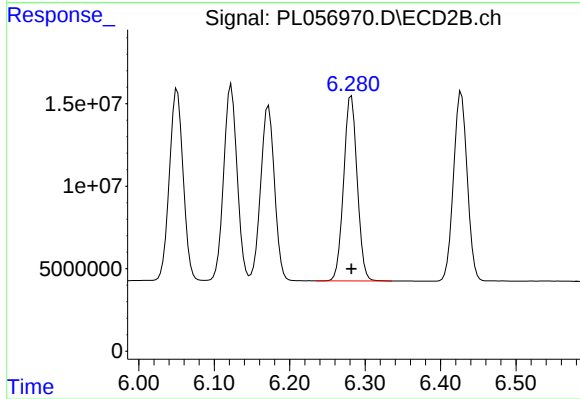


#12 4,4'-DDE

R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 139747781
Conc: 50.00 ng/ml

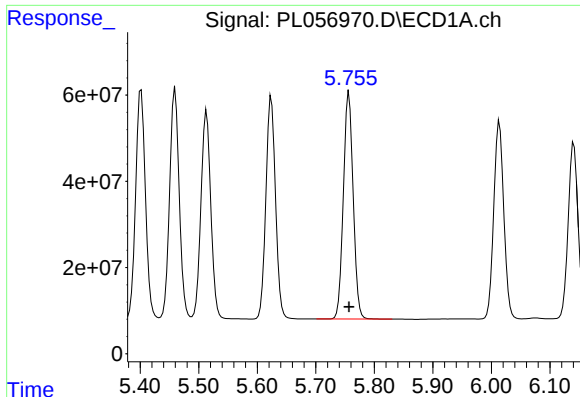


#13 Dieldrin

R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 612797579
Conc: 50.00 ng/ml

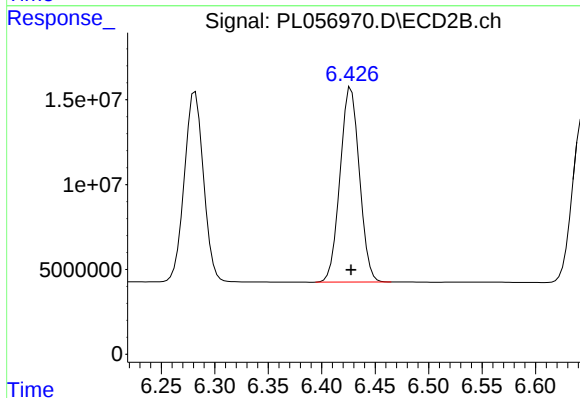


#13 Dieldrin

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 144737068
Conc: 50.00 ng/ml

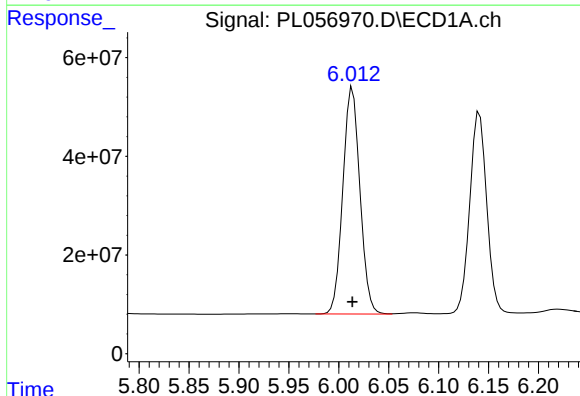


#14 Endrin

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 547044844
Conc: 50.00 ng/ml

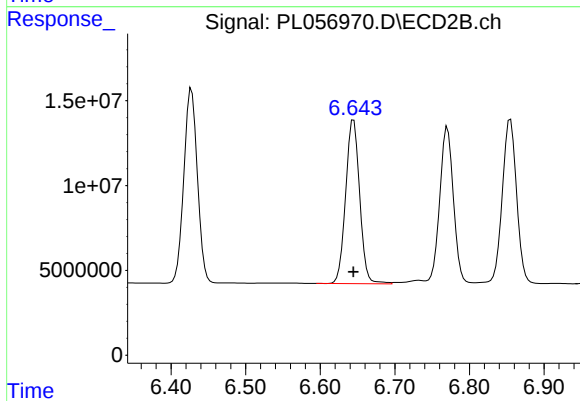


#14 Endrin

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 125801388
Conc: 50.00 ng/ml

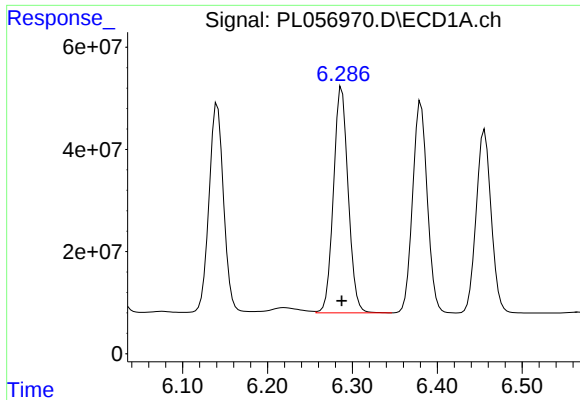


#15 Endosulfan II

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 533323193
Conc: 50.00 ng/ml

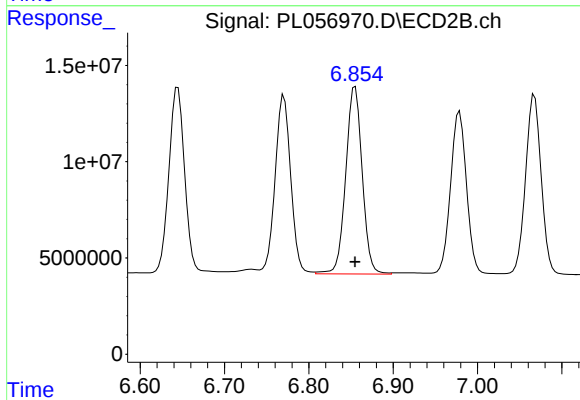


#15 Endosulfan II

R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 132176604
Conc: 50.00 ng/ml

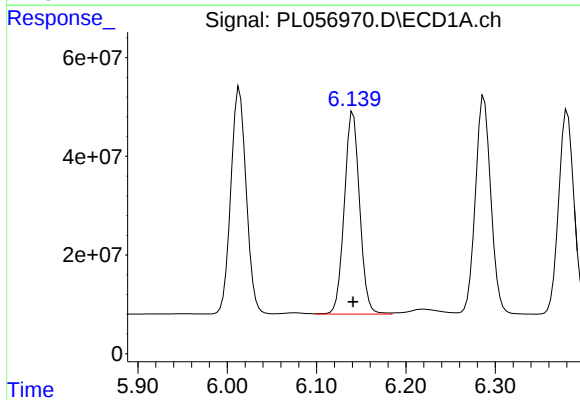


#16 4,4'-DDD

R.T.: 6.141 min
Delta R.T.: 0.000 min
Response: 489262527
Conc: 50.00 ng/ml

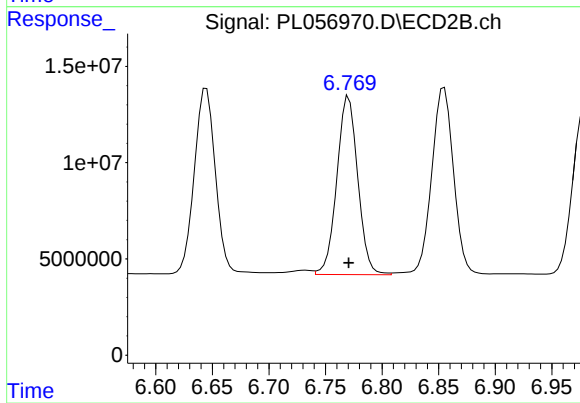


#16 4,4'-DDD

R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 119243115
Conc: 50.00 ng/ml

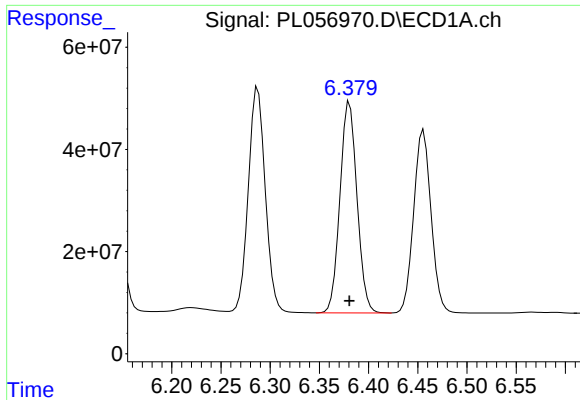


#17 4,4'-DDT

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 499060157
Conc: 50.00 ng/ml

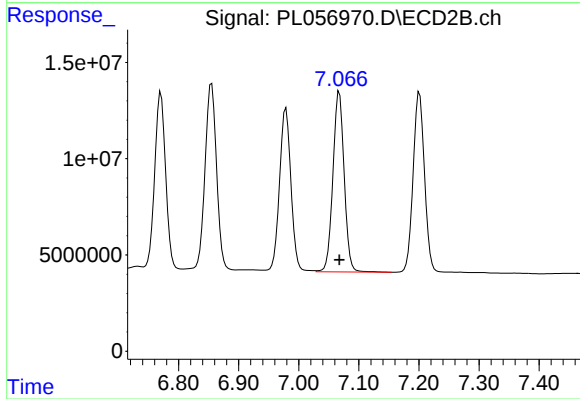


#17 4,4'-DDT

R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 122299867
Conc: 50.00 ng/ml

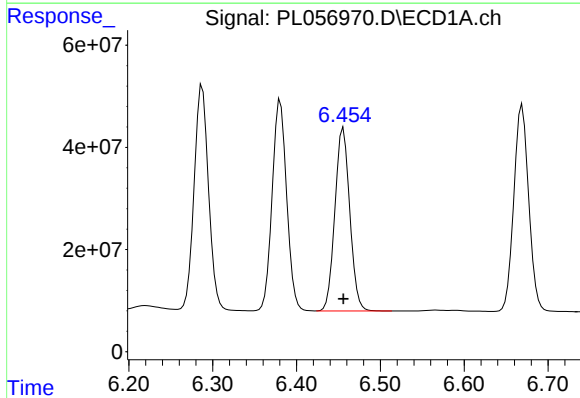


#18 Endrin aldehyde

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 441764809
Conc: 50.00 ng/ml

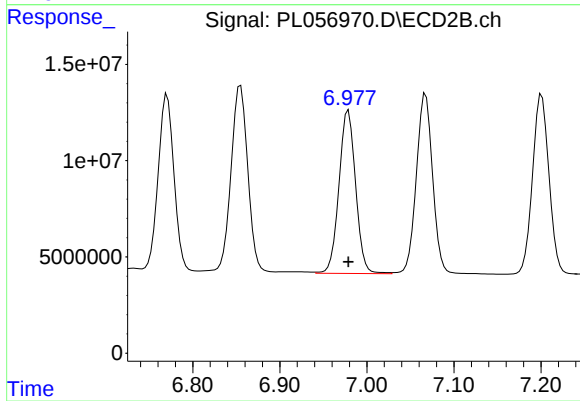


#18 Endrin aldehyde

R.T.: 6.979 min
Delta R.T.: 0.000 min
Response: 112638791
Conc: 50.00 ng/ml

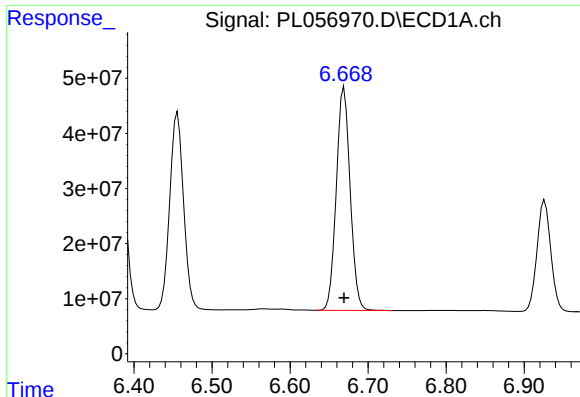


#19 Endosulfan Sulfate

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 499133066
Conc: 50.00 ng/ml

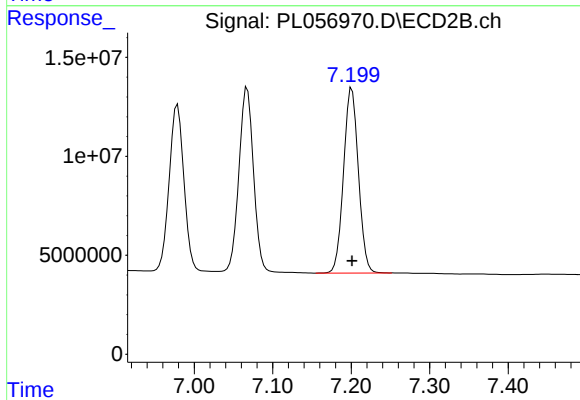


#19 Endosulfan Sulfate

R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 122813405
Conc: 50.00 ng/ml

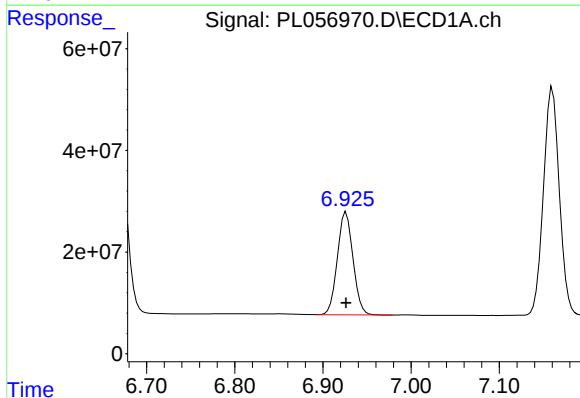


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 249328268
Conc: 50.00 ng/ml

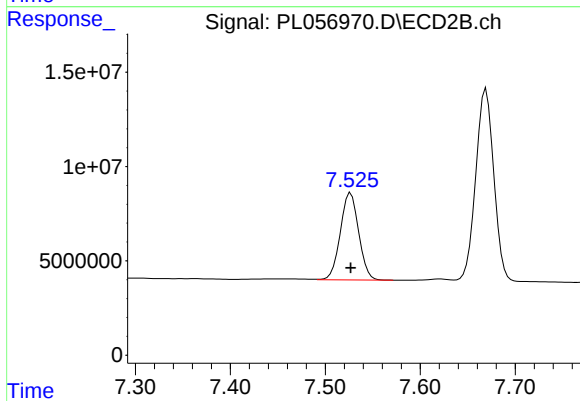


#20 Methoxychlor

R.T.: 7.527 min
Delta R.T.: 0.000 min
Response: 62099548
Conc: 50.00 ng/ml

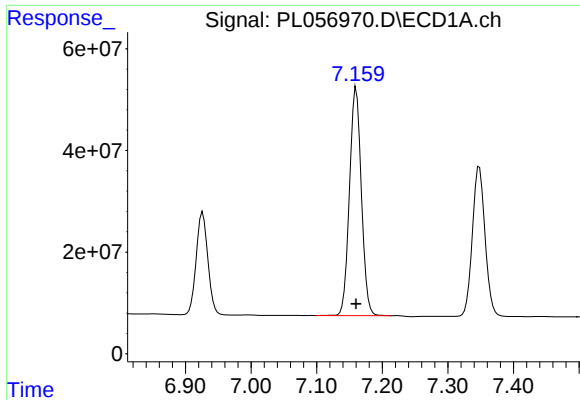


#21 Endrin ketone

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 564332521
Conc: 50.00 ng/ml

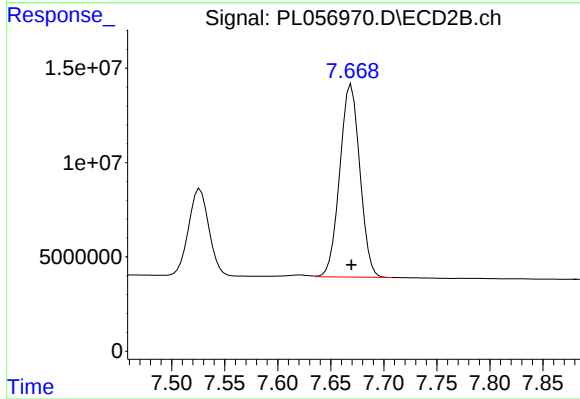


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 134493786
Conc: 50.00 ng/ml

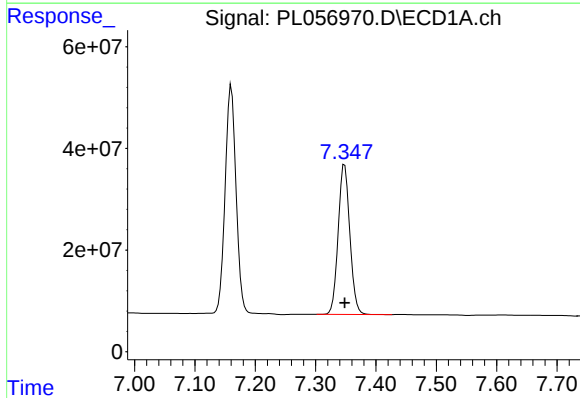


#22 Mirex

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 396405074
Conc: 50.00 ng/ml

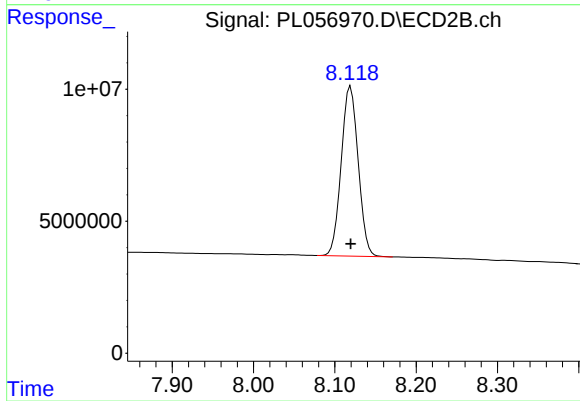


#22 Mirex

R.T.: 8.119 min
Delta R.T.: 0.000 min
Response: 93031121
Conc: 50.00 ng/ml

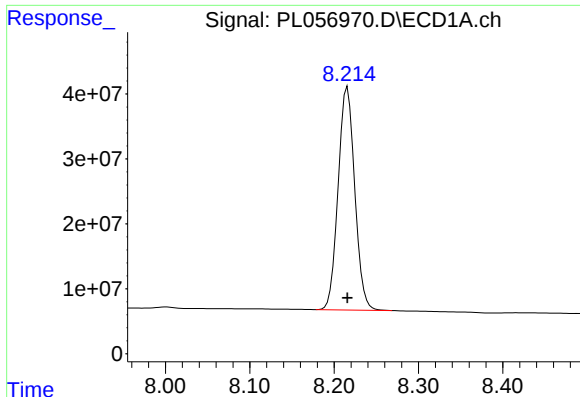

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 470561127
Conc: 50.00 ng/ml

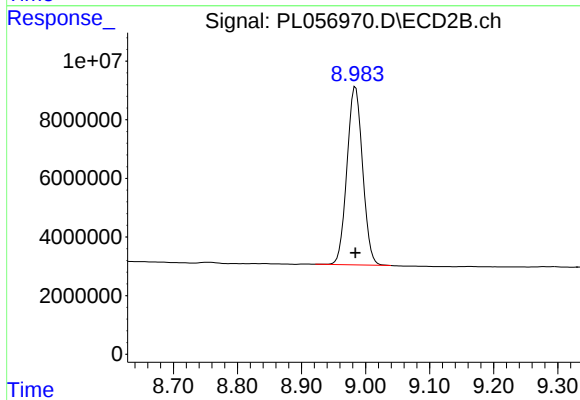

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 102707817
Conc: 50.00 ng/ml