

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL056973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2020 22:16
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 03:52:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:51:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	504.0E6	103.9E6	50.000	50.000
28)	SA Decachlor...	8.214	8.984	477.9E6	103.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.330	4.942	152.0E6	40103368	500.000	500.000
24)	Chlordane-2	4.832	5.407	176.3E6	47727118	500.000	500.000
25)	Chlordane-3	5.402	6.050	539.3E6	189.5E6	500.000	500.000
26)	Chlordane-4	5.459	6.123	459.5E6	229.3E6	500.000	500.000
27)	Chlordane-5	6.295	6.923	181.6E6	41714841	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL056973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2020 22:16
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 03:52:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:51:14 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

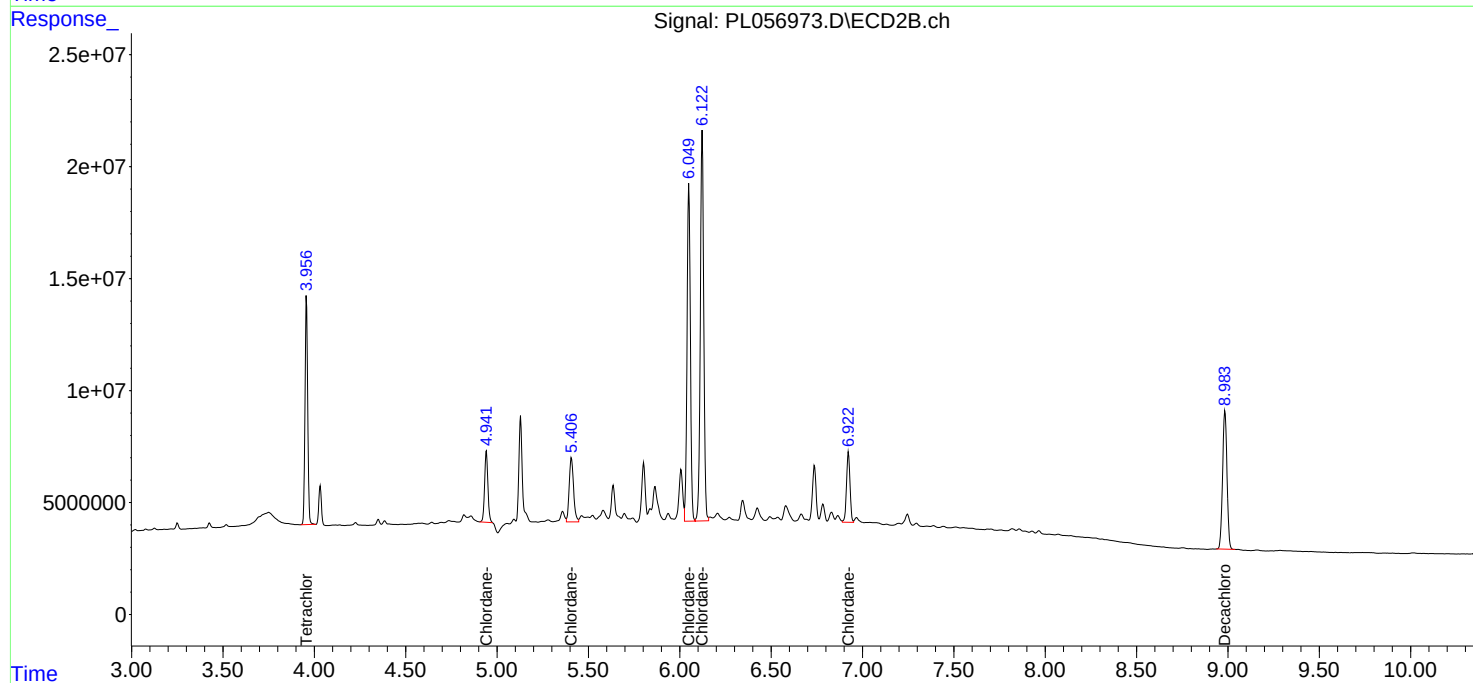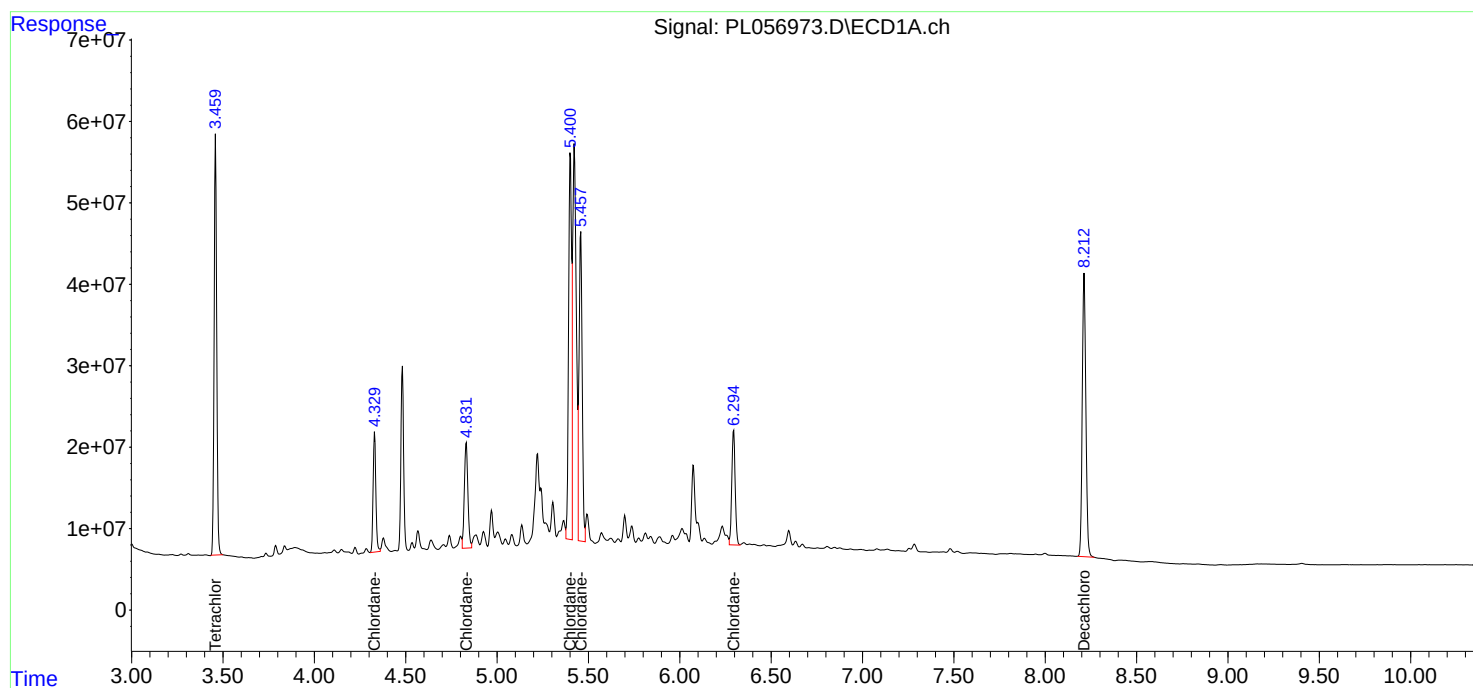

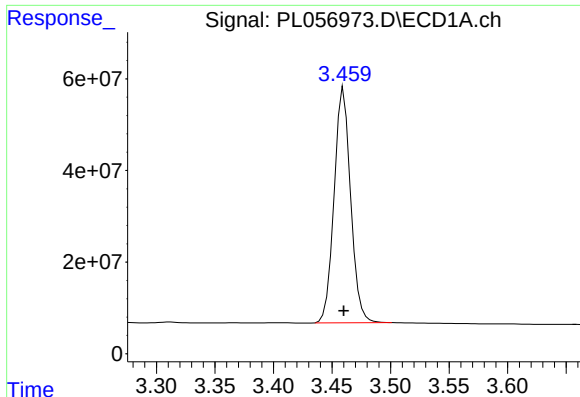


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 503960966
Conc: 50.00 ng/ml

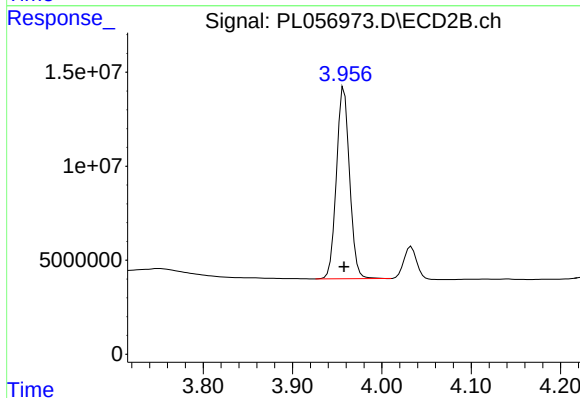


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 103929059
Conc: 50.00 ng/ml

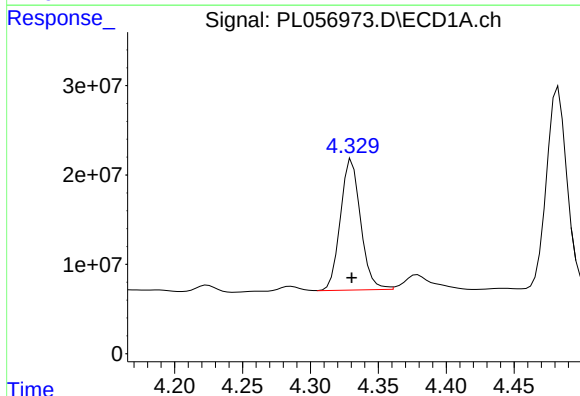


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 151975075
Conc: 500.00 ng/ml

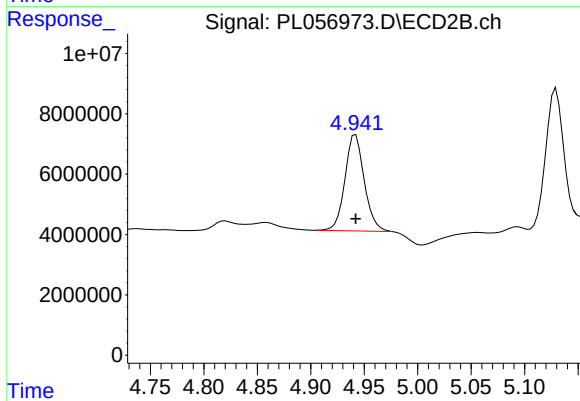


#23 Chlordane-1

R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 40103368
Conc: 500.00 ng/ml

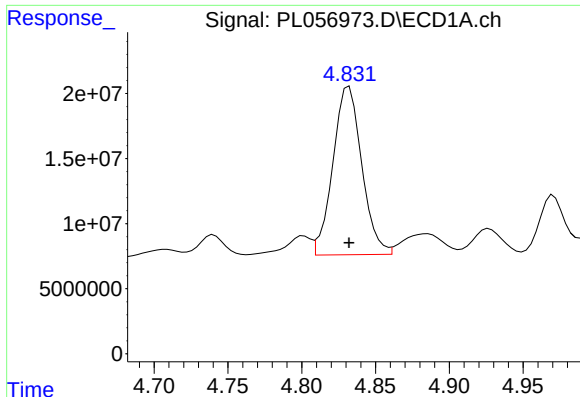


#24 Chlordane-2

R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: 176331733
Conc: 500.00 ng/ml

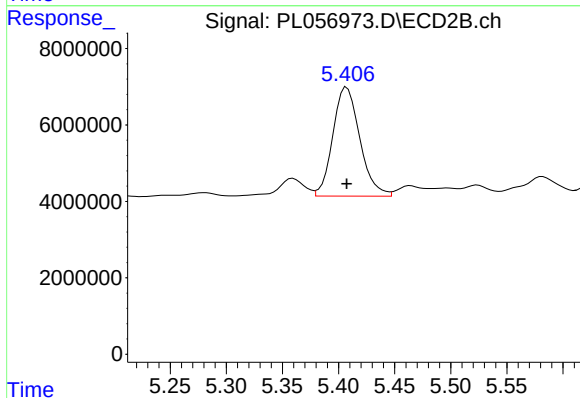


#24 Chlordane-2

R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 47727118
Conc: 500.00 ng/ml

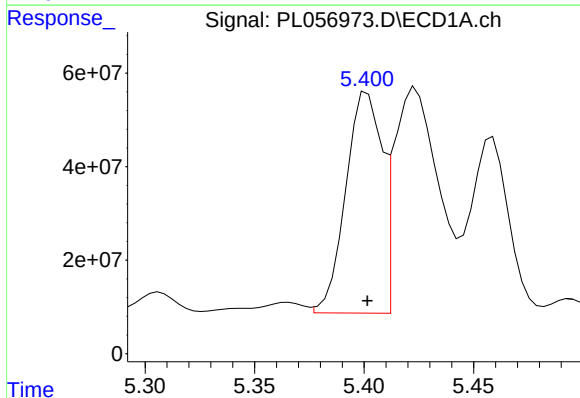


#25 Chlordane-3

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 539315637
Conc: 500.00 ng/ml

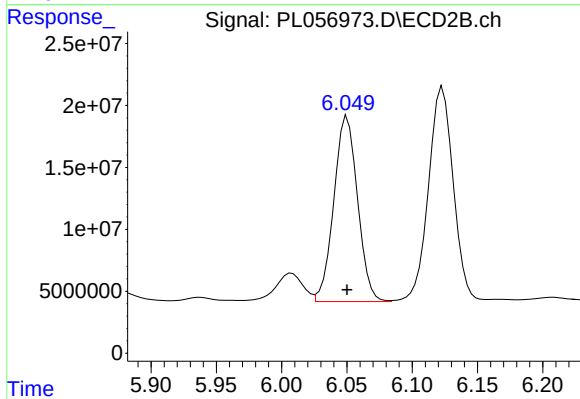


#25 Chlordane-3

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 189494417
Conc: 500.00 ng/ml

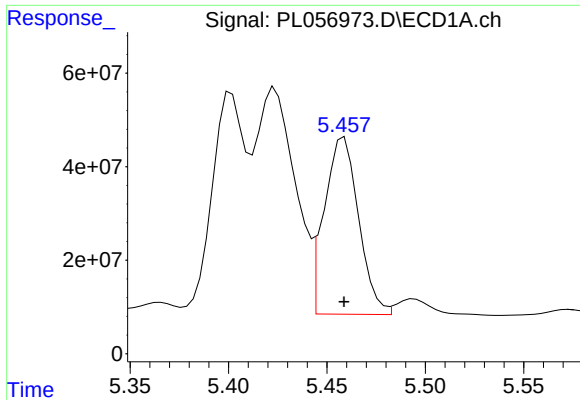


#26 Chlordane-4

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 459496632
Conc: 500.00 ng/ml

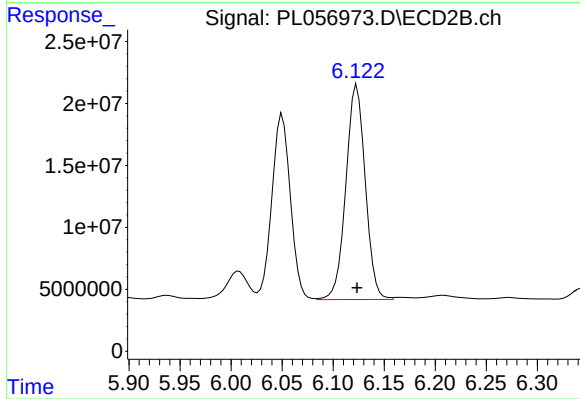


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 229268115
Conc: 500.00 ng/ml

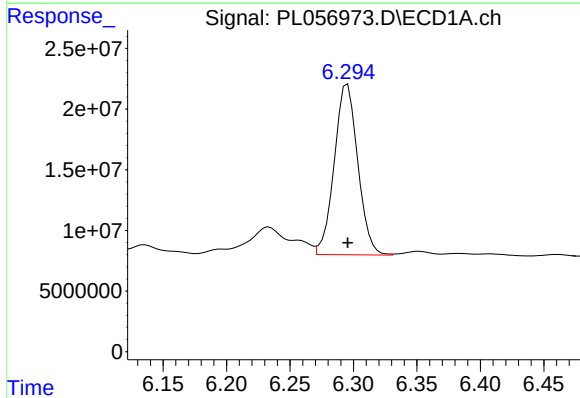


#27 Chlordane-5

R.T.: 6.295 min
Delta R.T.: 0.000 min
Response: 181612352
Conc: 500.00 ng/ml

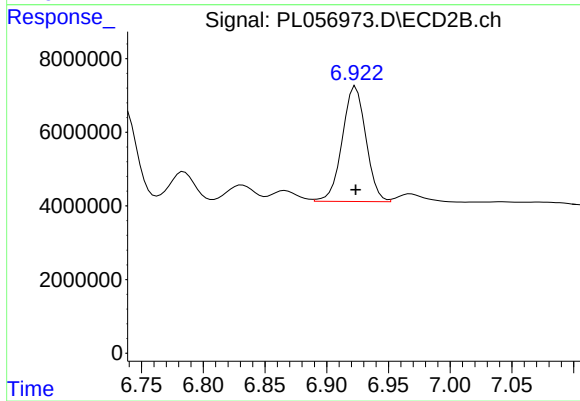


#27 Chlordane-5

R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 41714841
Conc: 500.00 ng/ml

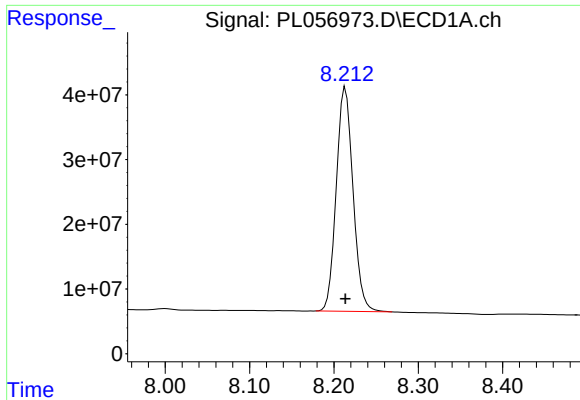

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 477923367
Conc: 50.00 ng/ml

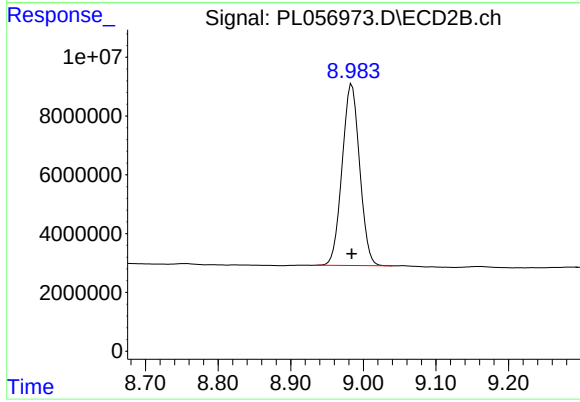

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 103445682
Conc: 50.00 ng/ml